
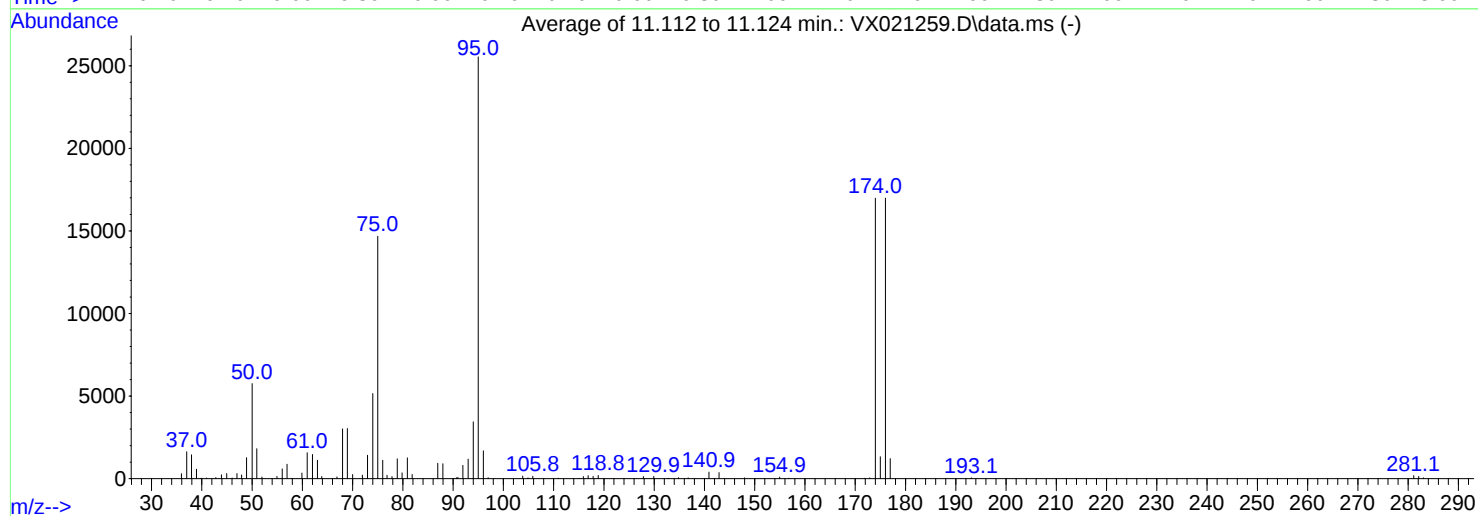


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031721\
Data File : VX021259.D
Acq On : 17 Mar 2021 09:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Title : SW846 8260
Last Update : Tue Mar 16 14:00:21 2021

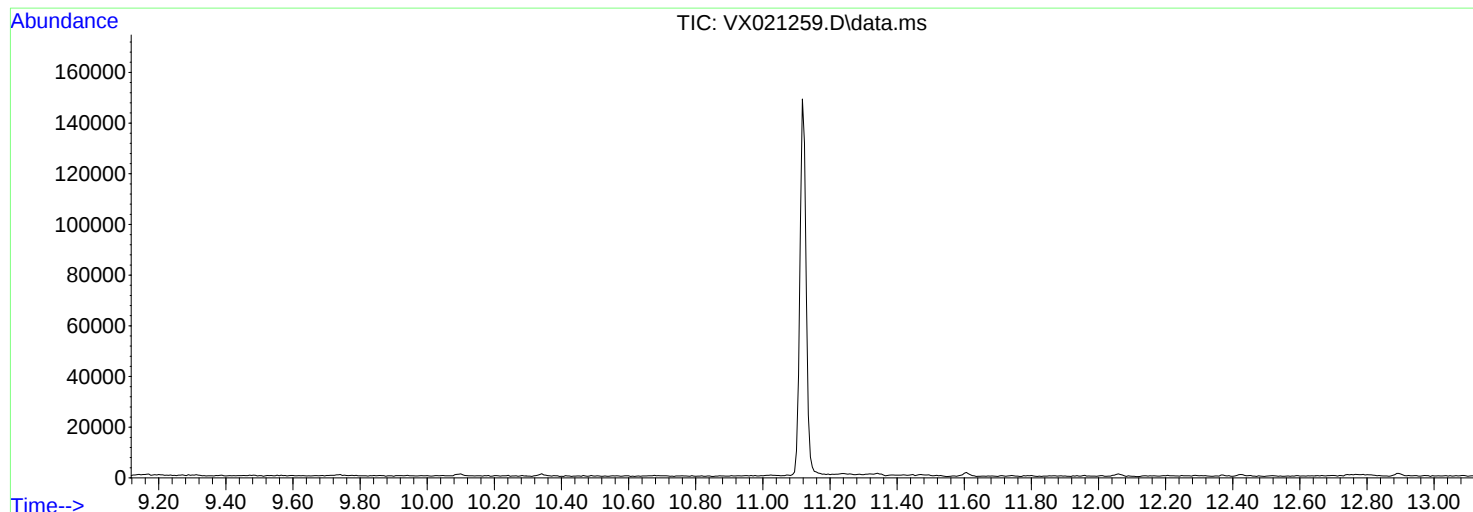

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	5756	PASS
75	95	30	60	57.5	14682	PASS
95	95	100	100	100.0	25541	PASS
96	95	5	9	6.6	1683	PASS
173	174	0.00	2	0.3	48	PASS
174	95	50	100	66.5	16986	PASS
175	174	5	9	7.8	1326	PASS
176	174	95	101	100.0	16984	PASS
177	176	5	9	7.1	1210	PASS