

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031722\  
 Data File : VX027513.D  
 Acq On : 18 Mar 2022 01:40  
 Operator : JC/MD  
 Sample : N1997-19  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124

Quant Time: Mar 18 03:42:01 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 17 15:02:59 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc      | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|--------|----------|
| -----                         |        |       |          |           |        |          |
| Internal Standards            |        |       |          |           |        |          |
| 1) Pentafluorobenzene         | 5.556  | 168   | 346822   | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.769  | 114   | 565381   | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 525650   | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 258957   | 50.000    | ug/l   | 0.00     |
| System Monitoring Compounds   |        |       |          |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958  | 65    | 212256   | 49.680    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 61 - 141 | Recovery  | =      | 99.360%  |
| 35) Dibromofluoromethane      | 5.391  | 113   | 189993   | 52.231    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 69 - 133 | Recovery  | =      | 104.460% |
| 50) Toluene-d8                | 8.653  | 98    | 681567   | 49.515    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 65 - 126 | Recovery  | =      | 99.020%  |
| 62) 4-Bromofluorobenzene      | 11.085 | 95    | 255311   | 50.463    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 58 - 135 | Recovery  | =      | 100.920% |
| Target Compounds              |        |       |          |           |        |          |
|                               |        |       |          |           | Qvalue |          |
| 3) Chloromethane              | 1.258  | 50    | 7201     | 2.437     | ug/l # | 42       |
| 5) Bromomethane               | 1.618  | 94    | 445      | Below Cal |        | 94       |
| 6) Chloroethane               | 1.904  | 64    | 1103     | 0.526     | ug/l # | 50       |
| 11) Tert butyl alcohol        | 2.965  | 59    | 38271    | 47.001    | ug/l   | 99       |
| 13) Acrolein                  | 2.209  | 56    | 208      | 0.329     | ug/l # | 1        |
| 14) Allyl chloride            | 2.709  | 41    | 2955     | 0.586     | ug/l # | 25       |
| 15) Acrylonitrile             | 3.099  | 53    | 3864     | 2.087     | ug/l # | 26       |
| 16) Acetone                   | 2.380  | 43    | 30570    | 17.554    | ug/l   | 93       |
| 17) Carbon Disulfide          | 2.514  | 76    | 6000     | 0.732     | ug/l   | 97       |
| 18) Methyl Acetate            | 2.709  | 43    | 2230     | 0.534     | ug/l # | 51       |
| 19) Methyl tert-butyl Ether   | 3.117  | 73    | 125999   | 11.596    | ug/l # | 33       |
| 20) Methylene Chloride        | 2.788  | 84    | 894      | 0.239     | ug/l # | 38       |
| 22) Diisopropyl ether         | 3.776  | 45    | 4840     | 0.492     | ug/l # | 82       |
| 23) Vinyl Acetate             | 3.770  | 43    | 3038     | 0.355     | ug/l # | 66       |
| 25) 2-Butanone                | 4.568  | 43    | 10694    | 4.081     | ug/l   | 98       |
| 26) 2,2-Dichloropropane       | 4.306  | 77    | 2298     | 0.470     | ug/l # | 52       |
| 29) Tetrahydrofuran           | 5.025  | 42    | 1553     | 0.924     | ug/l # | 70       |
| 31) Cyclohexane               | 5.477  | 56    | 115481   | 21.767    | ug/l   | 99       |
| 36) 1,1-Dichloropropene       | 5.562  | 75    | 25572    | 5.144     | ug/l # | 50       |
| 37) Ethyl Acetate             | 4.568  | 43    | 10694    | 2.159     | ug/l # | 65       |
| 38) Carbon Tetrachloride      | 5.556  | 117   | 34811    | 6.121     | ug/l # | 15       |
| 39) Methylcyclohexane         | 7.385  | 83    | 179977   | 28.792    | ug/l   | 94       |
| 40) Benzene                   | 6.044  | 78    | 722849   | 50.686    | ug/l   | 98       |
| 41) Methacrylonitrile         | 4.958  | 41    | 1164     | 0.431     | ug/l # | 40       |
| 42) 1,2-Dichloroethane        | 6.086  | 62    | 15663    | 2.931     | ug/l   | 91       |
| 43) Isopropyl Acetate         | 6.354  | 43    | 5651     | 0.709     | ug/l # | 62       |
| 47) Bromodichloromethane      | 7.775  | 83    | 1470     | 0.281     | ug/l # | 78       |
| 48) Methyl methacrylate       | 7.659  | 41    | 18419    | 4.669     | ug/l # | 62       |
| 51) 4-Methyl-2-Pentanone      | 8.580  | 43    | 11251    | 2.211     | ug/l   | 91       |
| 52) Toluene                   | 8.720  | 92    | 1777045  | 185.946   | ug/l   | 98       |
| 53) t-1,3-Dichloropropene     | 8.720  | 75    | 20291    | 3.784     | ug/l # | 1        |
| 55) 1,1,2-Trichloroethane     | 9.153  | 97    | 945      | 0.243     | ug/l   | 95       |
| 56) Ethyl methacrylate        | 9.104  | 69    | 6838     | 1.175     | ug/l # | 1        |
| 58) 2-Chloroethyl Vinyl ether | 8.305  | 63    | 88       | Below Cal | #      | 45       |
| 59) 2-Hexanone                | 9.445  | 43    | 25991    | 6.631     | ug/l   | 69       |
| 60) Dibromochloromethane      | 9.281  | 129   | 1244     | 0.290     | ug/l # | 9        |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031722\  
 Data File : VX027513.D  
 Acq On : 18 Mar 2022 01:40  
 Operator : JC/MD  
 Sample : N1997-19  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124

Quant Time: Mar 18 03:42:01 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 17 15:02:59 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|----------|--------|----------|
| -----                         |        |      |          |          |        |          |
| 64) Tetrachloroethene         | 9.275  | 164  | 1286     | 0.315    | ug/l   | 88       |
| 67) Ethyl Benzene             | 10.201 | 91   | 8708564  | 470.520  | ug/l # | 81       |
| 68) m/p-Xylenes               | 10.311 | 106  | 7397274  | 1015.057 | ug/l   | 77       |
| 69) o-Xylene                  | 10.646 | 106  | 2209326  | 312.237  | ug/l   | 95       |
| 70) Styrene                   | 10.646 | 104  | 116746   | 10.100   | ug/l # | 1        |
| 73) Isopropylbenzene          | 10.963 | 105  | 251798   | 13.350   | ug/l   | 99       |
| 74) N-amyl acetate            | 10.890 | 43   | 50393    | 7.535    | ug/l # | 39       |
| 75) 1,1,2,2-Tetrachloroethane | 11.232 | 83   | 1524     | 0.255    | ug/l # | 1        |
| 76) 1,2,3-Trichloropropane    | 11.305 | 75   | 6869     | 1.268    | ug/l # | 1        |
| 78) n-propylbenzene           | 11.305 | 91   | 1080117  | 52.166   | ug/l   | 98       |
| 79) 2-Chlorotoluene           | 11.384 | 91   | 593229   | 45.674   | ug/l # | 40       |
| 80) 1,3,5-Trimethylbenzene    | 11.457 | 105  | 3403497  | 214.394  | ug/l   | 98       |
| 81) trans-1,4-Dichloro-2-b... | 11.085 | 75   | 123912   | 69.477   | ug/l # | 15       |
| 82) 4-Chlorotoluene           | 11.457 | 91   | 370328   | 25.042   | ug/l # | 45       |
| 83) tert-Butylbenzene         | 11.719 | 119  | 180648   | 11.487   | ug/l   | 86       |
| 84) 1,2,4-Trimethylbenzene    | 11.756 | 105  | 6160021  | 389.089  | ug/l   | 94       |
| 85) sec-Butylbenzene          | 11.756 | 105  | 6160021  | 324.136  | ug/l # | 56       |
| 86) p-Isopropyltoluene        | 11.975 | 119  | 62257    | 3.814    | ug/l # | 77       |
| 88) 1,4-Dichlorobenzene       | 12.042 | 146  | 2283     | 0.256    | ug/l # | 53       |
| 89) n-Butylbenzene            | 12.323 | 91   | 237601   | 17.442   | ug/l # | 1        |
| 90) Hexachloroethane          | 12.536 | 117  | 36121    | 13.876   | ug/l # | 10       |
| 91) 1,2-Dichlorobenzene       | 12.335 | 146  | 3149     | 0.366    | ug/l # | 47       |
| 92) 1,2-Dibromo-3-Chloropr... | 12.926 | 75   | 3769     | 2.750    | ug/l # | 1        |
| 95) Naphthalene               | 13.780 | 128  | 2265986  | 126.264  | ug/l   | 100      |
| -----                         |        |      |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031722\  
 Data File : VX027513.D  
 Acq On : 18 Mar 2022 01:40  
 Operator : JC/MD  
 Sample : N1997-19  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124

Quant Time: Mar 18 03:42:01 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 17 15:02:59 2022  
 Response via : Initial Calibration




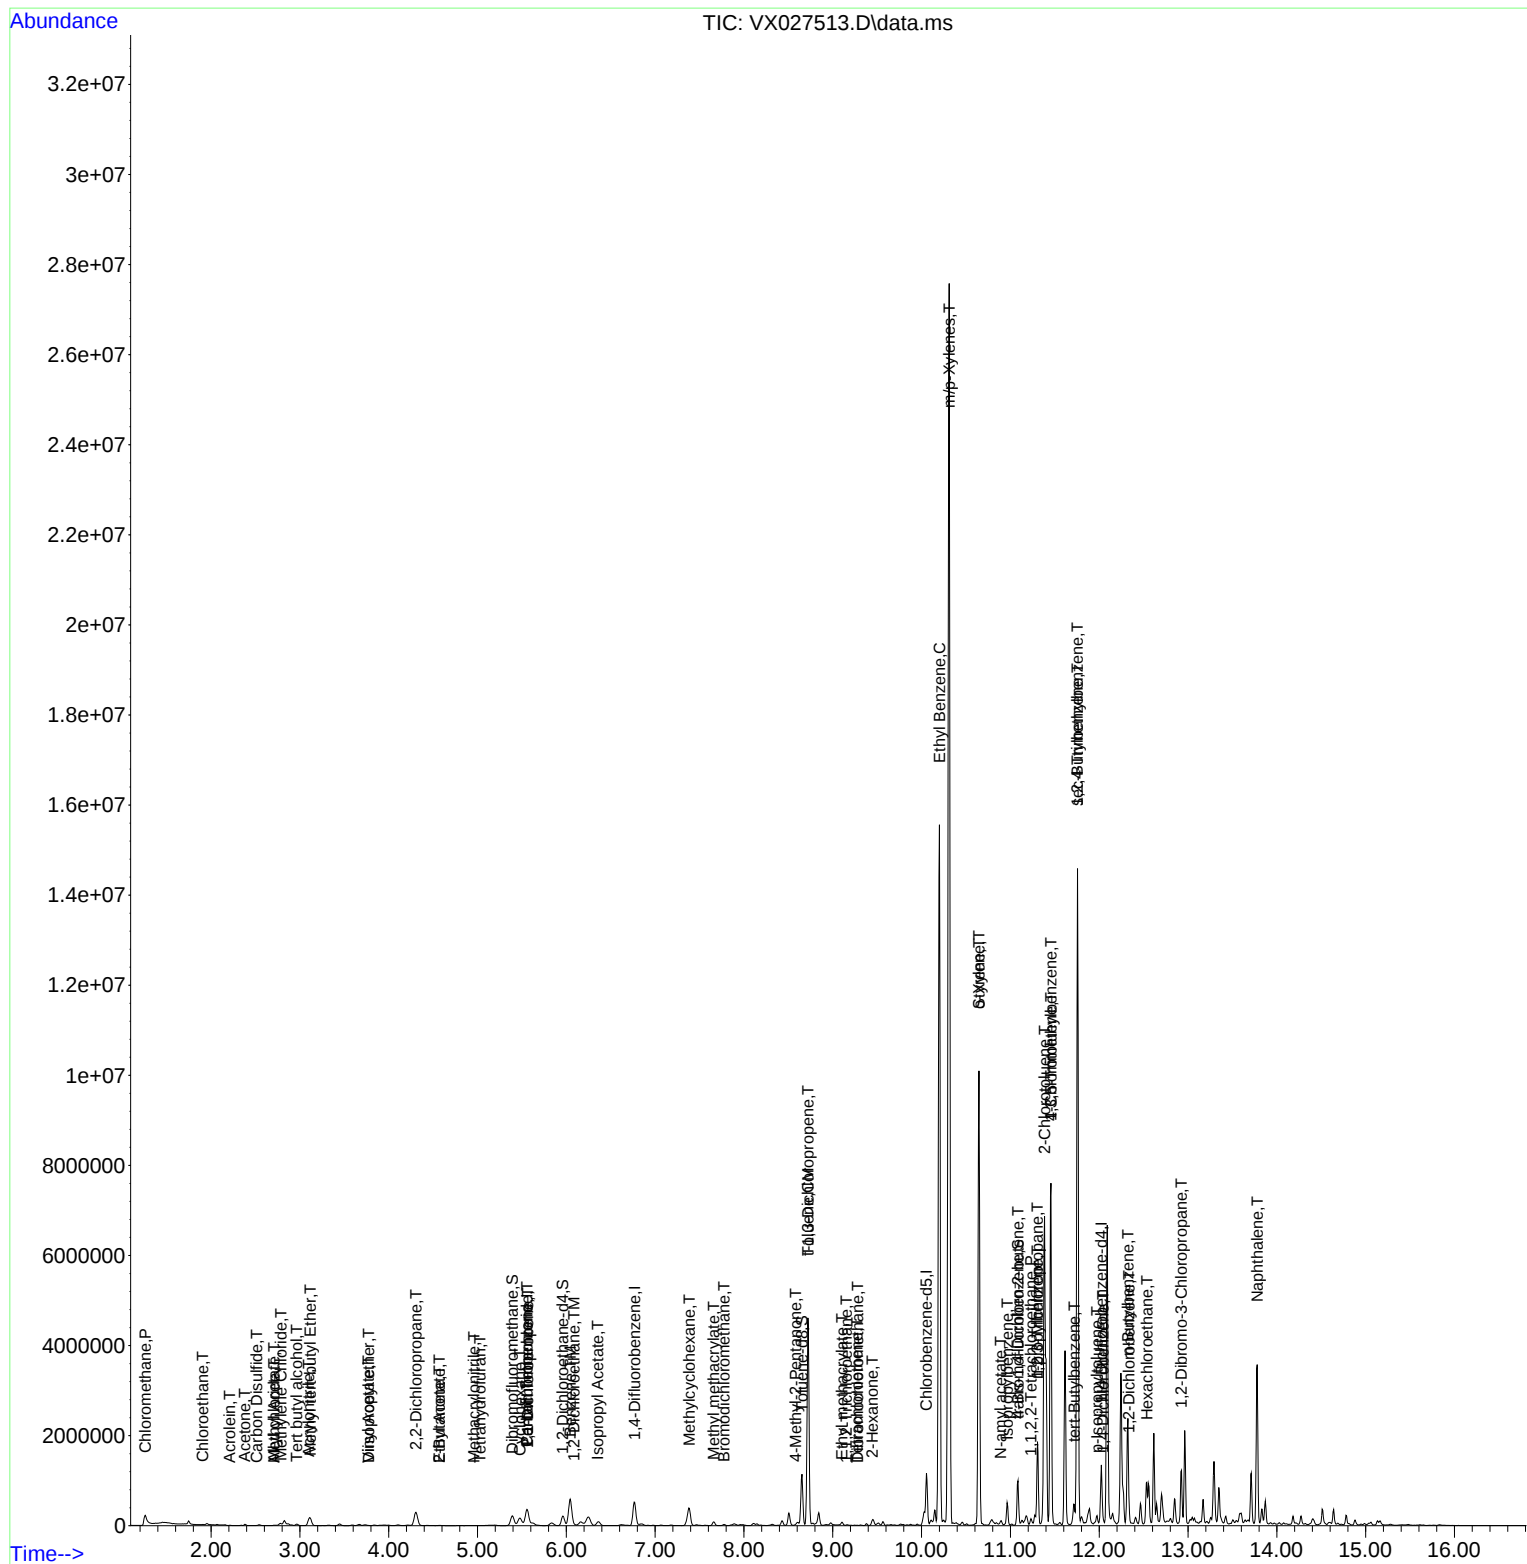


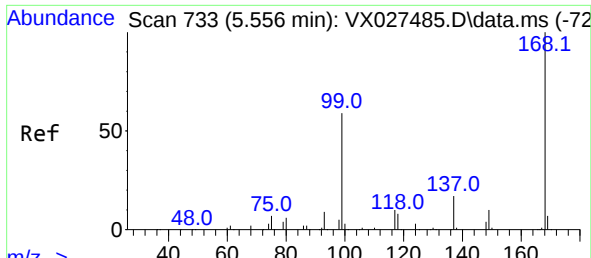

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.556 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:168 Resp: 346822  
Ion Ratio Lower Upper  
168 100  
99 57.4 41.7 62.5

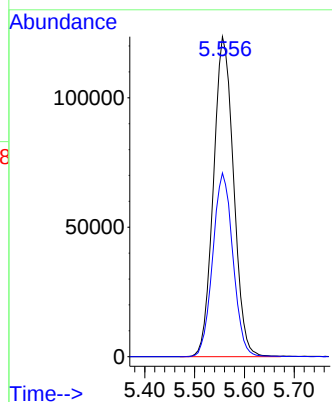

#3  
Chloromethane  
Concen: 2.437 ug/l  
RT: 1.258 min Scan# 28  
Delta R.T. -0.036 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 50 Resp: 7201  
Ion Ratio Lower Upper  
50 100  
52 0.0 26.4 39.6#


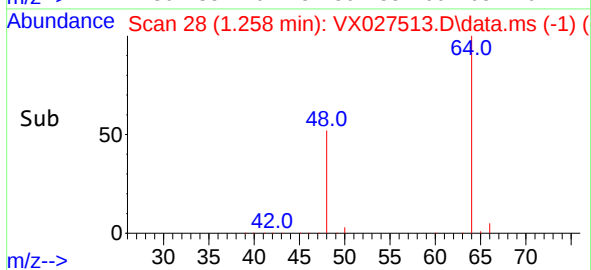
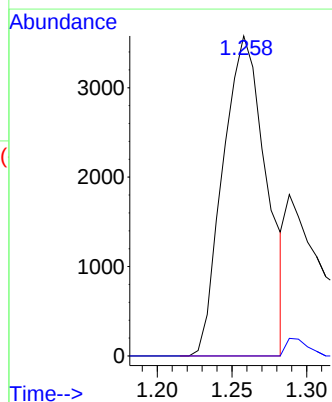



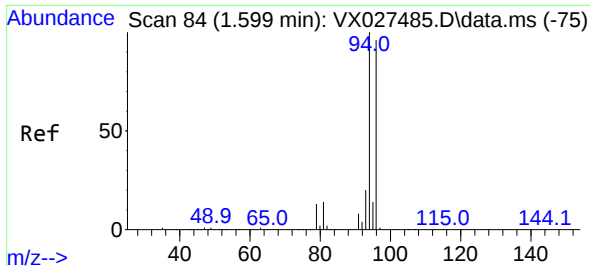

#5  
Bromomethane  
Concen: Below Cal  
RT: 1.618 min Scan# 81  
Delta R.T. 0.019 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 94 Resp: 445  
Ion Ratio Lower Upper  
94 100  
96 88.1 75.3 112.9

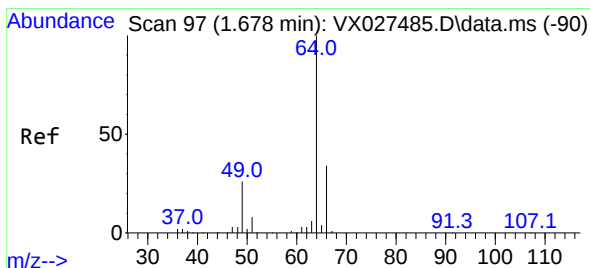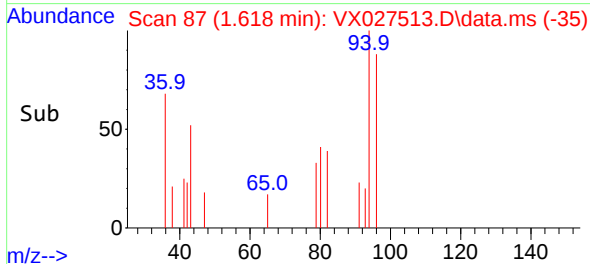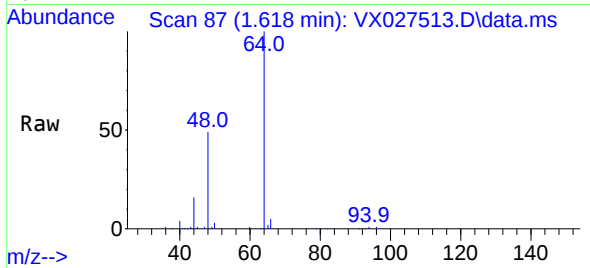

#6  
Chloroethane  
Concen: 0.526 ug/l  
RT: 1.904 min Scan# 134  
Delta R.T. 0.226 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 64 Resp: 1103  
Ion Ratio Lower Upper  
64 100  
66 4.1 25.3 37.9#


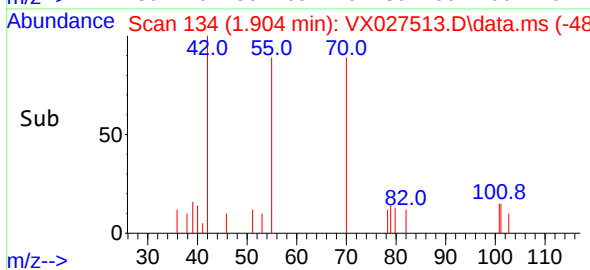

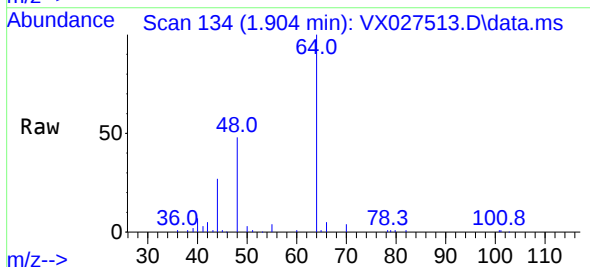




#11  
Tert butyl alcohol  
Concen: 47.001 ug/l  
RT: 2.965 min Scan# 30  
Delta R.T. -0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 59 Resp: 38271  
Ion Ratio Lower Upper  
59 100  
57 10.2 8.3 12.5

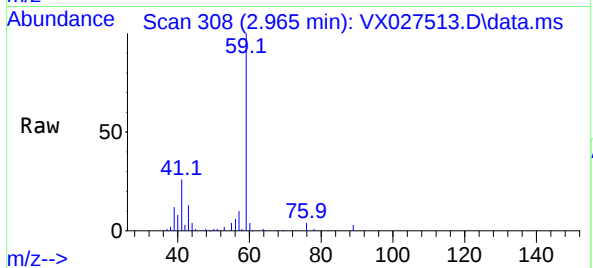

#13  
Acrolein  
Concen: 0.329 ug/l  
RT: 2.209 min Scan# 184  
Delta R.T. -0.024 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 56 Resp: 208  
Ion Ratio Lower Upper  
56 100  
55 1252.9 55.0 82.6#


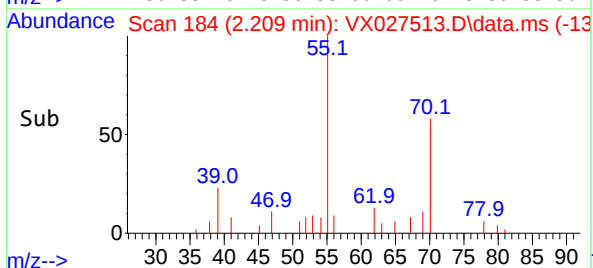
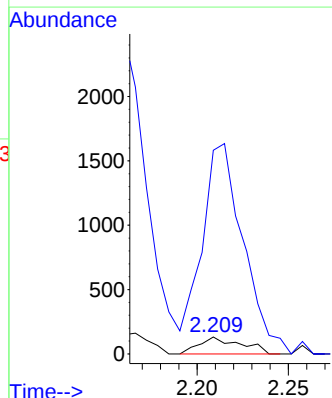





#14  
 Allyl chloride  
 Concen: 0.586 ug/l  
 RT: 2.709 min Scan# 2  
 Delta R.T. 0.049 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124


Tgt Ion: 41 Resp: 2955  
 Ion Ratio Lower Upper  
 41 100  
 39 0.0 50.4 75.6#  
 76 0.0 32.7 49.1#

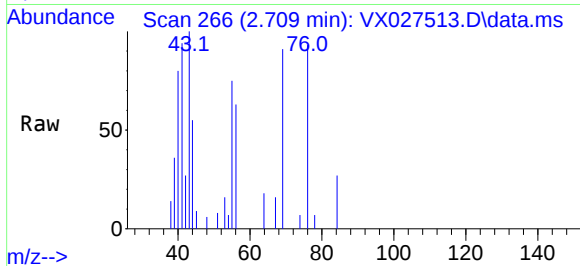

#15  
 Acrylonitrile  
 Concen: 2.087 ug/l  
 RT: 3.099 min Scan# 330  
 Delta R.T. 0.031 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40

Tgt Ion: 53 Resp: 3864  
 Ion Ratio Lower Upper  
 53 100  
 52 9.2 65.7 98.5#  
 51 68.6 28.4 42.6#


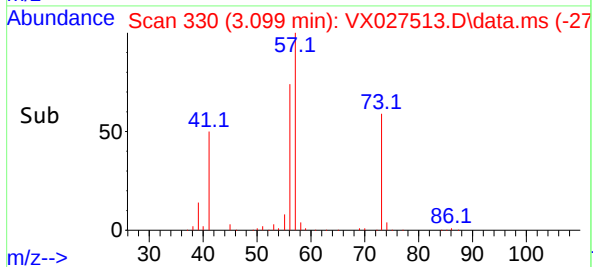

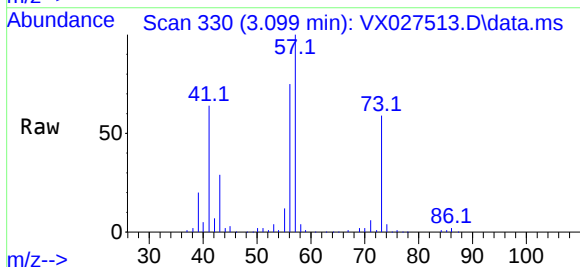




#16  
Acetone  
Concen: 17.554 ug/l  
RT: 2.380 min Scan# 212  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 43 Resp: 30570  
Ion Ratio Lower Upper  
43 100  
58 31.7 28.8 43.2

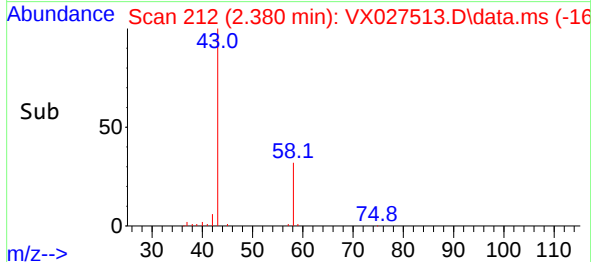

#17  
Carbon Disulfide  
Concen: 0.732 ug/l  
RT: 2.514 min Scan# 234  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 76 Resp: 6000  
Ion Ratio Lower Upper  
76 100  
78 7.7 7.2 10.8


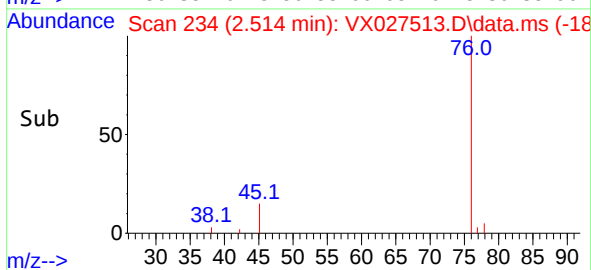






#18  
Methyl Acetate  
Concen: 0.534 ug/l  
RT: 2.709 min Scan# 21  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 43 Resp: 2230  
Ion Ratio Lower Upper  
43 100  
74 2.6 22.8 34.2#

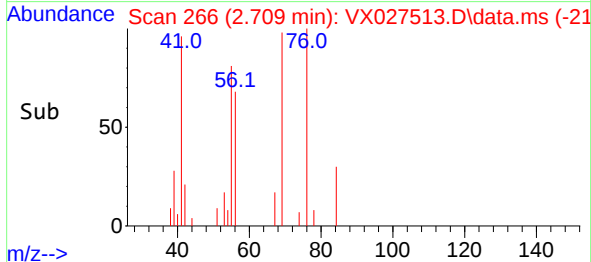

#19  
Methyl tert-butyl Ether  
Concen: 11.596 ug/l  
RT: 3.117 min Scan# 333  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 73 Resp: 125999  
Ion Ratio Lower Upper  
73 100  
57 52.4 16.8 25.2#


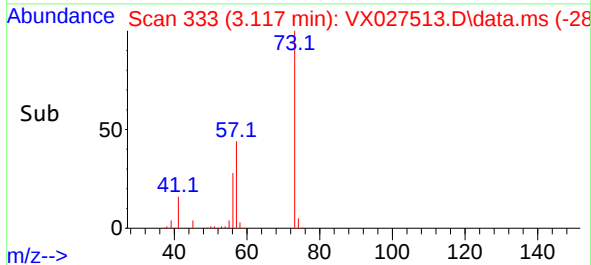

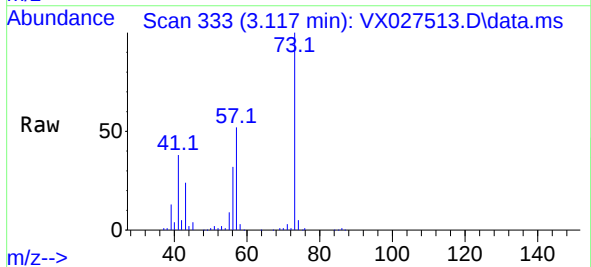




#20  
Methylene Chloride  
Concen: 0.239 ug/l  
RT: 2.788 min Scan# 21  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 84    | Resp: | 894    |
| Ion      | Ratio | Lower | Upper  |
| 84       | 100   |       |        |
| 49       | 84.3  | 85.5  | 128.3# |
| 51       | 91.5  | 26.6  | 39.8#  |
| 86       | 149.7 | 51.5  | 77.3#  |

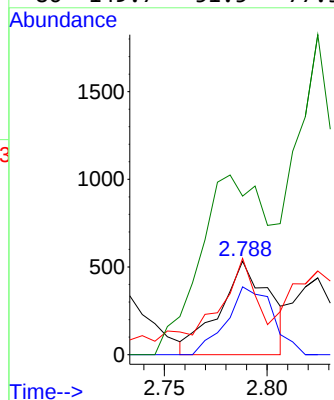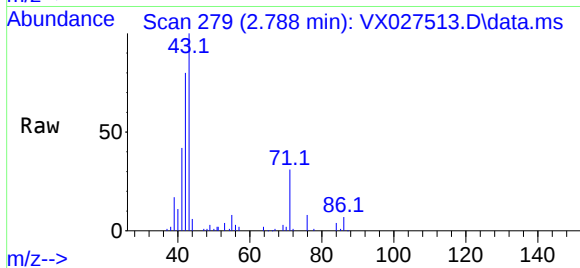

#22  
Diisopropyl ether  
Concen: 0.492 ug/l  
RT: 3.776 min Scan# 441  
Delta R.T. 0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 45    | Resp: | 4840  |
| Ion      | Ratio | Lower | Upper |
| 45       | 100   |       |       |
| 43       | 40.4  | 50.8  | 76.2# |
| 87       | 30.9  | 26.6  | 39.8  |
| 59       | 13.1  | 10.5  | 15.7  |



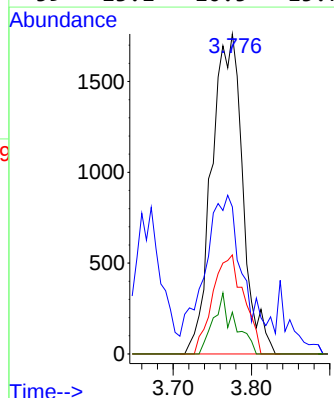
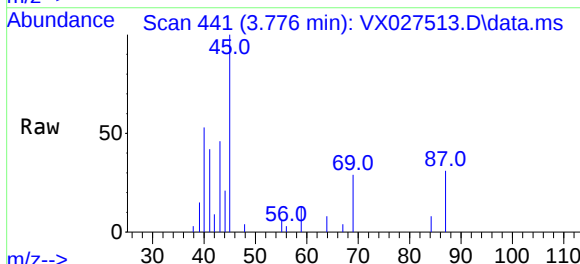




#23  
 Vinyl Acetate  
 Concen: 0.355 ug/l  
 RT: 3.770 min Scan# 43  
 Delta R.T. 0.043 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124


Tgt Ion: 43 Resp: 3038  
 Ion Ratio Lower Upper  
 43 100  
 86 0.0 10.8 16.2#

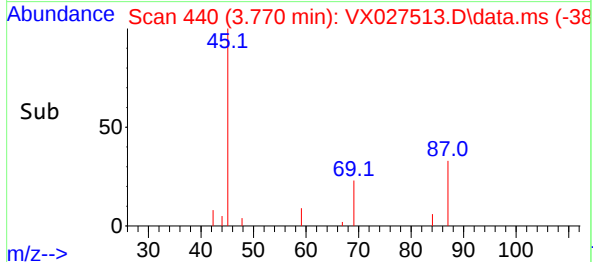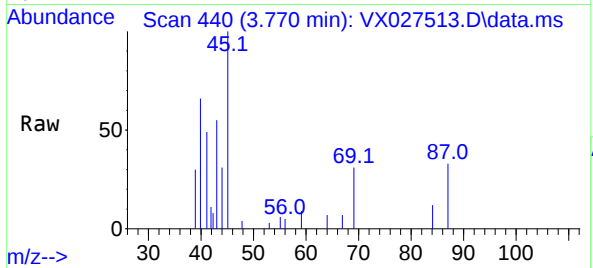

#25  
 2-Butanone  
 Concen: 4.081 ug/l  
 RT: 4.568 min Scan# 571  
 Delta R.T. 0.006 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40

Tgt Ion: 43 Resp: 10694  
 Ion Ratio Lower Upper  
 43 100  
 72 29.5 24.4 36.6

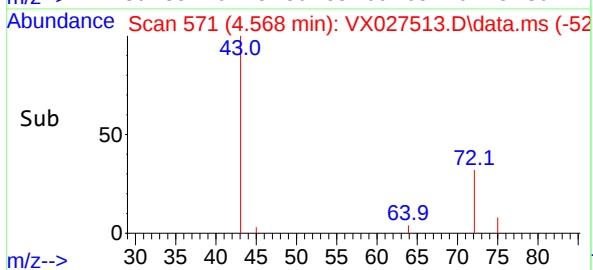



#26

2,2-Dichloropropane

Concen: 0.470 ug/l

RT: 4.306 min Scan# 51

Delta R.T. -0.171 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

Instrument :

MSVOA\_X

ClientSampleId :





MW-124

Tgt Ion: 77 Resp: 2298

Ion Ratio Lower Upper

77 100

97 0.0 11.8 35.4#

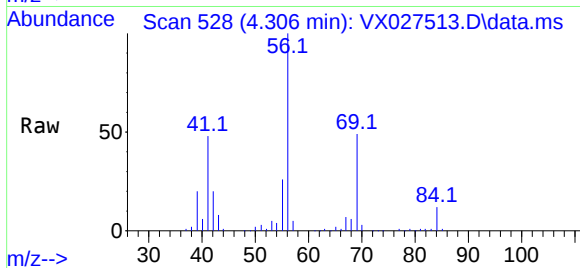

#29

Tetrahydrofuran

Concen: 0.924 ug/l

RT: 5.025 min Scan# 646

Delta R.T. 0.018 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40




Tgt Ion: 42 Resp: 1553


Ion Ratio Lower Upper

42 100

72 43.8 44.1 66.1#

71 18.9 40.5 60.7#


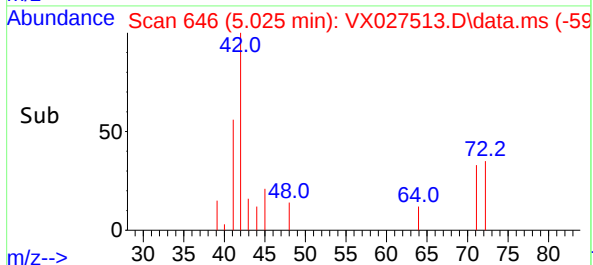
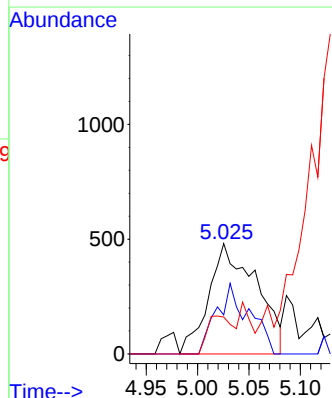
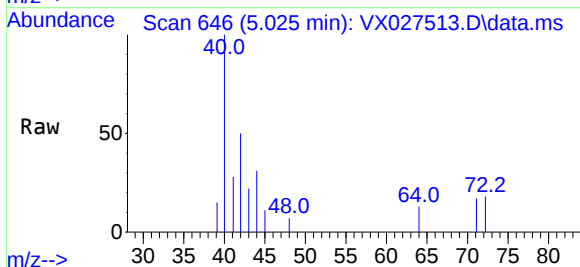




#31  
Cyclohexane  
Concen: 21.767 ug/l  
RT: 5.477 min Scan# 719  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 56 Resp: 115481  
Ion Ratio Lower Upper  
56 100  
69 31.2 26.7 40.1  
84 97.0 77.2 115.8

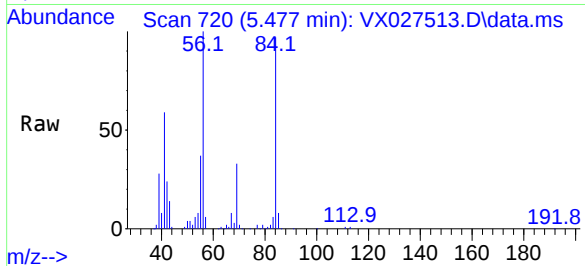

#33  
1,2-Dichloroethane-d4  
Concen: 49.680 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 65 Resp: 212256  
Ion Ratio Lower Upper  
65 100  
67 50.9 0.0 107.4


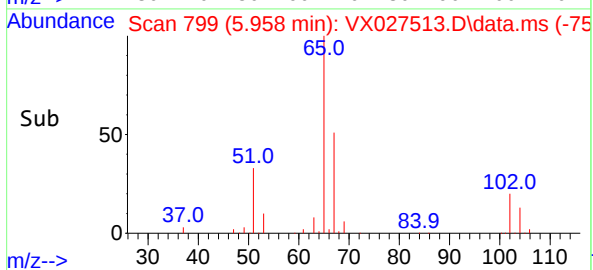

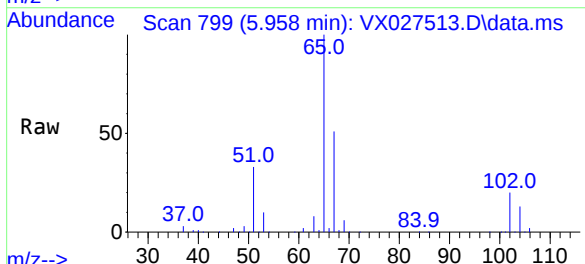




#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.769 min Scan# 91  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:114 Resp: 565381  
Ion Ratio Lower Upper  
114 100  
63 18.8 0.0 36.8  
88 15.7 0.0 32.4

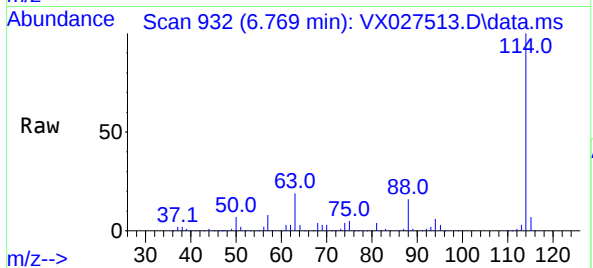

#35  
Dibromofluoromethane  
Concen: 52.231 ug/l  
RT: 5.391 min Scan# 706  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:113 Resp: 189993  
Ion Ratio Lower Upper  
113 100  
111 101.6 82.8 124.2  
192 19.6 16.9 25.3


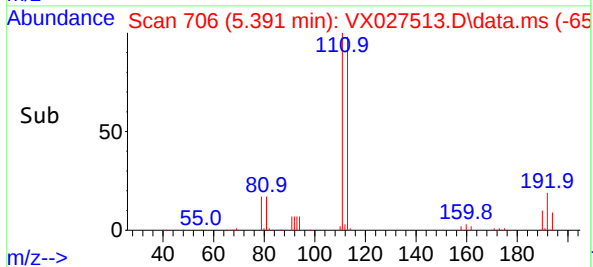

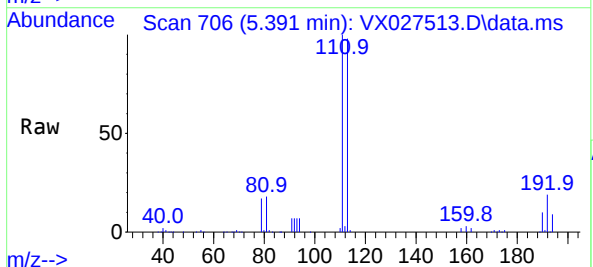


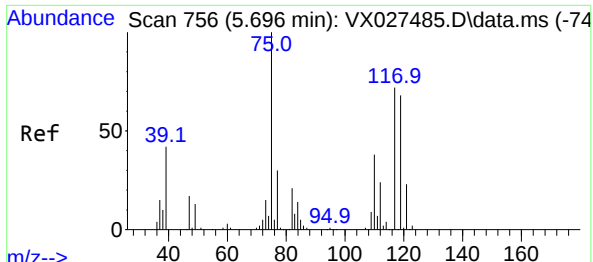

#36  
1,1-Dichloropropene  
Concen: 5.144 ug/l  
RT: 5.562 min Scan# 71  
Delta R.T. -0.134 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 75 Resp: 25572  
Ion Ratio Lower Upper  
75 100  
110 9.9 18.3 54.8#  
77 0.0 24.8 37.2#

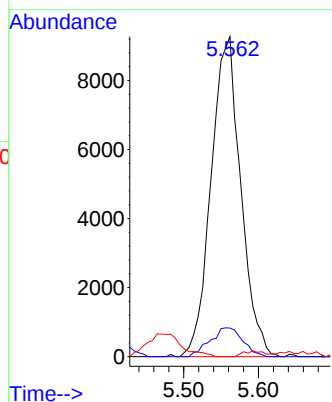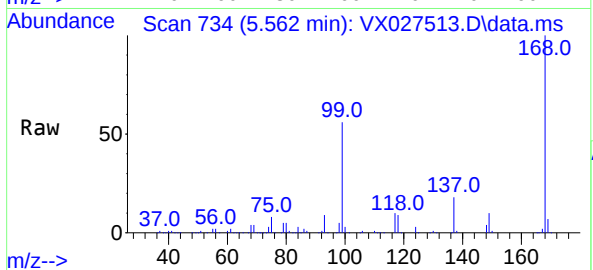

#37  
Ethyl Acetate  
Concen: 2.159 ug/l  
RT: 4.568 min Scan# 571  
Delta R.T. -0.152 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40


Tgt Ion: 43 Resp: 10694  
Ion Ratio Lower Upper  
43 100  
61 0.0 12.6 19.0#  
70 0.0 10.2 15.2#

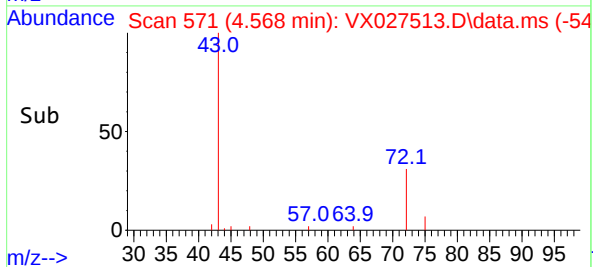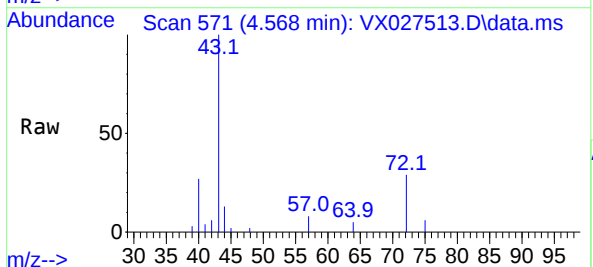



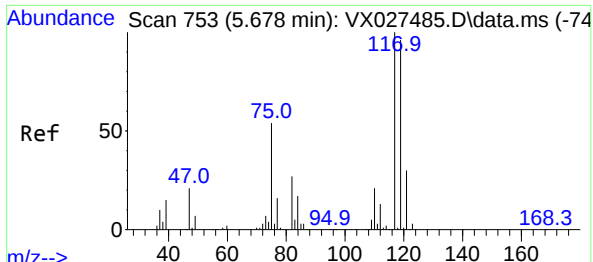


#38  
Carbon Tetrachloride  
Concen: 6.121 ug/l  
RT: 5.556 min Scan# 713  
Delta R.T. -0.122 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124



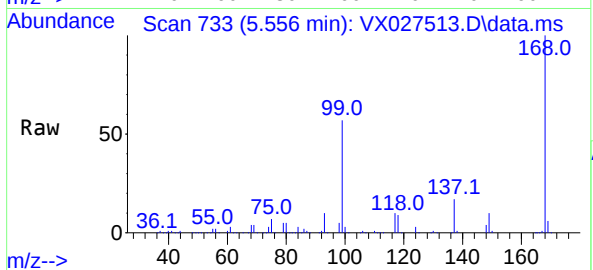



Tgt Ion:117 Resp: 34811  
Ion Ratio Lower Upper  
117 100  
119 4.6 77.3 115.9#  
121 0.0 24.2 36.2#



#39  
Methylcyclohexane  
Concen: 28.792 ug/l  
RT: 7.385 min Scan# 1033  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 83 Resp: 179977  
Ion Ratio Lower Upper  
83 100  
55 76.3 54.6 81.8  
98 47.4 37.4 56.2


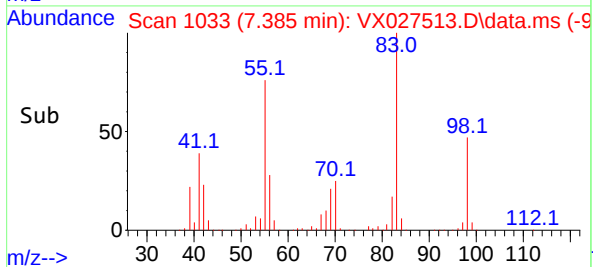

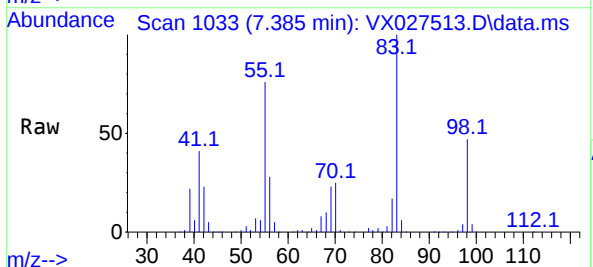




#40  
Benzene  
Concen: 50.686 ug/l  
RT: 6.044 min Scan# 813  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 78 Resp: 722849  
Ion Ratio Lower Upper  
78 100  
77 23.0 19.3 28.9

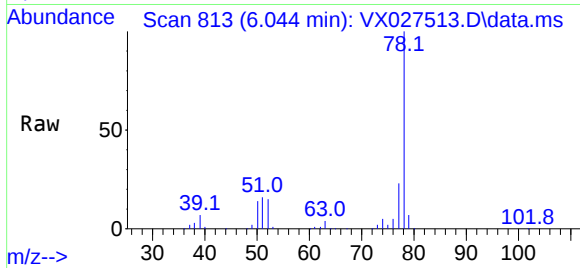

#41  
Methacrylonitrile  
Concen: 0.431 ug/l  
RT: 4.958 min Scan# 635  
Delta R.T. 0.031 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 41 Resp: 1164  
Ion Ratio Lower Upper  
41 100  
39 56.4 43.0 64.4  
67 0.0 70.2 105.4#  
52 0.0 26.0 39.0#

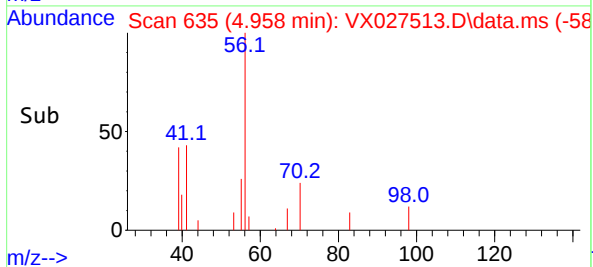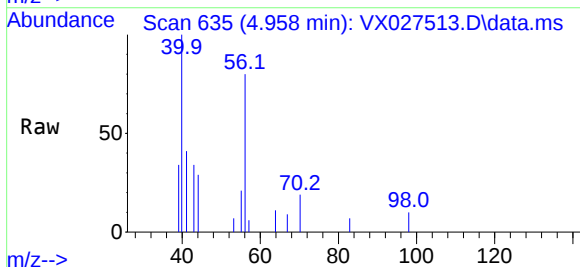



#42

1,2-Dichloroethane

Concen: 2.931 ug/l

RT: 6.086 min Scan# 81

Delta R.T. -0.006 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

Instrument :

MSVOA\_X

ClientSampleId :





MW-124

Tgt Ion: 62 Resp: 15663

Ion Ratio Lower Upper

62 100

98 13.5 0.0 20.4



#43

Isopropyl Acetate

Concen: 0.709 ug/l

RT: 6.354 min Scan# 864

Delta R.T. 0.012 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40




Tgt Ion: 43 Resp: 5651


Ion Ratio Lower Upper

43 100

61 1.5 18.5 27.7#

87 4.4 13.0 19.6#

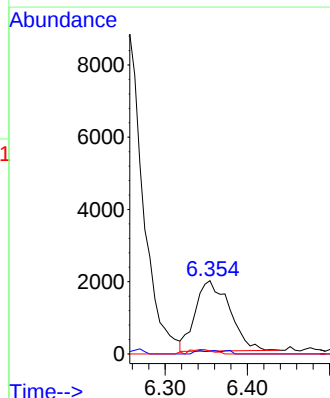



#47

Bromodichloromethane

Concen: 0.281 ug/l

RT: 7.775 min Scan# 1097

Delta R.T. -0.049 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40





Instrument :

MSVOA\_X

ClientSampleId :

MW-124

|             |                 |
|-------------|-----------------|
| Tgt Ion: 83 | Resp: 1470      |
| Ion Ratio   | Lower Upper     |
| 83          | 100             |
| 85          | 48.3 52.2 78.2# |
| 127         | 0.0 6.8 10.2#   |

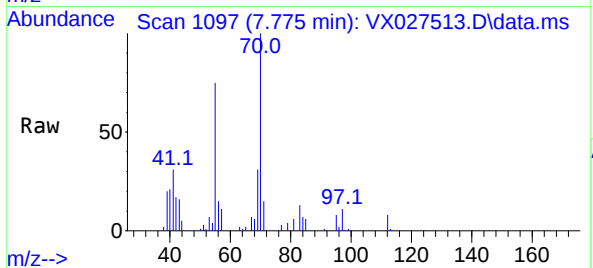

#48

Methyl methacrylate

Concen: 4.669 ug/l




RT: 7.659 min Scan# 1078


Delta R.T. -0.036 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

|             |                   |
|-------------|-------------------|
| Tgt Ion: 41 | Resp: 18419       |
| Ion Ratio   | Lower Upper       |
| 41          | 100               |
| 69          | 159.5 82.5 123.7# |
| 39          | 52.0 43.8 65.8    |


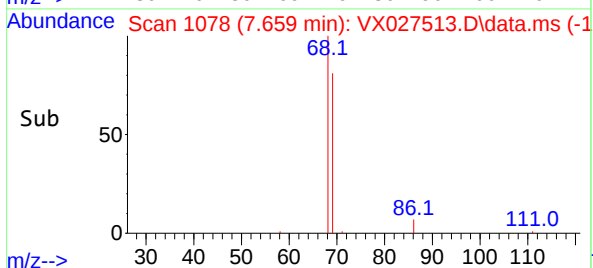
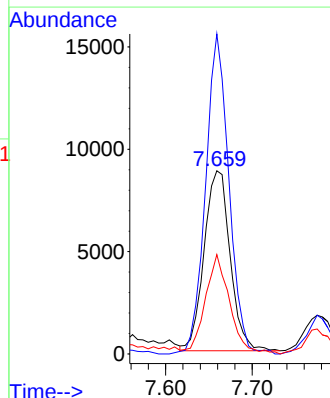





#50  
Toluene-d8  
Concen: 49.515 ug/l  
RT: 8.653 min Scan# 1241  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 98 Resp: 681567  
Ion Ratio Lower Upper  
98 100  
100 64.5 52.6 78.8

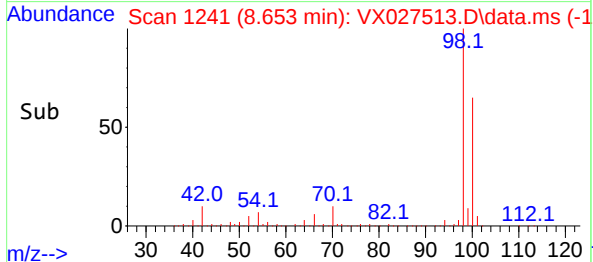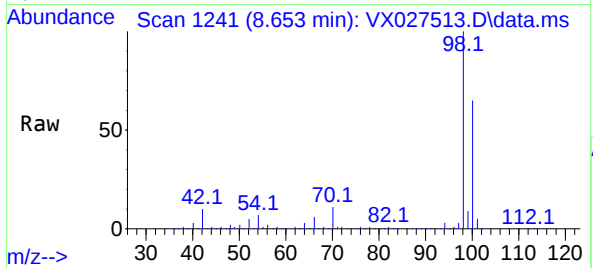

#51  
4-Methyl-2-Pentanone  
Concen: 2.211 ug/l  
RT: 8.580 min Scan# 1229  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 43 Resp: 11251  
Ion Ratio Lower Upper  
43 100  
58 39.3 36.1 54.1


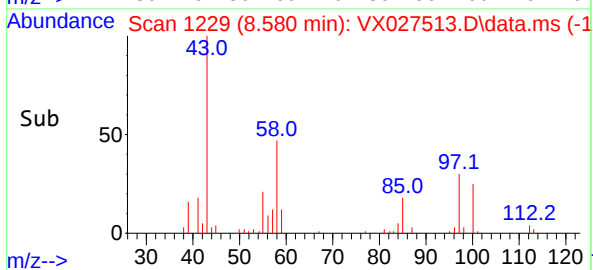






#52  
Toluene  
Concen: 185.946 ug/l  
RT: 8.720 min Scan# 1252  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 92 Resp: 1777045  
Ion Ratio Lower Upper  
92 100  
91 169.5 137.5 206.3

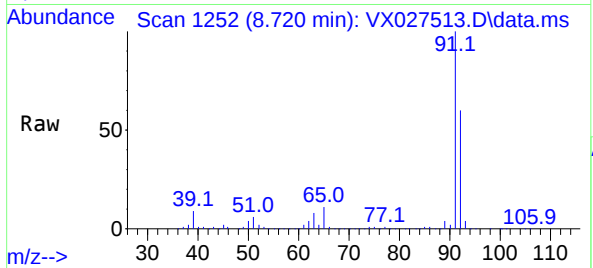

#53  
t-1,3-Dichloropropene  
Concen: 3.784 ug/l  
RT: 8.720 min Scan# 1252  
Delta R.T. -0.262 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 75 Resp: 20291  
Ion Ratio Lower Upper  
75 100  
77 157.9 25.4 38.0#

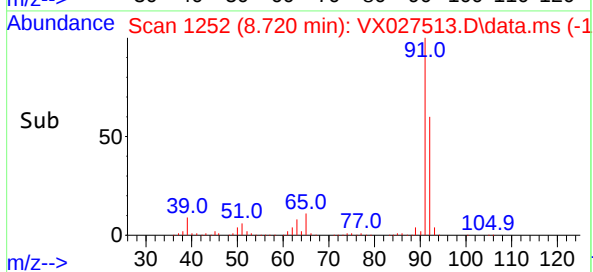







#55  
1,1,2-Trichloroethane  
Concen: 0.243 ug/l  
RT: 9.153 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion: 97 Resp: 945




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 97  | 100   |       |       |
| 83  | 86.6  | 66.2  | 99.4  |
| 85  | 44.6  | 42.9  | 64.3  |
| 99  | 62.1  | 49.0  | 73.6  |




#56  
Ethyl methacrylate  
Concen: 1.175 ug/l  
RT: 9.104 min Scan# 1315  
Delta R.T. -0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 69 Resp: 6838

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 69  | 100   |       |       |
| 41  | 127.7 | 43.8  | 65.6# |
| 39  | 79.6  | 22.2  | 33.2# |


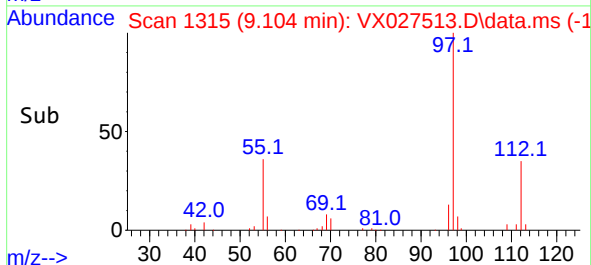
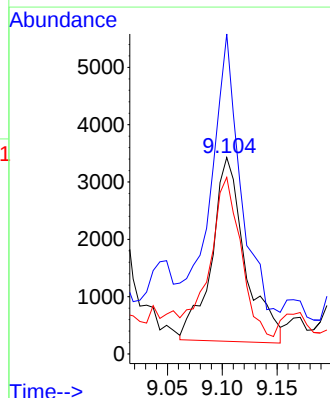
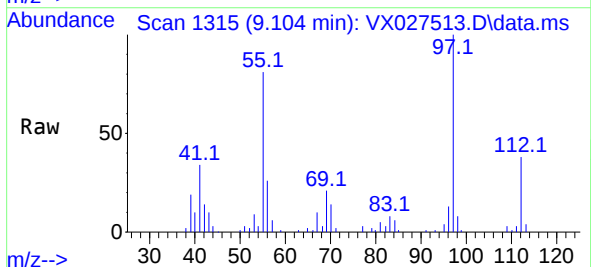




#58  
2-Chloroethyl Vinyl ether  
Concen: Below Cal  
RT: 8.305 min Scan# 1174  
Delta R.T. 0.061 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 63 Resp: 88  
Ion Ratio Lower Upper  
63 100  
106 0.0 23.9 35.9#

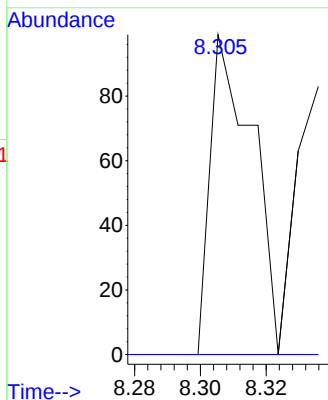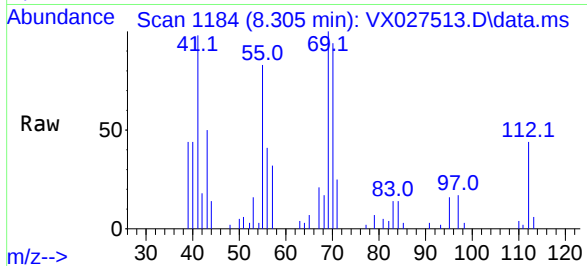

#59  
2-Hexanone  
Concen: 6.631 ug/l  
RT: 9.445 min Scan# 1371  
Delta R.T. 0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 43 Resp: 25991  
Ion Ratio Lower Upper  
43 100  
58 39.7 31.9 95.7


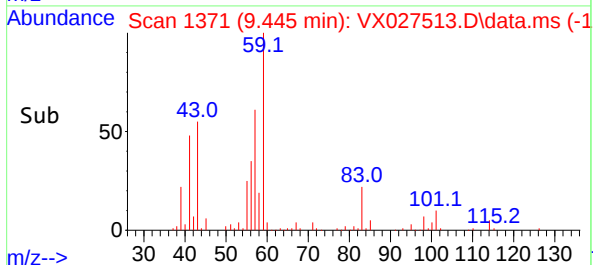
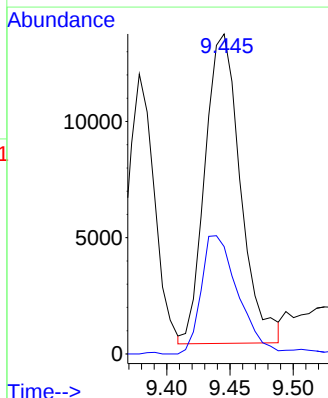
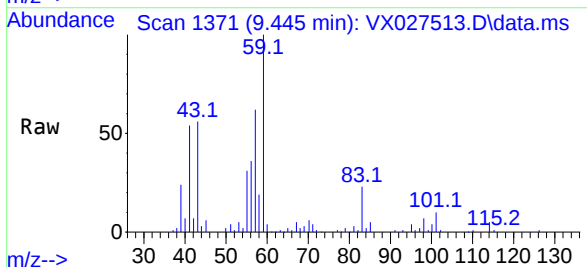




#60  
Dibromochloromethane  
Concen: 0.290 ug/l  
RT: 9.281 min Scan# 11  
Delta R.T. -0.244 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:129 Resp: 1244  
Ion Ratio Lower Upper  
129 100  
127 0.0 40.3 120.8#

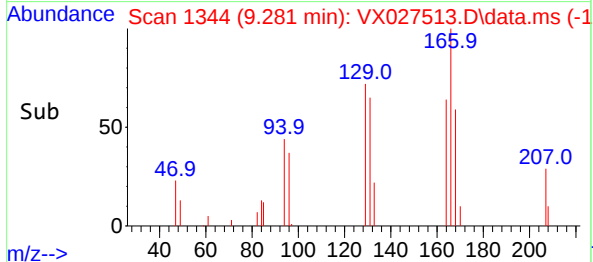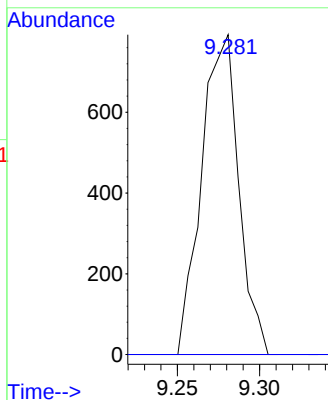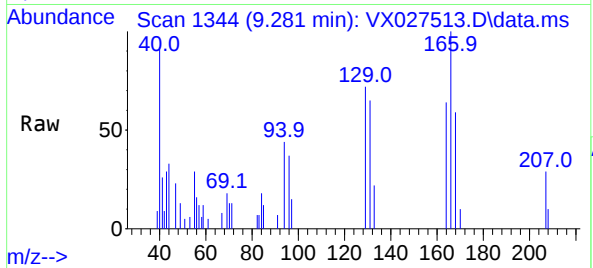

#62  
4-Bromofluorobenzene  
Concen: 50.463 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 95 Resp: 255311  
Ion Ratio Lower Upper  
95 100  
174 81.1 0.0 163.0  
176 78.4 0.0 155.0


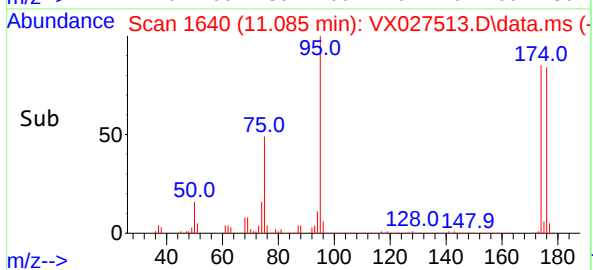
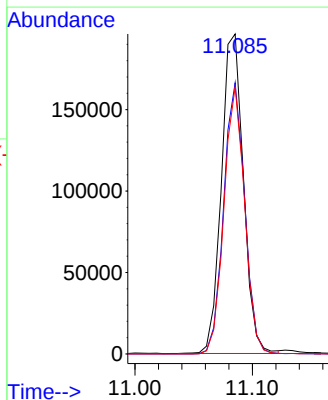





#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:117 Resp: 525650  
Ion Ratio Lower Upper  
117 100  
82 55.8 41.8 62.8  
119 32.9 24.8 37.2

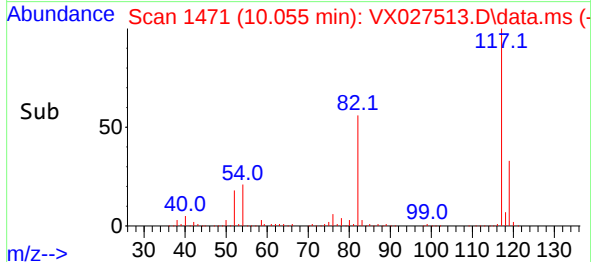

#64  
Tetrachloroethene  
Concen: 0.315 ug/l  
RT: 9.275 min Scan# 1343  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:164 Resp: 1286  
Ion Ratio Lower Upper  
164 100  
166 106.9 101.2 151.8  
129 78.2 73.0 109.4  
131 90.3 74.2 111.2



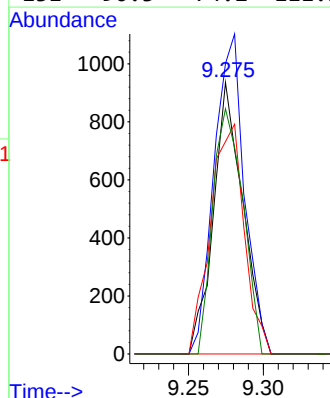





#67  
Ethyl Benzene  
Concen: 470.520 ug/l  
RT: 10.201 min Scan# 1495  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 91 Resp: 8708564  
Ion Ratio Lower Upper  
91 100  
106 41.2 24.6 36.8#

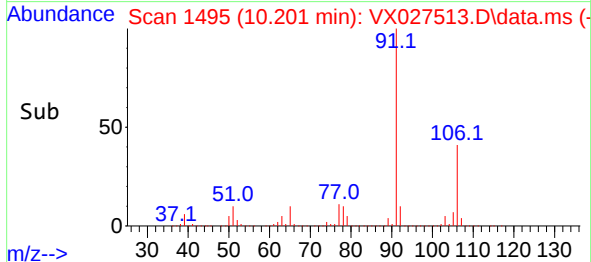

#68  
m/p-Xylenes  
Concen: 1015.057 ug/l  
RT: 10.311 min Scan# 1513  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:106 Resp: 7397274  
Ion Ratio Lower Upper  
106 100  
91 166.0 160.4 240.6


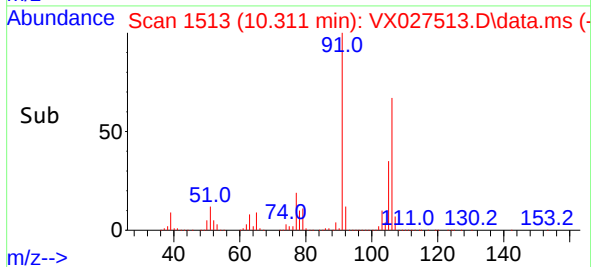

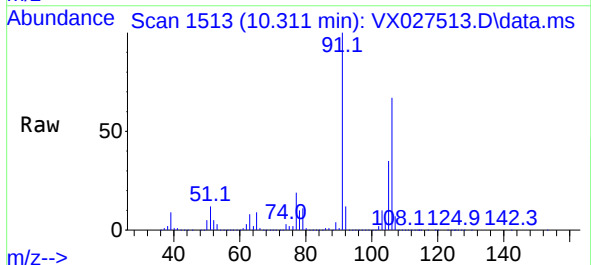




#69  
o-Xylene  
Concen: 312.237 ug/l  
RT: 10.646 min Scan# 1568  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:106 Resp: 2209326  
Ion Ratio Lower Upper  
106 100  
91 204.6 106.1 318.1

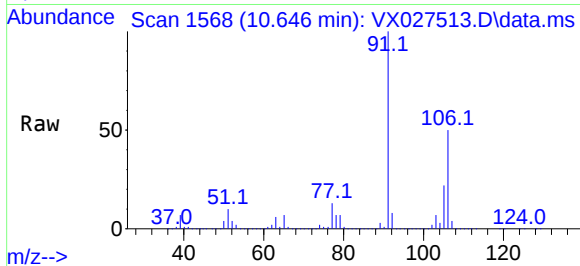

#70  
Styrene  
Concen: 10.100 ug/l  
RT: 10.646 min Scan# 1568  
Delta R.T. -0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:104 Resp: 116746  
Ion Ratio Lower Upper  
104 100  
78 277.9 38.6 57.8#  
103 268.5 43.8 65.8#


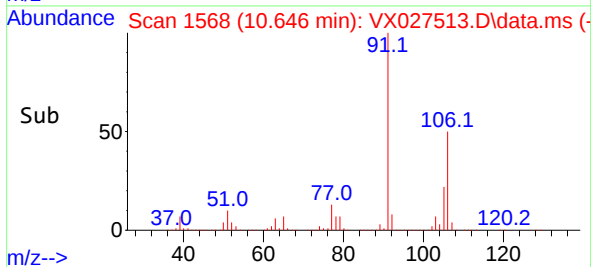

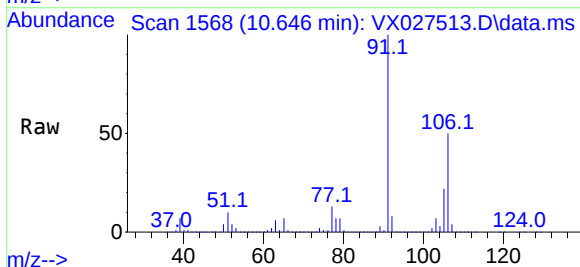




#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:152 Resp: 258957  
Ion Ratio Lower Upper  
152 100  
115 59.4 37.5 112.7  
150 155.1 0.0 338.2

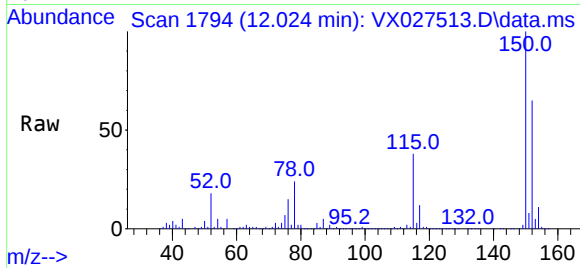

#73  
Isopropylbenzene  
Concen: 13.350 ug/l  
RT: 10.963 min Scan# 1620  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:105 Resp: 251798  
Ion Ratio Lower Upper  
105 100  
120 26.7 13.5 40.5




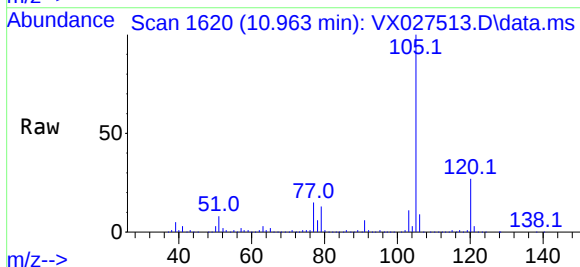




#74  
N-amy1 acetate  
Concen: 7.535 ug/l  
RT: 10.890 min Scan# 1608  
Delta R.T. 0.049 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 43 Resp: 50393  
Ion Ratio Lower Upper  
43 100  
70 0.0 42.5 63.7#  
55 6.6 23.1 34.7#  
61 0.0 22.8 34.2#

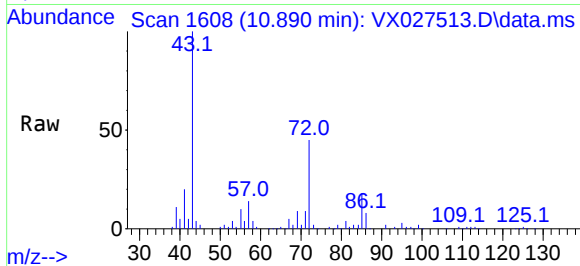

#75  
1,1,2,2-Tetrachloroethane  
Concen: 0.255 ug/l  
RT: 11.232 min Scan# 1664  
Delta R.T. 0.018 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 83 Resp: 1524  
Ion Ratio Lower Upper  
83 100  
131 0.0 5.1 15.3#  
85 1283.7 32.6 97.7#


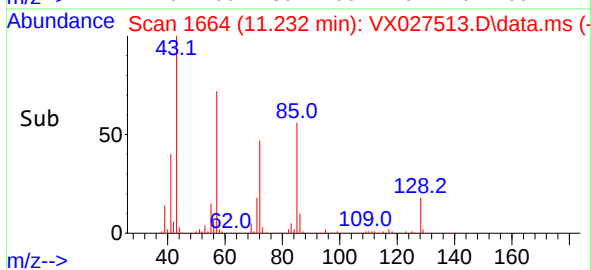

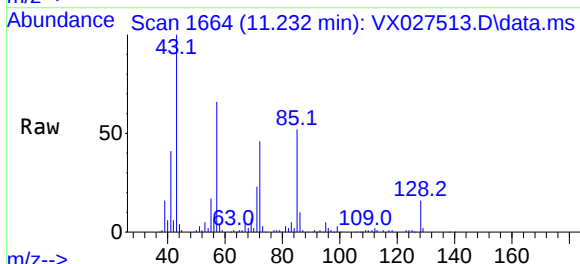




#76  
1,2,3-Trichloropropane  
Concen: 1.268 ug/l  
RT: 11.305 min Scan# 1676  
Delta R.T. 0.061 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 75 Resp: 6869  
Ion Ratio Lower Upper  
75 100  
77 628.8 19.4 58.2#

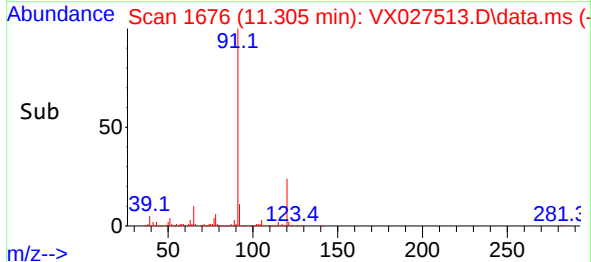

#78  
n-propylbenzene  
Concen: 52.166 ug/l  
RT: 11.305 min Scan# 1676  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 91 Resp: 1080117  
Ion Ratio Lower Upper  
91 100  
120 24.4 11.6 34.8


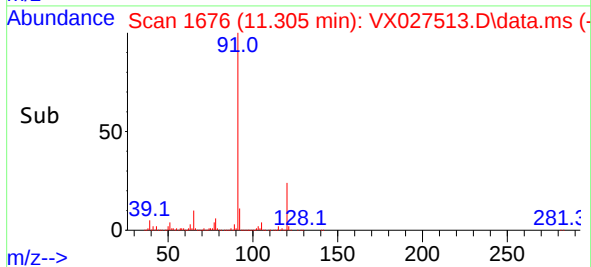

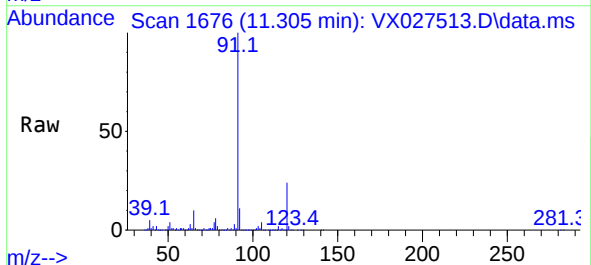




#79  
2-Chlorotoluene  
Concen: 45.674 ug/l  
RT: 11.384 min Scan# 1  
Delta R.T. 0.018 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 91 Resp: 593229  
Ion Ratio Lower Upper  
91 100  
126 0.0 17.3 51.9#

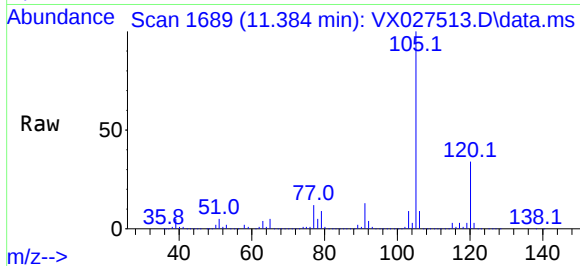

#80  
1,3,5-Trimethylbenzene  
Concen: 214.394 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:105 Resp: 3403497  
Ion Ratio Lower Upper  
105 100  
120 49.8 24.3 72.9


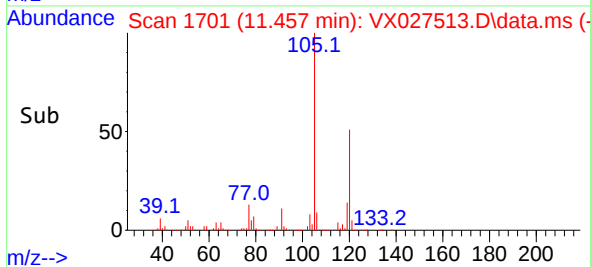

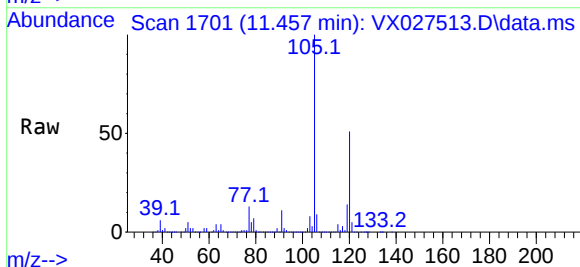




#81  
trans-1,4-Dichloro-2-butene  
Concen: 69.477 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.067 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion: 75 Resp: 123912  
Ion Ratio Lower Upper  
75 100  
53 1.2 69.0 103.4#  
89 0.0 37.0 55.6#

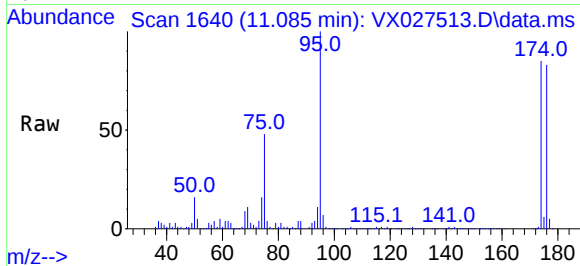

#82  
4-Chlorotoluene  
Concen: 25.042 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 91 Resp: 370328  
Ion Ratio Lower Upper  
91 100  
126 0.1 14.9 44.5#


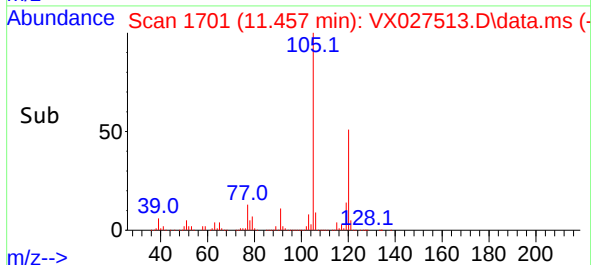
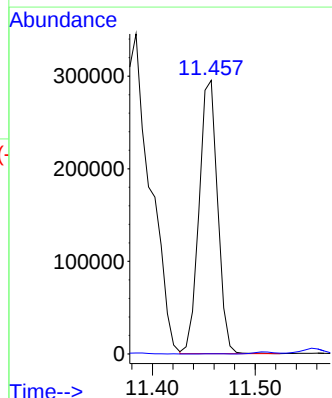
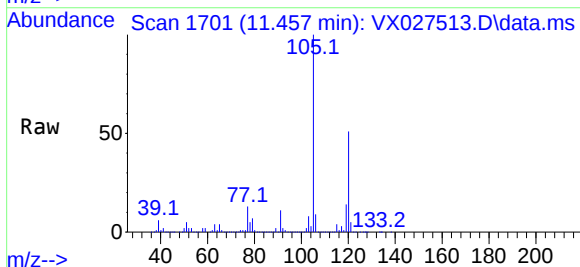




#83  
tert-Butylbenzene  
Concen: 11.487 ug/l  
RT: 11.719 min Scan# 1744  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:119 Resp: 180648  
Ion Ratio Lower Upper  
119 100  
91 66.8 26.9 80.6  
134 23.9 11.4 34.2

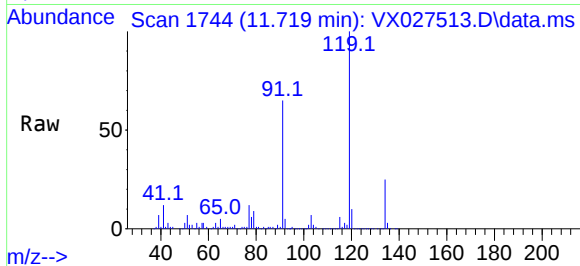

#84  
1,2,4-Trimethylbenzene  
Concen: 389.089 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:105 Resp: 6160021  
Ion Ratio Lower Upper  
105 100  
120 49.1 22.6 67.8


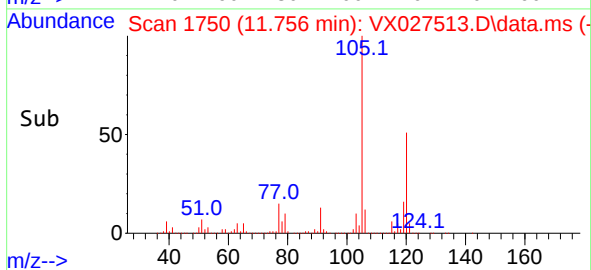

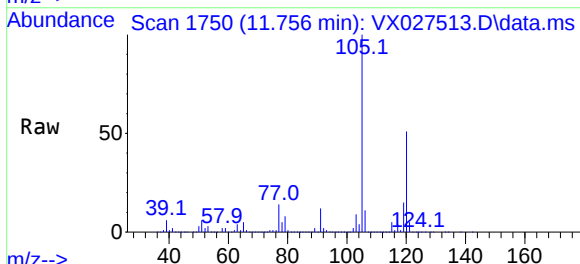




#85  
 sec-Butylbenzene  
 Concen: 324.136 ug/l  
 RT: 11.756 min Scan# 11750  
 Delta R.T. -0.134 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124


Tgt Ion:105 Resp: 6160021  
 Ion Ratio Lower Upper  
 105 100  
 134 0.0 10.2 30.4#

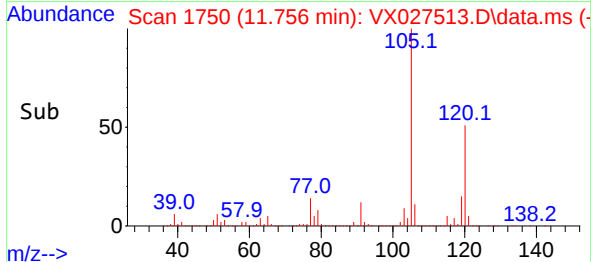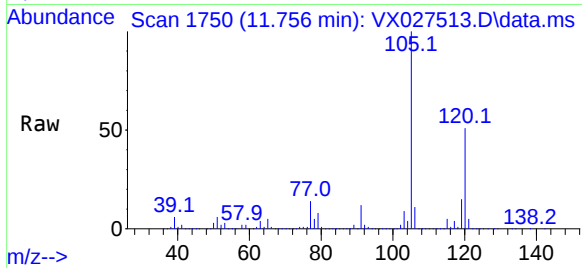

#86  
 p-Isopropyltoluene  
 Concen: 3.814 ug/l  
 RT: 11.975 min Scan# 1786  
 Delta R.T. -0.036 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40

Tgt Ion:119 Resp: 62257  
 Ion Ratio Lower Upper  
 119 100  
 134 27.6 13.0 39.0  
 91 0.0 11.3 33.9#


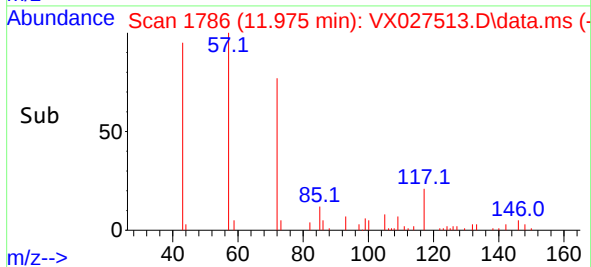

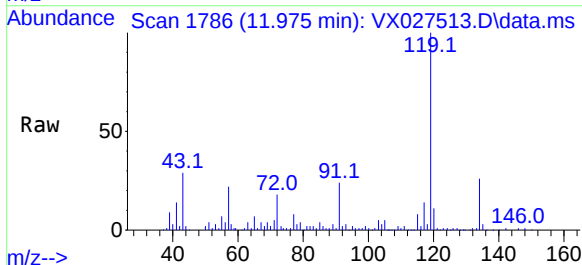




#88  
1,4-Dichlorobenzene  
Concen: 0.256 ug/l  
RT: 12.042 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:146 Resp: 2283  
Ion Ratio Lower Upper  
146 100  
111 0.0 19.2 57.6#  
148 93.5 32.3 96.9

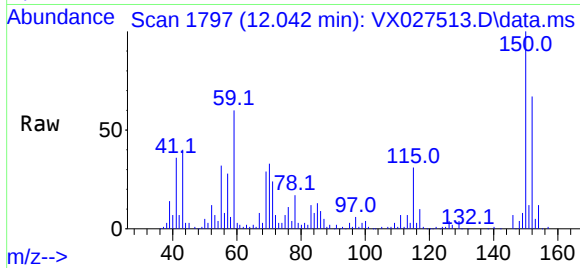

#89  
n-Butylbenzene  
Concen: 17.442 ug/l  
RT: 12.323 min Scan# 1843  
Delta R.T. -0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 91 Resp: 237601  
Ion Ratio Lower Upper  
91 100  
92 21.7 27.8 83.3#  
134 142.6 13.3 39.8#


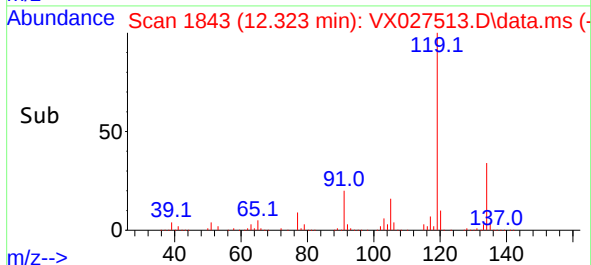
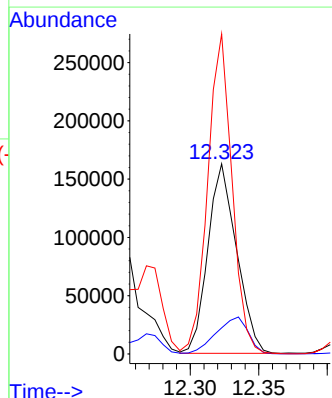
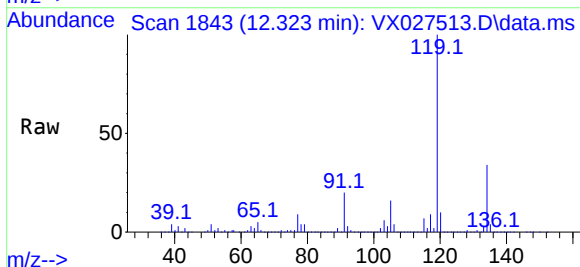




#90  
Hexachloroethane  
Concen: 13.876 ug/l  
RT: 12.536 min Scan# 117  
Delta R.T. -0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124


Tgt Ion:117 Resp: 36121  
Ion Ratio Lower Upper  
117 100  
201 0.0 39.5 118.5#

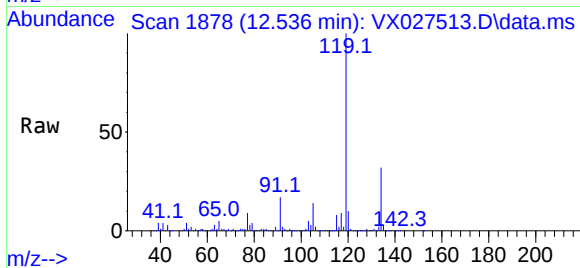

#91  
1,2-Dichlorobenzene  
Concen: 0.366 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion:146 Resp: 3149  
Ion Ratio Lower Upper  
146 100  
111 120.1 21.0 63.0#  
148 70.8 32.6 97.7

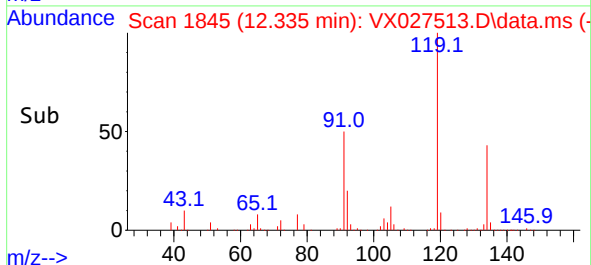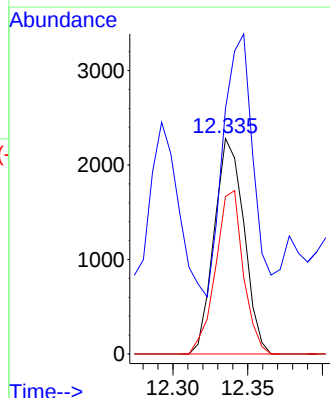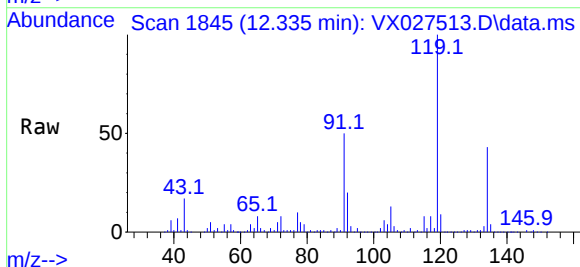



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.750 ug/l

RT: 12.926 min Scan# 1942

Delta R.T. -0.018 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

Instrument :

MSVOA\_X

ClientSampleId :

MW-124





Tgt Ion: 75 Resp: 3769

Ion Ratio Lower Upper

75 100

155 0.0 47.0 141.2#

157 0.0 57.9 173.6#

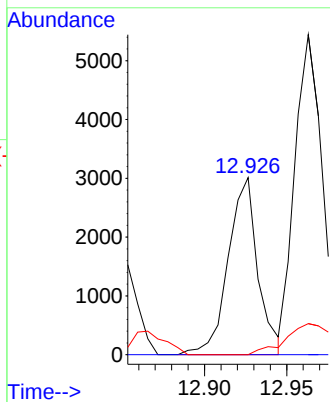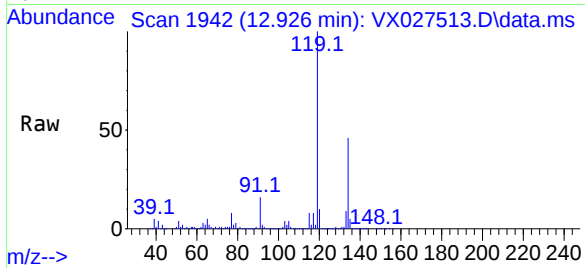

#95

Naphthalene

Concen: 126.264 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

Tgt Ion:128 Resp: 2265986

Ion Ratio Lower Upper

128 100

127 12.9 10.2 15.4

129 11.2 8.7 13.1

