

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
 Data File : VX027492.D
 Acq On : 17 Mar 2022 17:17
 Operator : JC/MD
 Sample : VX0317WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0317WBL01

Quant Time: Mar 18 02:05:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	347936	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	570099	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	507537	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	232663	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	215329	50.237	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	100.480%
35) Dibromofluoromethane	5.391	113	189327	51.617	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	103.240%
50) Toluene-d8	8.653	98	660755	47.606	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.220%
62) 4-Bromofluorobenzene	11.079	95	238944	46.837	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	93.680%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
Data File : VX027492.D
Acq On : 17 Mar 2022 17:17
Operator : JC/MD
Sample : VX0317WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0317WBL01

Quant Time: Mar 18 02:05:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration




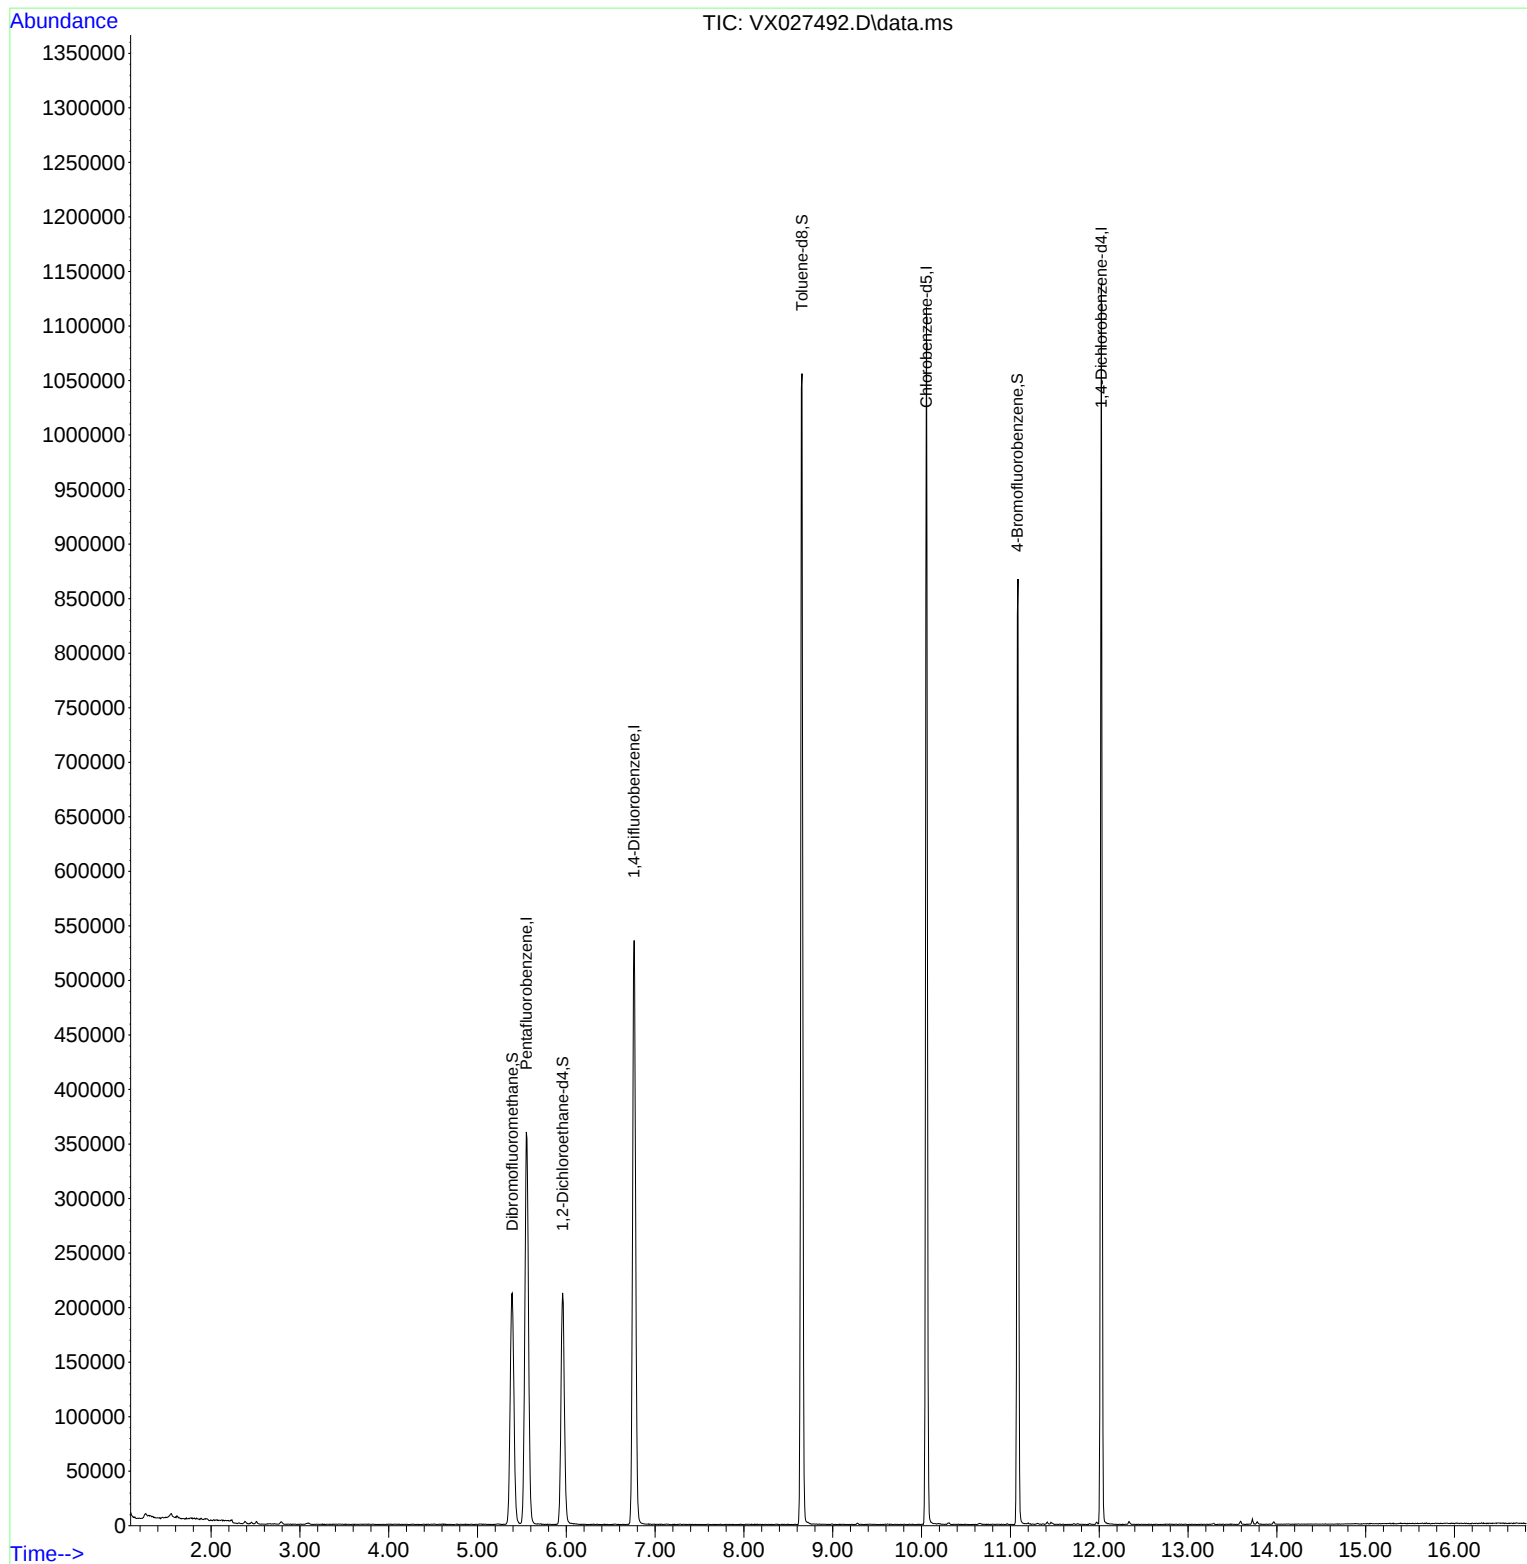




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17




Instrument :
MSVOA_X
ClientSampleId :
VX0317WBL01


Tgt Ion:168 Resp: 347936
Ion Ratio Lower Upper
168 100
99 56.7 41.7 62.5

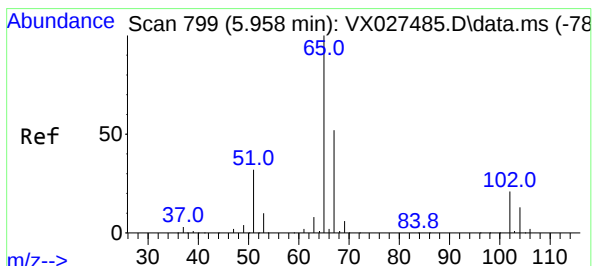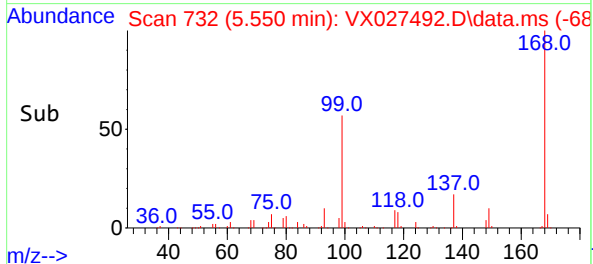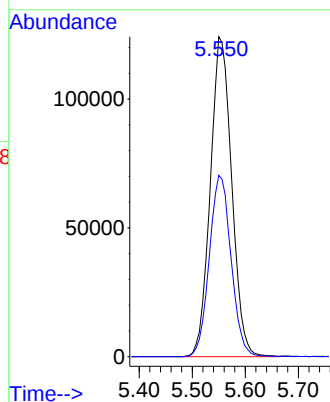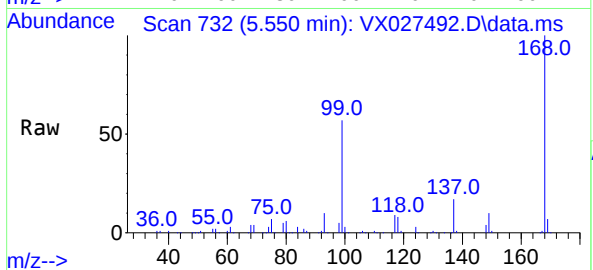

#33
1,2-Dichloroethane-d4
Concen: 50.237 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17

Tgt Ion: 65 Resp: 215329
Ion Ratio Lower Upper
65 100
67 51.2 0.0 107.4


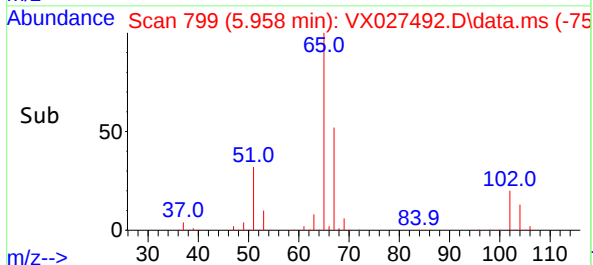
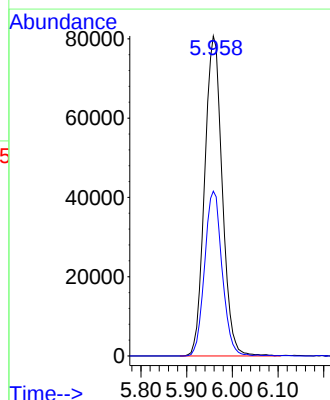
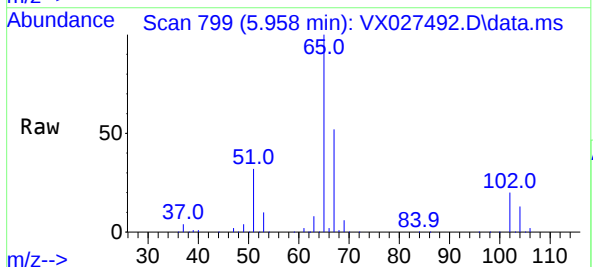


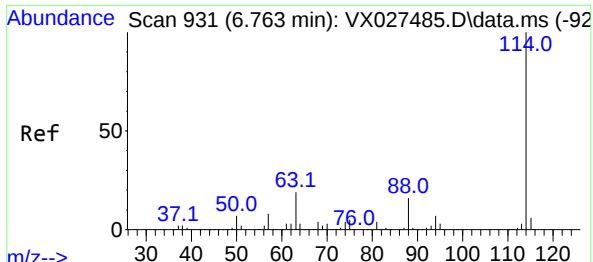

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17




Instrument :
MSVOA_X
ClientSampleId :
VX0317WBL01


Tgt Ion:114 Resp: 570099
Ion Ratio Lower Upper
114 100
63 18.9 0.0 36.8
88 15.9 0.0 32.4

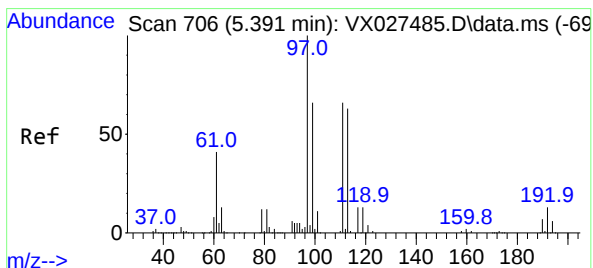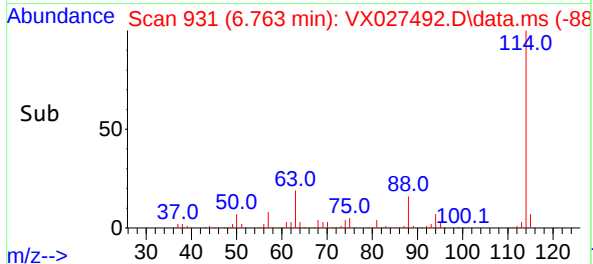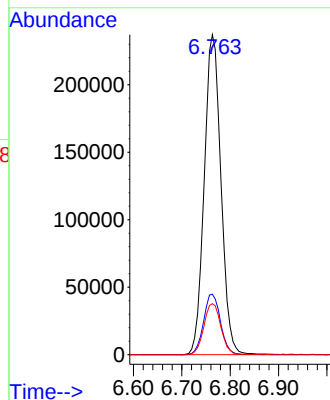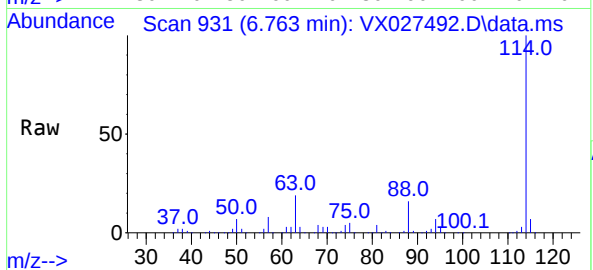

#35
Dibromofluoromethane
Concen: 51.617 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17

Tgt Ion:113 Resp: 189327
Ion Ratio Lower Upper
113 100
111 102.4 82.8 124.2
192 19.7 16.9 25.3


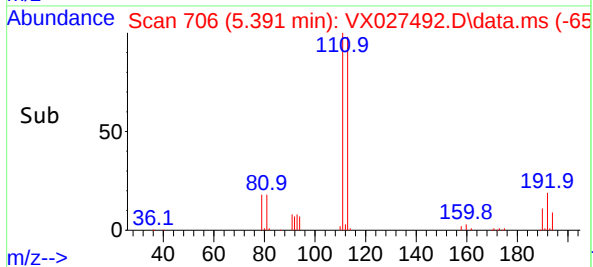
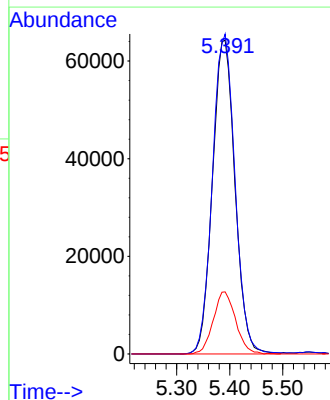
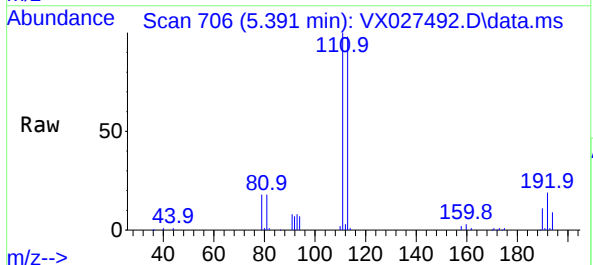


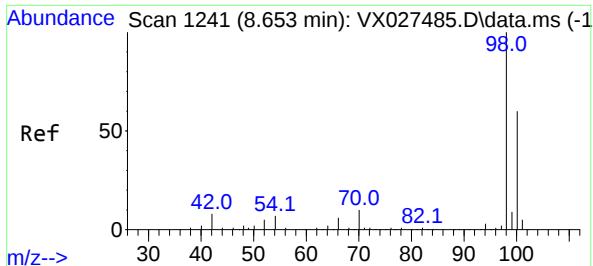

#50
Toluene-d8
Concen: 47.606 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17




Instrument :
MSVOA_X
ClientSampleId :
VX0317WBL01


Tgt Ion: 98 Resp: 660755
Ion Ratio Lower Upper
98 100
100 64.5 52.6 78.8

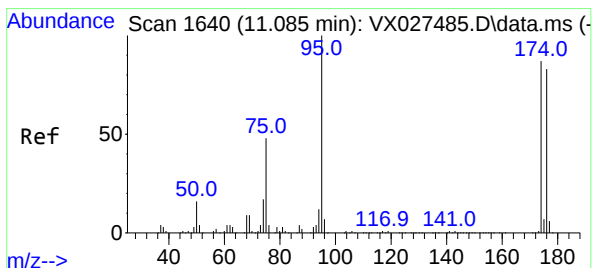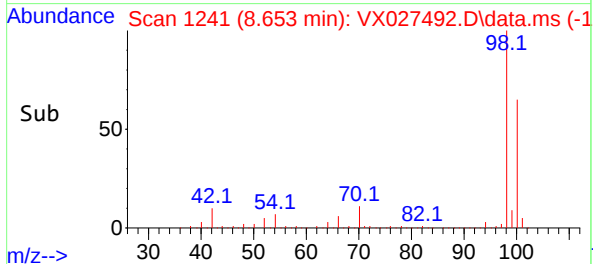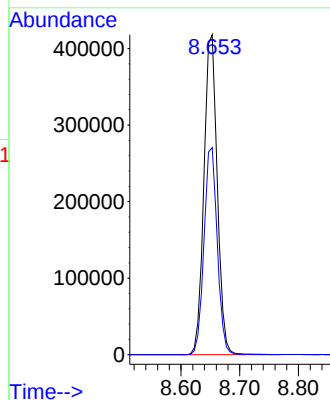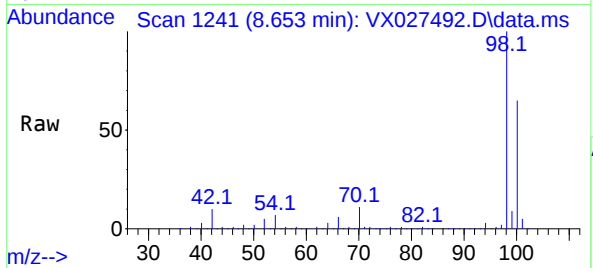

#62
4-Bromofluorobenzene
Concen: 46.837 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17

Tgt Ion: 95 Resp: 238944
Ion Ratio Lower Upper
95 100
174 81.2 0.0 163.0
176 79.5 0.0 155.0


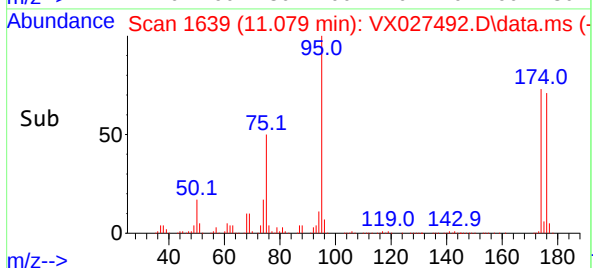
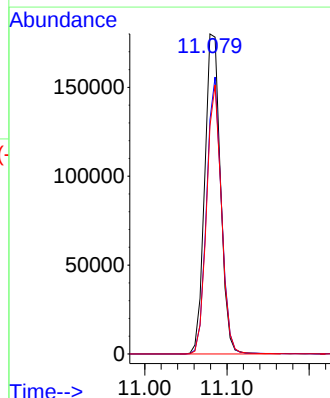
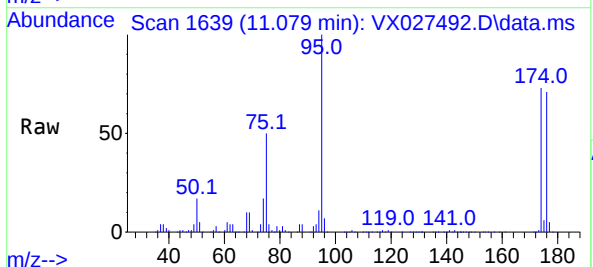


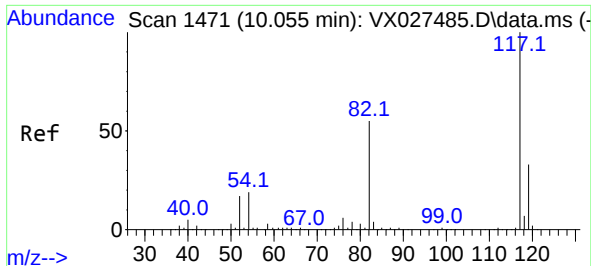

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17

Instrument :
MSVOA_X
ClientSampleId :
VX0317WBL01

Tgt Ion:117 Resp: 507537
Ion Ratio Lower Upper
117 100
82 54.7 41.8 62.8
119 31.7 24.8 37.2

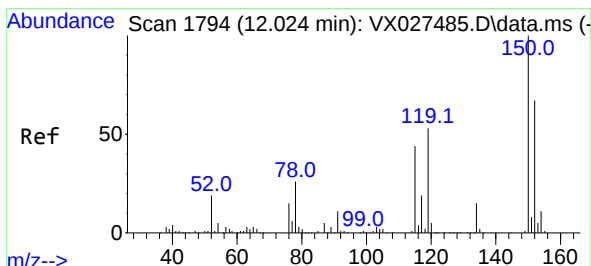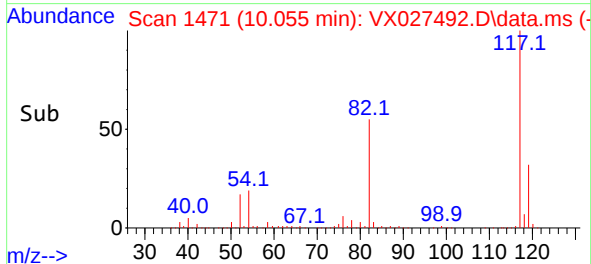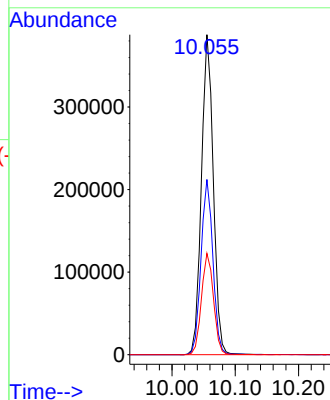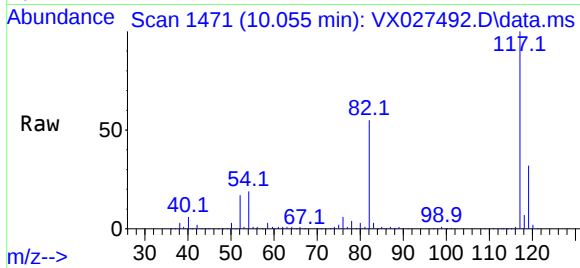

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027492.D
Acq: 17 Mar 2022 17:17

Tgt Ion:152 Resp: 232663
Ion Ratio Lower Upper
152 100
115 59.9 37.5 112.7
150 154.7 0.0 338.2

