

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031722\  
 Data File : VX027513.D  
 Acq On : 18 Mar 2022 01:40  
 Operator : JC/MD  
 Sample : N1997-19  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124

Manual Integrations  
 APPROVED

Reviewed By : John Carlone 03/18/2022  
 Supervised By : Mahesh Dadoda 03/18/2022

Quant Time: Mar 18 03:42:01 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 17 15:02:59 2022  
 Response via : Initial Calibration

| Compound                    | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-----------------------------|----------------|------|------------|----------|--------|----------|
| -----                       |                |      |            |          |        |          |
| Internal Standards          |                |      |            |          |        |          |
| 1) Pentafluorobenzene       | 5.556          | 168  | 346822     | 50.000   | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene     | 6.769          | 114  | 565381     | 50.000   | ug/l   | 0.00     |
| 63) Chlorobenzene-d5        | 10.055         | 117  | 525650     | 50.000   | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4  | 12.024         | 152  | 258957     | 50.000   | ug/l   | 0.00     |
|                             |                |      |            |          |        |          |
| System Monitoring Compounds |                |      |            |          |        |          |
| 33) 1,2-Dichloroethane-d4   | 5.958          | 65   | 212256     | 49.680   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 61 - 141 |      | Recovery = | 99.360%  |        |          |
| 35) Dibromofluoromethane    | 5.391          | 113  | 189993     | 52.231   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 69 - 133 |      | Recovery = | 104.460% |        |          |
| 50) Toluene-d8              | 8.653          | 98   | 681567     | 49.515   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 65 - 126 |      | Recovery = | 99.020%  |        |          |
| 62) 4-Bromofluorobenzene    | 11.085         | 95   | 255311     | 50.463   | ug/l   | 0.00     |
| Spiked Amount 50.000        | Range 58 - 135 |      | Recovery = | 100.920% |        |          |
|                             |                |      |            |          |        |          |
| Target Compounds            |                |      |            |          | Qvalue |          |
| 11) Tert butyl alcohol      | 2.965          | 59   | 38271      | 47.001   | ug/l   | 99       |
| 16) Acetone                 | 2.380          | 43   | 30570      | 17.554   | ug/l   | 93       |
| 17) Carbon Disulfide        | 2.514          | 76   | 6000       | 0.732    | ug/l   | 97       |
| 19) Methyl tert-butyl Ether | 3.117          | 73   | 125999     | 11.596   | ug/l # | 33       |
| 22) Diisopropyl ether       | 3.776          | 45   | 4840       | 0.492    | ug/l # | 82       |
| 25) 2-Butanone              | 4.568          | 43   | 10694      | 4.081    | ug/l   | 98       |
| 31) Cyclohexane             | 5.477          | 56   | 115481     | 21.767   | ug/l   | 99       |
| 39) Methylcyclohexane       | 7.385          | 83   | 179977     | 28.792   | ug/l   | 94       |
| 40) Benzene                 | 6.044          | 78   | 722849     | 50.686   | ug/l   | 98       |
| 42) 1,2-Dichloroethane      | 6.086          | 62   | 15663      | 2.931    | ug/l   | 91       |
| 51) 4-Methyl-2-Pentanone    | 8.580          | 43   | 11251      | 2.211    | ug/l   | 91       |
| 52) Toluene                 | 8.720          | 92   | 1777045    | 185.946  | ug/l   | 98       |
| 59) 2-Hexanone              | 9.445          | 43   | 25991      | 6.631    | ug/l   | 69       |
| 64) Tetrachloroethene       | 9.275          | 164  | 1286       | 0.315    | ug/l   | 88       |
| 67) Ethyl Benzene           | 10.201         | 91   | 8708564    | 470.520  | ug/l # | 81       |
| 68) m/p-Xylenes             | 10.311         | 106  | 7397274    | 1015.057 | ug/l   | 77       |
| 69) o-Xylene                | 10.646         | 106  | 2209326    | 312.237  | ug/l   | 95       |
| 73) Isopropylbenzene        | 10.963         | 105  | 251798     | 13.350   | ug/l   | 99       |
| 78) n-propylbenzene         | 11.305         | 91   | 1080117    | 52.166   | ug/l   | 98       |
| 80) 1,3,5-Trimethylbenzene  | 11.457         | 105  | 3403497    | 214.394  | ug/l   | 98       |
| 83) tert-Butylbenzene       | 11.719         | 119  | 180648     | 11.487   | ug/l   | 86       |
| 84) 1,2,4-Trimethylbenzene  | 11.756         | 105  | 6160021    | 389.089  | ug/l   | 94       |
| 85) sec-Butylbenzene        | 11.890         | 105  | 36023m     | 1.896    | ug/l   |          |
| 86) p-Isopropyltoluene      | 12.012         | 119  | 18329m     | 1.123    | ug/l   |          |
| 95) Naphthalene             | 13.780         | 128  | 2265986    | 126.264  | ug/l   | 100      |
| -----                       |                |      |            |          |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031722\  
Data File : VX027513.D  
Acq On : 18 Mar 2022 01:40  
Operator : JC/MD  
Sample : N1997-19  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1


Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Quant Time: Mar 18 03:42:01 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
Quant Title : SW846 8260  
QLast Update : Thu Mar 17 15:02:59 2022  
Response via : Initial Calibration

Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

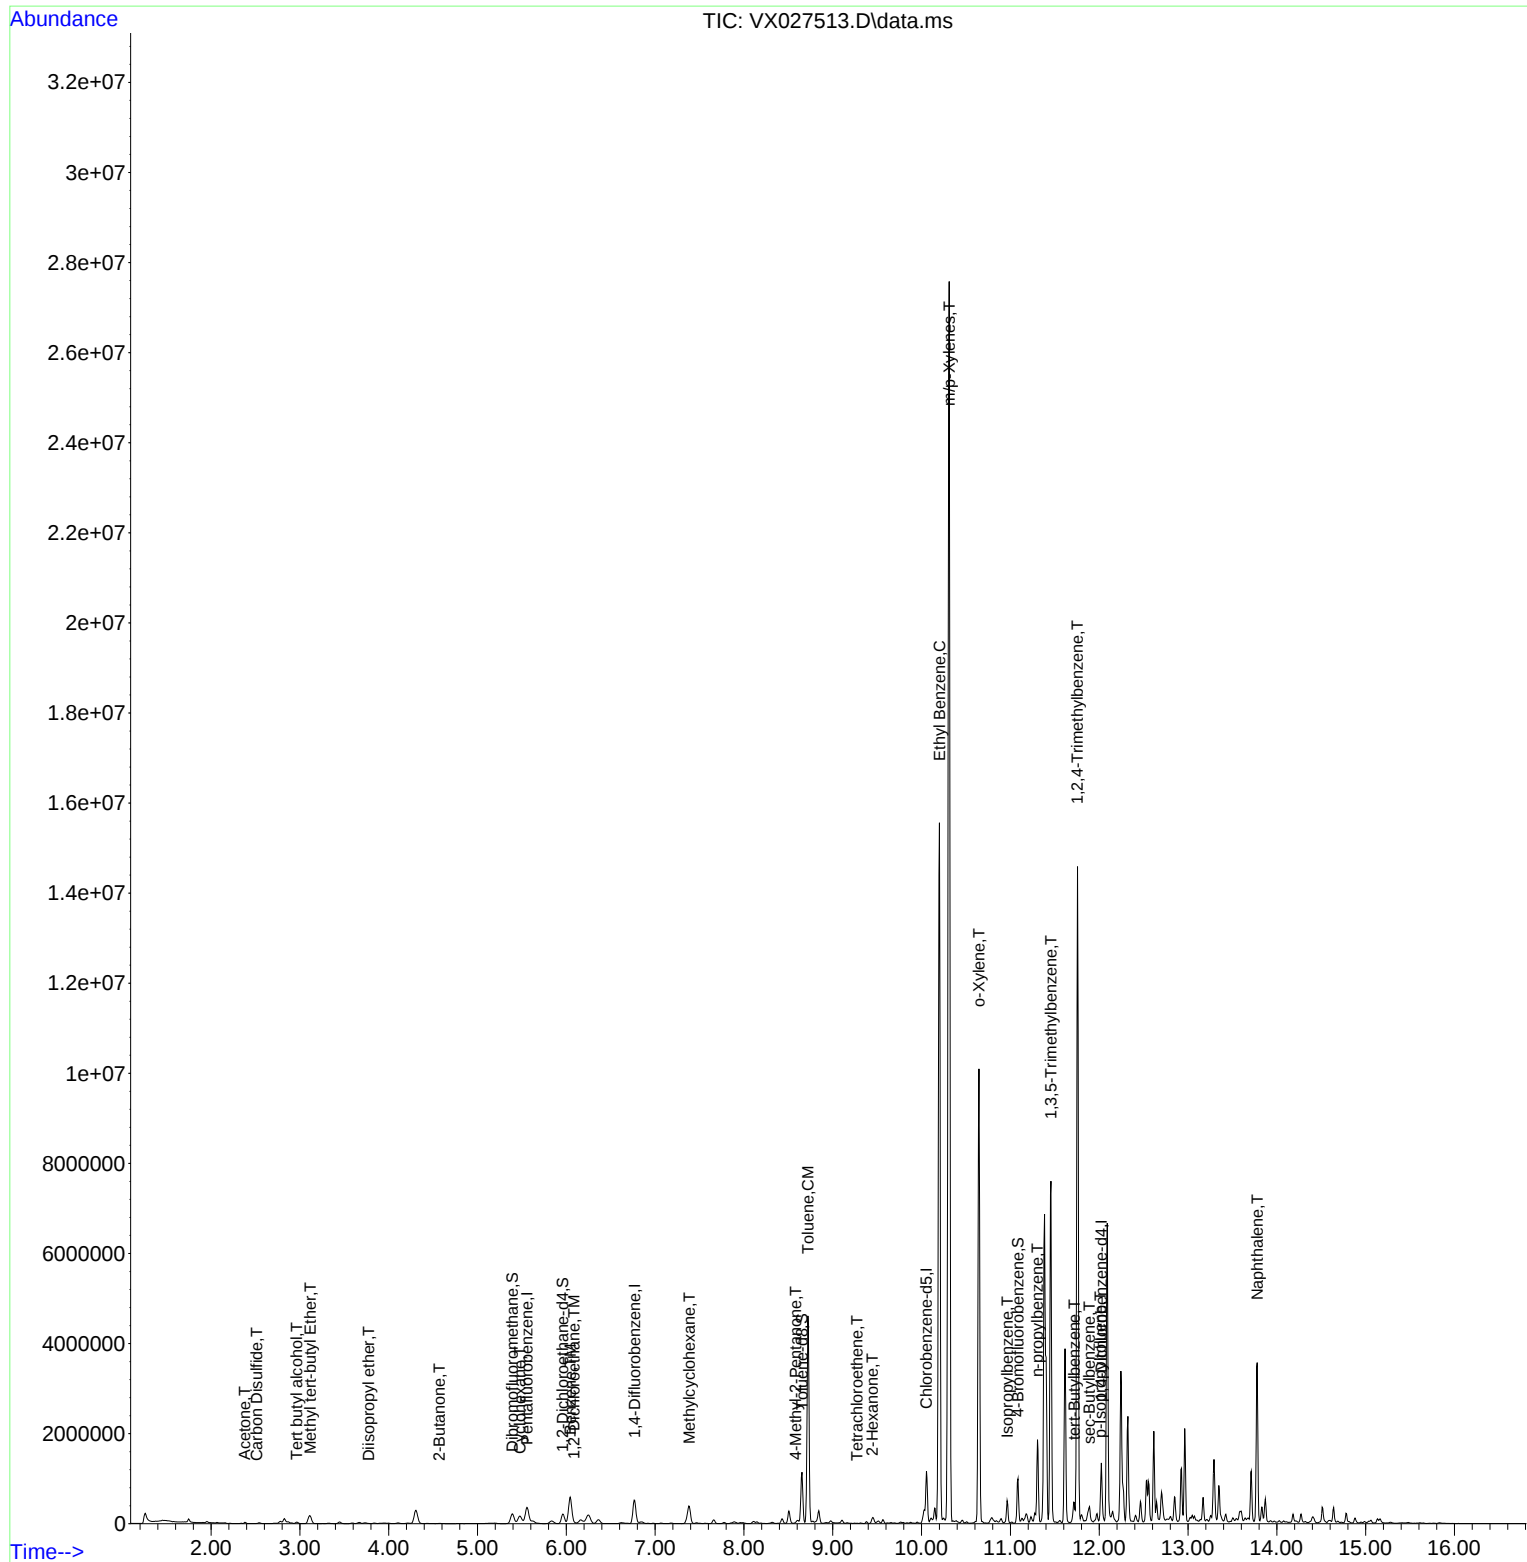

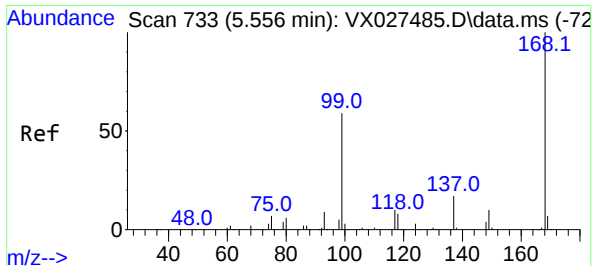

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.556 min Scan# 713  
Delta R.T. -0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

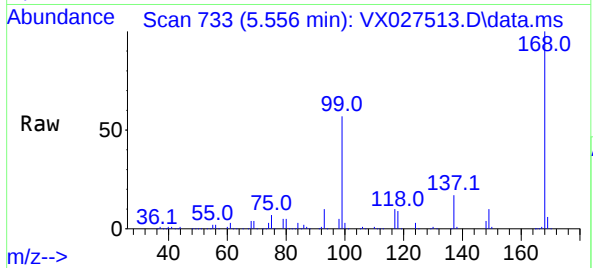


Tgt Ion:168 Resp: 34682  
Ion Ratio Lower Upper  
168 100  
99 57.4 41.7 62.5

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

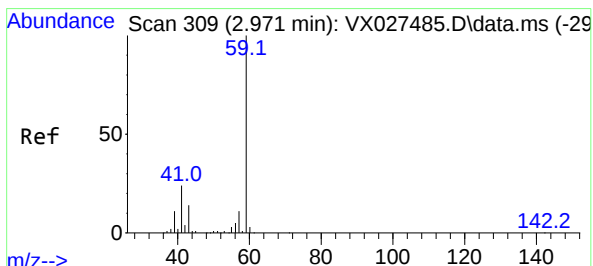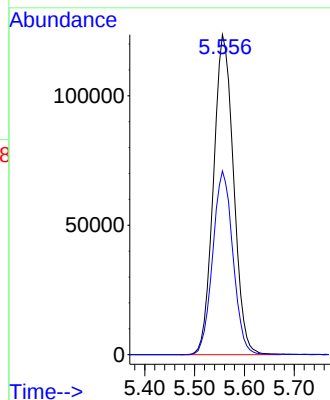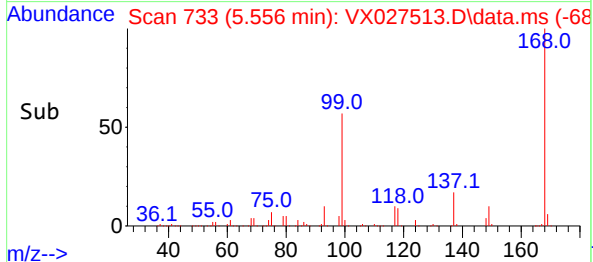


#11  
Tert butyl alcohol  
Concen: 47.001 ug/l  
RT: 2.965 min Scan# 308  
Delta R.T. -0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

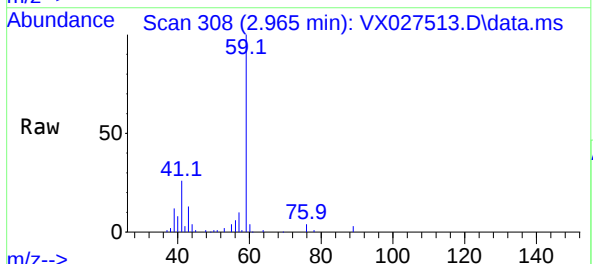

Tgt Ion: 59 Resp: 38271  
Ion Ratio Lower Upper  
59 100  
57 10.2 8.3 12.5

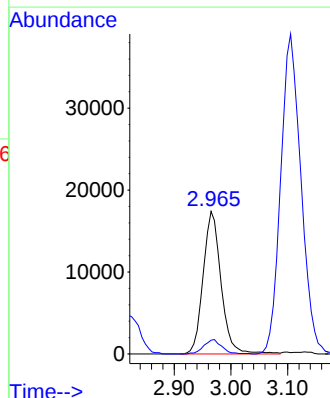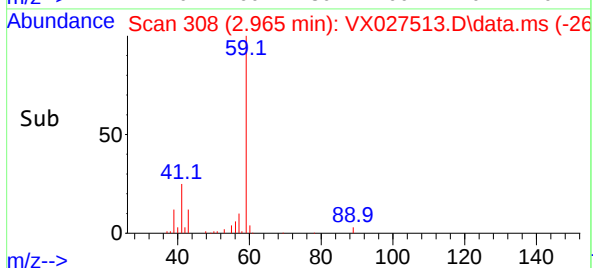







#16  
Acetone  
Concen: 17.554 ug/l  
RT: 2.380 min Scan# 21  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion: 43 Resp: 30570  
Ion Ratio Lower Upper  
43 100  
58 31.7 28.8 43.2




Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022



#17  
Carbon Disulfide  
Concen: 0.732 ug/l  
RT: 2.514 min Scan# 234  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40


Tgt Ion: 76 Resp: 6000  
Ion Ratio Lower Upper  
76 100  
78 7.7 7.2 10.8

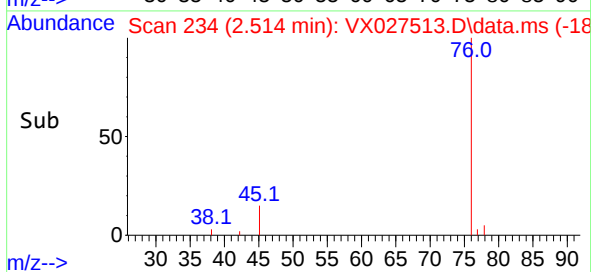



#19  
Methyl tert-butyl Ether  
Concen: 11.596 ug/l  
RT: 3.117 min Scan# 311  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124




Tgt Ion: 73 Resp: 12599  
Ion Ratio Lower Upper  
73 100  
57 52.4 16.8 25.2

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

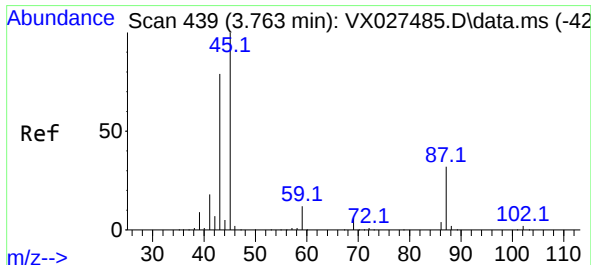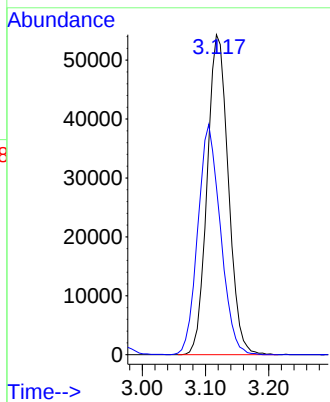


#22  
Diisopropyl ether  
Concen: 0.492 ug/l  
RT: 3.776 min Scan# 441  
Delta R.T. 0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

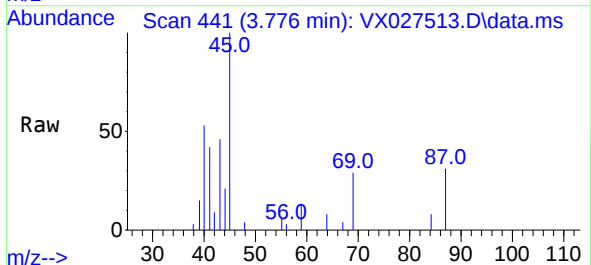

Tgt Ion: 45 Resp: 4840  
Ion Ratio Lower Upper  
45 100  
43 40.4 50.8 76.2#  
87 30.9 26.6 39.8  
59 13.1 10.5 15.7

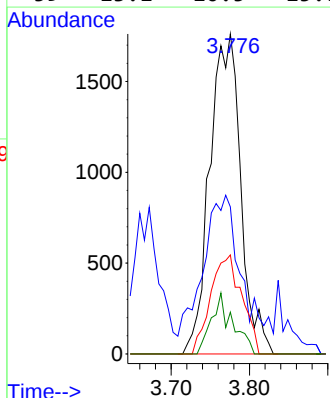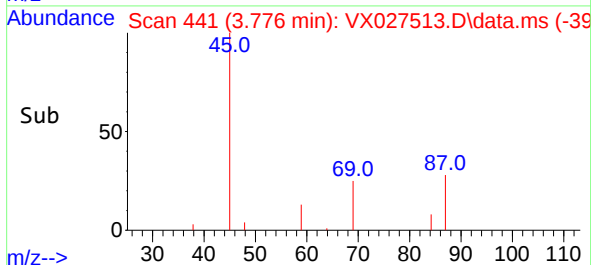







#25  
2-Butanone  
Concen: 4.081 ug/l  
RT: 4.568 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion: 43 Resp: 10694  
Ion Ratio Lower Upper  
43 100  
72 29.5 24.4 36.6




Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022



#31  
Cyclohexane  
Concen: 21.767 ug/l  
RT: 5.477 min Scan# 720  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Tgt Ion: 56 Resp: 115481  
Ion Ratio Lower Upper  
56 100  
69 31.2 26.7 40.1  
84 97.0 77.2 115.8

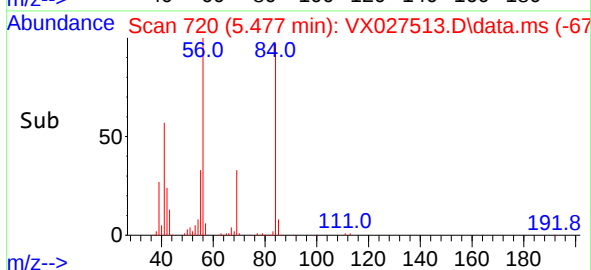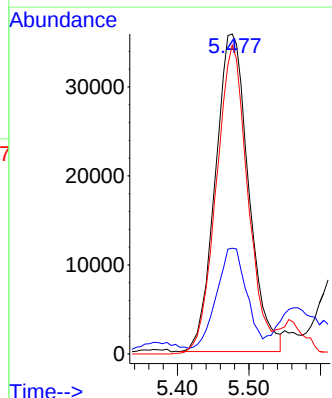



#33

1,2-Dichloroethane-d4

Concen: 49.680 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40

Instrument :

MSVOA\_X

ClientSampleId :

MW-124

Tgt Ion: 65 Resp: 212250

Ion Ratio Lower Upper

65 100





67 50.9 0.0 107.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 03/18/2022

Supervised By :Mahesh Dadoda 03/18/2022

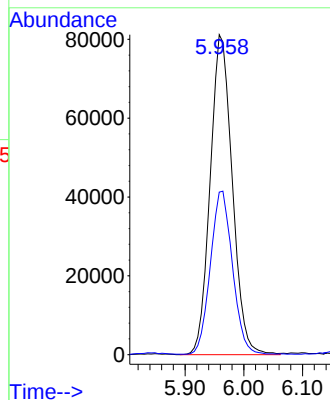

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX027513.D

Acq: 18 Mar 2022 01:40




Tgt Ion:114 Resp: 565381


Ion Ratio Lower Upper

114 100

63 18.8 0.0 36.8


88 15.7 0.0 32.4

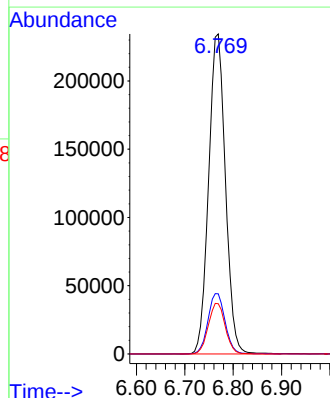

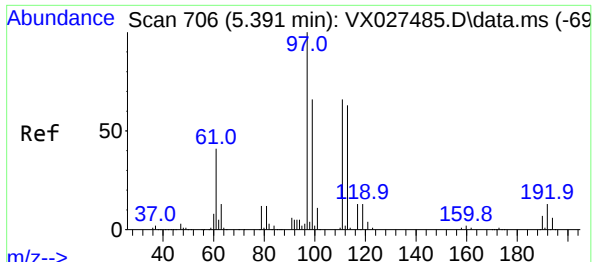

#35  
Dibromofluoromethane  
Concen: 52.231 ug/l  
RT: 5.391 min Scan# 706  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

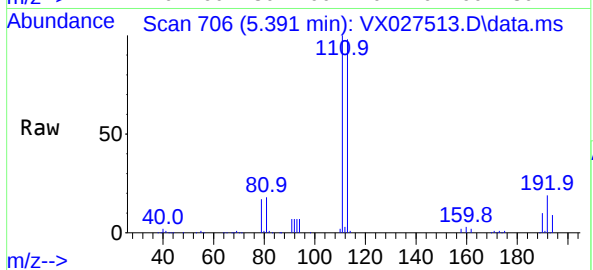


Tgt Ion: 113 Resp: 18999  
Ion Ratio Lower Upper  
113 100  
111 101.6 82.8 124.2  
192 19.6 16.9 25.3

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

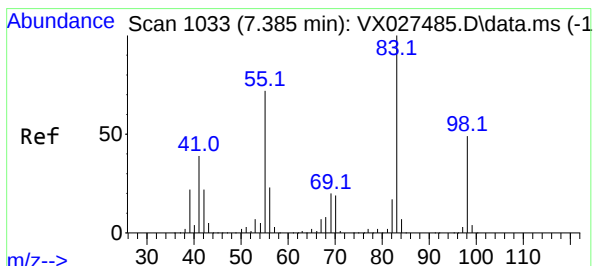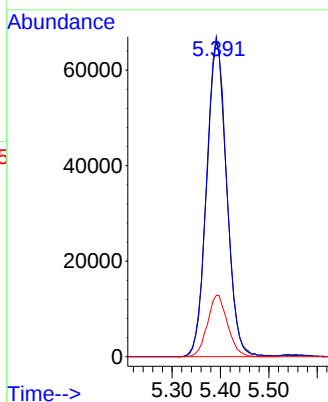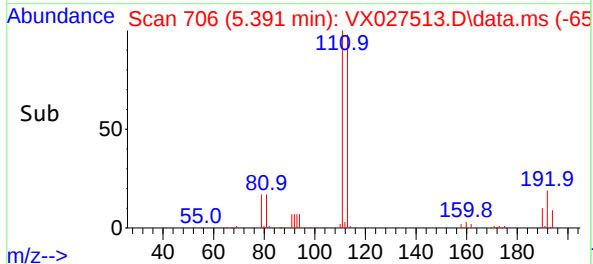


#39  
Methylcyclohexane  
Concen: 28.792 ug/l  
RT: 7.385 min Scan# 1033  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

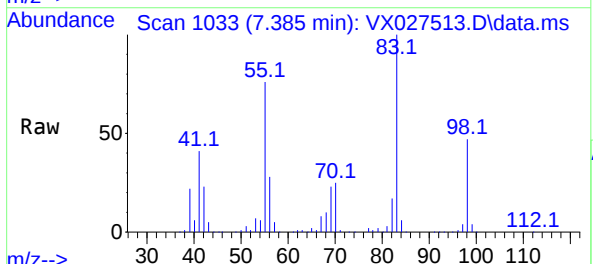

Tgt Ion: 83 Resp: 179977  
Ion Ratio Lower Upper  
83 100  
55 76.3 54.6 81.8  
98 47.4 37.4 56.2

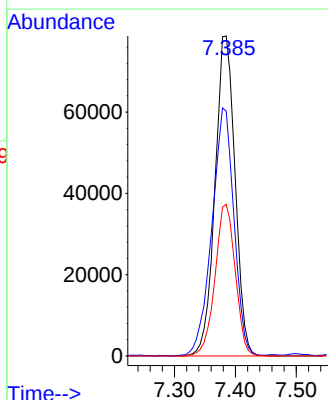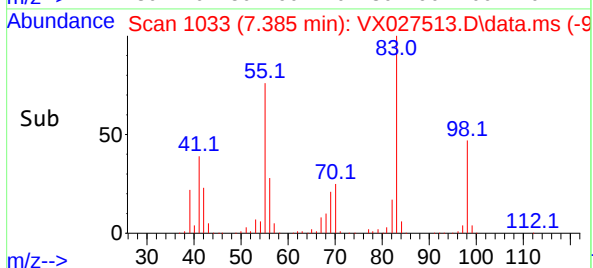







#40  
Benzene  
Concen: 50.686 ug/l  
RT: 6.044 min Scan# 813  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion: 78 Resp: 722849  
Ion Ratio Lower Upper  
78 100  
77 23.0 19.3 28.9




Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

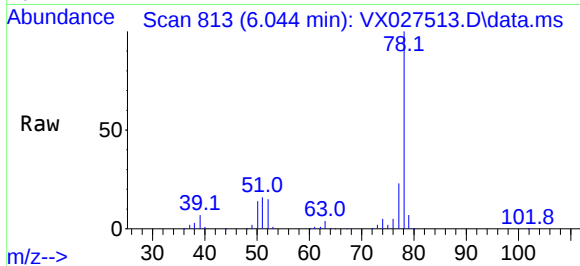

#42  
1,2-Dichloroethane  
Concen: 2.931 ug/l  
RT: 6.086 min Scan# 820  
Delta R.T. -0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40


Tgt Ion: 62 Resp: 15663  
Ion Ratio Lower Upper  
62 100  
98 13.5 0.0 20.4

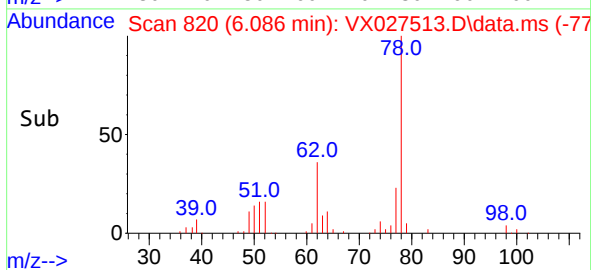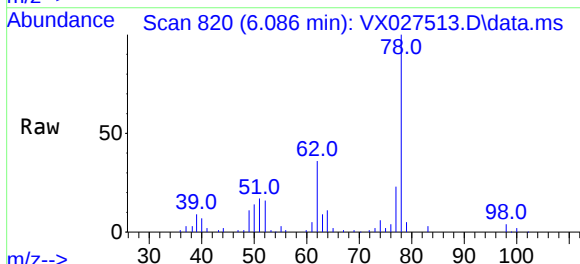

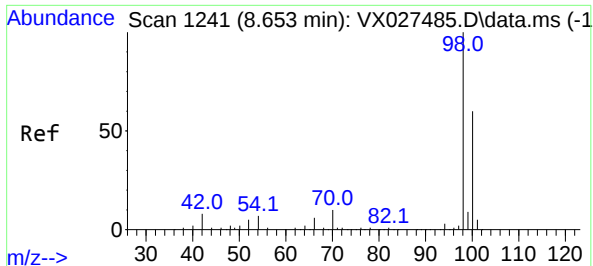

#50  
Toluene-d8  
Concen: 49.515 ug/l  
RT: 8.653 min Scan# 1241  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

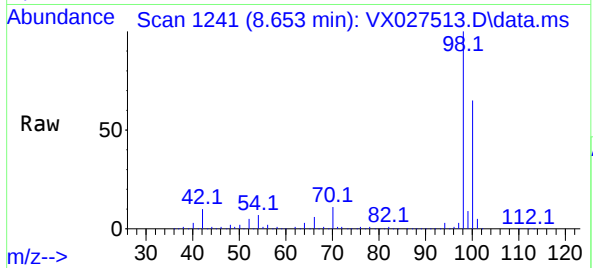


Tgt Ion: 98 Resp: 68156  
Ion Ratio Lower Upper  
98 100  
100 64.5 52.6 78.8

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

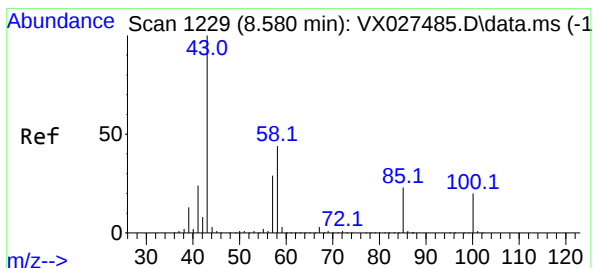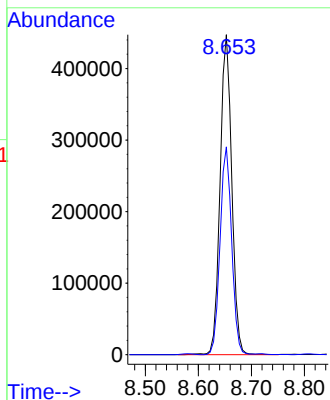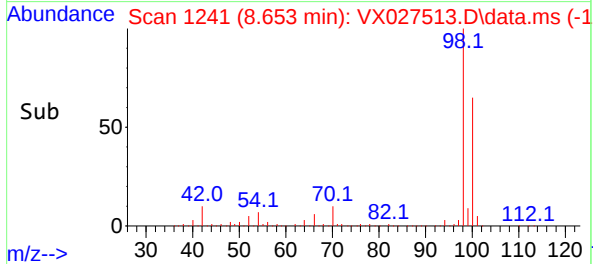


#51  
4-Methyl-2-Pentanone  
Concen: 2.211 ug/l  
RT: 8.580 min Scan# 1229  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

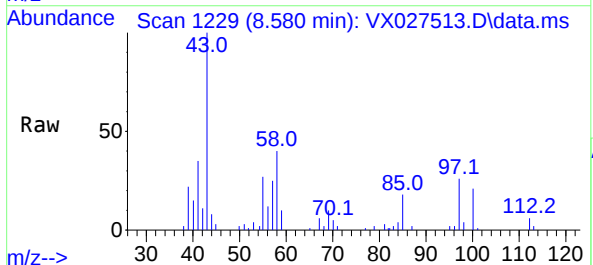


Tgt Ion: 43 Resp: 11251  
Ion Ratio Lower Upper  
43 100  
58 39.3 36.1 54.1

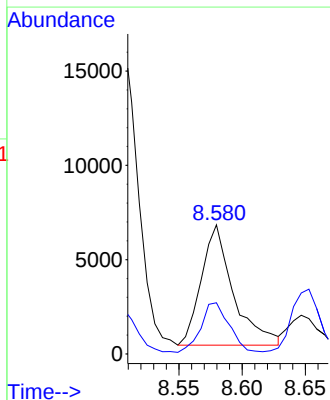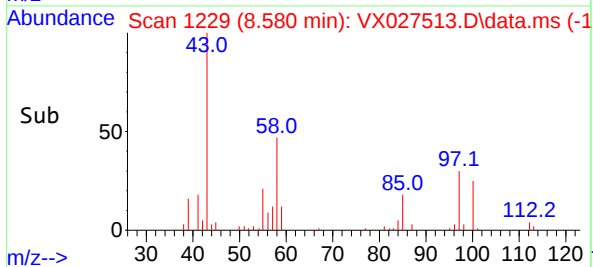

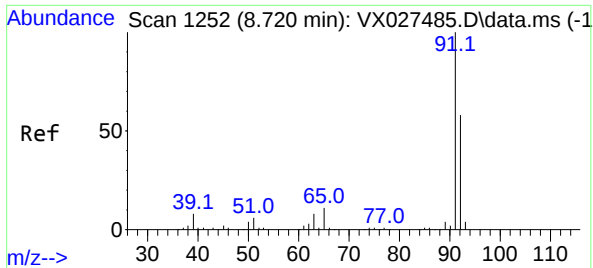

#52  
Toluene  
Concen: 185.946 ug/l  
RT: 8.720 min Scan# 1177  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

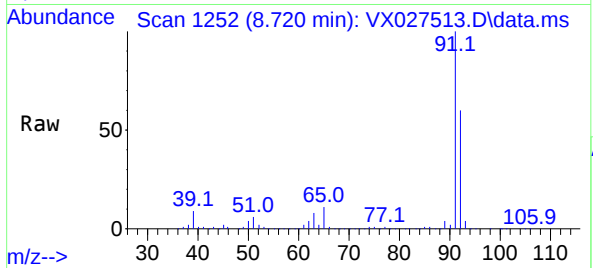


Tgt Ion: 92 Resp: 1777045  
Ion Ratio Lower Upper  
92 100  
91 169.5 137.5 206.3

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

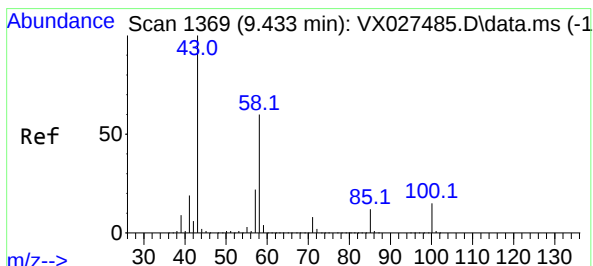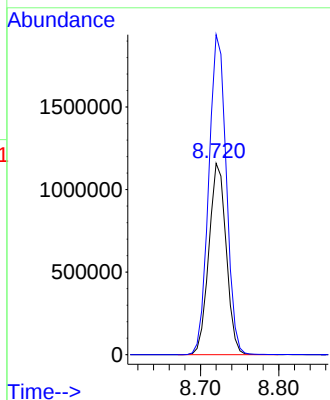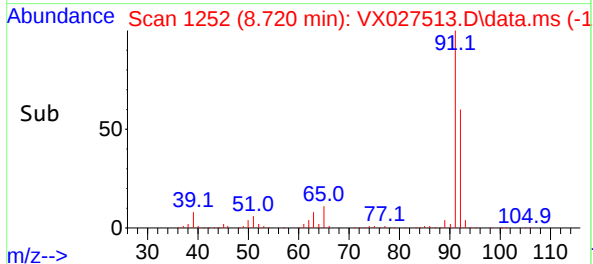


#59  
2-Hexanone  
Concen: 6.631 ug/l  
RT: 9.445 min Scan# 1371  
Delta R.T. 0.012 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

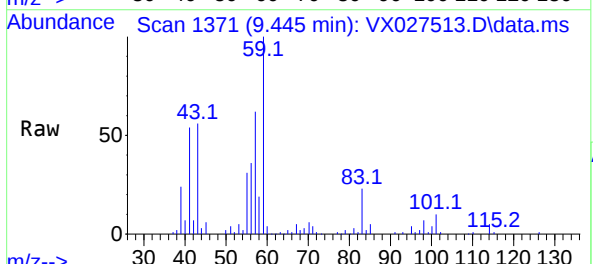


Tgt Ion: 43 Resp: 25991  
Ion Ratio Lower Upper  
43 100  
58 39.7 31.9 95.7

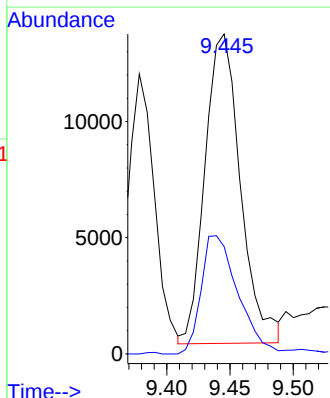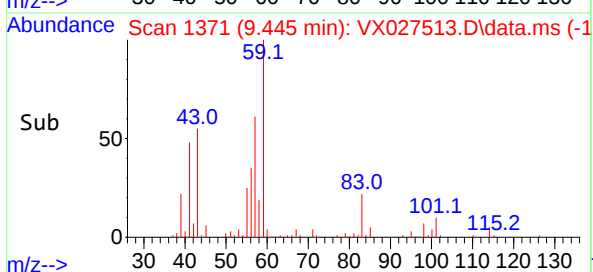



#62  
4-Bromofluorobenzene  
Concen: 50.463 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

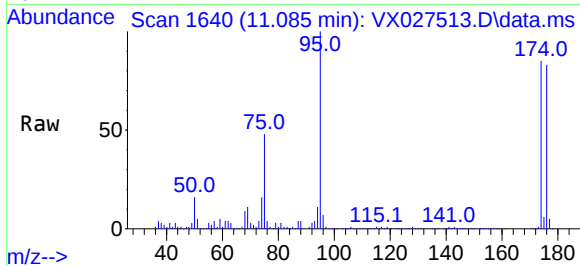


Tgt Ion: 95 Resp: 25531  
Ion Ratio Lower Upper  
95 100  
174 81.1 0.0 163.0  
176 78.4 0.0 155.0

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

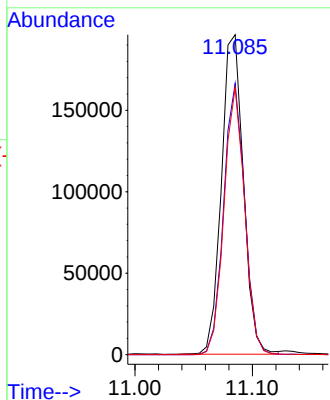


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

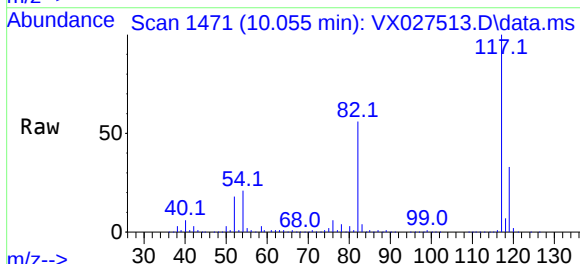


Tgt Ion:117 Resp: 525650  
Ion Ratio Lower Upper  
117 100  
82 55.8 41.8 62.8  
119 32.9 24.8 37.2

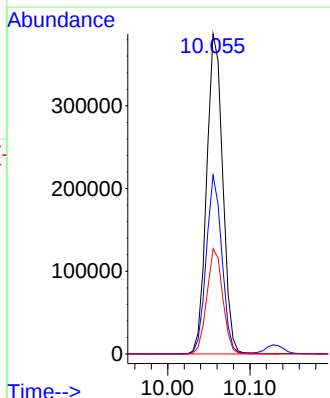



#64  
Tetrachloroethene  
Concen: 0.315 ug/l  
RT: 9.275 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124




Tgt Ion:164 Resp: 1280  
Ion Ratio Lower Upper  
164 100  
166 106.9 101.2 151.8  
129 78.2 73.0 109.4  
131 90.3 74.2 111.2

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

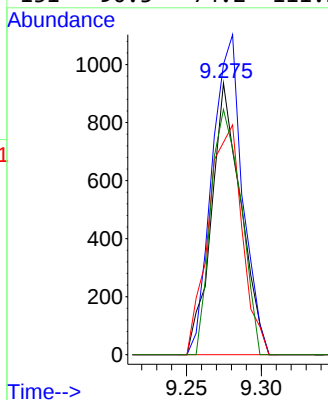


#67  
Ethyl Benzene  
Concen: 470.520 ug/l  
RT: 10.201 min Scan# 1495  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

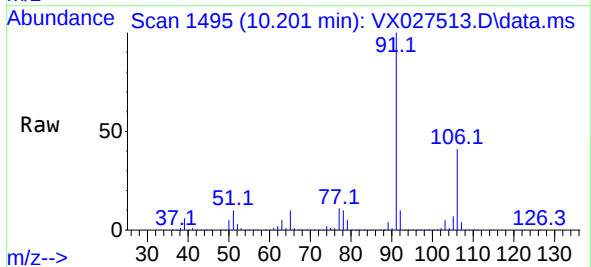

Tgt Ion: 91 Resp: 8708564  
Ion Ratio Lower Upper  
91 100  
106 41.2 24.6 36.8#

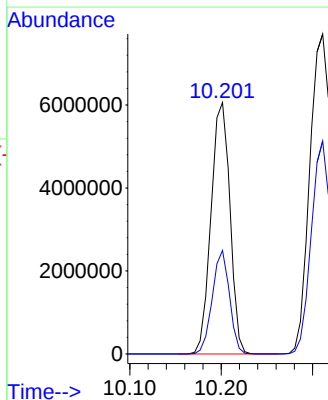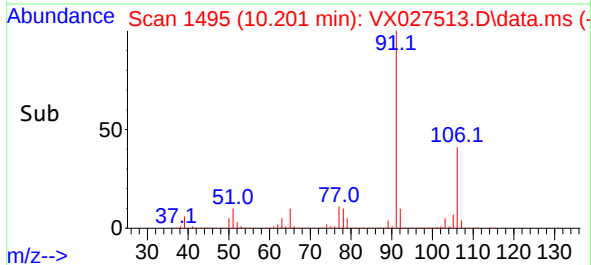







#68  
m/p-Xylenes  
Concen: 1015.057 ug/l  
RT: 10.311 min Scan# 1512  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion:106 Resp: 7397274  
Ion Ratio Lower Upper  
106 100  
91 166.0 160.4 240.6




Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

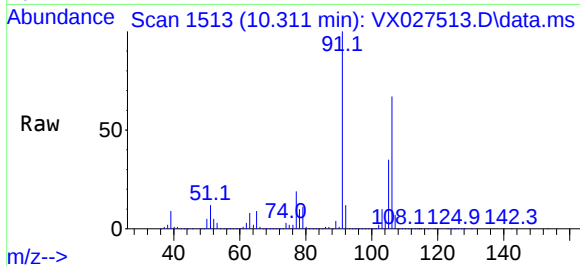

#69  
o-Xylene  
Concen: 312.237 ug/l  
RT: 10.646 min Scan# 1568  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40


Tgt Ion:106 Resp: 2209326  
Ion Ratio Lower Upper  
106 100  
91 204.6 106.1 318.1

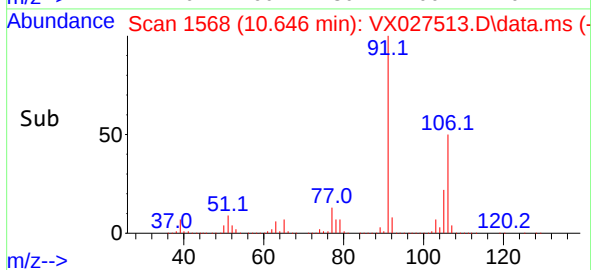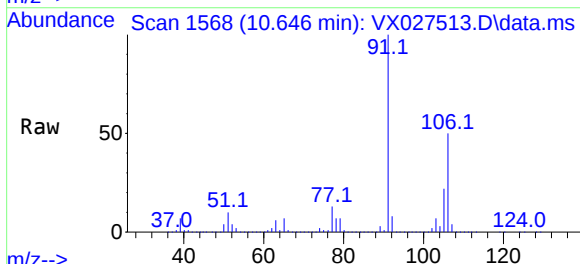



#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124




Tgt Ion:152 Resp: 25895  
Ion Ratio Lower Upper  
152 100  
115 59.4 37.5 112.7  
150 155.1 0.0 338.2

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

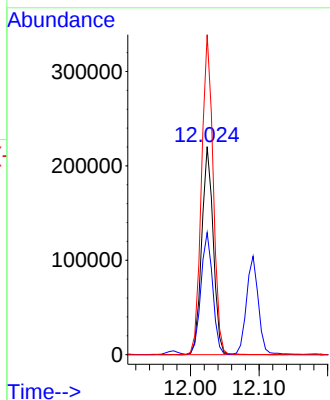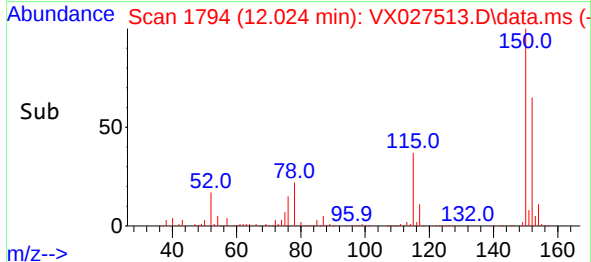


#73  
Isopropylbenzene  
Concen: 13.350 ug/l  
RT: 10.963 min Scan# 1620  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40



Tgt Ion:105 Resp: 251798  
Ion Ratio Lower Upper  
105 100  
120 26.7 13.5 40.5

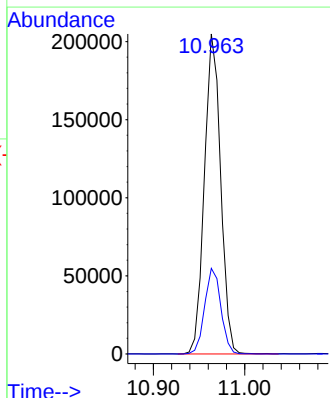







#78  
n-propylbenzene  
Concen: 52.166 ug/l  
RT: 11.305 min Scan# 117  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

Tgt Ion: 91 Resp: 108011  
Ion Ratio Lower Upper  
91 100  
120 24.4 11.6 34.8




Manual Integrations  
APPROVED


Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

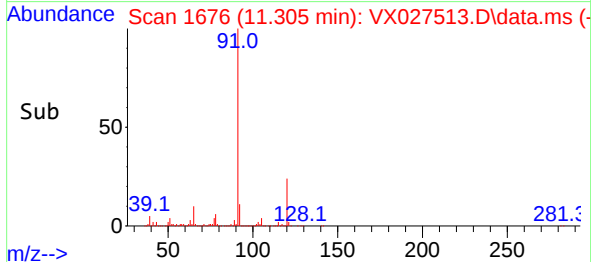

#80  
1,3,5-Trimethylbenzene  
Concen: 214.394 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. 0.006 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40


Tgt Ion:105 Resp: 3403497  
Ion Ratio Lower Upper  
105 100  
120 49.8 24.3 72.9

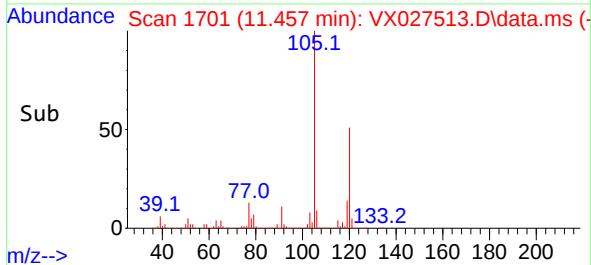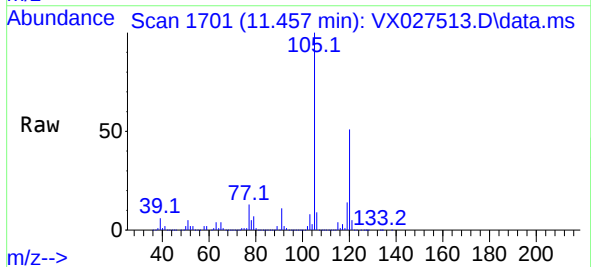



#83  
tert-Butylbenzene  
Concen: 11.487 ug/l  
RT: 11.719 min Scan# 1744  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40




Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124

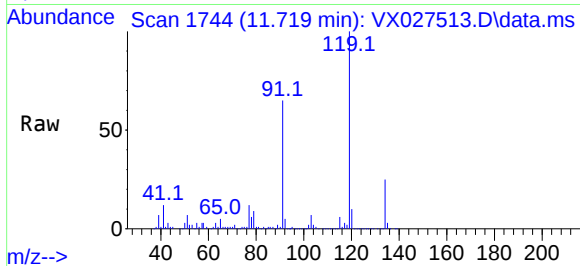


Tgt Ion:119 Resp: 180648  
Ion Ratio Lower Upper  
119 100  
91 66.8 26.9 80.6  
134 23.9 11.4 34.2

Manual Integrations  
APPROVED



Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

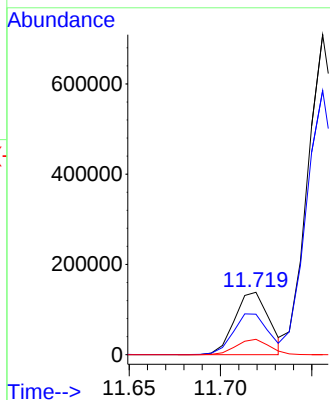


#84  
1,2,4-Trimethylbenzene  
Concen: 389.089 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

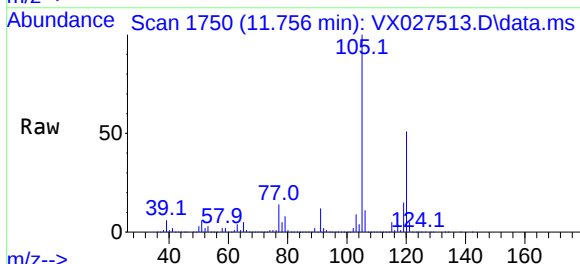

Tgt Ion:105 Resp: 6160021  
Ion Ratio Lower Upper  
105 100  
120 49.1 22.6 67.8

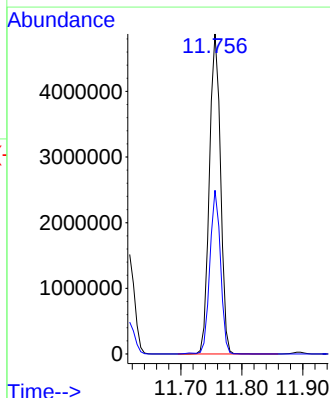







#85  
 sec-Butylbenzene  
 Concen: 1.896 ug/l m  
 RT: 11.890 min Scan# 1772  
 Delta R.T. 0.000 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-124

Tgt Ion:105 Resp: 3602  
 Ion Ratio Lower Upper  
 105 100  
 134 0.0 10.2 30.4




Manual Integrations  
 APPROVED


Reviewed By :John Carlone 03/18/2022  
 Supervised By :Mahesh Dadoda 03/18/2022

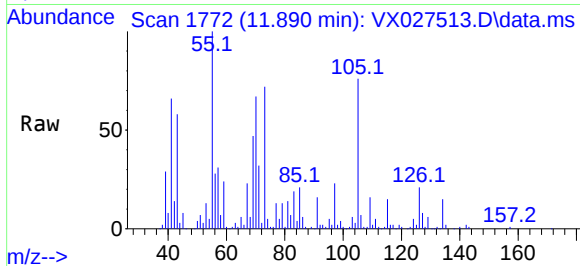

#86  
 p-Isopropyltoluene  
 Concen: 1.123 ug/l m  
 RT: 12.012 min Scan# 1792  
 Delta R.T. 0.000 min  
 Lab File: VX027513.D  
 Acq: 18 Mar 2022 01:40


Tgt Ion:119 Resp: 18329  
 Ion Ratio Lower Upper  
 119 100  
 134 93.7 13.0 39.0#  
 91 0.0 11.3 33.9#

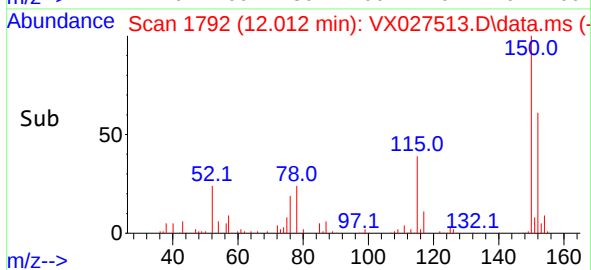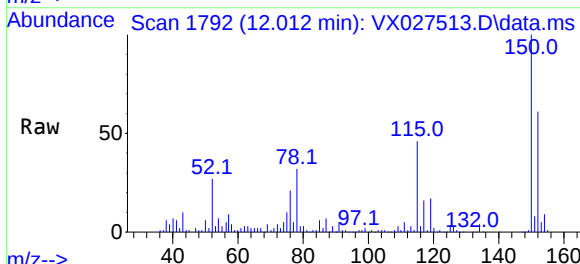



#95  
Naphthalene  
Concen: 126.264 ug/l  
RT: 13.780 min Scan# 2082  
Delta R.T. 0.000 min  
Lab File: VX027513.D  
Acq: 18 Mar 2022 01:40

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-124



Tgt Ion:128 Resp: 2265980  
Ion Ratio Lower Upper  
128 100  
127 12.9 10.2 15.4  
129 11.2 8.7 13.1

Manual Integrations  
APPROVED

Reviewed By :John Carlone 03/18/2022  
Supervised By :Mahesh Dadoda 03/18/2022

