

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
 Data File : VX027501.D
 Acq On : 17 Mar 2022 20:57
 Operator : JC/MD
 Sample : N1997-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-106S

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	22	31	42	rBV2	40323	163182	10.66%	1.872%
2	1.746	105	108	118	rVB3	17357	31984	2.09%	0.367%
3	2.538	230	238	248	rBV2	9544	24288	1.59%	0.279%
4	2.867	286	292	302	rVB	7989	15394	1.01%	0.177%
5	5.391	694	706	723	rBV2	195406	572469	37.40%	6.567%
6	5.556	723	733	751	rVB	317928	901775	58.91%	10.344%
7	5.964	787	800	814	rBV	196910	528300	34.51%	6.060%
8	6.251	836	847	860	rBV3	28400	87492	5.72%	1.004%
9	6.763	919	931	945	rBV	478532	1151764	75.24%	13.211%
10	7.988	1125	1132	1140	rVB2	25617	50939	3.33%	0.584%
11	8.110	1144	1152	1161	rVV	43444	87954	5.75%	1.009%
12	8.653	1226	1241	1256	rBV	977753	1530825	100.00%	17.559%
13	9.464	1368	1374	1379	rBV	11341	17443	1.14%	0.200%
14	10.055	1465	1471	1486	rBV	987251	1318254	86.11%	15.121%
15	11.018	1623	1629	1634	rBV	11741	16704	1.09%	0.192%
16	11.085	1634	1640	1653	rVV	783761	1009035	65.91%	11.574%
17	12.024	1789	1794	1808	rVB	1009107	1210181	79.05%	13.881%




Sum of corrected areas: 8717983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
Data File : VX027501.D
Acq On : 17 Mar 2022 20:57
Operator : JC/MD
Sample : N1997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-106S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

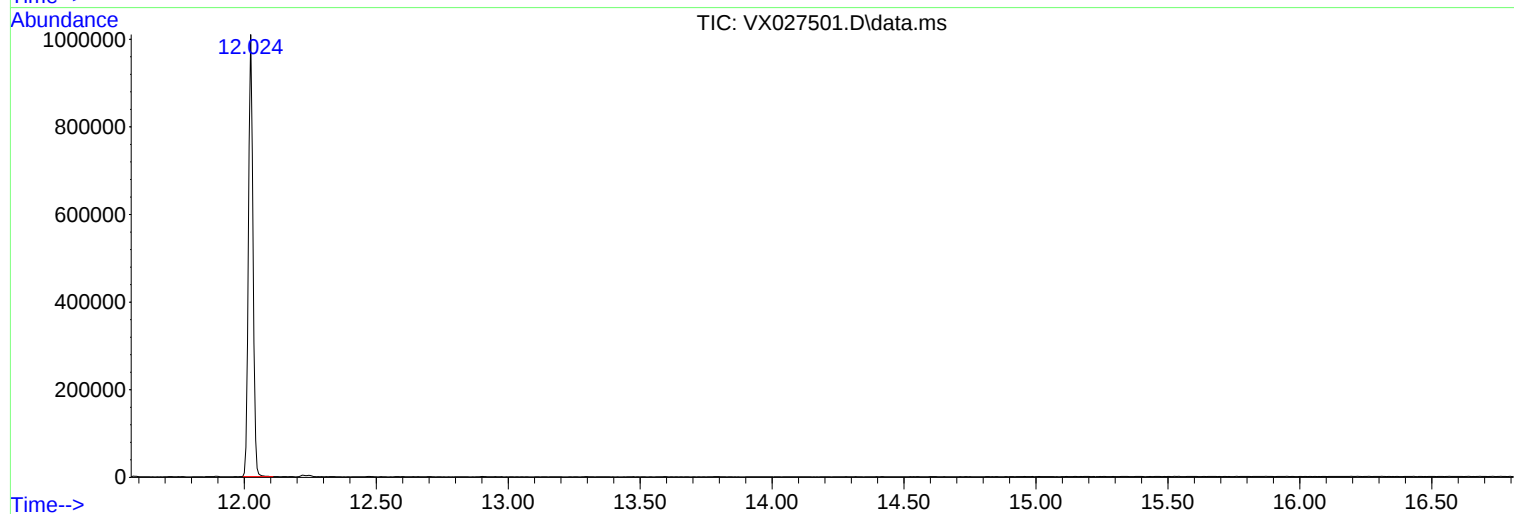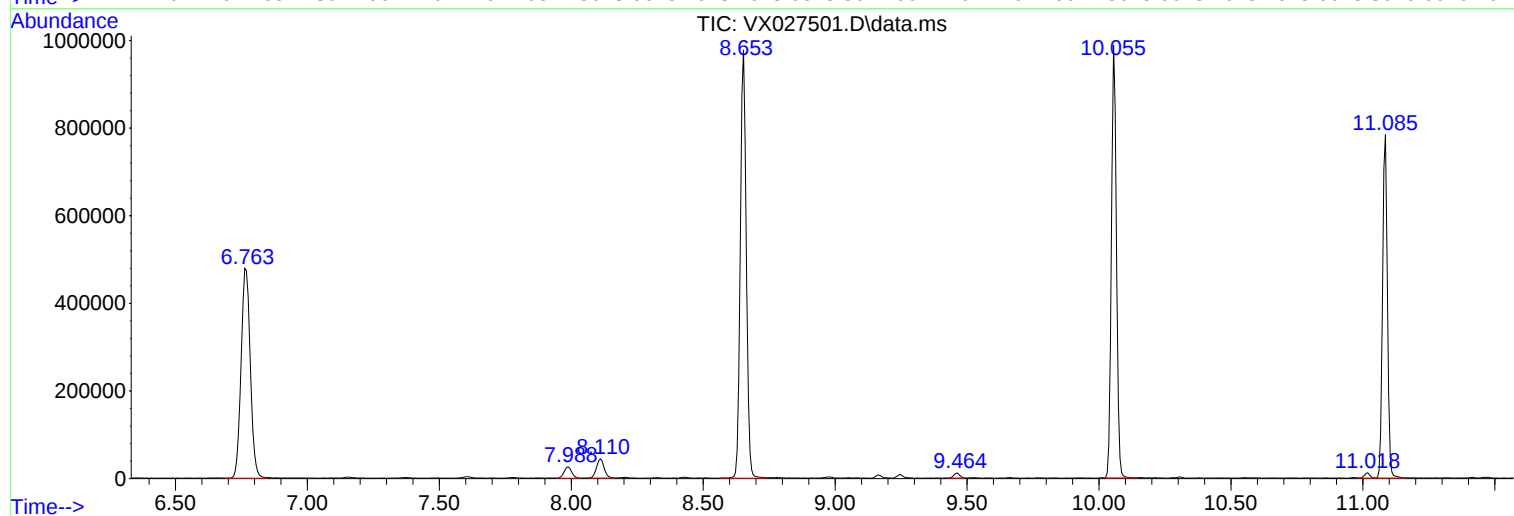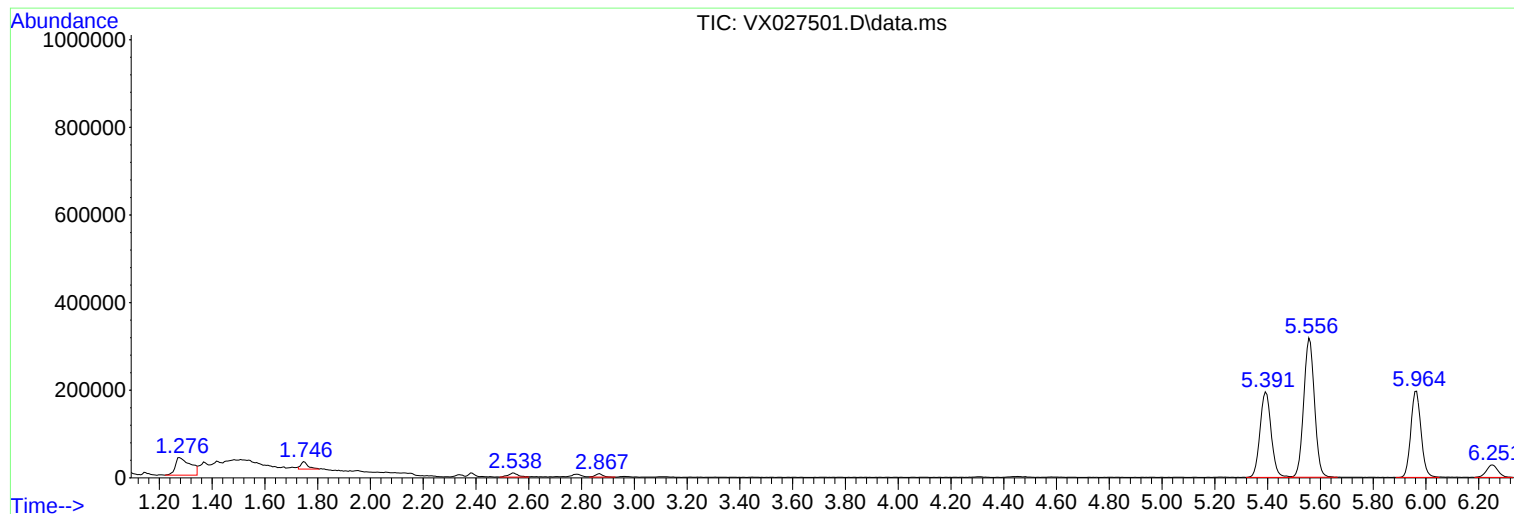

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
Data File : VX027501.D
Acq On : 17 Mar 2022 20:57
Operator : JC/MD
Sample : N1997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-106S









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Aminomethanesulfonic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.276	9.05 ug/l	163182	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	83
2			Sulfur dioxide	64	O2S	007446-09-5	83
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

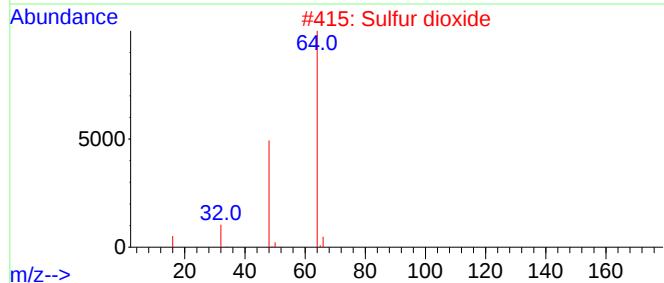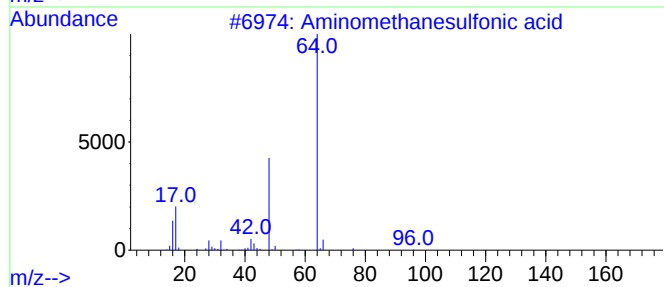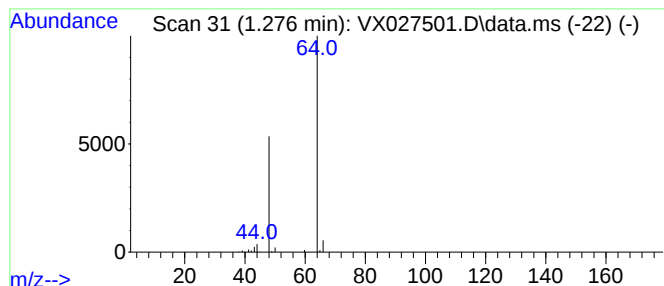

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
Data File : VX027501.D
Acq On : 17 Mar 2022 20:57
Operator : JC/MD
Sample : N1997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-106S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Aminomethanesul...	1.276	9.1	ug/l	163182	1	5.556	901775	50.0