


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031722\
 Data File : VX027490.D
 Acq On : 17 Mar 2022 16:14
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260
 Last Update : Thu Mar 17 15:02:59 2022

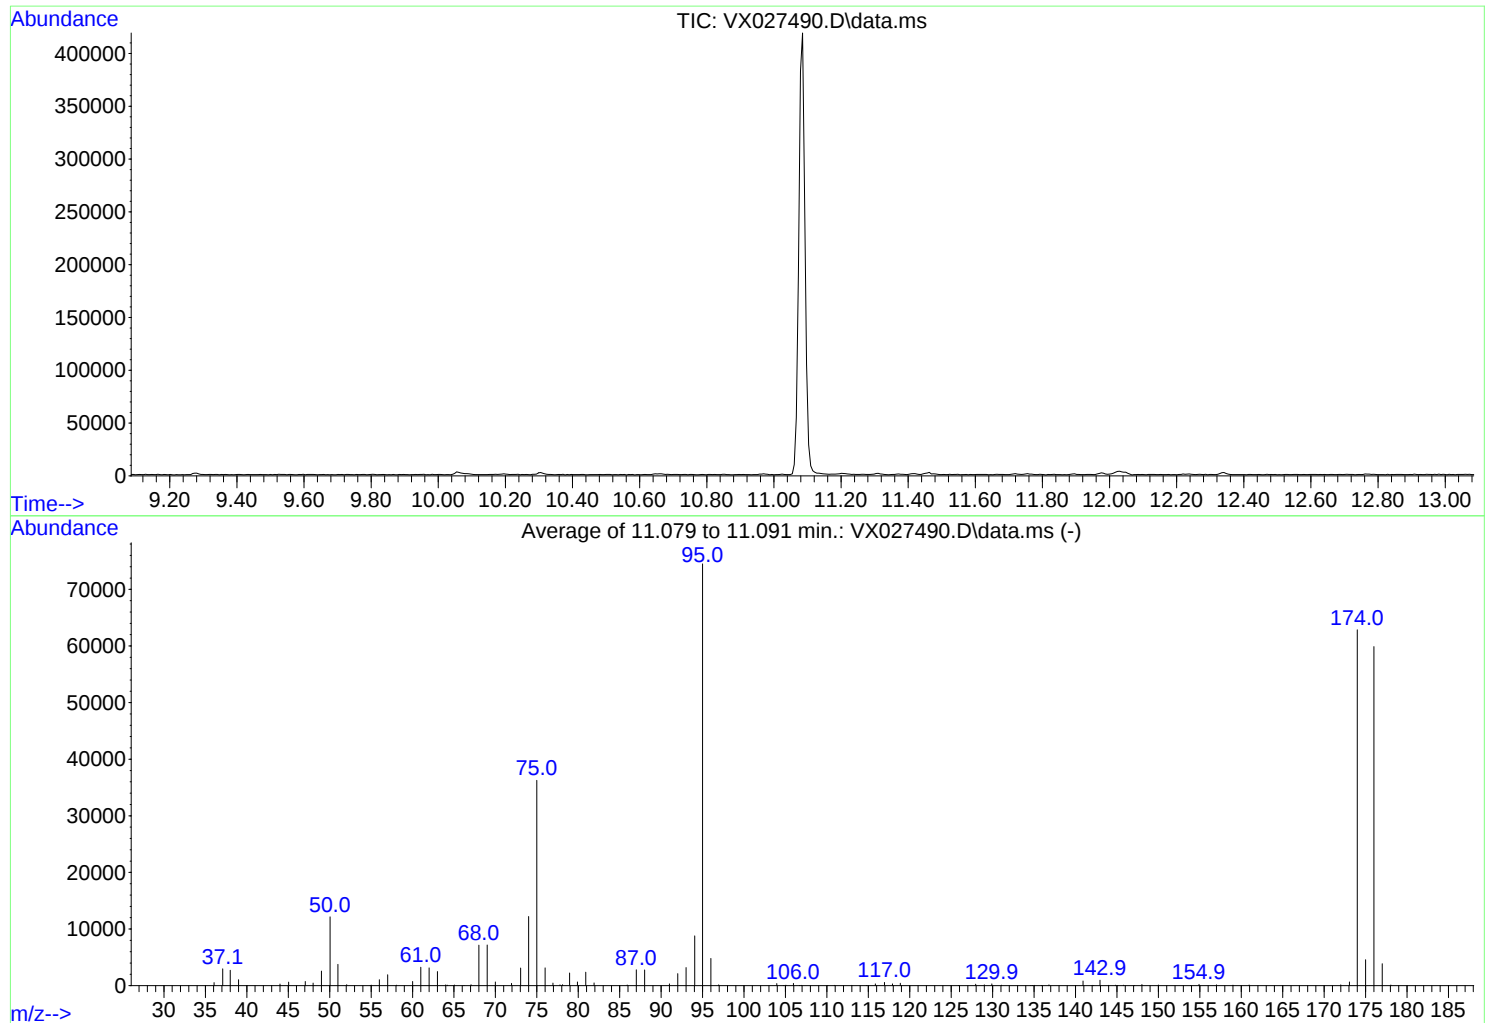

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	12166	PASS
75	95	30	60	48.7	36272	PASS
95	95	100	100	100.0	74512	PASS
96	95	5	9	6.4	4798	PASS
173	174	0.00	2	1.1	667	PASS
174	95	50	100	84.4	62864	PASS
175	174	5	9	7.3	4595	PASS
176	174	95	101	95.3	59885	PASS
177	176	5	9	6.5	3880	PASS