

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031723\
 Data File : VX034578.D
 Acq On : 17 Mar 2023 12:48
 Operator : JC/MD
 Sample : PB151466TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB151466TB

Quant Time: Mar 19 23:58:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	247521	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	420997	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	377961	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	159191	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	171042	47.499	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	95.000%		
35) Dibromofluoromethane	5.385	113	132348	47.614	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.220%		
50) Toluene-d8	8.647	98	512293	49.370	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.740%		
62) 4-Bromofluorobenzene	11.079	95	199589	47.620	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	95.240%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.295	50	440	Below Cal		96
11) Tert butyl alcohol	2.959	59	2594	3.459	ug/l	98
13) Acrolein	2.240	56	337	0.568	ug/l #	13
15) Acrylonitrile	3.081	53	408	0.252	ug/l #	80
16) Acetone	2.374	43	92260	54.392	ug/l	99
17) Carbon Disulfide	2.514	76	2412	0.316	ug/l #	93
18) Methyl Acetate	2.703	43	3732	0.673	ug/l	99
20) Methylene Chloride	2.788	84	13684	4.157	ug/l	97
25) 2-Butanone	4.562	43	9868	4.066	ug/l #	90
29) Tetrahydrofuran	5.032	42	1331	0.889	ug/l #	78
36) 1,1-Dichloropropene	5.544	75	20442	4.788	ug/l #	51
37) Ethyl Acetate	4.709	43	66818	14.326	ug/l	97
38) Carbon Tetrachloride	5.544	117	24765	5.831	ug/l #	16
43) Isopropyl Acetate	6.336	43	283835	35.922	ug/l	100
48) Methyl methacrylate	7.793	41	237927	62.610	ug/l #	47
49) 1,4-Dioxane	7.647	88	52	0.651	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	226270	49.365	ug/l #	50
53) t-1,3-Dichloropropene	8.952	75	2270	0.470	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	95129	18.190	ug/l #	61
57) 1,3-Dichloropropane	9.482	76	12398	2.273	ug/l #	43
58) 2-Chloroethyl Vinyl ether	8.257	63	1783	0.687	ug/l	95
59) 2-Hexanone	9.482	43	177851	50.195	ug/l #	52
74) N-amyl acetate	10.640	43	74430	12.630	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	108485	29.680	ug/l #	34
81) trans-1,4-Dichloro-2-b...	11.079	75	108485	80.292	ug/l #	8
93) 1,2,4-Trichlorobenzene	13.591	180	835	0.239	ug/l	90
94) Hexachlorobutadiene	13.725	225	630	0.447	ug/l	81
95) Naphthalene	13.780	128	2363	0.202	ug/l #	86
96) 1,2,3-Trichlorobenzene	13.969	180	866	0.253	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031723\
Data File : VX034578.D
Acq On : 17 Mar 2023 12:48
Operator : JC/MD
Sample : PB151466TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB151466TB

Quant Time: Mar 19 23:58:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




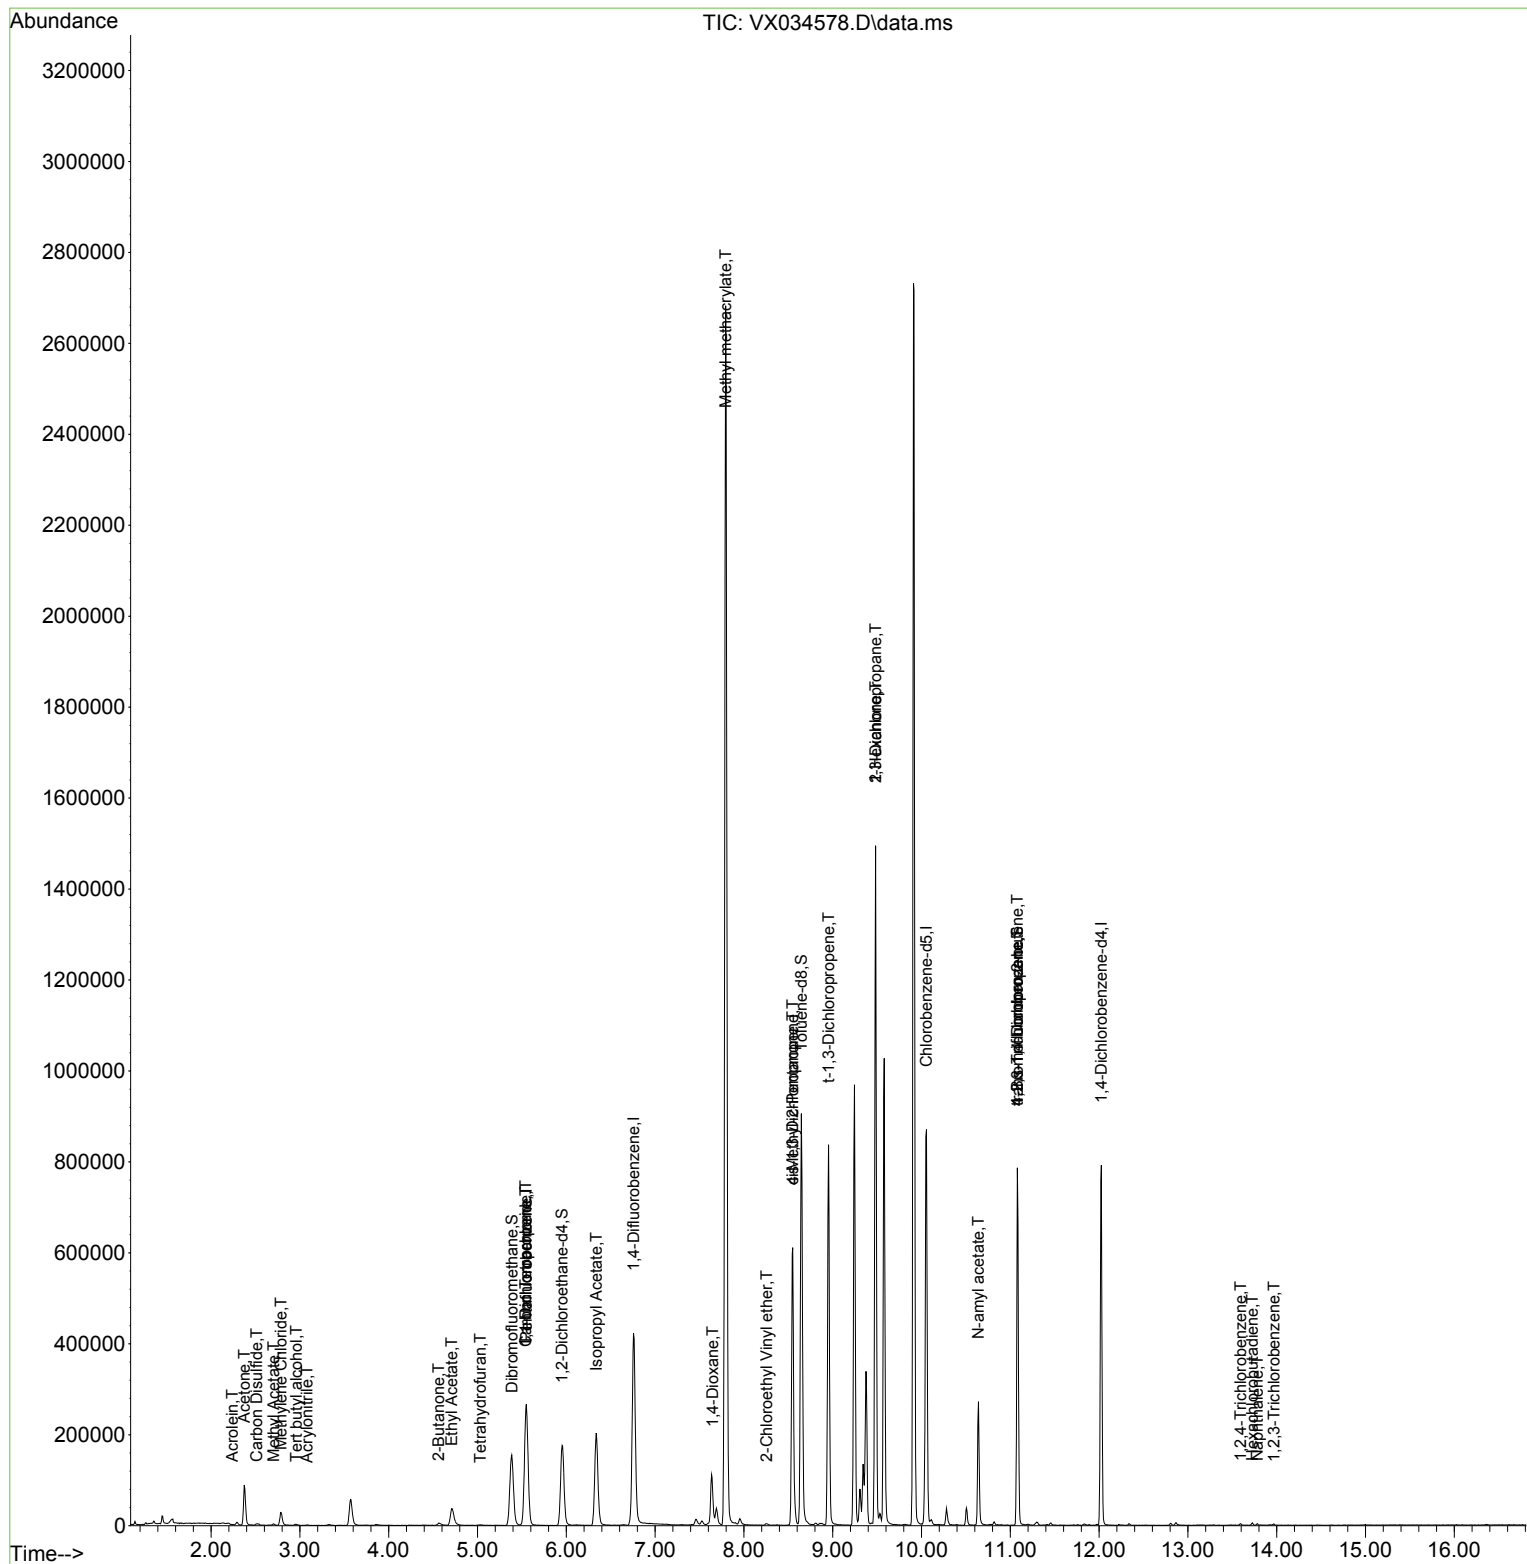




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion:168 Resp: 247521
Ion Ratio Lower Upper
168 100
99 59.1 45.7 68.5

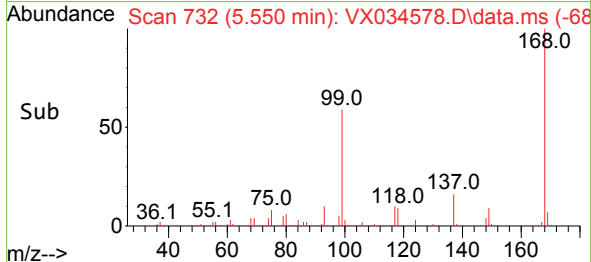

#3
Chloromethane
Concen: Below Cal
RT: 1.295 min Scan# 34
Delta R.T. -0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion: 50 Resp: 440
Ion Ratio Lower Upper
50 100
52 29.9 25.9 38.9

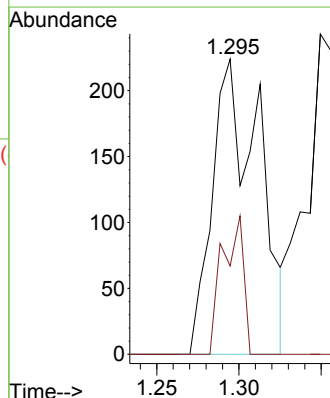

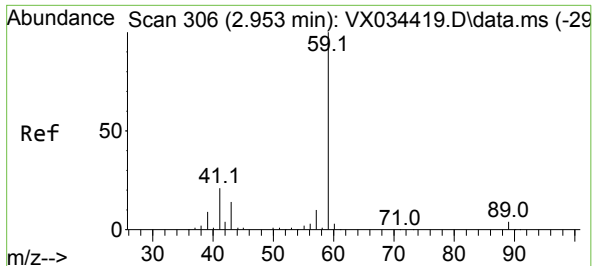

#11

Tert butyl alcohol

Concen: 3.459 ug/l

RT: 2.959 min Scan# 306

Delta R.T. 0.006 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :





PB151466TB

Tgt Ion: 59 Resp: 2594

Ion Ratio Lower Upper

59 100

57 10.9 8.1 12.1

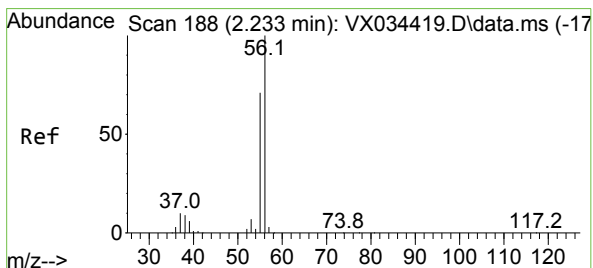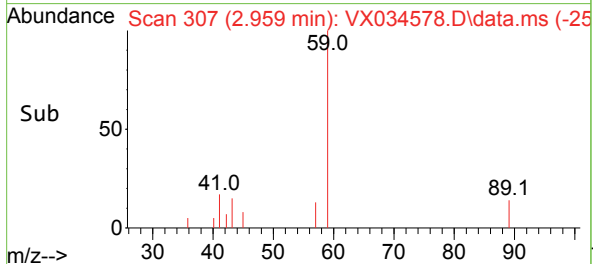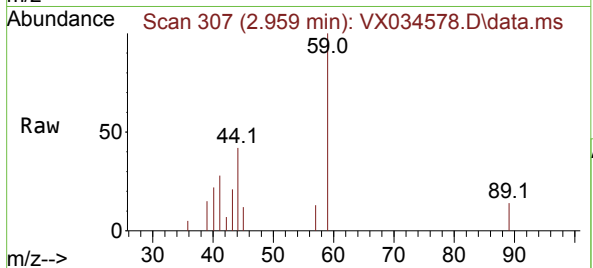

#13

Acrolein

Concen: 0.568 ug/l

RT: 2.240 min Scan# 189

Delta R.T. 0.007 min

Lab File: VX034578.D




Acq: 17 Mar 2023 12:48


Tgt Ion: 56 Resp: 337

Ion Ratio Lower Upper

56 100

55 142.4 56.6 85.0#


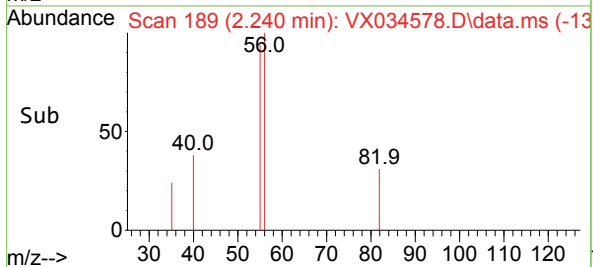

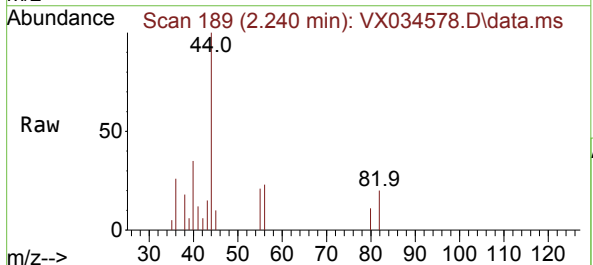




#15
Acrylonitrile
Concen: 0.252 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.025 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion: 53 Resp: 408
Ion Ratio Lower Upper
53 100
52 84.8 66.2 99.2
51 0.0 28.3 42.5#

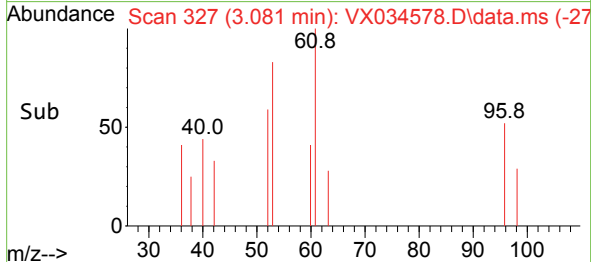

#16
Acetone
Concen: 54.392 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion: 43 Resp: 92260
Ion Ratio Lower Upper
43 100
58 30.1 24.7 37.1

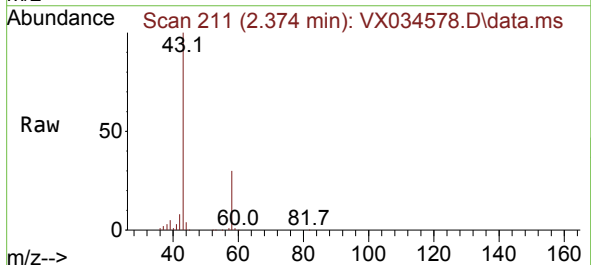



#17

Carbon Disulfide

Concen: 0.316 ug/l

RT: 2.514 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :





PB151466TB

Tgt Ion: 76 Resp: 2412

Ion Ratio Lower Upper

76 100

78 11.6 7.2 10.8#

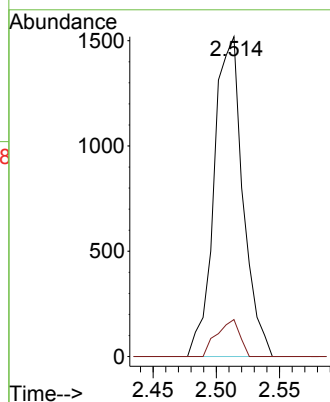

#18

Methyl Acetate

Concen: 0.673 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.006 min

Lab File: VX034578.D




Acq: 17 Mar 2023 12:48


Tgt Ion: 43 Resp: 3732

Ion Ratio Lower Upper

43 100

74 22.4 18.3 27.5









#20
Methylene Chloride
Concen: 4.157 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion:	84	Resp:	13684
Ion	Ratio	Lower	Upper
84	100		
49	127.0	103.8	155.8
51	35.4	31.8	47.8
86	64.8	51.4	77.2



#25
2-Butanone
Concen: 4.066 ug/l
RT: 4.562 min Scan# 570
Delta R.T. 0.018 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion:	43	Resp:	9868
Ion	Ratio	Lower	Upper
43	100		
72	29.0	19.3	28.9#





#29

Tetrahydrofuran

Concen: 0.889 ug/l

RT: 5.032 min Scan# 641

Delta R.T. 0.037 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :

PB151466TB





Tgt Ion: 42 Resp: 1331

Ion Ratio Lower Upper

42 100

72 29.2 34.5 51.7#

71 25.9 32.1 48.1#

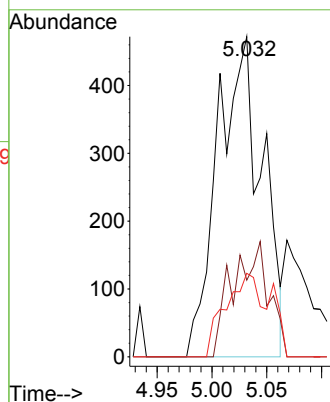

#33

1,2-Dichloroethane-d4

Concen: 47.499 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX034578.D




Acq: 17 Mar 2023 12:48


Tgt Ion: 65 Resp: 171042

Ion Ratio Lower Upper

65 100

67 52.3 0.0 104.0



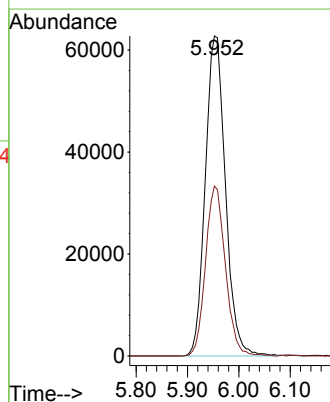





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion:114 Resp: 420997
Ion Ratio Lower Upper
114 100
63 21.6 0.0 42.2
88 17.1 0.0 33.2

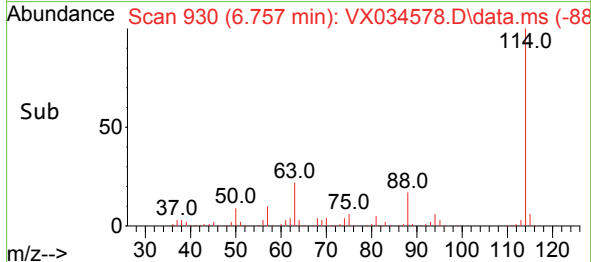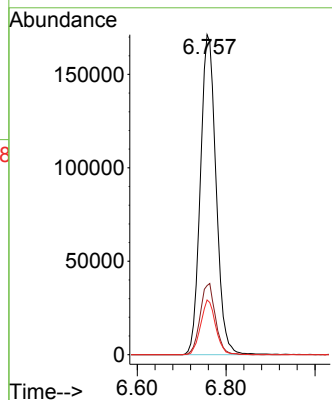

#35
Dibromofluoromethane
Concen: 47.614 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion:113 Resp: 132348
Ion Ratio Lower Upper
113 100
111 103.0 83.7 125.5
192 18.8 15.4 23.2



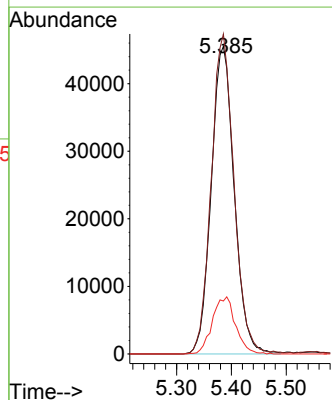
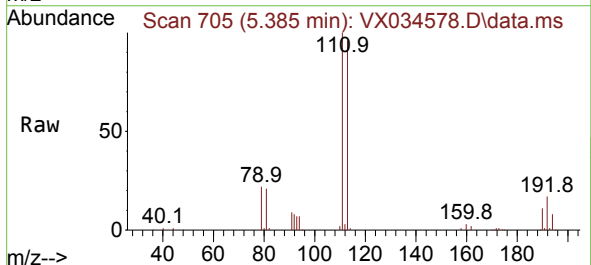




#36
1,1-Dichloropropene
Concen: 4.788 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion: 75 Resp: 20442
Ion Ratio Lower Upper
75 100
110 10.4 17.5 52.5#
77 0.0 24.3 36.5#

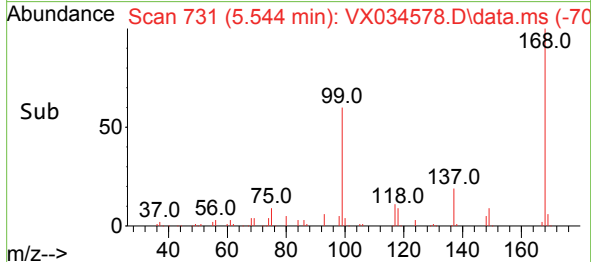

#37
Ethyl Acetate
Concen: 14.326 ug/l
RT: 4.709 min Scan# 594
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48


Tgt Ion: 43 Resp: 66818
Ion Ratio Lower Upper
43 100
61 13.9 10.2 15.4
70 11.4 8.2 12.4

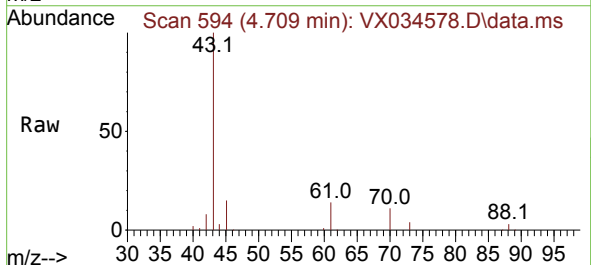






#38
Carbon Tetrachloride
Concen: 5.831 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Instrument :
MSVOA_X
ClientSampleId :
PB151466TB







Tgt Ion:117 Resp: 24765
Ion Ratio Lower Upper
117 100
119 4.6 76.6 114.8#
121 0.0 23.8 35.6#



#43
Isopropyl Acetate
Concen: 35.922 ug/l
RT: 6.336 min Scan# 861
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion: 43 Resp: 283835
Ion Ratio Lower Upper
43 100
61 18.8 15.2 22.8
87 12.2 9.8 14.8


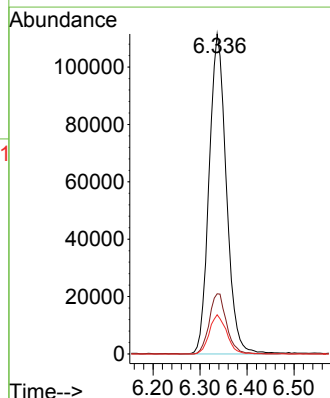






#48
Methyl methacrylate
Concen: 62.610 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.104 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion: 41 Resp: 237927
Ion Ratio Lower Upper
41 100
69 0.2 62.2 93.4#
39 56.0 47.7 71.5

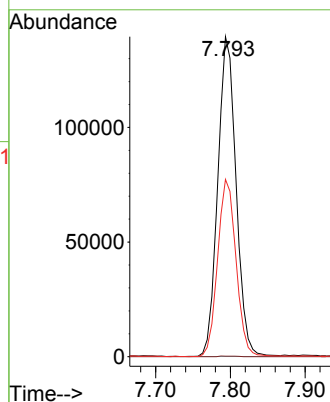

#49
1,4-Dioxane
Concen: 0.651 ug/l
RT: 7.647 min Scan# 1076
Delta R.T. -0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion: 88 Resp: 52
Ion Ratio Lower Upper
88 100
43 0.0 27.7 41.5#
58 10853.8 56.8 85.2#



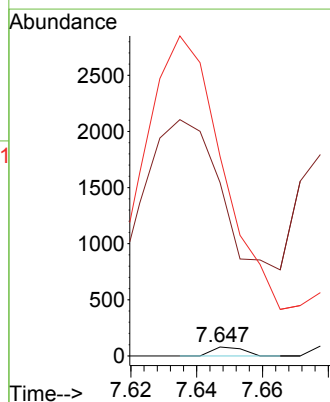





#50
Toluene-d8
Concen: 49.370 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion: 98 Resp: 512293
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

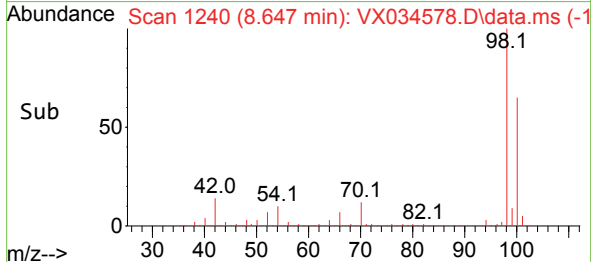

#51
4-Methyl-2-Pentanone
Concen: 49.365 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.018 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion: 43 Resp: 226270
Ion Ratio Lower Upper
43 100
58 8.3 30.6 46.0#




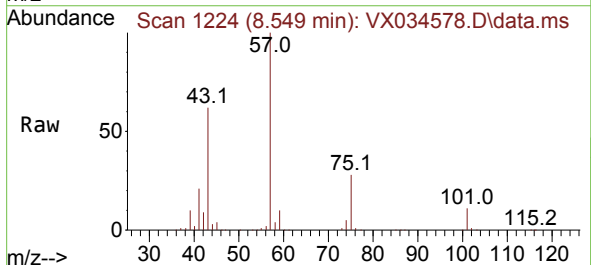




#53
 t-1,3-Dichloropropene
 Concen: 0.470 ug/l
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX034578.D
 Acq: 17 Mar 2023 12:48




Instrument :
 MSVOA_X
 ClientSampleId :
 PB151466TB


Tgt Ion: 75 Resp: 2270
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.4 38.2#

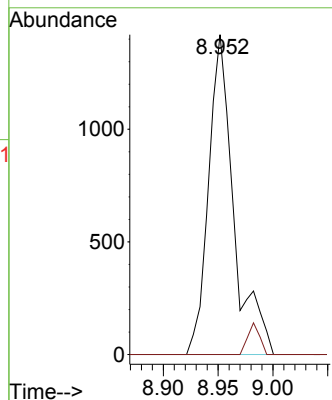

#54
 cis-1,3-Dichloropropene
 Concen: 18.190 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.189 min
 Lab File: VX034578.D
 Acq: 17 Mar 2023 12:48

Tgt Ion: 75 Resp: 95129
 Ion Ratio Lower Upper
 75 100
 77 0.3 25.0 37.4#
 39 34.1 44.6 66.8#

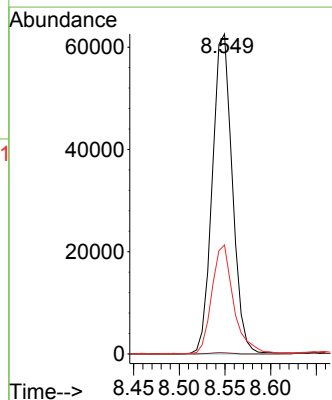



#57

1,3-Dichloropropane

Concen: 2.273 ug/l

RT: 9.482 min Scan# 1176

Delta R.T. 0.177 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :





PB151466TB

Tgt Ion: 76 Resp: 12398

Ion Ratio Lower Upper

76 100

78 0.2 25.8 38.8#

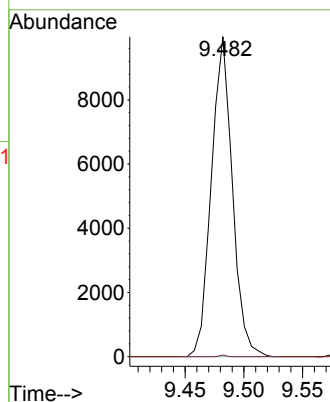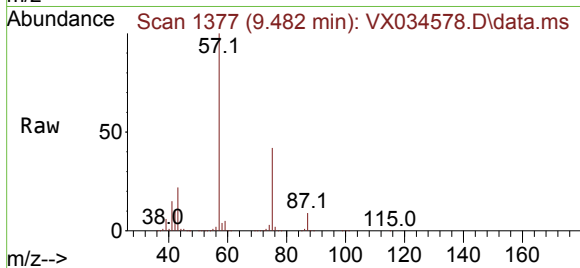

#58

2-Chloroethyl Vinyl ether

Concen: 0.687 ug/l

RT: 8.257 min Scan# 1176

Delta R.T. 0.018 min

Lab File: VX034578.D




Acq: 17 Mar 2023 12:48


Tgt Ion: 63 Resp: 1783

Ion Ratio Lower Upper

63 100

106 30.5 22.2 33.2

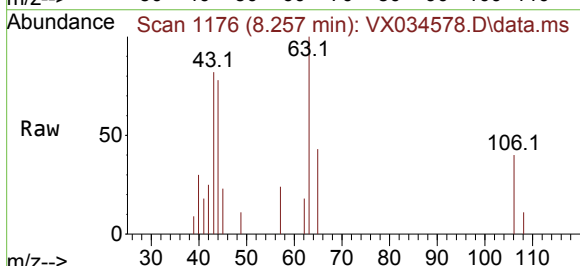



#59

2-Hexanone

Concen: 50.195 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.055 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :





PB151466TB

Tgt Ion: 43 Resp: 177851

Ion Ratio Lower Upper

43 100

58 18.6 26.3 78.9#

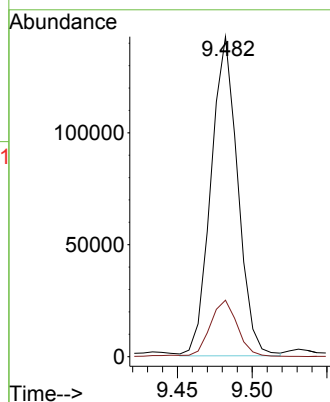

#62

4-Bromofluorobenzene

Concen: 47.620 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX034578.D

Acq: 17 Mar 2023 12:48




Tgt Ion: 95 Resp: 199589


Ion Ratio Lower Upper

95 100

174 75.0 0.0 147.4

176 72.6 0.0 140.6









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion:117 Resp: 377961
Ion Ratio Lower Upper
117 100
82 57.9 45.0 67.4
119 32.8 26.0 39.0

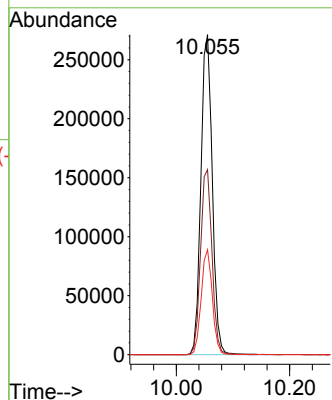

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Tgt Ion:152 Resp: 159191
Ion Ratio Lower Upper
152 100
115 61.2 45.0 135.0
150 155.4 0.0 352.4

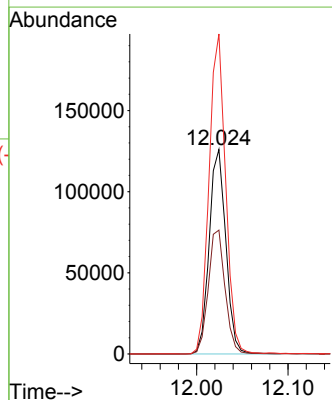



#74

N-amy1 acetate

Concen: 12.630 ug/l

RT: 10.640 min Scan# 1

Delta R.T. -0.201 min

Lab File: VX034578.D


Acq: 17 Mar 2023 12:48

Instrument :

MSVOA_X

ClientSampleId :

PB151466TB

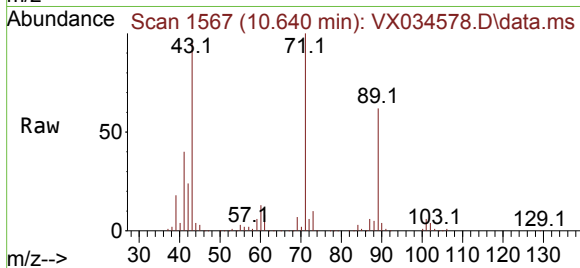

Tgt Ion: 43 Resp: 74430




Ion Ratio Lower Upper

43 100

70 1.4 32.1 48.1#

55 4.2 18.3 27.5#

61 9.1 18.8 28.2#



#76

1,2,3-Trichloropropane

Concen: 29.680 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX034578.D




Acq: 17 Mar 2023 12:48


Tgt Ion: 75 Resp: 108485

Ion Ratio Lower Upper

75 100

77 1.1 21.6 64.8#



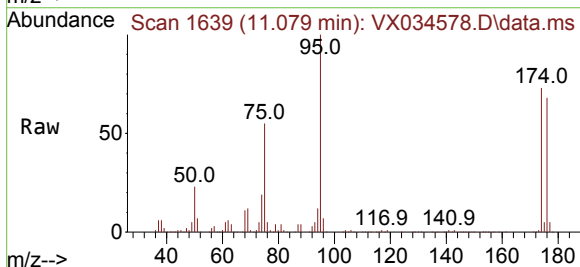





#81
trans-1,4-Dichloro-2-butene
Concen: 80.292 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48




Instrument :
MSVOA_X
ClientSampleId :
PB151466TB


Tgt Ion: 75 Resp: 108485
Ion Ratio Lower Upper
75 100
53 0.0 82.6 124.0#
89 0.0 36.9 55.3#

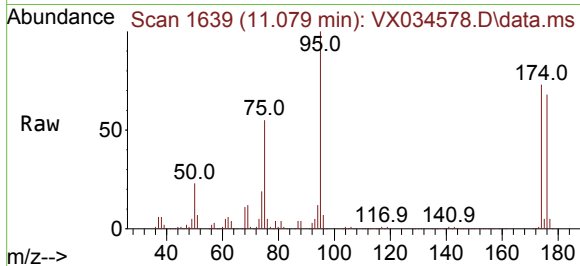

#93
1,2,4-Trichlorobenzene
Concen: 0.239 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48


Tgt Ion:180 Resp: 835
Ion Ratio Lower Upper
180 100
182 102.0 47.0 141.0
145 23.8 15.9 47.7

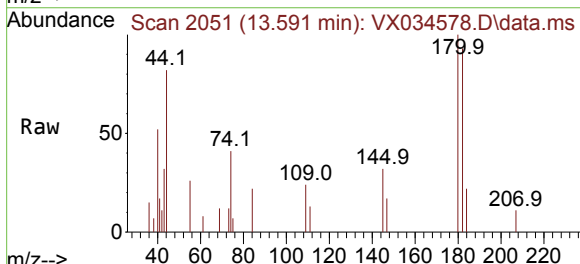






#94
Hexachlorobutadiene
Concen: 0.447 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48


Instrument :
MSVOA_X
ClientSampleId :
PB151466TB





Tgt Ion:225 Resp: 630
Ion Ratio Lower Upper
225 100
223 50.3 32.1 96.5
227 79.4 31.8 95.4

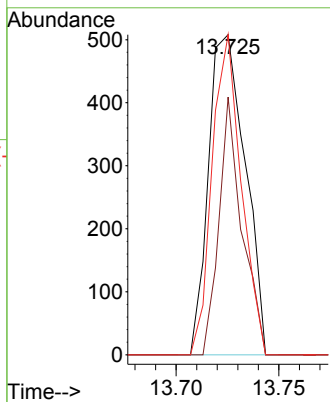


#95
Naphthalene
Concen: 0.202 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

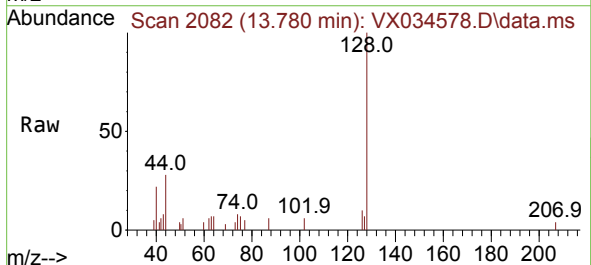


Tgt Ion:128 Resp: 2363
Ion Ratio Lower Upper
128 100
127 9.0 10.2 15.4#
129 3.3 8.6 13.0#





#96
1,2,3-Trichlorobenzene
Concen: 0.253 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX034578.D
Acq: 17 Mar 2023 12:48

Instrument :
MSVOA_X
ClientSampleId :
PB151466TB



Tgt Ion:	180	Resp:	866
Ion Ratio	Lower	Upper	
180	100		
182	91.8	48.0	144.2
145	31.8	17.7	53.1

