

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031723\
 Data File : VX034605.D
 Acq On : 18 Mar 2023 02:32
 Operator : JC/MD
 Sample : 01932-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CE-43-031423

Quant Time: Mar 20 00:13:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	221296	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	6.763	114	378010	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	342375	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	144263	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	156510	48.614	ug/l	0.01
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.220%
35) Dibromofluoromethane	5.391	113	121602	48.723	ug/l	0.01
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.440%
50) Toluene-d8	8.647	98	465437	49.956	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.920%
62) 4-Bromofluorobenzene	11.079	95	173706	46.157	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.320%
Target Compounds						
					Qvalue	
3) Chloromethane	1.313	50	431	Below Cal	#	42
11) Tert butyl alcohol	2.953	59	1760	2.625	ug/l #	92
13) Acrolein	2.233	56	257	0.485	ug/l #	19
15) Acrylonitrile	3.056	53	364	0.251	ug/l #	68
16) Acetone	2.379	43	81878	53.991	ug/l	97
17) Carbon Disulfide	2.514	76	1833	0.269	ug/l	96
18) Methyl Acetate	2.703	43	3205	0.647	ug/l	96
20) Methylene Chloride	2.788	84	20756	7.052	ug/l	98
25) 2-Butanone	4.574	43	8849	4.078	ug/l	91
29) Tetrahydrofuran	5.025	42	1086	0.811	ug/l #	83
36) 1,1-Dichloropropene	5.550	75	18765	4.895	ug/l #	51
37) Ethyl Acetate	4.714	43	60829	14.525	ug/l	98
38) Carbon Tetrachloride	5.556	117	23005	6.032	ug/l #	15
43) Isopropyl Acetate	6.342	43	255611	36.029	ug/l	99
48) Methyl methacrylate	7.799	41	216526	63.458	ug/l #	47
49) 1,4-Dioxane	7.641	88	112	1.563	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	200469	48.709	ug/l #	51
53) t-1,3-Dichloropropene	8.951	75	1727	0.398	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	84195	17.930	ug/l #	62
57) 1,3-Dichloropropane	9.482	76	10768	2.199	ug/l #	43
58) 2-Chloroethyl Vinyl ether	8.256	63	2257	0.968	ug/l	98
59) 2-Hexanone	9.482	43	149673	47.046	ug/l #	51
74) N-amyl acetate	10.640	43	57223	10.715	ug/l #	54
76) 1,2,3-Trichloropropane	11.079	75	94897	28.649	ug/l #	34
81) trans-1,4-Dichloro-2-b...	11.079	75	94897	77.503	ug/l #	8
93) 1,2,4-Trichlorobenzene	13.591	180	817	0.258	ug/l	94
94) Hexachlorobutadiene	13.725	225	556	0.436	ug/l	83
95) Naphthalene	13.780	128	2244	0.211	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	724	0.234	ug/l	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031723\
Data File : VX034605.D
Acq On : 18 Mar 2023 02:32
Operator : JC/MD
Sample : 01932-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423

Quant Time: Mar 20 00:13:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




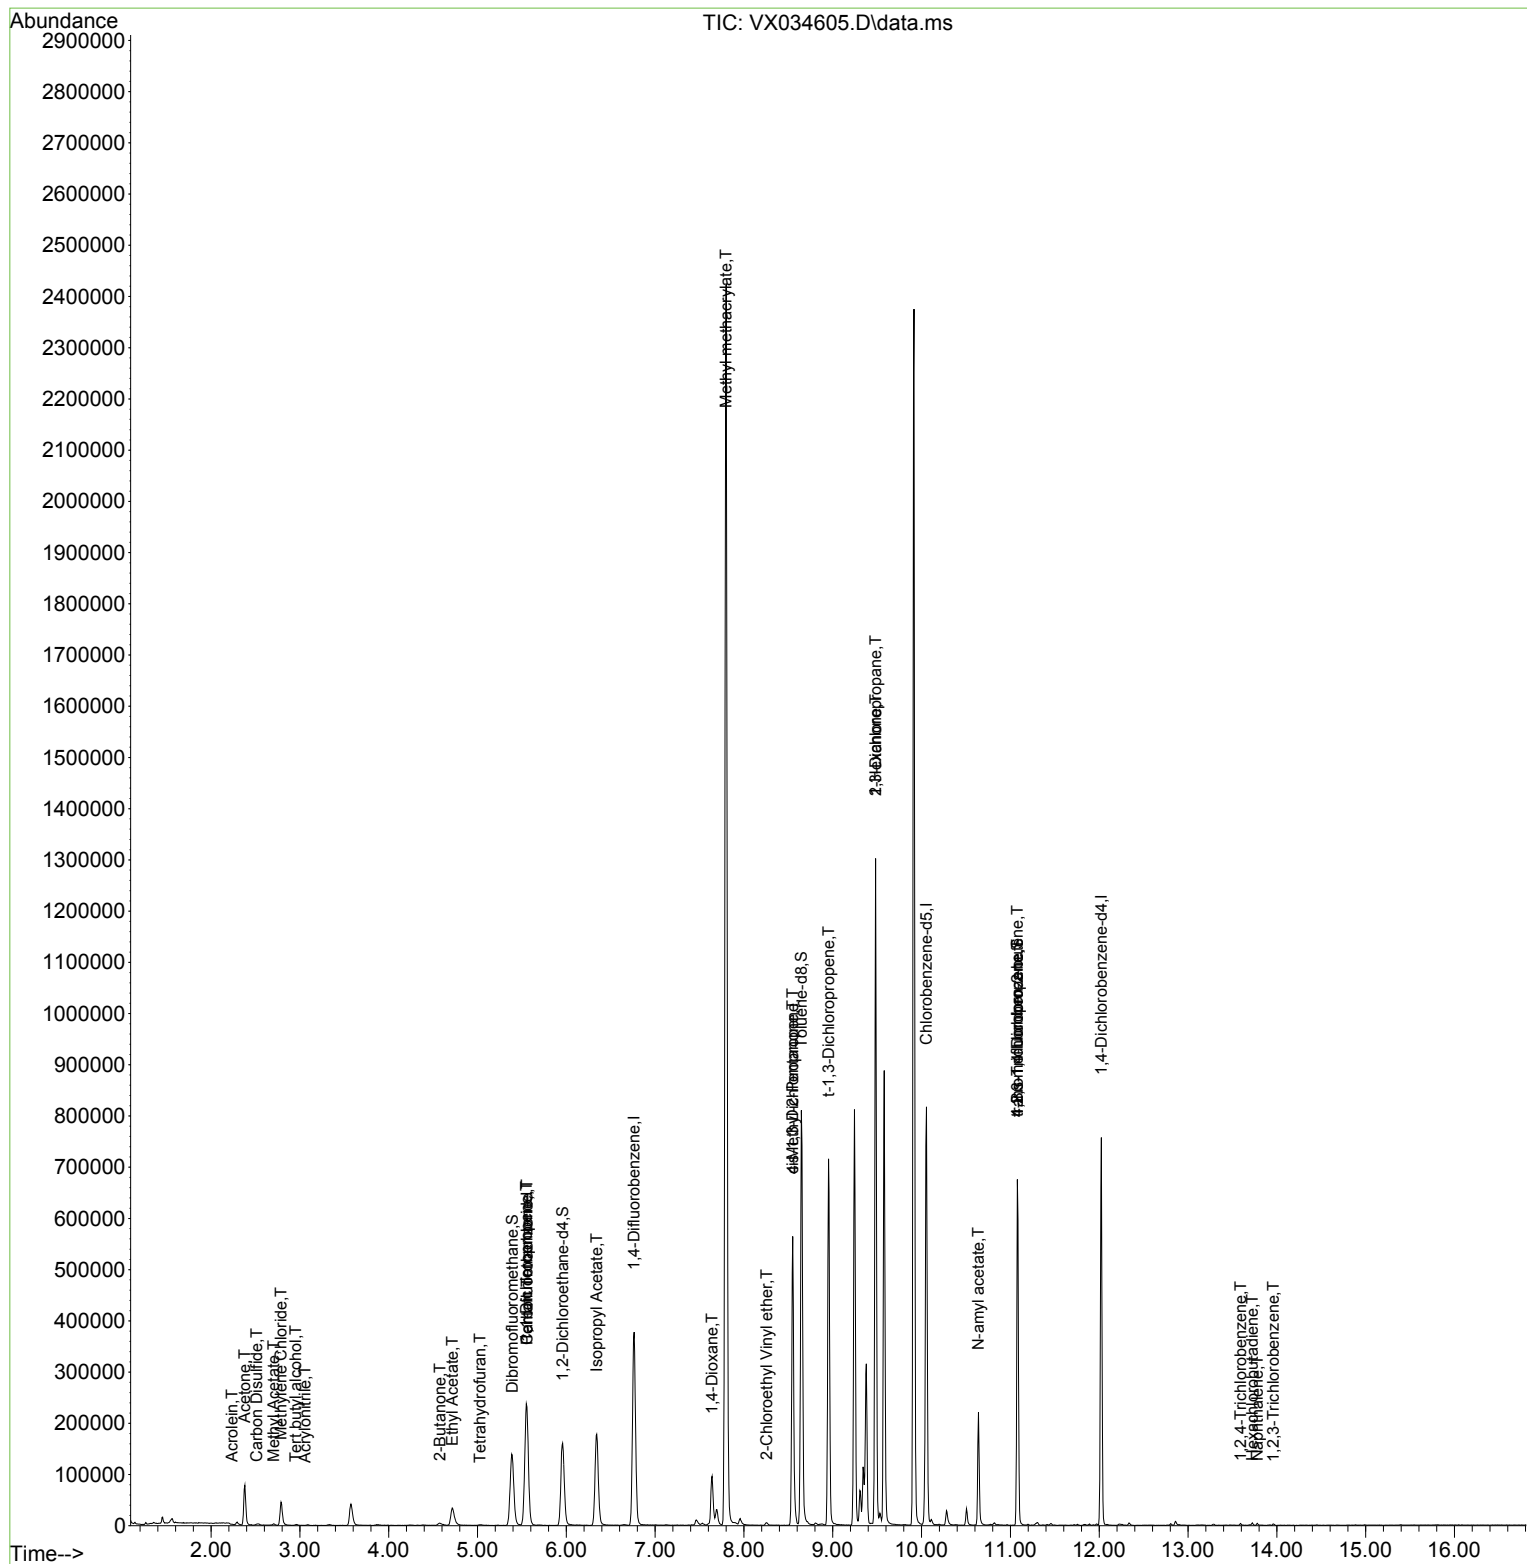




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion:168 Resp: 221296
Ion Ratio Lower Upper
168 100
99 58.3 45.7 68.5

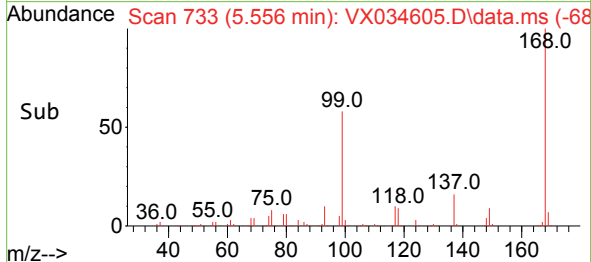

#3
Chloromethane
Concen: Below Cal
RT: 1.313 min Scan# 37
Delta R.T. 0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion: 50 Resp: 431
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#





#11

Tert butyl alcohol

Concen: 2.625 ug/l

RT: 2.953 min Scan# 306

Delta R.T. -0.000 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :





CE-43-031423

Tgt Ion: 59 Resp: 1760

Ion Ratio Lower Upper

59 100

57 13.2 8.1 12.1#

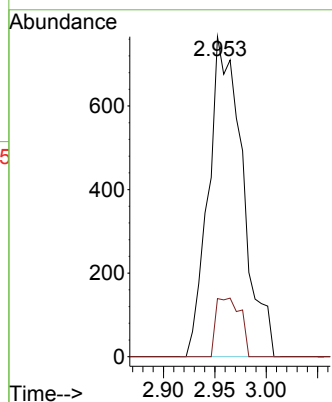

#13

Acrolein

Concen: 0.485 ug/l

RT: 2.233 min Scan# 188

Delta R.T. 0.000 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 56 Resp: 257

Ion Ratio Lower Upper

56 100

55 137.4 56.6 85.0#





#15

Acrylonitrile

Concen: 0.251 ug/l

RT: 3.056 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :

CE-43-031423





Tgt Ion: 53 Resp: 364

Ion Ratio Lower Upper

53 100

52 65.1 66.2 99.2#

51 0.0 28.3 42.5#

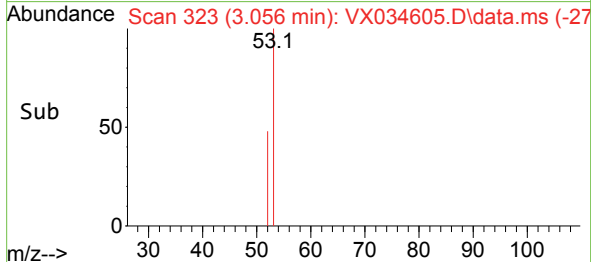

#16

Acetone

Concen: 53.991 ug/l

RT: 2.379 min Scan# 212

Delta R.T. 0.006 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 43 Resp: 81878

Ion Ratio Lower Upper

43 100

58 29.3 24.7 37.1


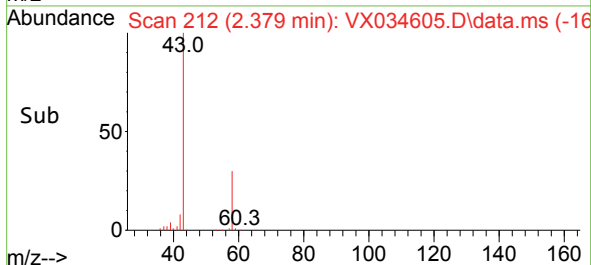
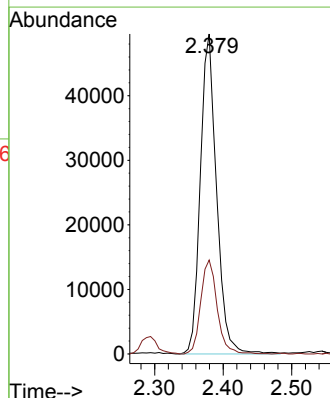
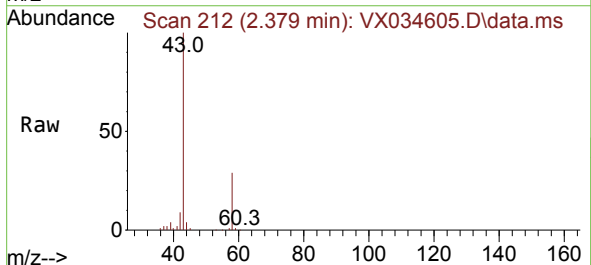


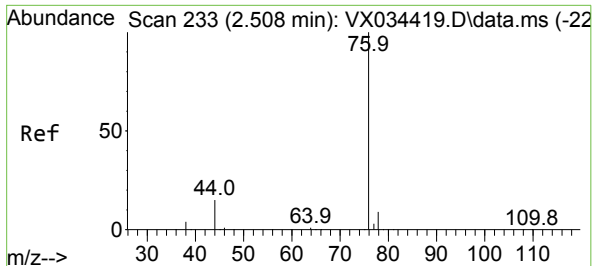

#17
Carbon Disulfide
Concen: 0.269 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion: 76 Resp: 1833
Ion Ratio Lower Upper
76 100
78 10.4 7.2 10.8

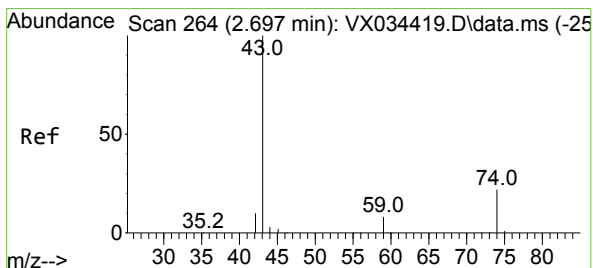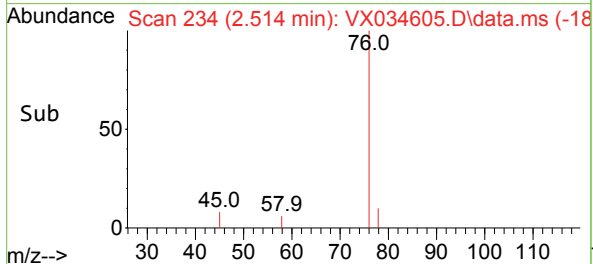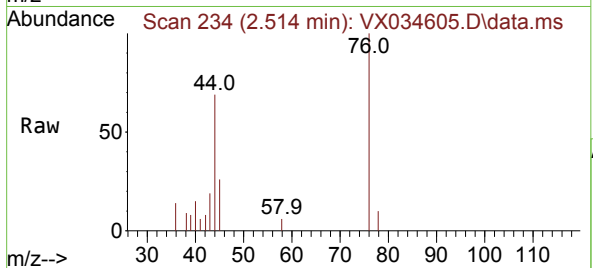

#18
Methyl Acetate
Concen: 0.647 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion: 43 Resp: 3205
Ion Ratio Lower Upper
43 100
74 24.6 18.3 27.5

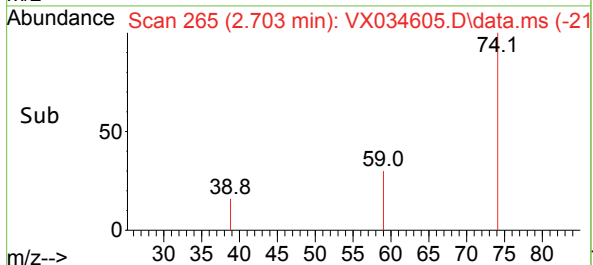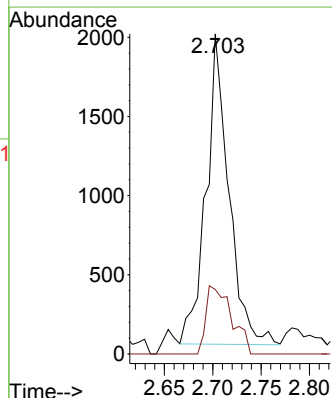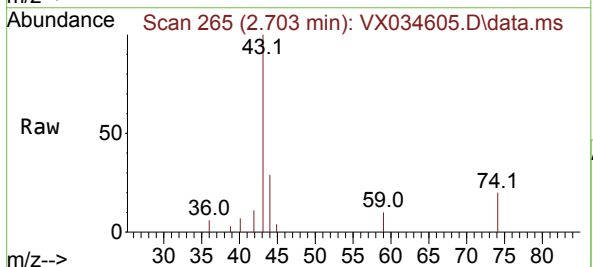



#20

Methylene Chloride

Concen: 7.052 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :

CE-43-031423

Tgt Ion: 84 Resp: 20756





Ion Ratio Lower Upper

84 100

49 131.2 103.8 155.8

51 38.2 31.8 47.8

86 66.4 51.4 77.2



#25

2-Butanone

Concen: 4.078 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.030 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 43 Resp: 8849

Ion Ratio Lower Upper

43 100

72 28.5 19.3 28.9





#29

Tetrahydrofuran

Concen: 0.811 ug/l

RT: 5.025 min Scan# 641

Delta R.T. 0.030 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :

CE-43-031423





Tgt Ion: 42 Resp: 1086

Ion Ratio Lower Upper

42 100

72 32.7 34.5 51.7#

71 28.9 32.1 48.1#

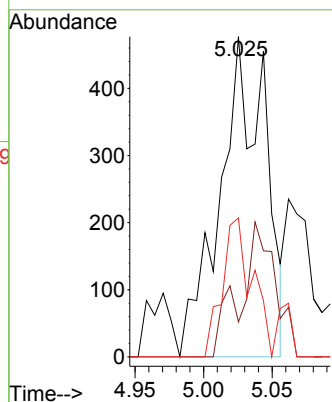

#33

1,2-Dichloroethane-d4

Concen: 48.614 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.012 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 65 Resp: 156510

Ion Ratio Lower Upper

65 100

67 50.7 0.0 104.0




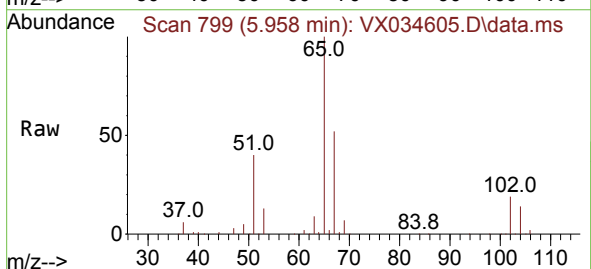




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion:114 Resp: 378010
Ion Ratio Lower Upper
114 100
63 21.5 0.0 42.2
88 15.5 0.0 33.2

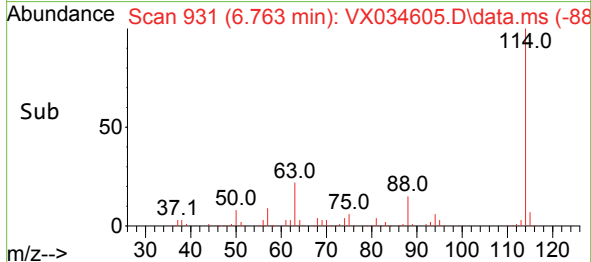

#35
Dibromofluoromethane
Concen: 48.723 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion:113 Resp: 121602
Ion Ratio Lower Upper
113 100
111 101.0 83.7 125.5
192 18.5 15.4 23.2


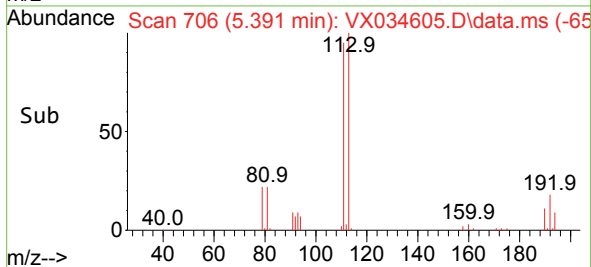

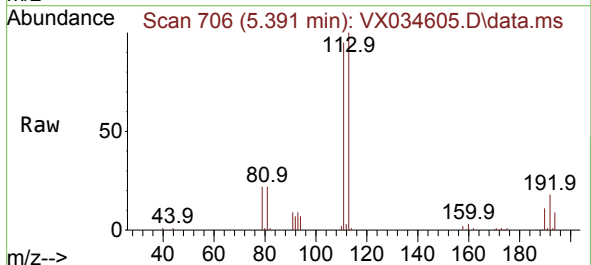




#36
1,1-Dichloropropene
Concen: 4.895 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion: 75 Resp: 18765
Ion Ratio Lower Upper
75 100
110 9.7 17.5 52.5#
77 0.0 24.3 36.5#

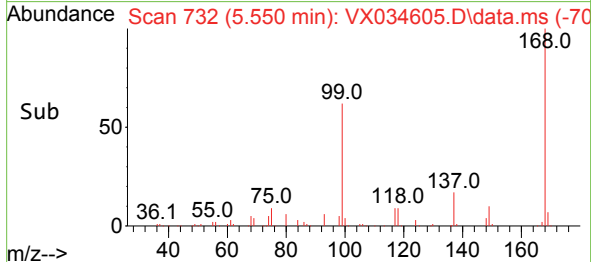

#37
Ethyl Acetate
Concen: 14.525 ug/l
RT: 4.714 min Scan# 595
Delta R.T. 0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32


Tgt Ion: 43 Resp: 60829
Ion Ratio Lower Upper
43 100
61 13.9 10.2 15.4
70 10.8 8.2 12.4

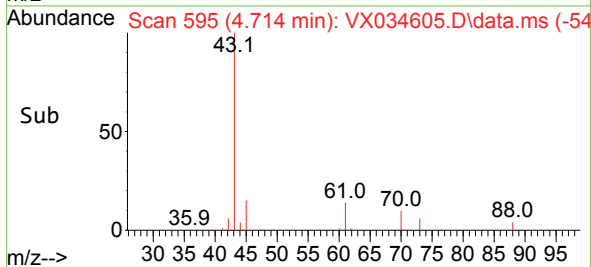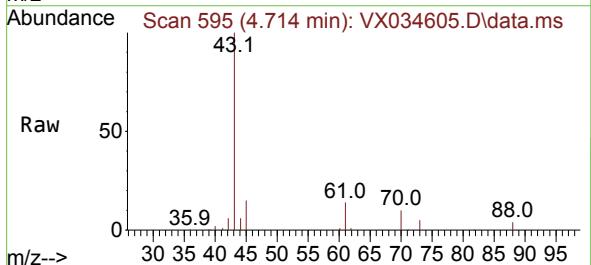






#38
Carbon Tetrachloride
Concen: 6.032 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.116 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423







Tgt Ion:117 Resp: 23005
Ion Ratio Lower Upper
117 100
119 4.1 76.6 114.8#
121 0.0 23.8 35.6#



#43
Isopropyl Acetate
Concen: 36.029 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion: 43 Resp: 255611
Ion Ratio Lower Upper
43 100
61 18.6 15.2 22.8
87 12.2 9.8 14.8




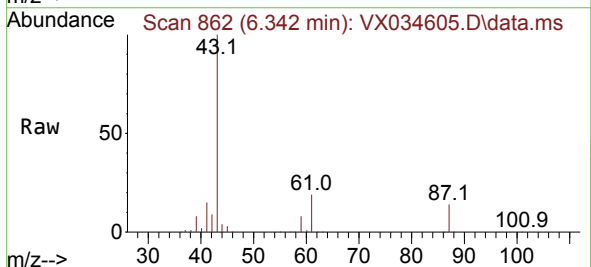




#48
Methyl methacrylate
Concen: 63.458 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.110 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion: 41 Resp: 216526
Ion Ratio Lower Upper
41 100
69 0.1 62.2 93.4#
39 54.7 47.7 71.5

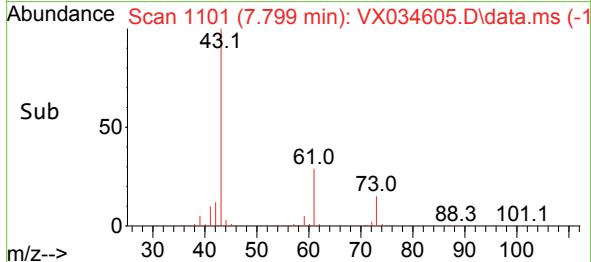

#49
1,4-Dioxane
Concen: 1.563 ug/l
RT: 7.641 min Scan# 1075
Delta R.T. -0.012 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion: 88 Resp: 112
Ion Ratio Lower Upper
88 100
43 0.0 27.7 41.5#
58 3752.7 56.8 85.2#


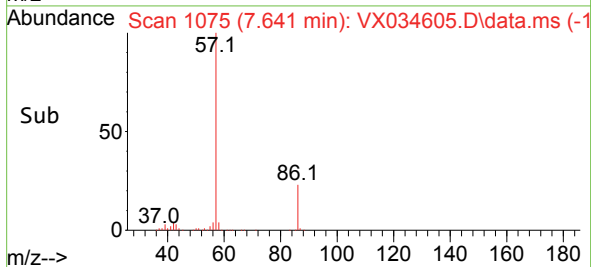

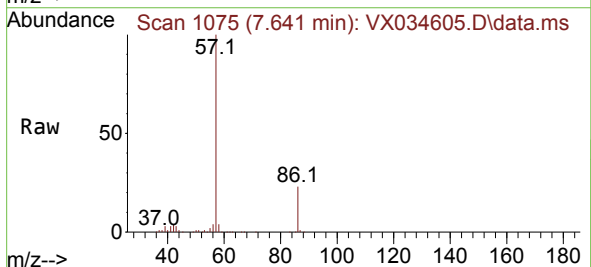


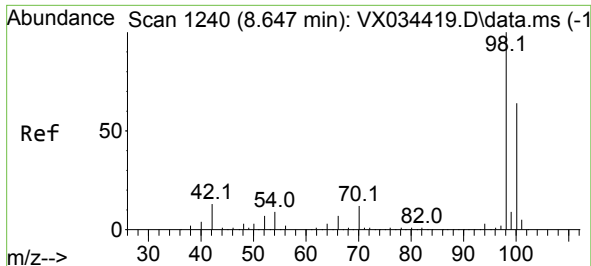

#50
Toluene-d8
Concen: 49.956 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion: 98 Resp: 465437
Ion Ratio Lower Upper
98 100
100 65.2 52.5 78.7

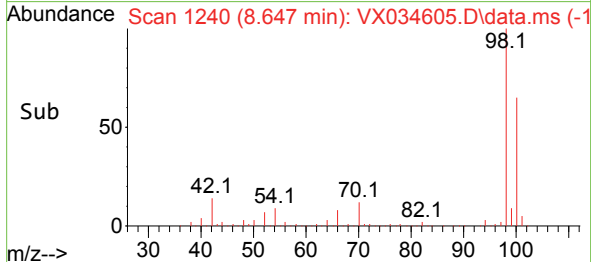

#51
4-Methyl-2-Pentanone
Concen: 48.709 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.018 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion: 43 Resp: 200469
Ion Ratio Lower Upper
43 100
58 8.4 30.6 46.0#


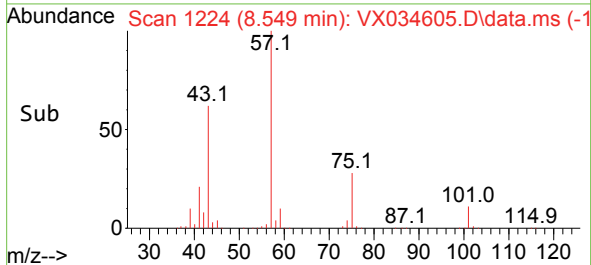

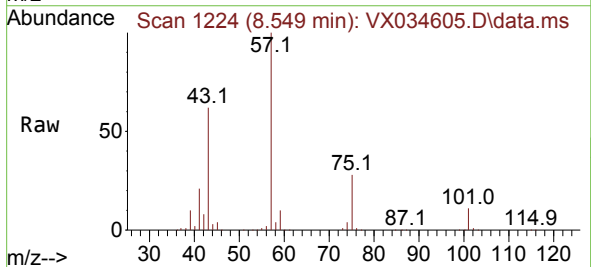




#53
 t-1,3-Dichloropropene
 Concen: 0.398 ug/l
 RT: 8.951 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX034605.D
 Acq: 18 Mar 2023 02:32




Instrument :
 MSVOA_X
 ClientSampleId :
 CE-43-031423


Tgt Ion: 75 Resp: 1727
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.4 38.2#



#54
 cis-1,3-Dichloropropene
 Concen: 17.930 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.189 min
 Lab File: VX034605.D
 Acq: 18 Mar 2023 02:32

Tgt Ion: 75 Resp: 84195
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.0 37.4#
 39 35.1 44.6 66.8#

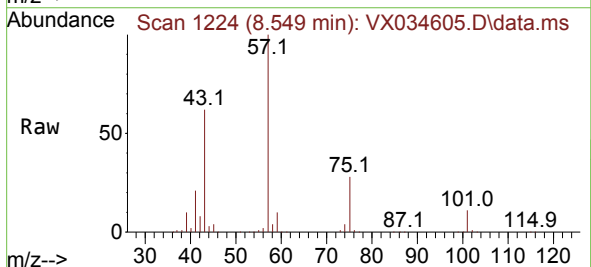



#57

1,3-Dichloropropane

Concen: 2.199 ug/l

RT: 9.482 min Scan# 1177

Delta R.T. 0.177 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :





CE-43-031423

Tgt Ion: 76 Resp: 10768

Ion Ratio Lower Upper

76 100

78 0.4 25.8 38.8#

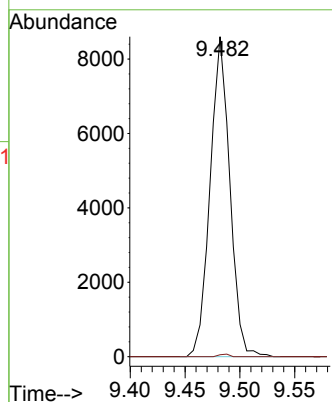

#58

2-Chloroethyl Vinyl ether

Concen: 0.968 ug/l

RT: 8.256 min Scan# 1176

Delta R.T. 0.018 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 63 Resp: 2257

Ion Ratio Lower Upper

63 100

106 26.6 22.2 33.2





#59

2-Hexanone

Concen: 47.046 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.055 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :





CE-43-031423

Tgt Ion: 43 Resp: 149673

Ion Ratio Lower Upper

43 100

58 18.2 26.3 78.9#

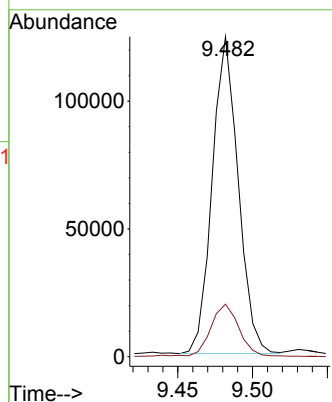

#62

4-Bromofluorobenzene

Concen: 46.157 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32




Tgt Ion: 95 Resp: 173706


Ion Ratio Lower Upper

95 100

174 75.6 0.0 147.4

176 72.3 0.0 140.6









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion:117 Resp: 342375
Ion Ratio Lower Upper
117 100
82 57.1 45.0 67.4
119 32.4 26.0 39.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32

Tgt Ion:152 Resp: 144263
Ion Ratio Lower Upper
152 100
115 60.3 45.0 135.0
150 159.1 0.0 352.4

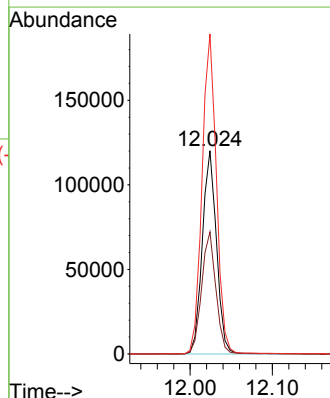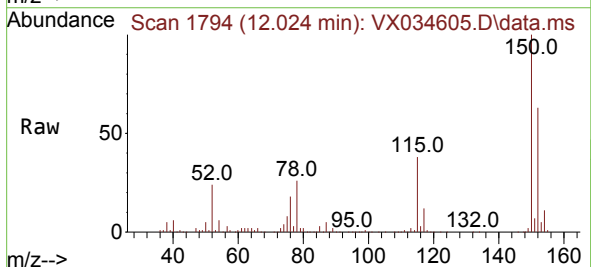



#74

N-amy1 acetate

Concen: 10.715 ug/l

RT: 10.640 min Scan# 1

Delta R.T. -0.201 min

Lab File: VX034605.D

Acq: 18 Mar 2023 02:32

Instrument :

MSVOA_X

ClientSampleId :

CE-43-031423

Tgt Ion: 43 Resp: 57223





Ion Ratio Lower Upper

43 100

70 1.8 32.1 48.1#

55 4.5 18.3 27.5#

61 9.6 18.8 28.2#

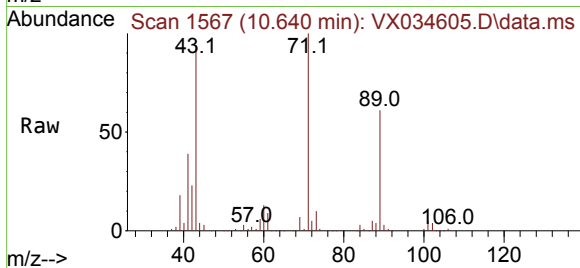

#76

1,2,3-Trichloropropane

Concen: 28.649 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX034605.D




Acq: 18 Mar 2023 02:32


Tgt Ion: 75 Resp: 94897

Ion Ratio Lower Upper

75 100

77 1.0 21.6 64.8#




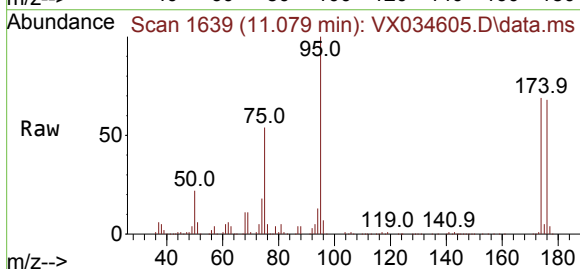




#81
 trans-1,4-Dichloro-2-butene
 Concen: 77.503 ug/l
 RT: 11.079 min Scan# 1
 Delta R.T. 0.061 min
 Lab File: VX034605.D
 Acq: 18 Mar 2023 02:32




Instrument :
 MSVOA_X
 ClientSampleId :
 CE-43-031423


Tgt Ion: 75 Resp: 94897
 Ion Ratio Lower Upper
 75 100
 53 0.0 82.6 124.0#
 89 0.0 36.9 55.3#

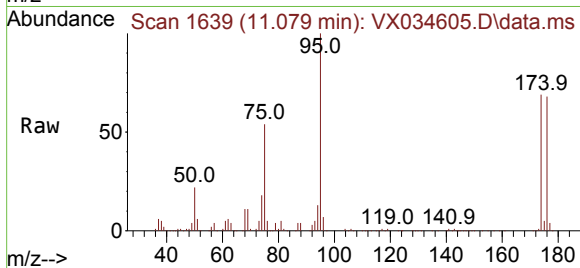

#93
 1,2,4-Trichlorobenzene
 Concen: 0.258 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. 0.006 min
 Lab File: VX034605.D
 Acq: 18 Mar 2023 02:32

Tgt Ion:180 Resp: 817
 Ion Ratio Lower Upper
 180 100
 182 88.6 47.0 141.0
 145 28.0 15.9 47.7


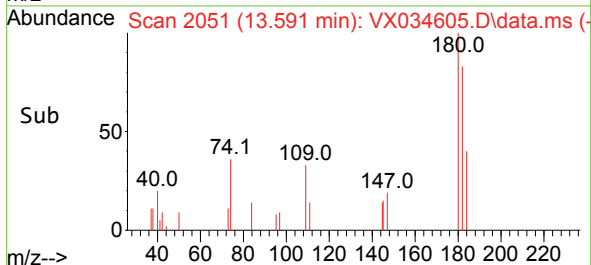

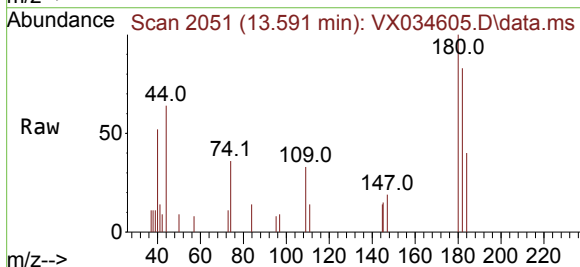




#94
Hexachlorobutadiene
Concen: 0.436 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32




Instrument :
MSVOA_X
ClientSampleId :
CE-43-031423


Tgt Ion:	225	Resp:	556
Ion	Ratio	Lower	Upper
225	100		
223	75.7	32.1	96.5
227	48.6	31.8	95.4

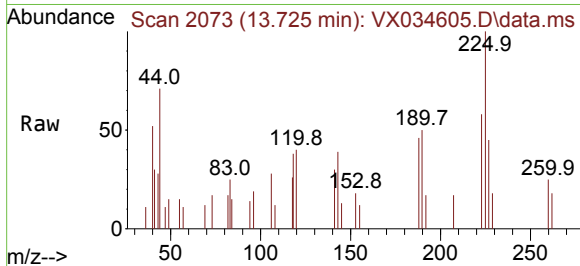

#95
Naphthalene
Concen: 0.211 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX034605.D
Acq: 18 Mar 2023 02:32


Tgt Ion:	128	Resp:	2244
Ion	Ratio	Lower	Upper
128	100		
127	12.8	10.2	15.4
129	10.2	8.6	13.0

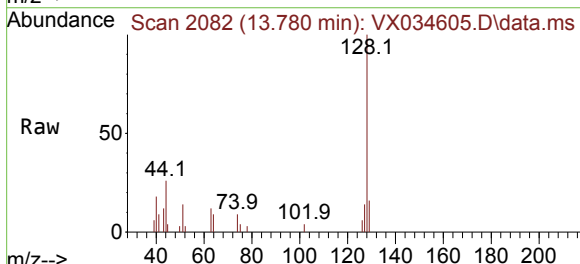



#96
 1,2,3-Trichlorobenzene
 Concen: 0.234 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX034605.D
 Acq: 18 Mar 2023 02:32

Instrument :
 MSVOA_X
 ClientSampleId :
 CE-43-031423



Tgt Ion:180 Resp: 724
 Ion Ratio Lower Upper
 180 100
 182 75.3 48.0 144.2
 145 30.5 17.7 53.1

