


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031723\
Data File : VX034600.D
Acq On : 17 Mar 2023 23:17
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

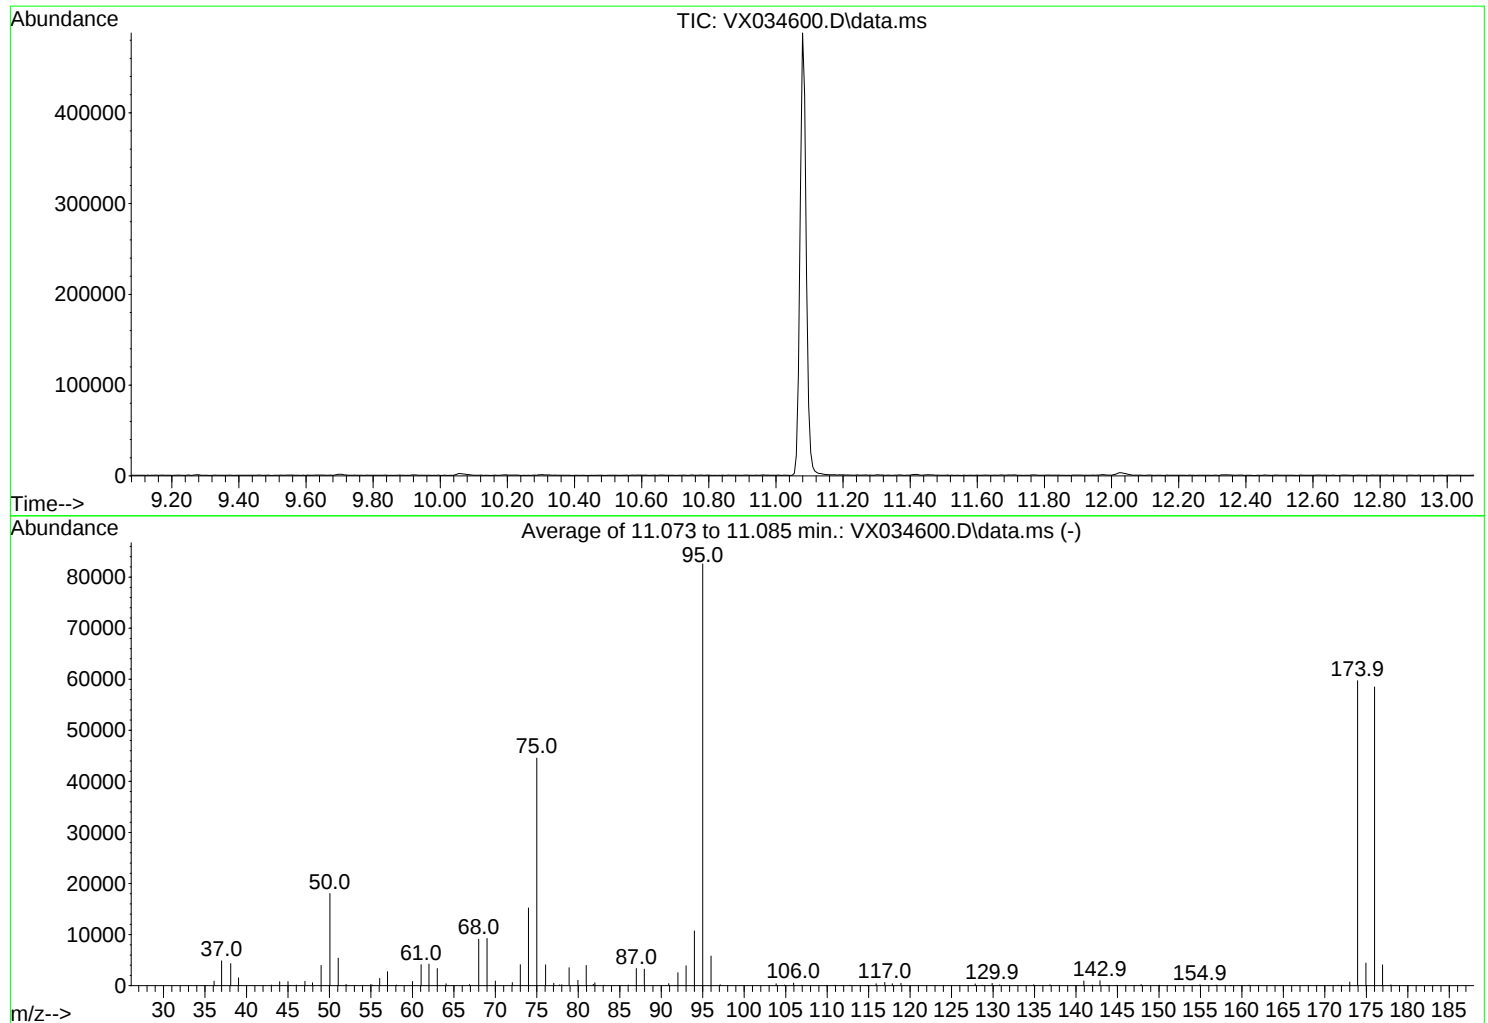

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	18057	PASS
75	95	30	60	53.9	44557	PASS
95	95	100	100	100.0	82600	PASS
96	95	5	9	7.0	5805	PASS
173	174	0.00	2	1.2	730	PASS
174	95	50	100	72.3	59723	PASS
175	174	5	9	7.4	4411	PASS
176	174	95	101	98.0	58515	PASS
177	176	5	9	7.0	4067	PASS