

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031725\
 Data File : VX045298.D
 Acq On : 17 Mar 2025 11:39
 Operator : JC/MD
 Sample : VX0317MBL01
 Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0317MBL01

Quant Time: Mar 18 01:22:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	71165	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	137682	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	125229	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53343	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	59138	52.243	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	104.480%
35) Dibromofluoromethane	5.379	113	48552	52.737	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.480%
50) Toluene-d8	8.647	98	169665	50.834	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.660%
62) 4-Bromofluorobenzene	11.079	95	60052	54.297	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	108.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031725\
Data File : VX045298.D
Acq On : 17 Mar 2025 11:39
Operator : JC/MD
Sample : VX0317MBL01
Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0317MBL01

Quant Time: Mar 18 01:22:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




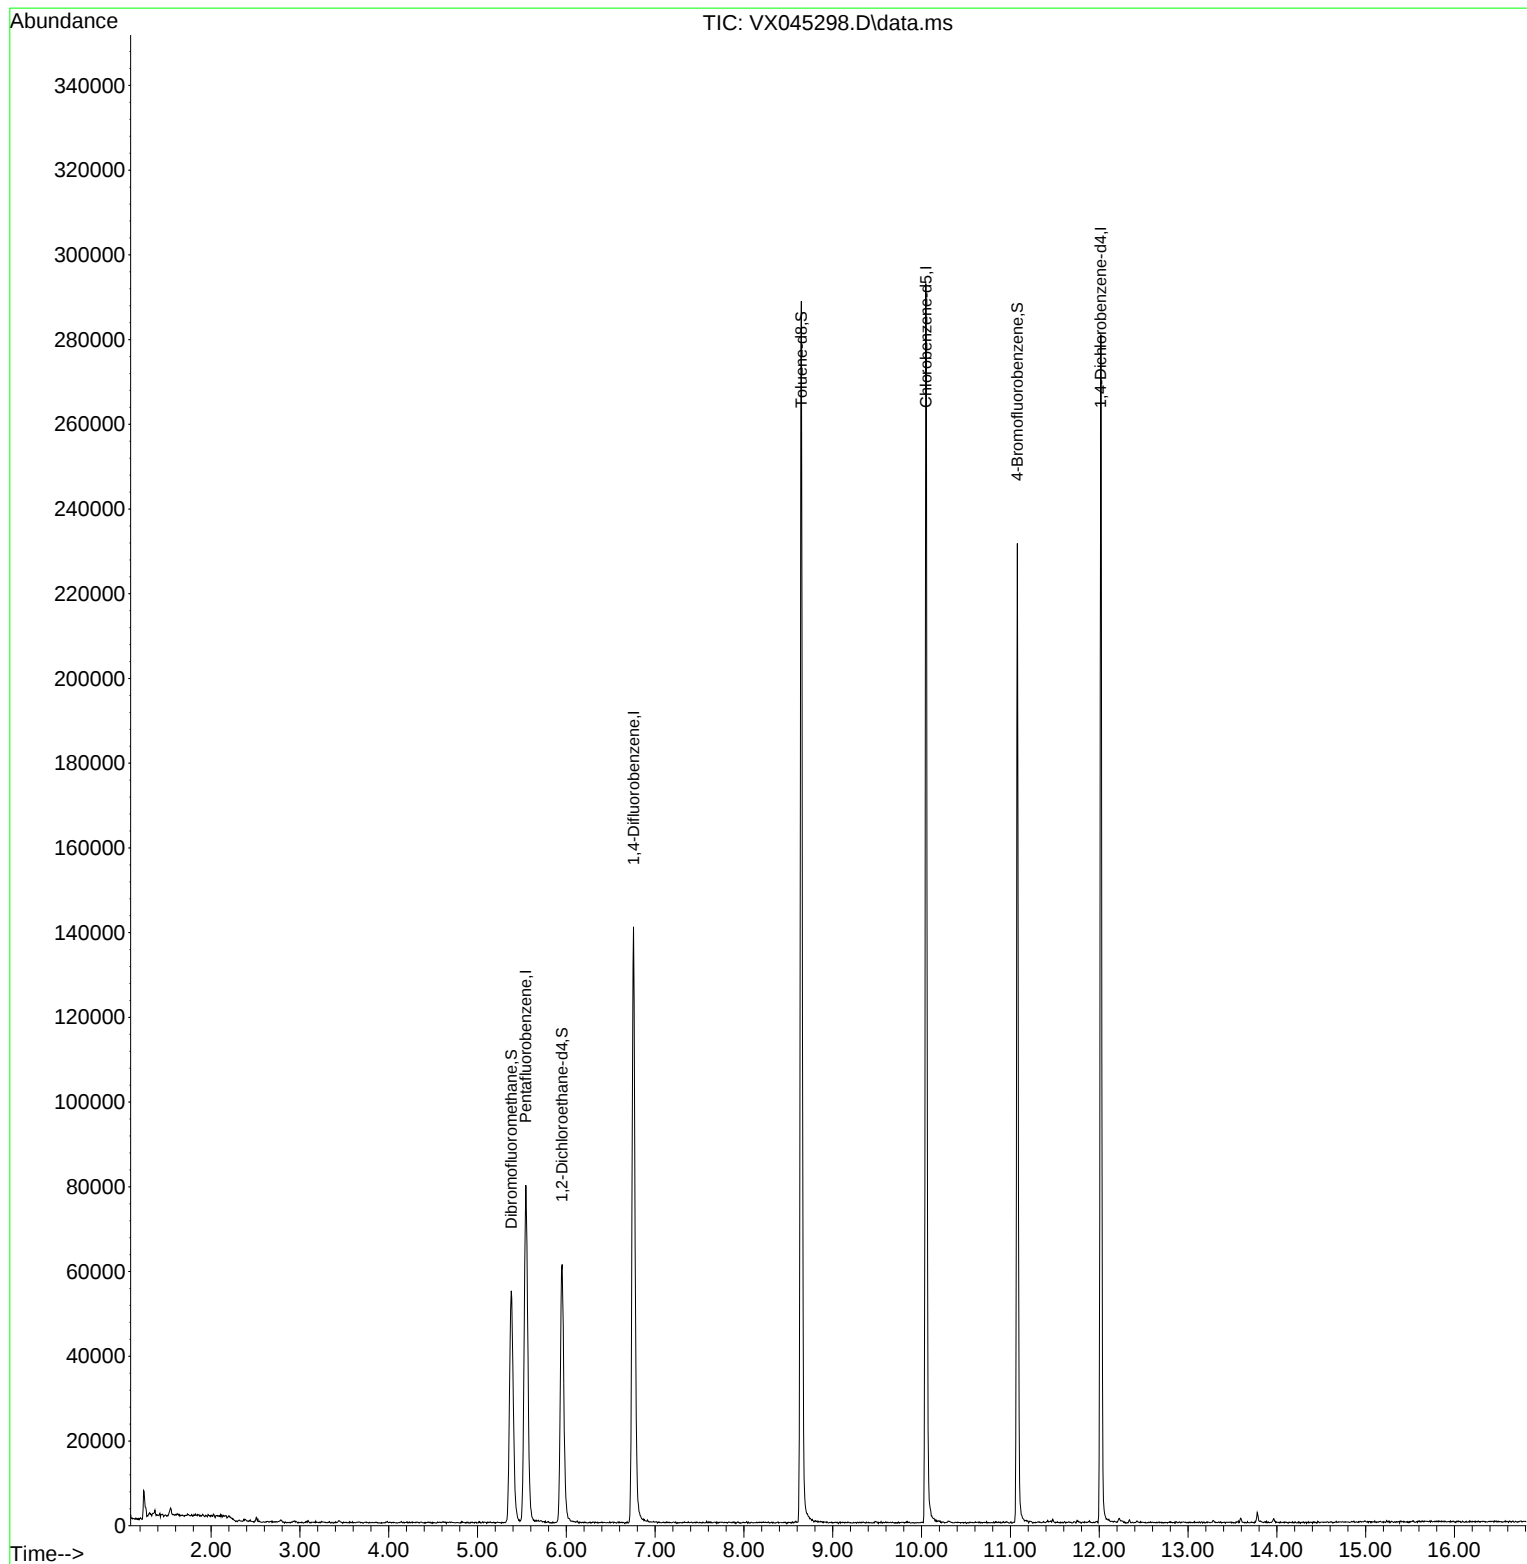


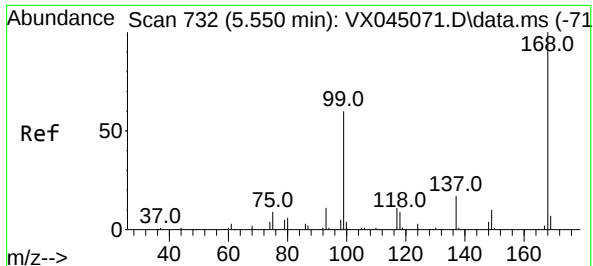

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 712
Delta R.T. -0.006 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39




Instrument :
MSVOA_X
ClientSampleId :
VX0317MBL01

Tgt Ion:168 Resp: 71165
Ion Ratio Lower Upper
168 100
99 60.2 48.2 72.4

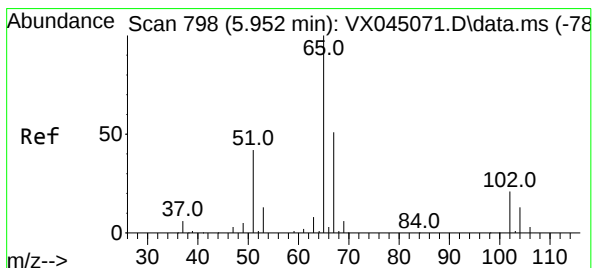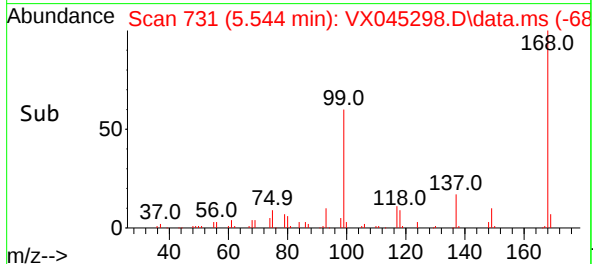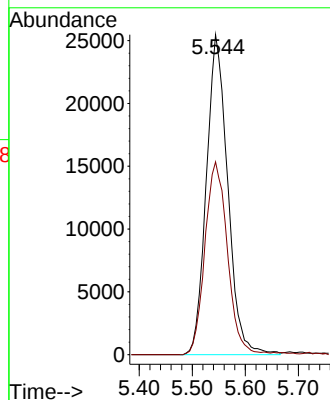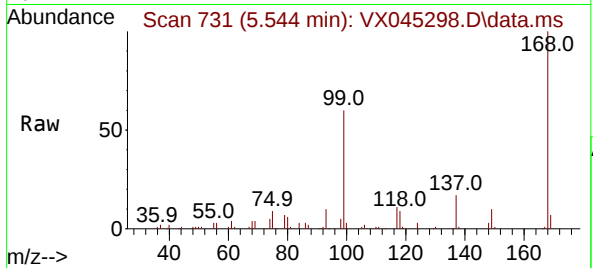

#33
1,2-Dichloroethane-d4
Concen: 52.243 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39

Tgt Ion: 65 Resp: 59138
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.2

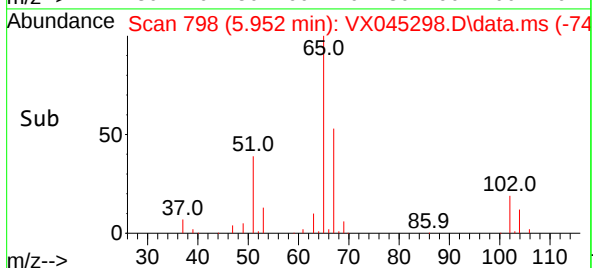
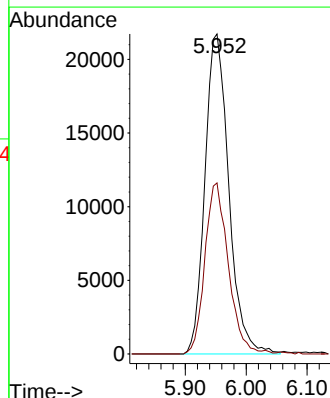
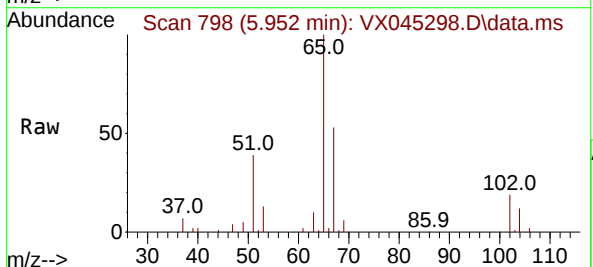




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39




Instrument :
MSVOA_X
ClientSampleId :
VX0317MBL01


Tgt Ion:114 Resp: 137682
Ion Ratio Lower Upper
114 100
63 22.7 0.0 41.8
88 16.2 0.0 32.8

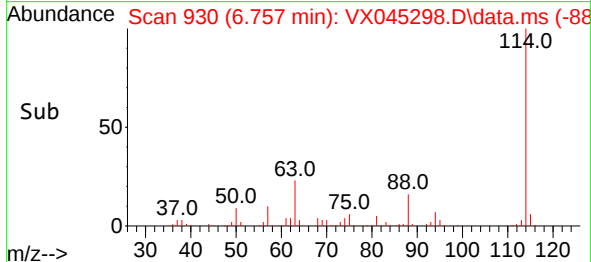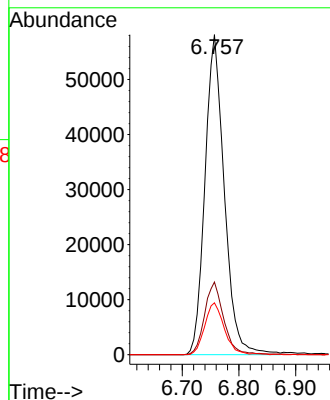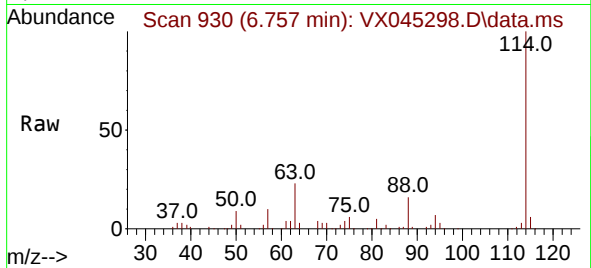

#35
Dibromofluoromethane
Concen: 52.737 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39

Tgt Ion:113 Resp: 48552
Ion Ratio Lower Upper
113 100
111 102.5 81.8 122.6
192 17.0 14.3 21.5


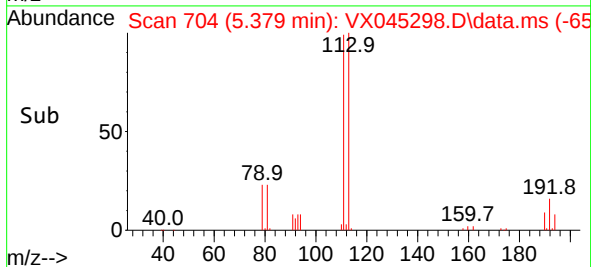
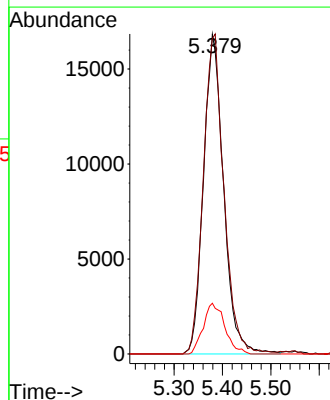
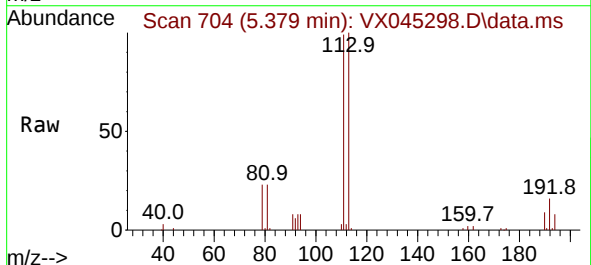


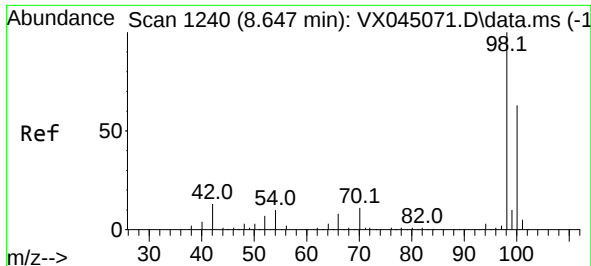

#50
Toluene-d8
Concen: 50.834 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39




Instrument :
MSVOA_X
ClientSampleId :
VX0317MBL01


Tgt Ion: 98 Resp: 169665
Ion Ratio Lower Upper
98 100
100 64.1 52.0 78.0

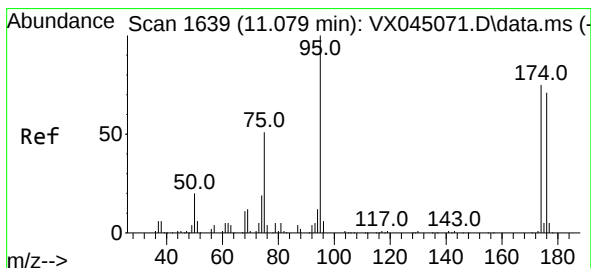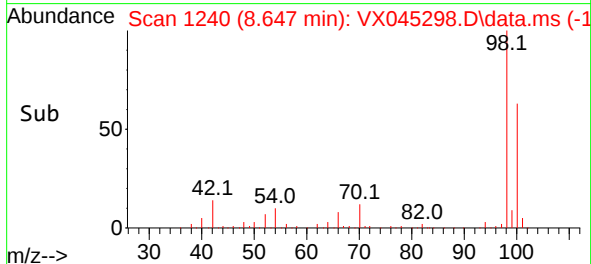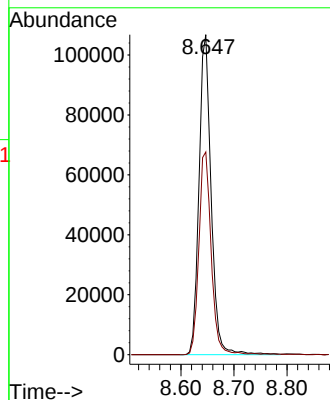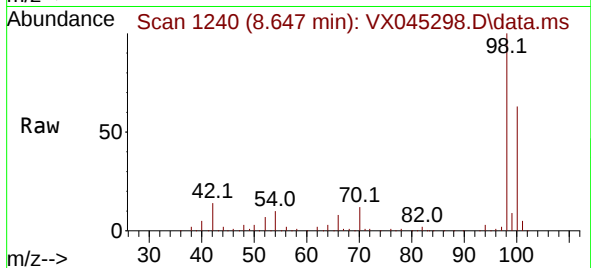

#62
4-Bromofluorobenzene
Concen: 54.297 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39

Tgt Ion: 95 Resp: 60052
Ion Ratio Lower Upper
95 100
174 71.3 0.0 148.2
176 70.0 0.0 141.4


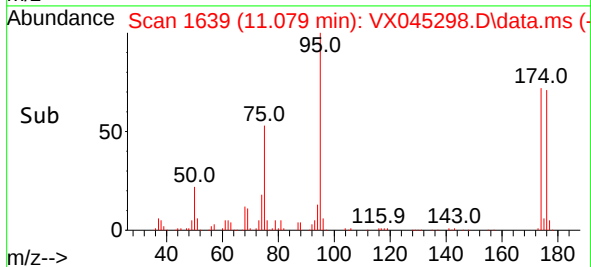
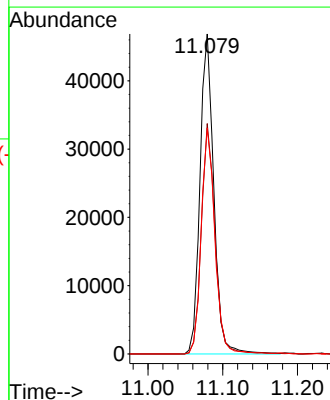
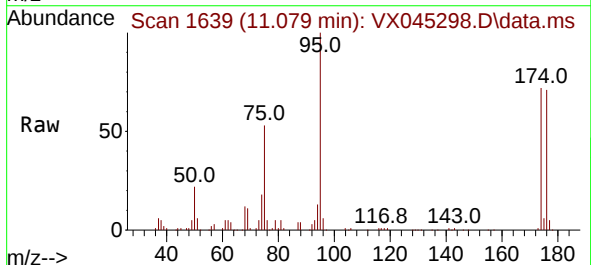


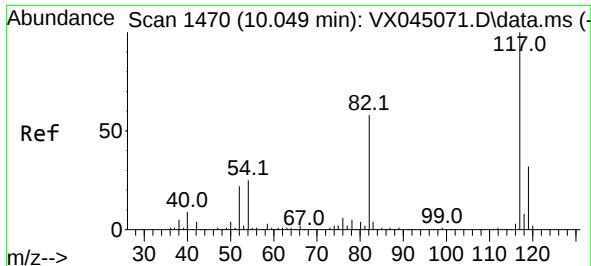

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39

Instrument :
MSVOA_X
ClientSampleId :
VX0317MBL01

Tgt Ion:117 Resp: 125229
Ion Ratio Lower Upper
117 100
82 58.6 46.3 69.5
119 32.4 25.7 38.5

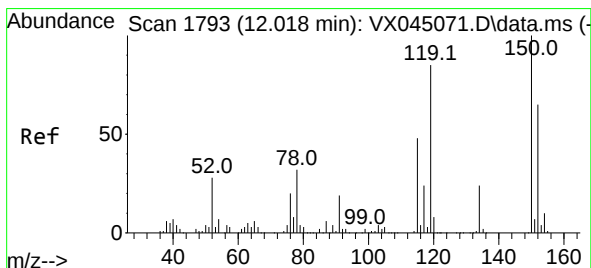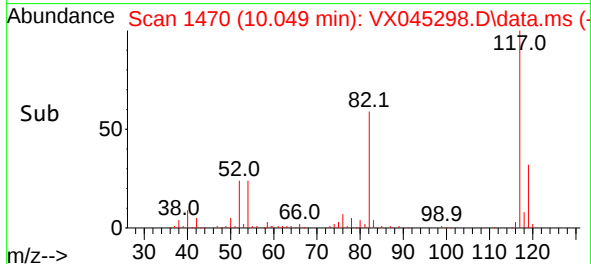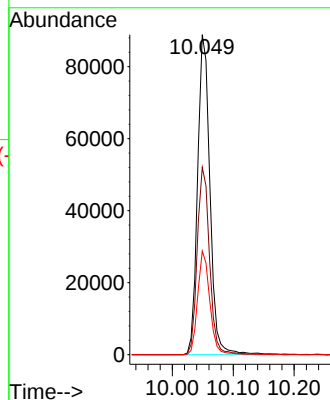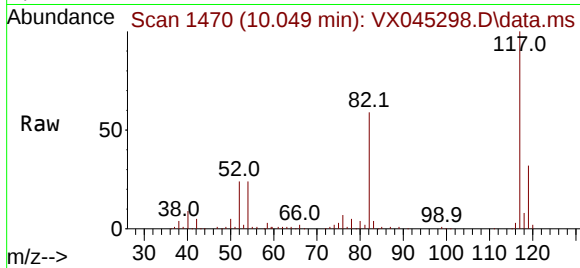

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045298.D
Acq: 17 Mar 2025 11:39

Tgt Ion:152 Resp: 53343
Ion Ratio Lower Upper
152 100
115 62.8 44.2 132.6
150 156.4 0.0 349.0

