

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031819\
 Data File : VX008163.D
 Acq On : 18 Mar 2019 12:32
 Operator : JC/SP
 Sample : IBLK
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Mar 19 03:42:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X031819W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Mon Mar 18 14:34:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.02	128	57017	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.86	114	317758	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	267672	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.07	65	143147	30.18	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	100.60%
60) 4-Bromofluorobenzene	11.13	95	126588	28.34	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	94.47%
63) Toluene-d8	8.71	98	396820	30.51	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	101.70%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031819\
Data File : VX008163.D
Acq On : 18 Mar 2019 12:32
Operator : JC/SP
Sample : IBLK
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Mar 19 03:42:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X031819W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Mon Mar 18 14:34:46 2019
Response via : Initial Calibration

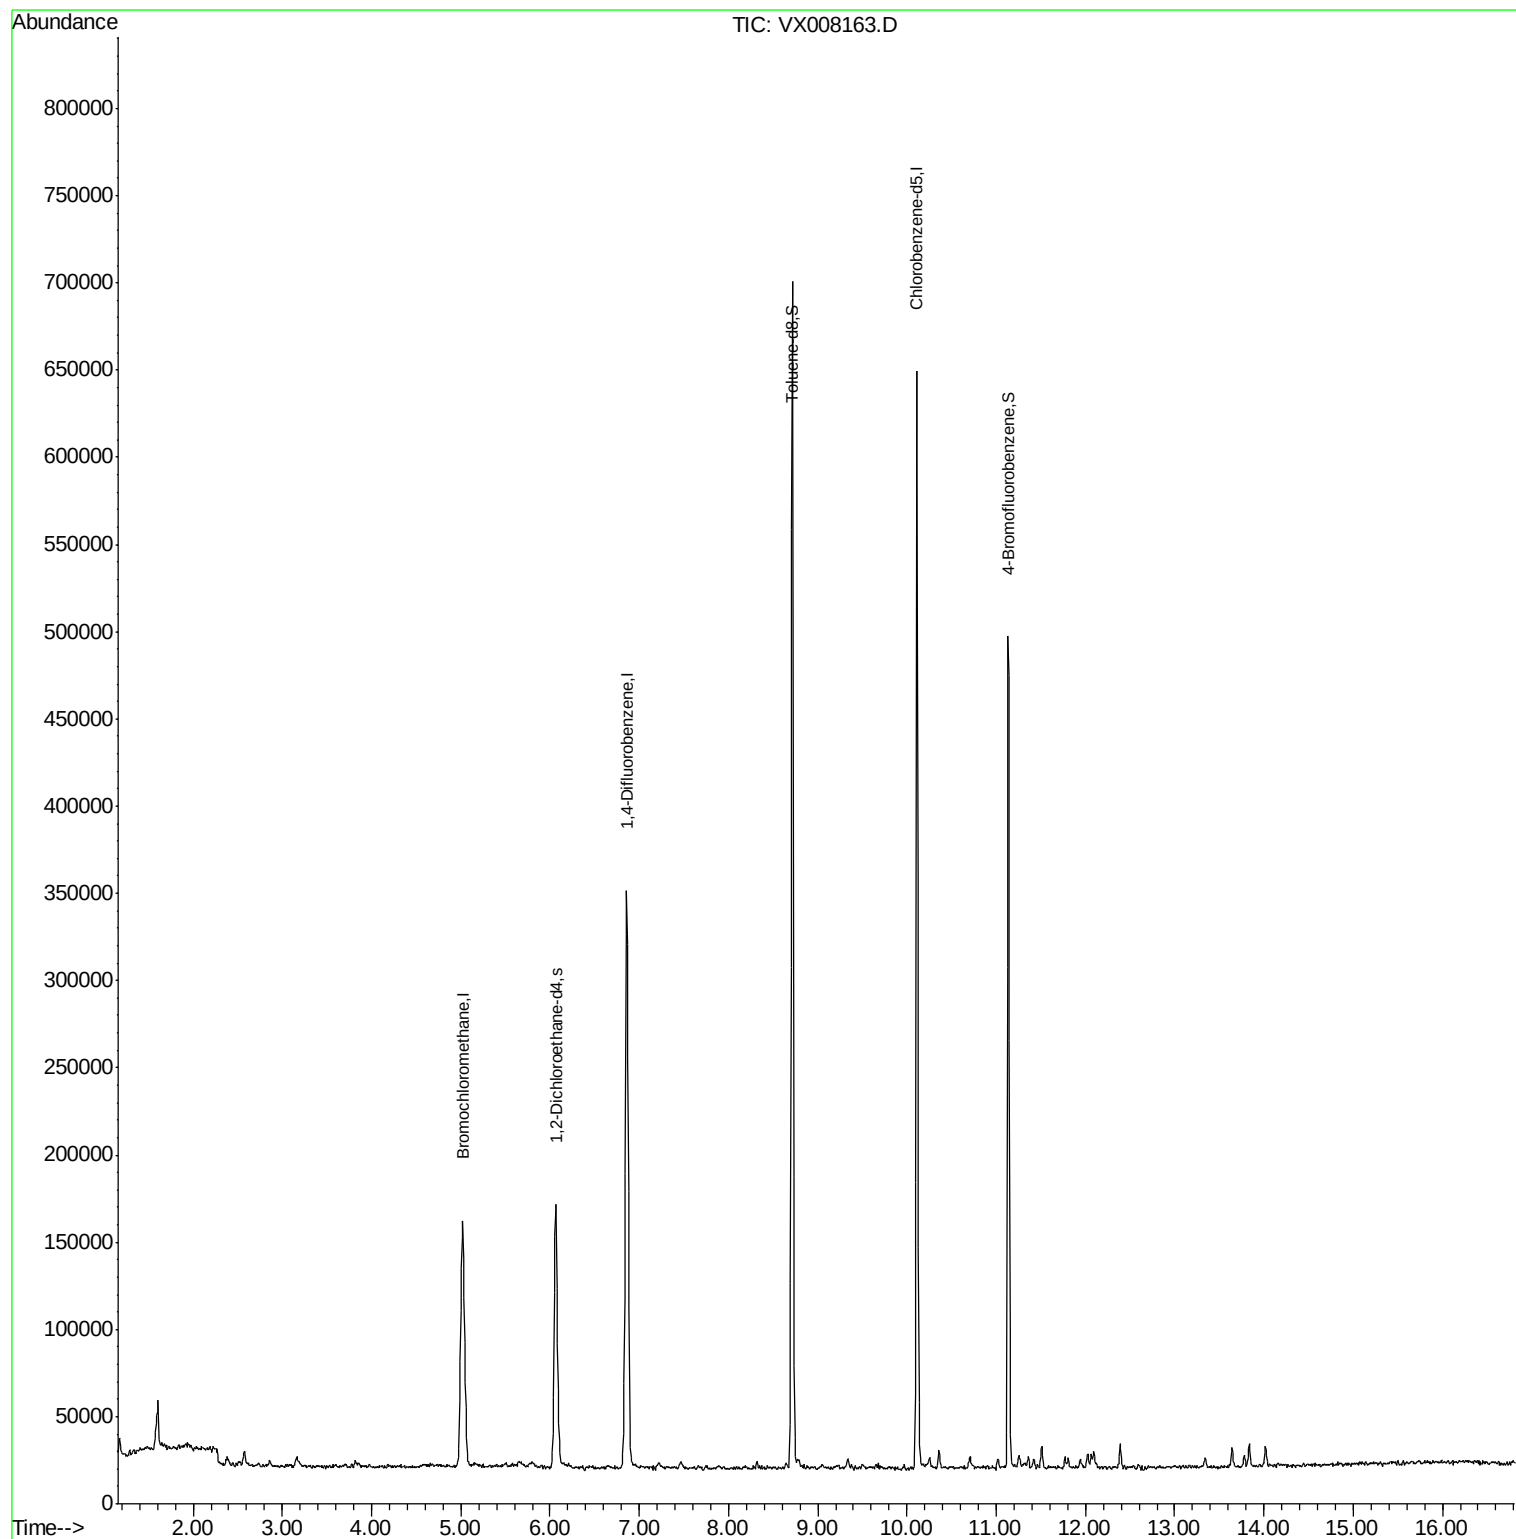

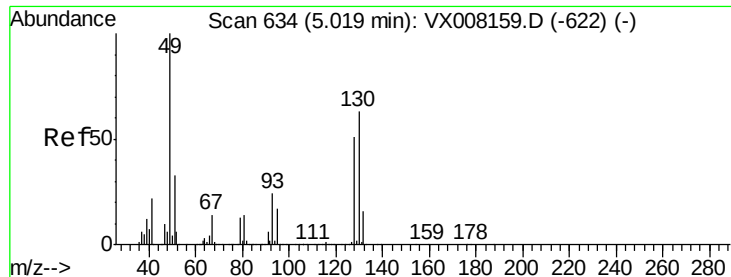

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.02 min Scan# 634

Delta R.T. -0.00 min

Lab File: VX008163.D

Acq: 18 Mar 2019 12:32

Instrument :

MSVOA_X

ClientSampleId :

IBLK


Tot Ion:128 Resp: 57017

Ion Ratio Lower Upper

128 100

49 196.8 0.0 350.8




130 130.7 0.0 325.8

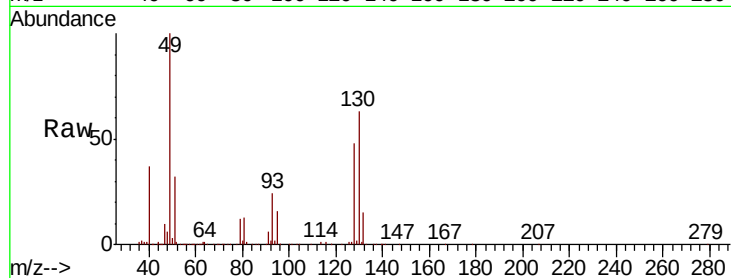

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

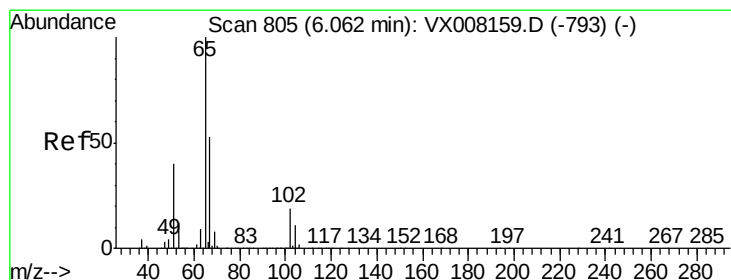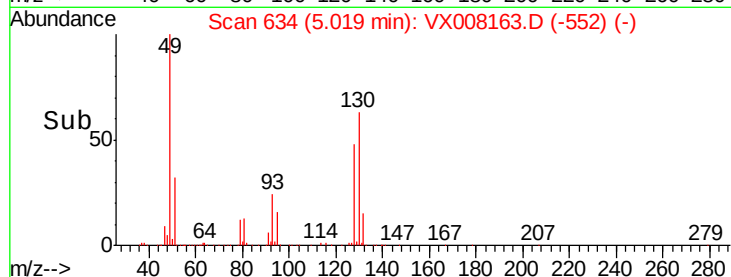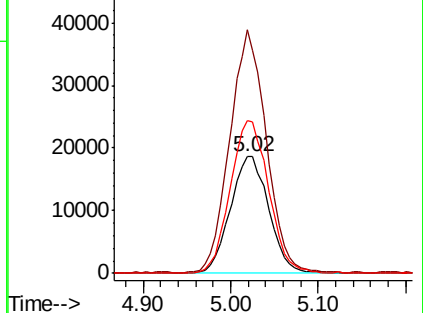

#27

1,2-Dichloroethane-d4

Concen: 30.182 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX008163.D


Acq: 18 Mar 2019 12:32

Tgt Ion: 65 Resp: 143147

Ion Ratio Lower Upper



65 100


67 53.9 42.9 64.3

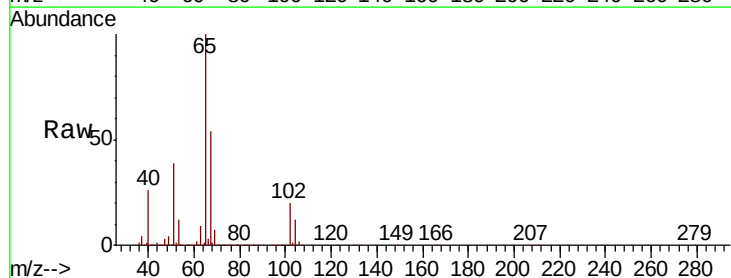

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



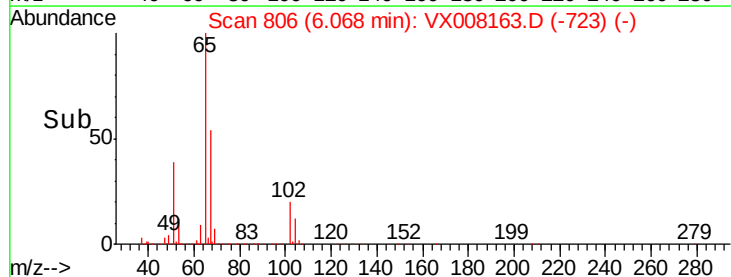
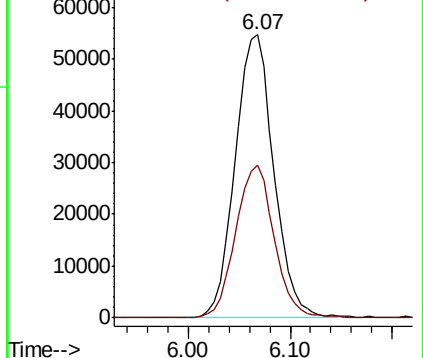


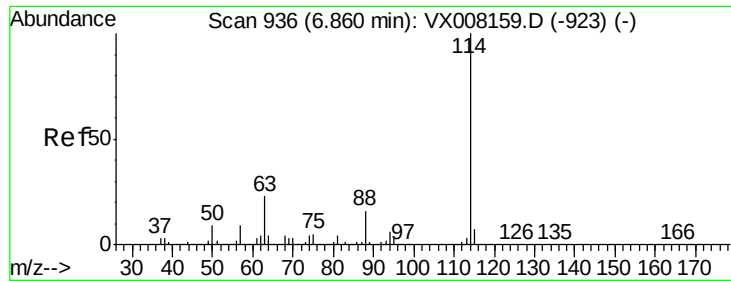

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008163.D
 Acq: 18 Mar 2019 12:32




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tot Ion	Ratio	Lower	Upper
114	100		
63	23.1	14.2	21.4#
88	16.8	11.9	17.9

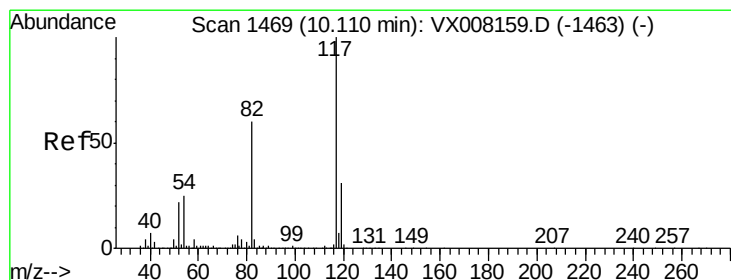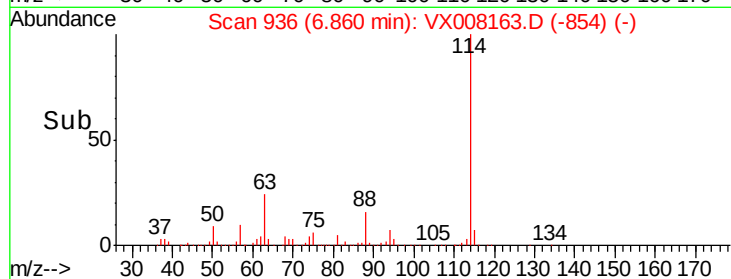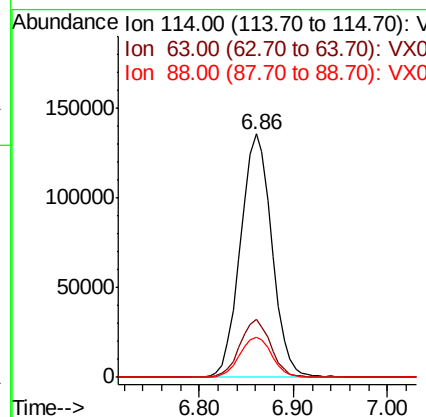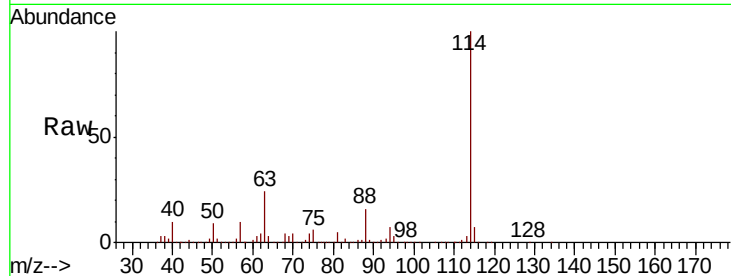

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VX008163.D
 Acq: 18 Mar 2019 12:32

Tgt Ion	Ratio	Lower	Upper
117	100		
82	61.1	40.4	60.6#
119	32.5	25.8	38.6


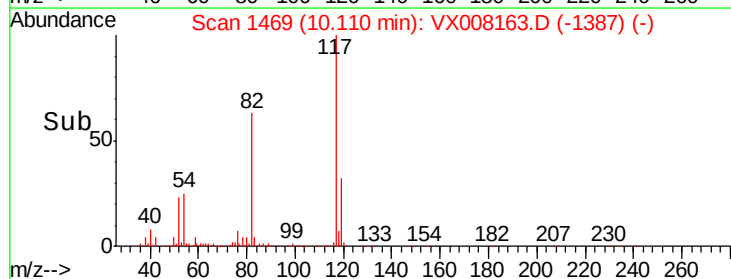
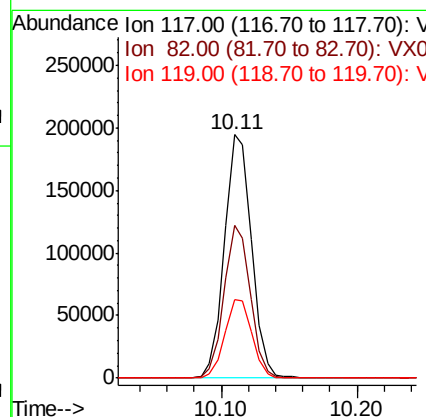
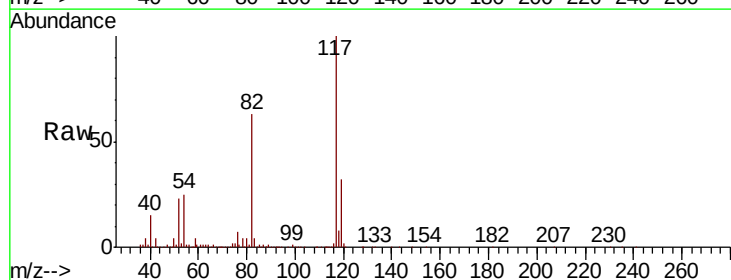


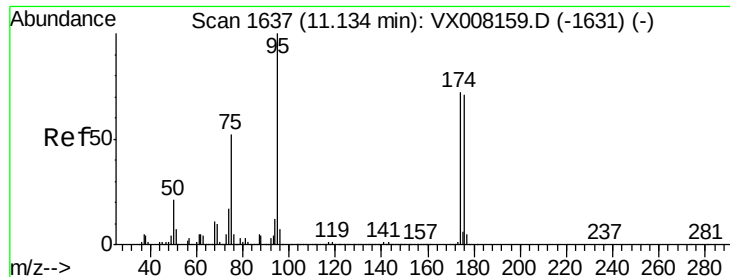

#60
4-Bromofluorobenzene
Concen: 28.337 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008163.D
Acq: 18 Mar 2019 12:32

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tot Ion	95	Resp	126588
Ion Ratio	Lower	Upper	
95	100		
174	77.0	74.9	112.3
176	75.4	70.7	106.1

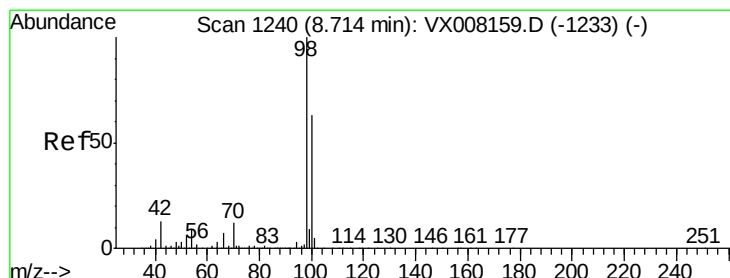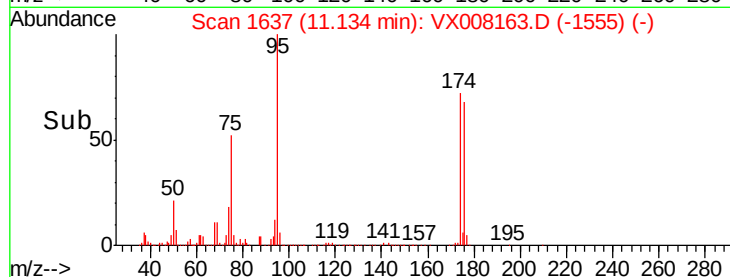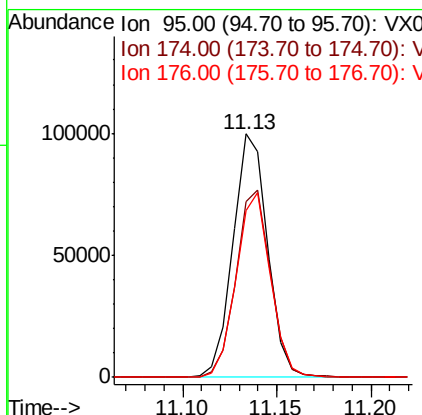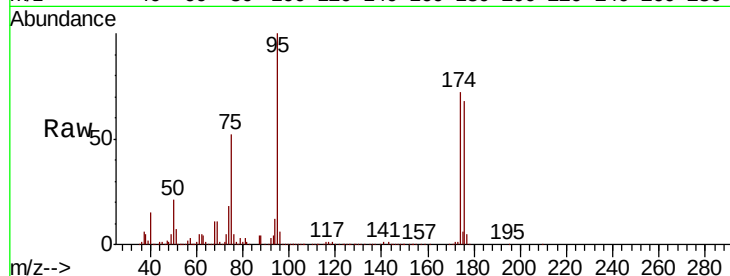

#63
Toluene-d8
Concen: 30.512 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX008163.D
Acq: 18 Mar 2019 12:32

Tgt Ion	98	Resp	396820
Ion Ratio	Lower	Upper	
98	100		
100	63.1	50.9	76.3

