


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX031819\
 Data File : VX008157.D
 Acq On : 18 Mar 2019 09:51
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X031819W.M
 Title : SW846 8260
 Last Update : Wed Nov 21 08:15:54 2018

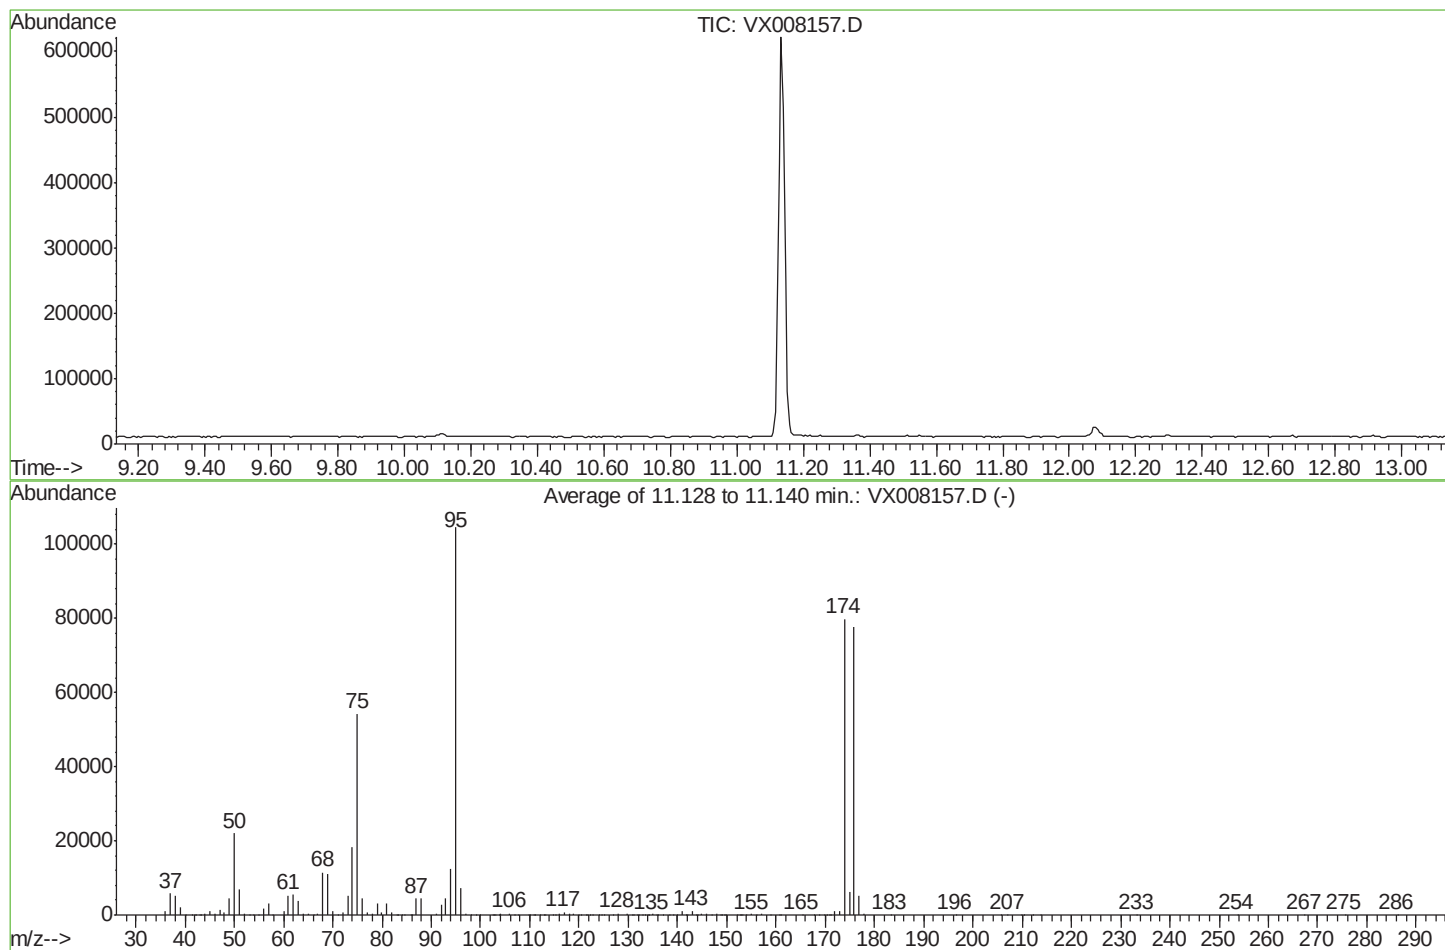

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	21988	PASS
75	95	30	60	51.9	54198	PASS
95	95	100	100	100.0	104509	PASS
96	95	5	9	6.9	7183	PASS
173	174	0.00	2	1.5	1177	PASS
174	95	50	100	76.4	79850	PASS
175	174	5	9	7.7	6182	PASS
176	174	95	101	97.3	77709	PASS
177	176	5	9	6.5	5078	PASS