

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031821\
 Data File : VX021276.D
 Acq On : 18 Mar 2021 11:51
 Operator : JC/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX021276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.123	4	6	14	rVB	9009	10709	4.72%	0.538%
2	1.311	36	38	47	rVB4	1929	2793	1.23%	0.140%
3	1.387	47	51	57	rVB	30357	31166	13.73%	1.566%
4	1.693	99	103	109	rBV	21922	27272	12.02%	1.370%
5	2.340	207	213	229	rVB	54876	90047	39.68%	4.524%
6	2.546	243	248	255	rVB	1761	3459	1.52%	0.174%
7	2.829	291	296	304	rBV4	2864	6294	2.77%	0.316%
8	4.529	574	585	599	rBV	28380	84758	37.35%	4.258%
9	5.135	676	688	702	rBV	32939	99603	43.89%	5.004%
10	6.041	830	842	857	rBV4	77860	226932	100.00%	11.400%
11	6.829	967	976	989	rBV	64742	153995	67.86%	7.736%
12	7.182	1029	1036	1044	rVB8	1258	3009	1.33%	0.151%
13	7.365	1059	1067	1078	rBV	49486	109113	48.08%	5.481%
14	8.288	1217	1224	1231	rVV2	5633	9356	4.12%	0.470%
15	8.370	1231	1238	1253	rVB	35750	60090	26.48%	3.019%
16	8.694	1286	1293	1310	rBV	129045	202815	89.37%	10.189%
17	8.994	1338	1344	1354	rBV	21691	34891	15.38%	1.753%
18	9.424	1409	1417	1436	rBV	154819	216563	95.43%	10.879%
19	10.094	1525	1531	1544	rBV	133621	188089	82.88%	9.449%
20	10.688	1627	1632	1638	rVB6	1894	2761	1.22%	0.139%
21	11.230	1719	1724	1733	rBV	47163	58939	25.97%	2.961%
22	12.006	1849	1856	1860	rBV2	1967	2562	1.13%	0.129%
23	12.059	1860	1865	1874	rVB	148282	183784	80.99%	9.233%
24	12.359	1910	1916	1923	rBV	131331	169032	74.49%	8.492%
25	13.153	2046	2051	2055	rBV2	2700	3652	1.61%	0.183%
26	13.630	2124	2132	2138	rBV3	3618	5119	2.26%	0.257%
27	14.001	2191	2195	2199	rBV3	2787	3771	1.66%	0.189%




Sum of corrected areas: 1990574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031821\
Data File : VX021276.D
Acq On : 18 Mar 2021 11:51
Operator : JC/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

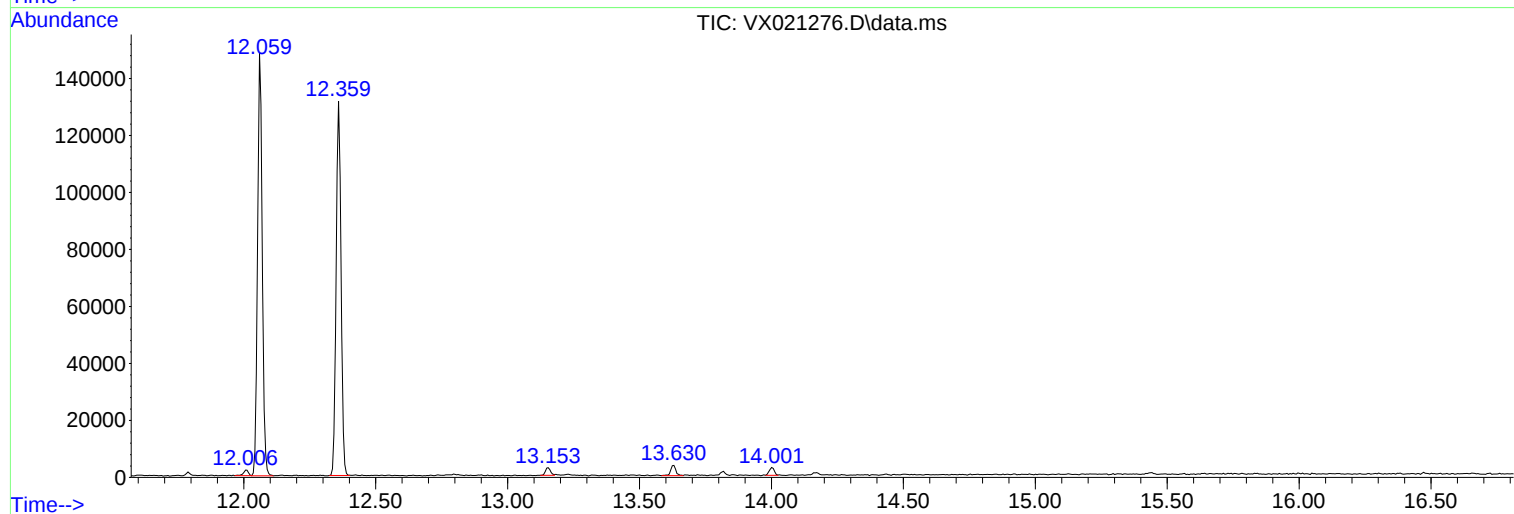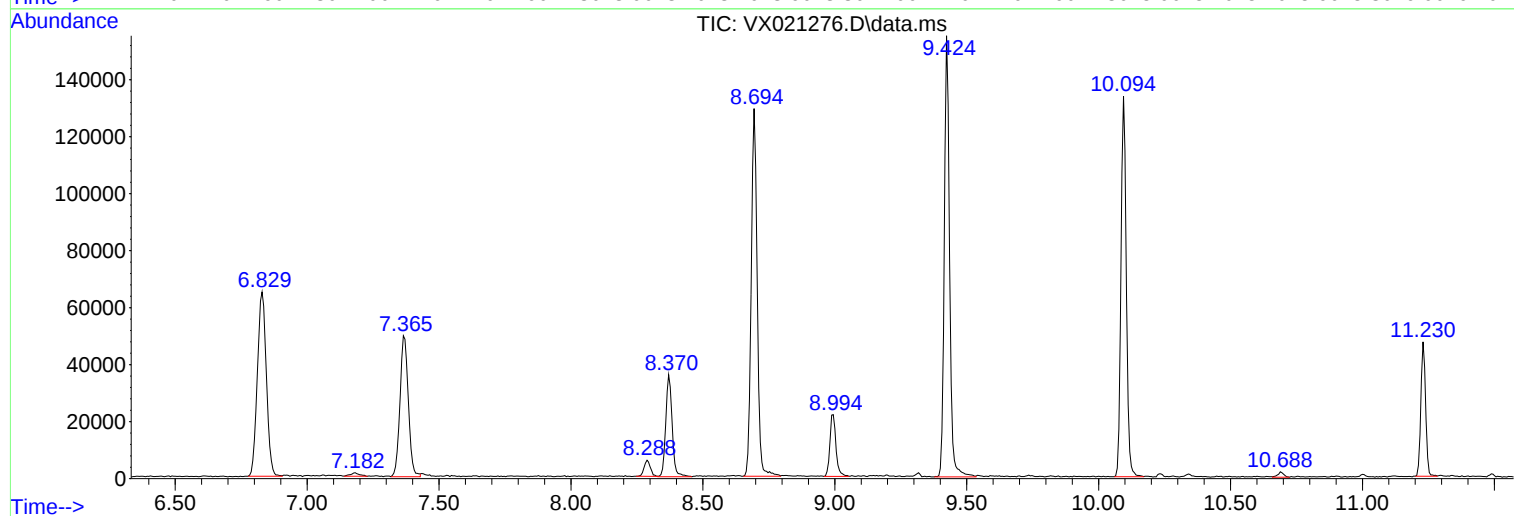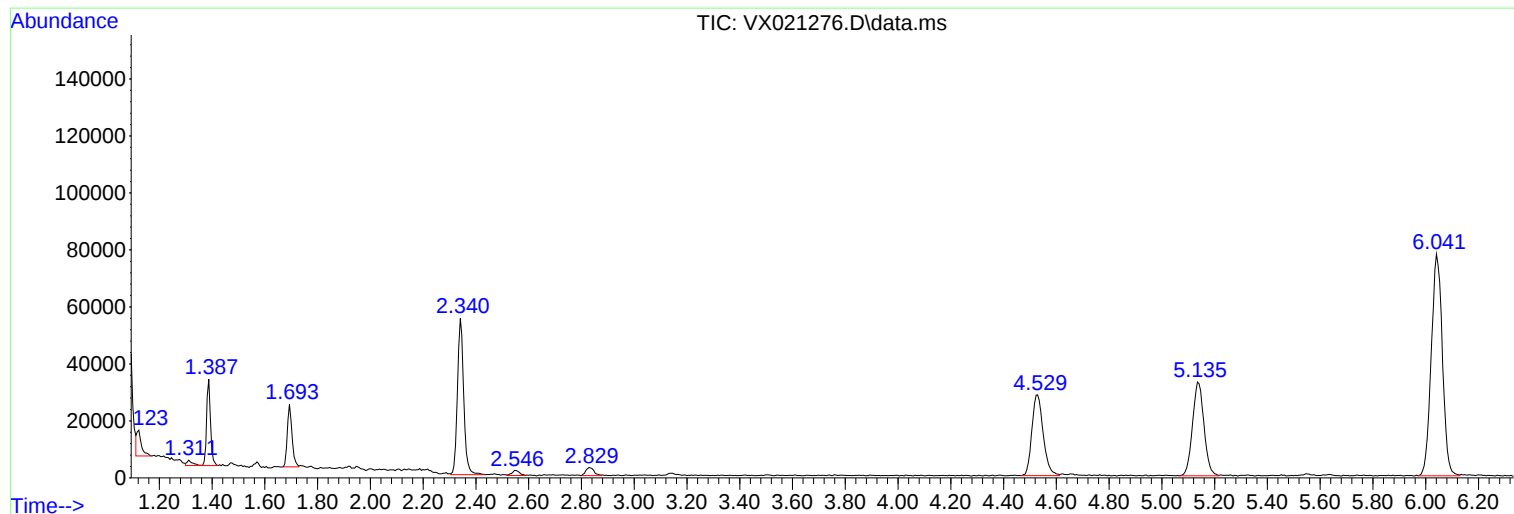

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031821\
Data File : VX021276.D
Acq On : 18 Mar 2021 11:51
Operator : JC/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031821\
Data File : VX021276.D
Acq On : 18 Mar 2021 11:51
Operator : JC/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
