

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
 Data File : VX027524.D
 Acq On : 18 Mar 2022 13:44
 Operator : JC/MD
 Sample : N1997-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 19 03:06:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	339356	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	564426	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	530909	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	280834	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	205753	49.217	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.440%
35) Dibromofluoromethane	5.385	113	182018	50.123	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.240%
50) Toluene-d8	8.653	98	663824	48.307	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.620%
62) 4-Bromofluorobenzene	11.085	95	265884	52.642	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	105.280%

Target Compounds			Qvalue			
5) Bromomethane	1.593	94	667	Below Cal		99
10) Methyl Iodide	2.447	142	2566	0.590 ug/l #		91
11) Tert butyl alcohol	2.989	59	1871	2.348 ug/l #		72
16) Acetone	2.392	43	2261	1.327 ug/l		100
19) Methyl tert-butyl Ether	3.123	73	8101	0.762 ug/l		94
20) Methylene Chloride	2.782	84	1456	0.397 ug/l #		76
29) Tetrahydrofuran	5.032	42	734	0.446 ug/l #		47
31) Cyclohexane	5.471	56	5261	1.013 ug/l #		76
36) 1,1-Dichloropropene	5.550	75	23957	4.828 ug/l #		51
38) Carbon Tetrachloride	5.550	117	33964	5.982 ug/l #		16
39) Methylcyclohexane	7.379	83	7623	1.222 ug/l		96
40) Benzene	6.038	78	34245	2.405 ug/l		92
42) 1,2-Dichloroethane	6.105	62	1221	0.229 ug/l		93
48) Methyl methacrylate	7.665	41	806	0.205 ug/l #		69
52) Toluene	8.720	92	83142	8.715 ug/l		100
55) 1,1,2-Trichloroethane	9.104	97	1172	0.302 ug/l #		24
58) 2-Chloroethyl Vinyl ether	8.257	63	30	Below Cal #		45
59) 2-Hexanone	9.446	43	1281	0.327 ug/l #		55
67) Ethyl Benzene	10.195	91	465811	24.918 ug/l		99
68) m/p-Xylenes	10.305	106	382422	51.956 ug/l		99
69) o-Xylene	10.647	106	104254	14.588 ug/l		99
70) Styrene	10.647	104	5594	0.479 ug/l #		1
73) Isopropylbenzene	10.964	105	10899	0.533 ug/l		99
76) 1,2,3-Trichloropropane	11.079	75	129280	22.009 ug/l #		38
78) n-propylbenzene	11.305	91	46896	2.088 ug/l		98
79) 2-Chlorotoluene	11.378	91	28079	1.993 ug/l #		42
80) 1,3,5-Trimethylbenzene	11.451	105	163174	9.478 ug/l		98
81) trans-1,4-Dichloro-2-b...	11.079	75	129280	66.840 ug/l #		15
82) 4-Chlorotoluene	11.451	91	17794	1.110 ug/l #		48
83) tert-Butylbenzene	11.713	119	8464	0.496 ug/l		86
84) 1,2,4-Trimethylbenzene	11.756	105	314656	18.327 ug/l		99
85) sec-Butylbenzene	11.756	105	314656	15.267 ug/l #		56
89) n-Butylbenzene	12.323	91	11912	0.806 ug/l #		9
90) Hexachloroethane	12.530	117	2130	0.754 ug/l #		10
92) 1,2-Dibromo-3-Chloropr...	12.969	75	338	0.227 ug/l #		1
95) Naphthalene	13.780	128	93713	4.815 ug/l		99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
Data File : VX027524.D
Acq On : 18 Mar 2022 13:44
Operator : JC/MD
Sample : N1997-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Mar 19 03:06:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Mar 19 03:06:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration





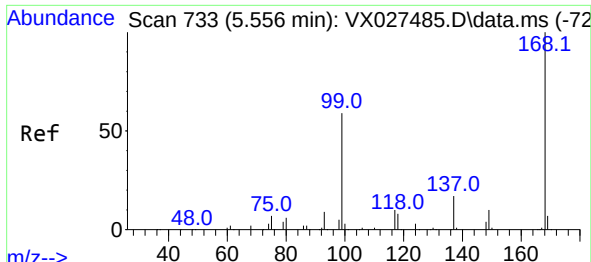


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :



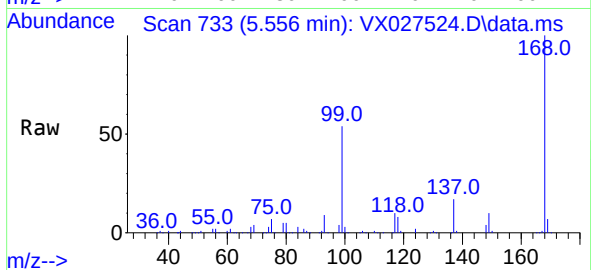



Tgt Ion:168 Resp: 339356
Ion Ratio Lower Upper
168 100
99 54.3 41.7 62.5

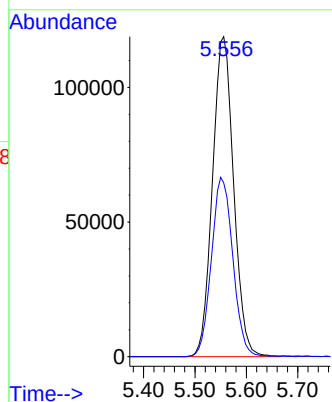

#5
Bromomethane
Concen: Below Cal
RT: 1.593 min Scan# 83
Delta R.T. -0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44


Tgt Ion: 94 Resp: 667
Ion Ratio Lower Upper
94 100
96 95.1 75.3 112.9

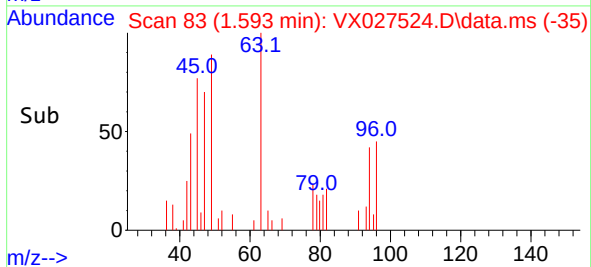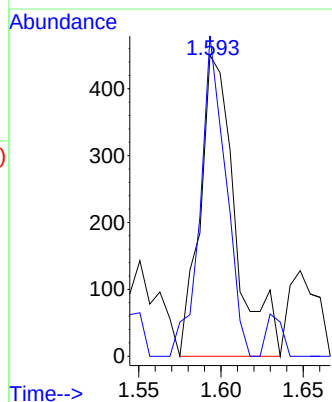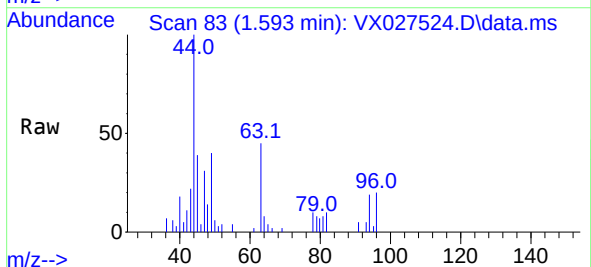






#10
Methyl Iodide
Concen: 0.590 ug/l
RT: 2.447 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44


Instrument :
MSVOA_X
ClientSampleId :

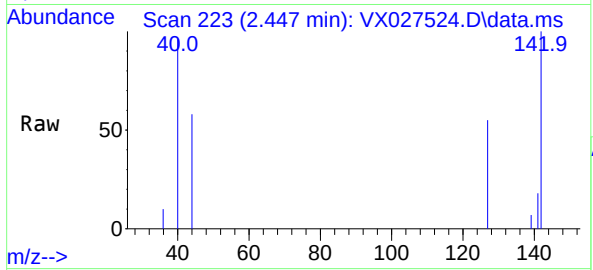



Tgt Ion:142 Resp: 2566
Ion Ratio Lower Upper
142 100
127 36.7 33.9 50.9
141 10.0 11.4 17.2#

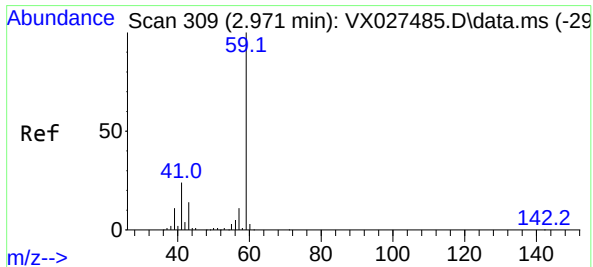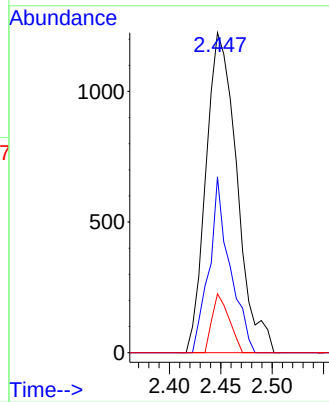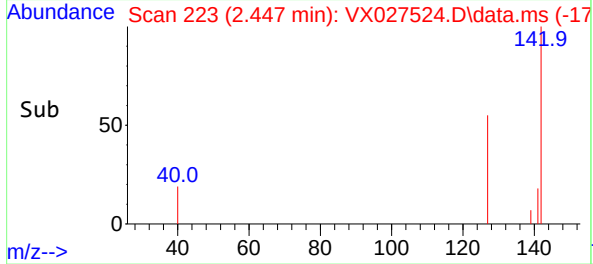


#11
Tert butyl alcohol
Concen: 2.348 ug/l
RT: 2.989 min Scan# 312
Delta R.T. 0.019 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

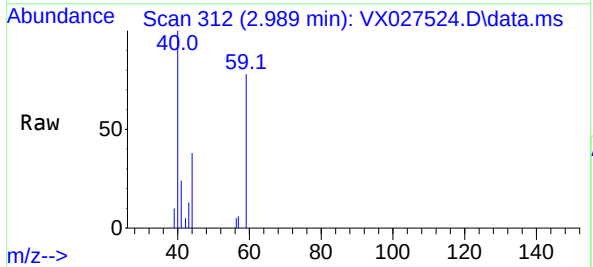

Tgt Ion: 59 Resp: 1871
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



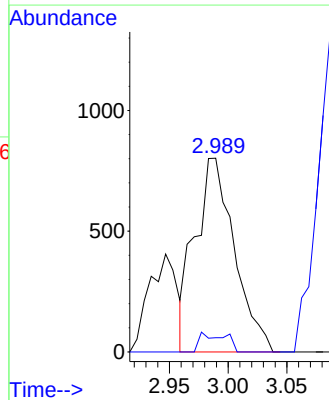
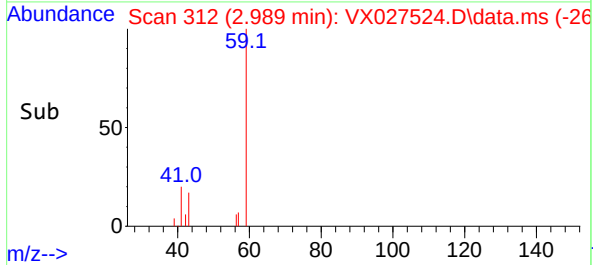




#16
Acetone
Concen: 1.327 ug/l
RT: 2.392 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2261
Ion Ratio Lower Upper
43 100
58 35.9 28.8 43.2

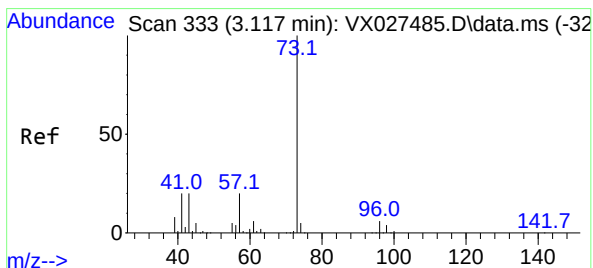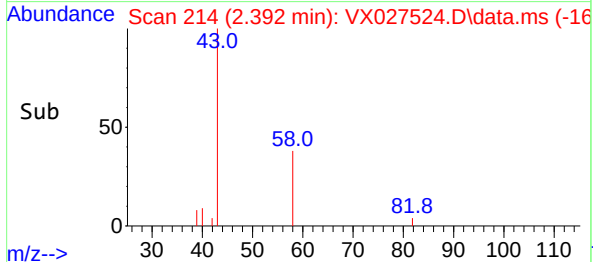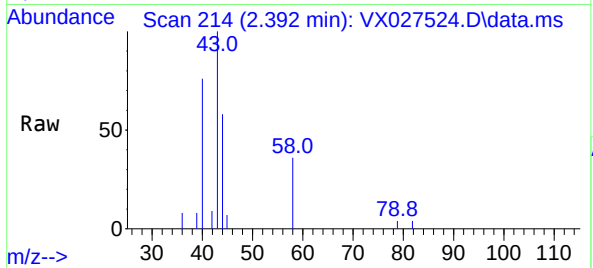

#19
Methyl tert-butyl Ether
Concen: 0.762 ug/l
RT: 3.123 min Scan# 334
Delta R.T. 0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44


Tgt Ion: 73 Resp: 8101
Ion Ratio Lower Upper
73 100
57 23.7 16.8 25.2

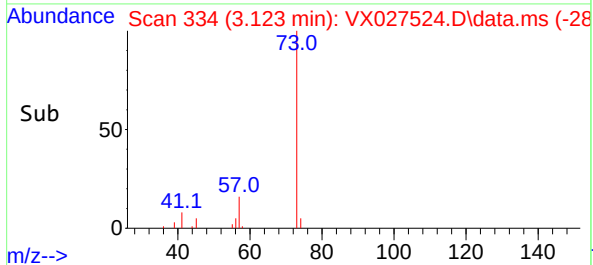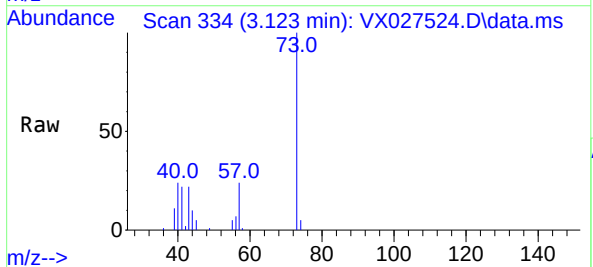






#20
Methylene Chloride
Concen: 0.397 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :

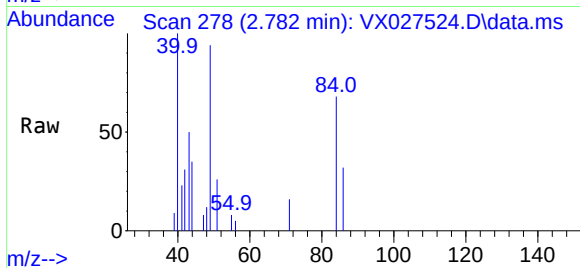

Tgt Ion: 84 Resp: 1456




Ion	Ratio	Lower	Upper
84	100		
49	138.1	85.5	128.3#
51	37.7	26.6	39.8
86	47.8	51.5	77.3#

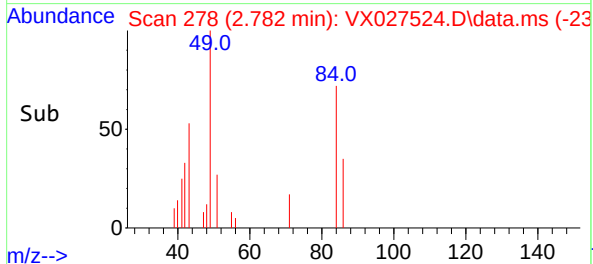


#29
Tetrahydrofuran
Concen: 0.446 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.025 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 42 Resp: 734


Ion	Ratio	Lower	Upper
42	100		
72	20.2	44.1	66.1#
71	10.9	40.5	60.7#

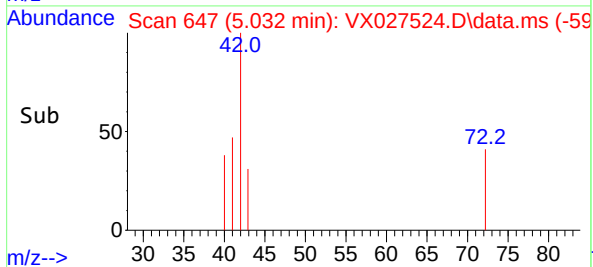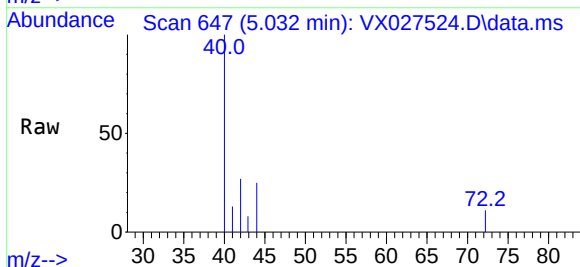






#31
Cyclohexane
Concen: 1.013 ug/l
RT: 5.471 min Scan# 719
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 5261
Ion Ratio Lower Upper
56 100
69 16.2 26.7 40.1#
84 74.8 77.2 115.8#



#33
1,2-Dichloroethane-d4
Concen: 49.217 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 65 Resp: 205753
Ion Ratio Lower Upper
65 100
67 52.6 0.0 107.4


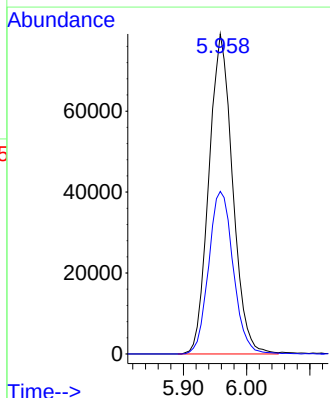




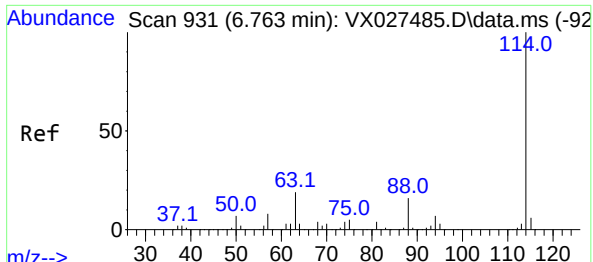

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 564426
Ion Ratio Lower Upper
114 100
63 18.9 0.0 36.8
88 15.9 0.0 32.4

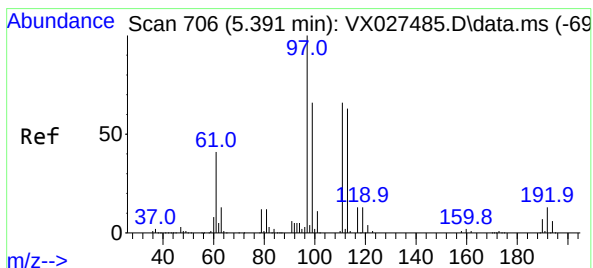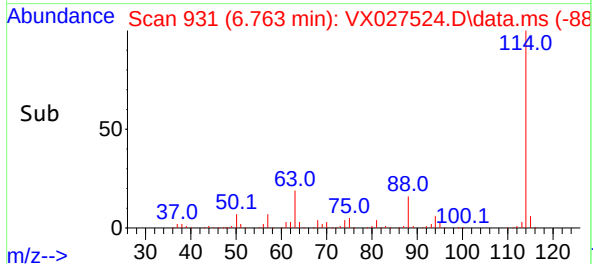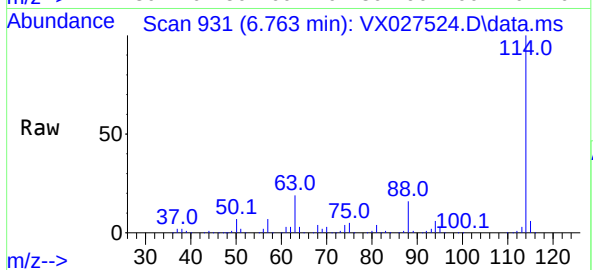

#35
Dibromofluoromethane
Concen: 50.123 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44


Tgt Ion:113 Resp: 182018
Ion Ratio Lower Upper
113 100
111 102.3 82.8 124.2
192 20.2 16.9 25.3

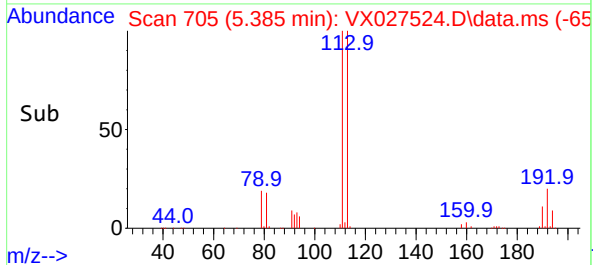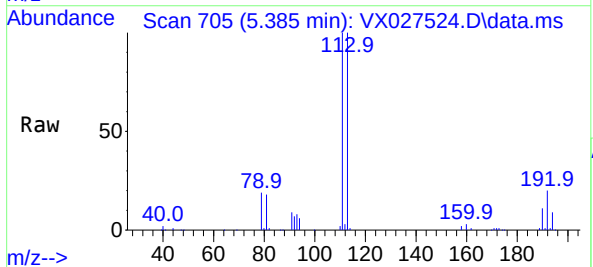






#36
1,1-Dichloropropene
Concen: 4.828 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 23957
Ion Ratio Lower Upper
75 100
110 10.7 18.3 54.8#
77 0.0 24.8 37.2#

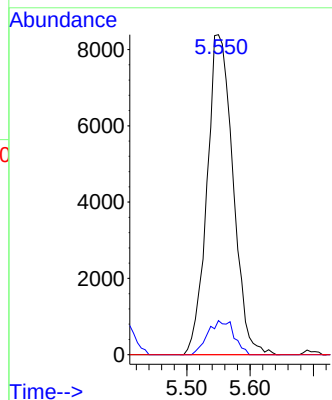

#38
Carbon Tetrachloride
Concen: 5.982 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 117 Resp: 33964
Ion Ratio Lower Upper
117 100
119 5.4 77.3 115.9#
121 0.0 24.2 36.2#

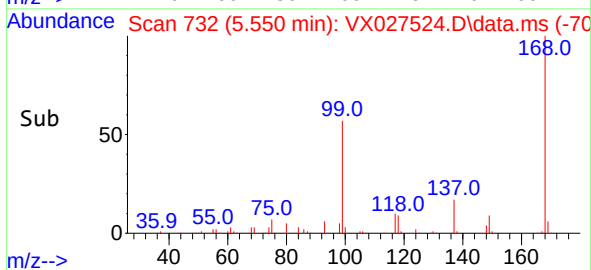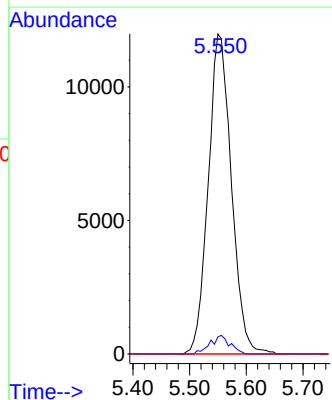



#39

Methylcyclohexane

Concen: 1.222 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX027524.D

Acq: 18 Mar 2022 13:44

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 7623

Ion Ratio Lower Upper

83 100

55 71.3 54.6 81.8

98 49.1 37.4 56.2

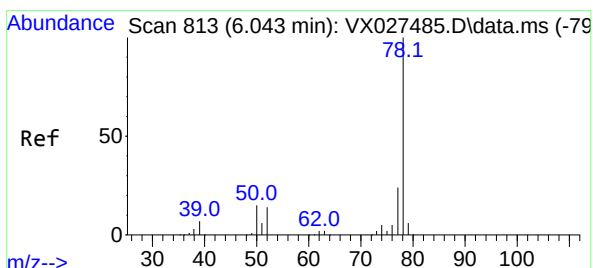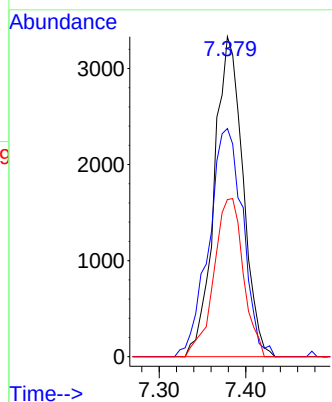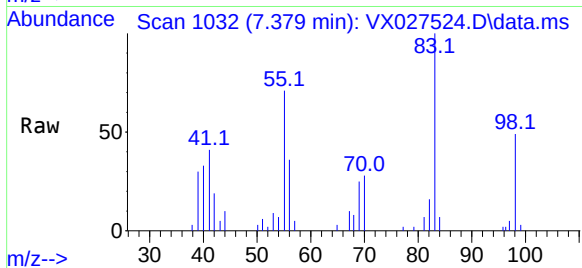

#40

Benzene

Concen: 2.405 ug/l

RT: 6.038 min Scan# 812

Delta R.T. -0.006 min

Lab File: VX027524.D




Acq: 18 Mar 2022 13:44


Tgt Ion: 78 Resp: 34245

Ion Ratio Lower Upper

78 100

77 20.0 19.3 28.9

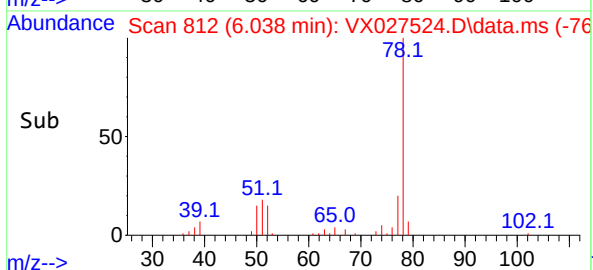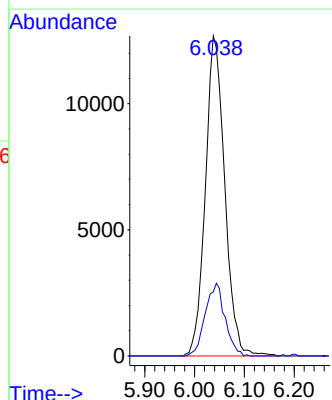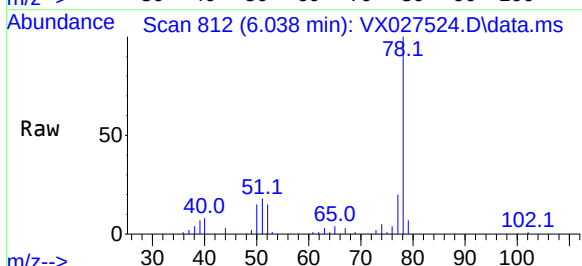



#42

1,2-Dichloroethane

Concen: 0.229 ug/l

RT: 6.105 min Scan# 81

Delta R.T. 0.012 min

Lab File: VX027524.D

Acq: 18 Mar 2022 13:44

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 1221

Ion Ratio Lower Upper

62 100

98 7.5 0.0 20.4

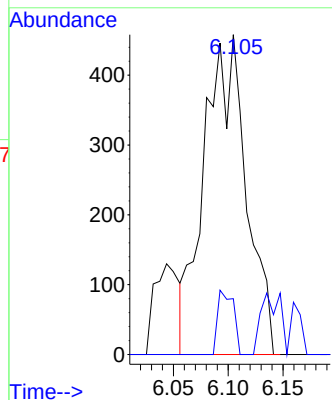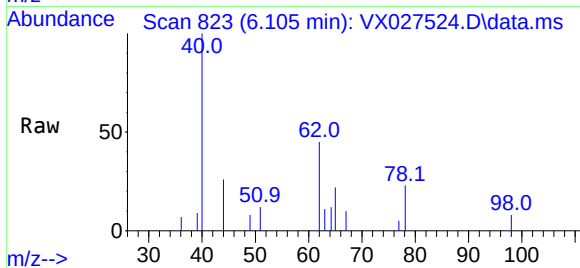

#48

Methyl methacrylate

Concen: 0.205 ug/l

RT: 7.665 min Scan# 1079

Delta R.T. -0.030 min

Lab File: VX027524.D

Acq: 18 Mar 2022 13:44




Tgt Ion: 41 Resp: 806


Ion Ratio Lower Upper

41 100

69 143.8 82.5 123.7#

39 65.8 43.8 65.8



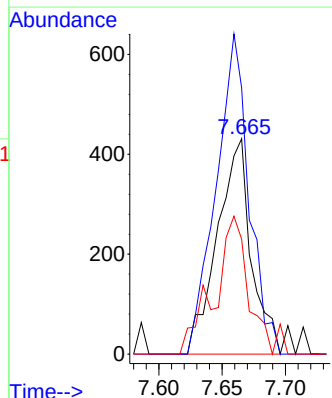
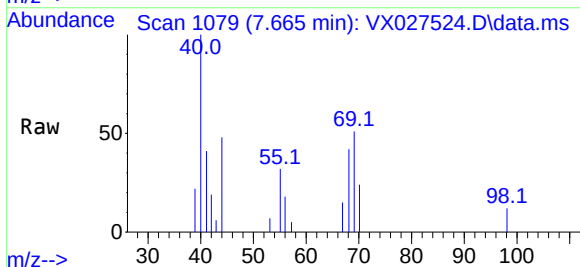




#50
Toluene-d8
Concen: 48.307 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 663824
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8

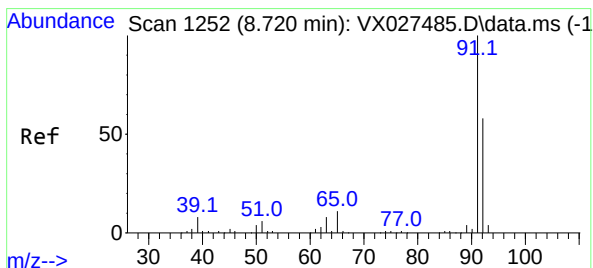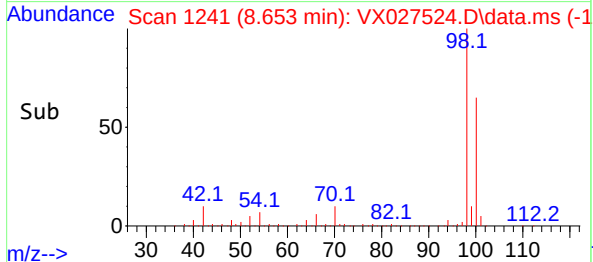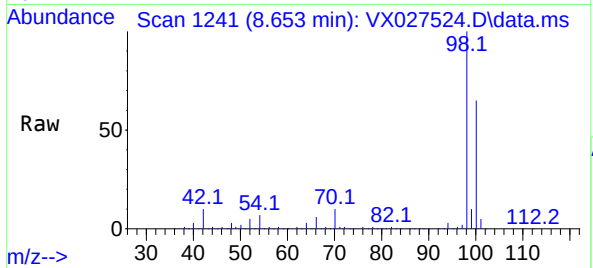

#52
Toluene
Concen: 8.715 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 92 Resp: 83142
Ion Ratio Lower Upper
92 100
91 172.4 137.5 206.3

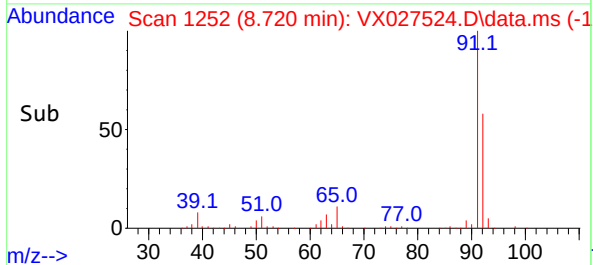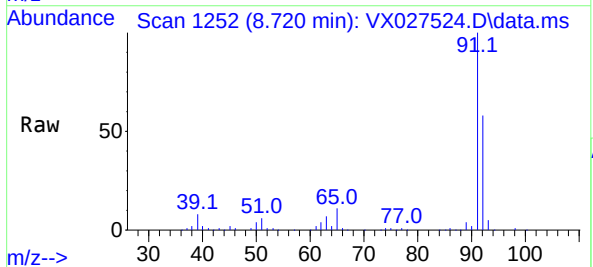







#55
1,1,2-Trichloroethane
Concen: 0.302 ug/l
RT: 9.104 min Scan# 1172
Delta R.T. -0.049 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 97 Resp: 1172




Ion	Ratio	Lower	Upper
97	100		
83	7.6	66.2	99.4#
85	10.6	42.9	64.3#
99	0.0	49.0	73.6#

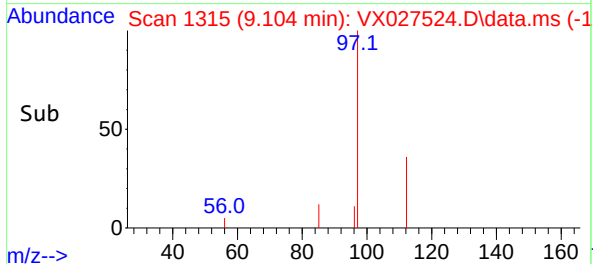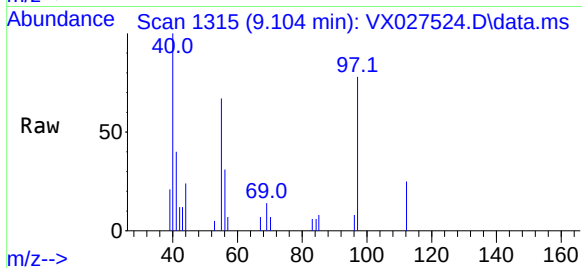


#58
2-Chloroethyl Vinyl ether
Concen: Below Cal
RT: 8.257 min Scan# 1176
Delta R.T. 0.013 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 63 Resp: 30

Ion	Ratio	Lower	Upper
63	100		
106	0.0	23.9	35.9#


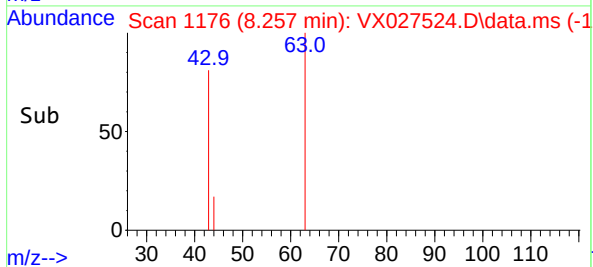

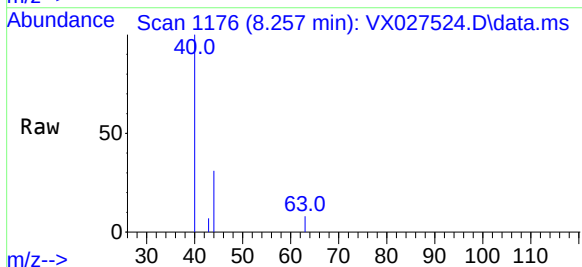




#59
2-Hexanone
Concen: 0.327 ug/l
RT: 9.446 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1281
Ion Ratio Lower Upper
43 100
58 29.0 31.9 95.7#

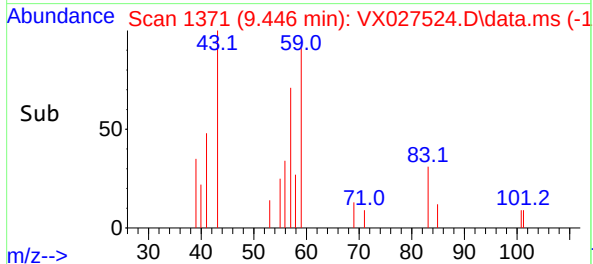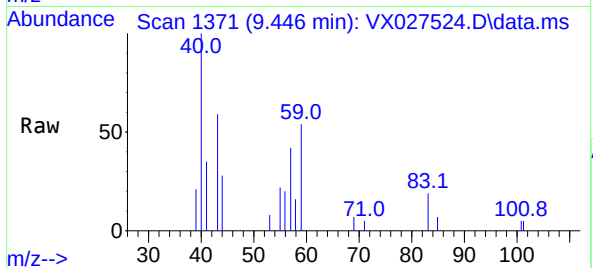

#62
4-Bromofluorobenzene
Concen: 52.642 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 95 Resp: 265884
Ion Ratio Lower Upper
95 100
174 81.2 0.0 163.0
176 79.0 0.0 155.0


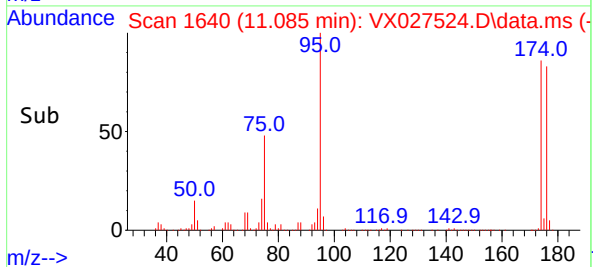

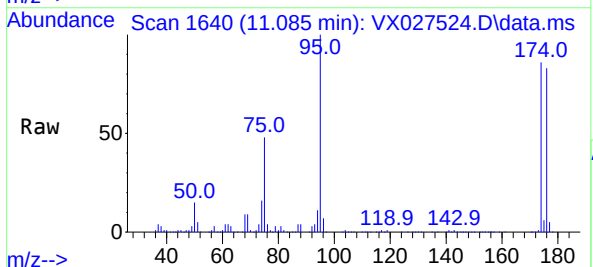




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 530909
Ion Ratio Lower Upper
117 100
82 55.0 41.8 62.8
119 32.0 24.8 37.2

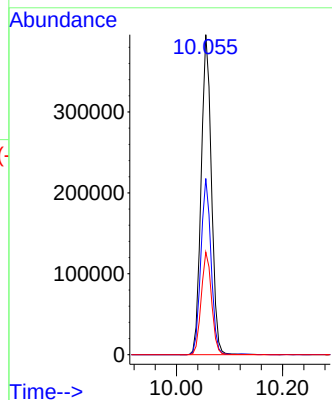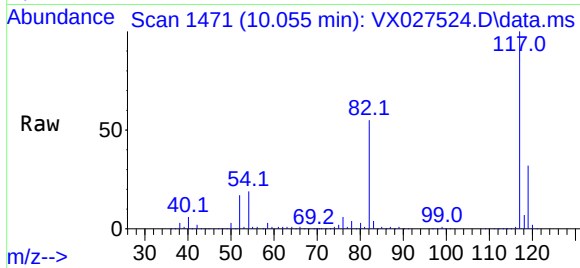

#67
Ethyl Benzene
Concen: 24.918 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 91 Resp: 465811
Ion Ratio Lower Upper
91 100
106 31.2 24.6 36.8



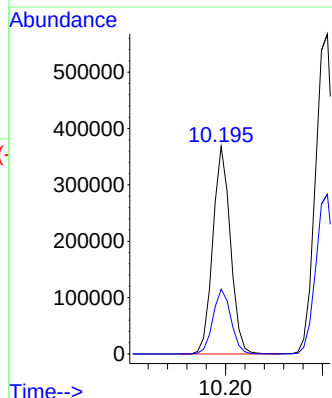
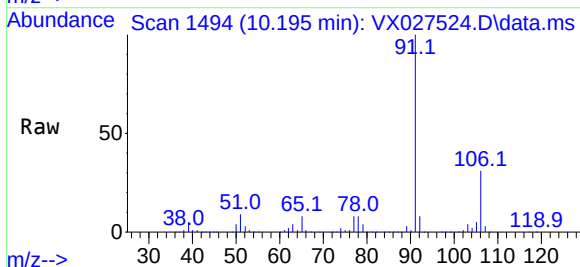




#68
m/p-Xylenes
Concen: 51.956 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 382422
Ion Ratio Lower Upper
106 100
91 202.0 160.4 240.6

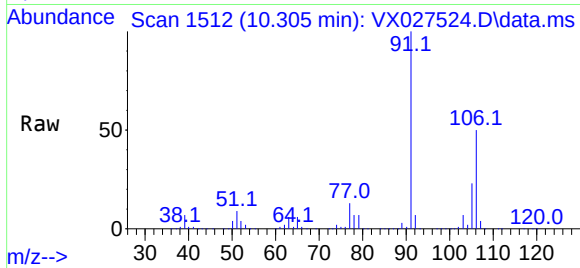

#69
o-Xylene
Concen: 14.588 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion:106 Resp: 104254
Ion Ratio Lower Upper
106 100
91 211.2 106.1 318.1


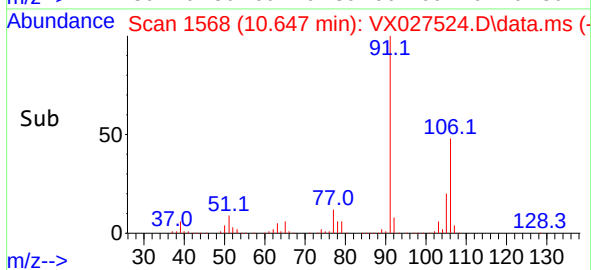

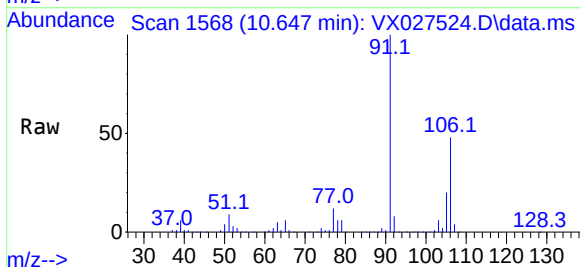




#70
Styrene
Concen: 0.479 ug/l
RT: 10.647 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 5594
Ion Ratio Lower Upper
104 100
78 263.7 38.6 57.8#
103 256.3 43.8 65.8#

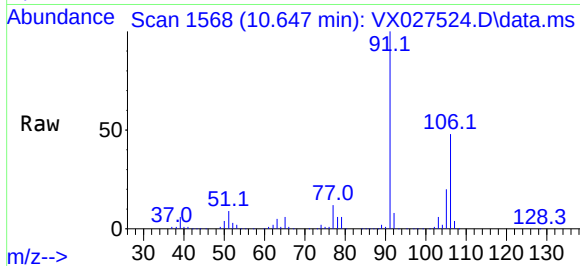

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion:152 Resp: 280834
Ion Ratio Lower Upper
152 100
115 59.9 37.5 112.7
150 157.4 0.0 338.2



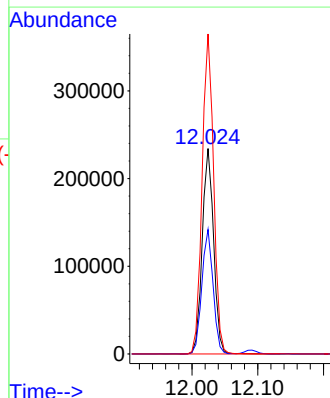
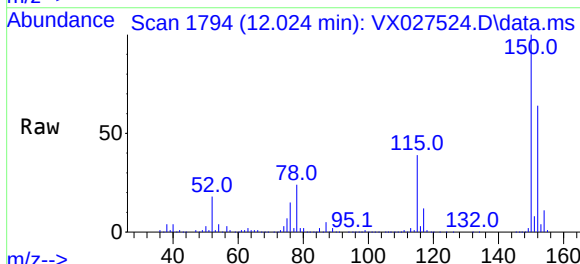




#73
Isopropylbenzene
Concen: 0.533 ug/l
RT: 10.964 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 10899
Ion Ratio Lower Upper
105 100
120 27.4 13.5 40.5

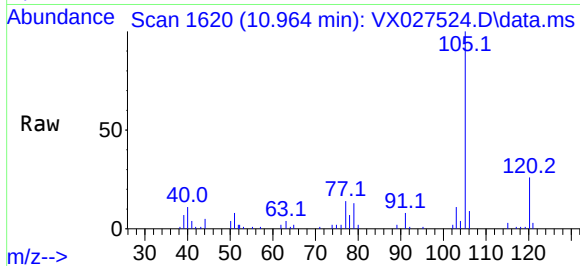

#76
1,2,3-Trichloropropane
Concen: 22.009 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.164 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 75 Resp: 129280
Ion Ratio Lower Upper
75 100
77 1.2 19.4 58.2#


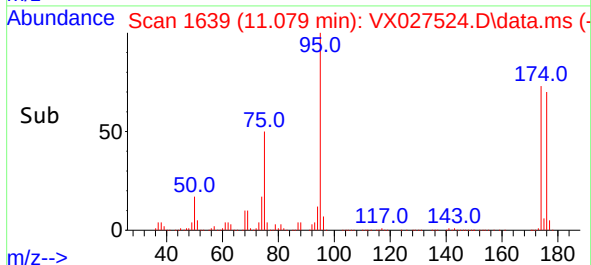

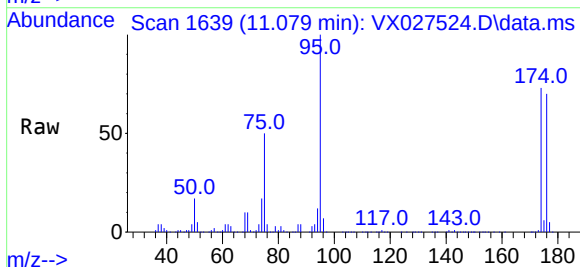




#78
n-propylbenzene
Concen: 2.088 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 46896
Ion Ratio Lower Upper
91 100
120 24.1 11.6 34.8

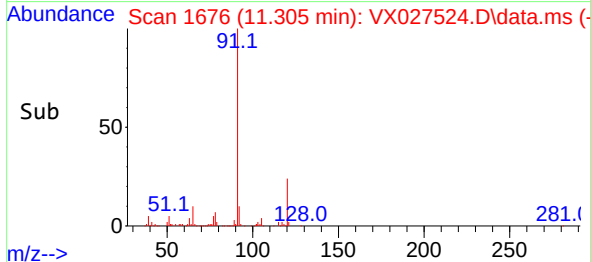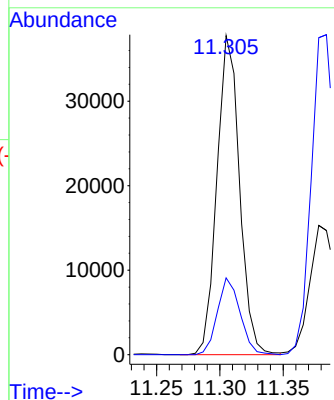

#79
2-Chlorotoluene
Concen: 1.993 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 91 Resp: 28079
Ion Ratio Lower Upper
91 100
126 0.9 17.3 51.9#


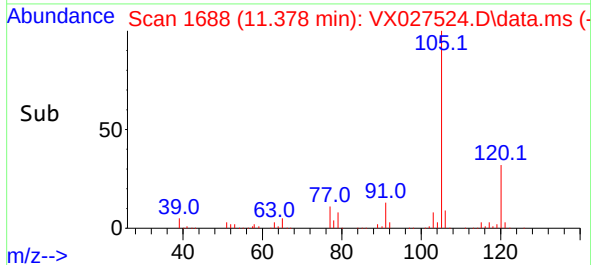
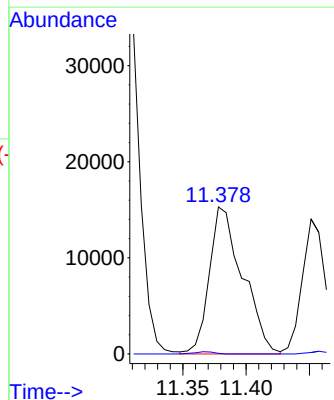
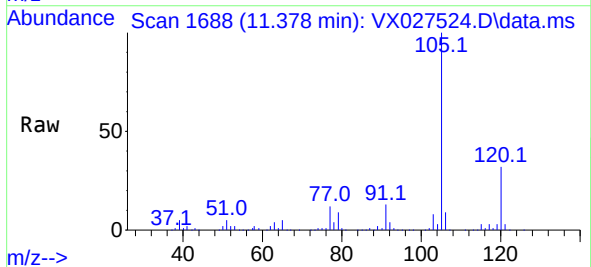




#80
1,3,5-Trimethylbenzene
Concen: 9.478 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 163174
Ion Ratio Lower Upper
105 100
120 47.5 24.3 72.9

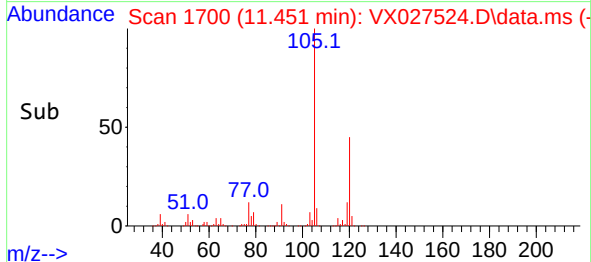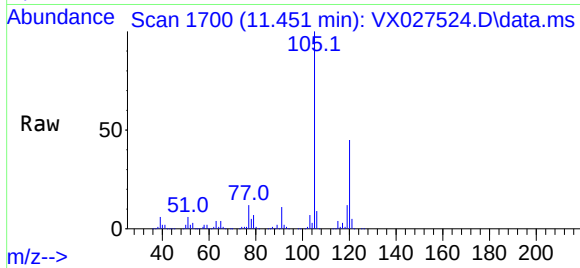

#81
trans-1,4-Dichloro-2-butene
Concen: 66.840 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 75 Resp: 129280
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#


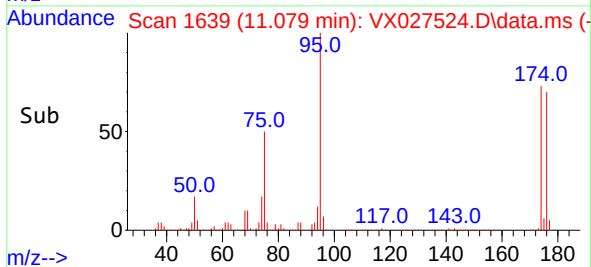

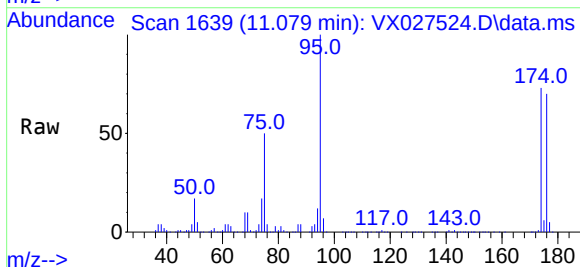




#82
4-Chlorotoluene
Concen: 1.110 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 17794
Ion Ratio Lower Upper
91 100
126 1.7 14.9 44.5#

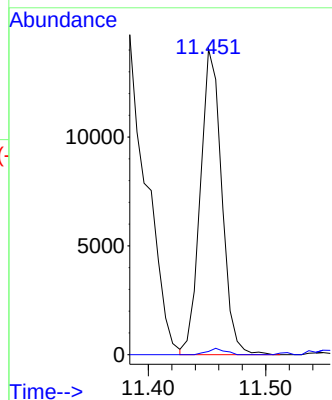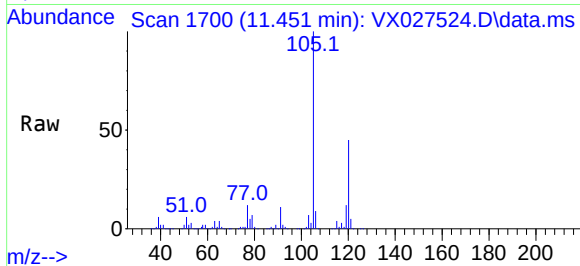

#83
tert-Butylbenzene
Concen: 0.496 ug/l
RT: 11.713 min Scan# 1743
Delta R.T. -0.006 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 119 Resp: 8464
Ion Ratio Lower Upper
119 100
91 66.5 26.9 80.6
134 24.7 11.4 34.2



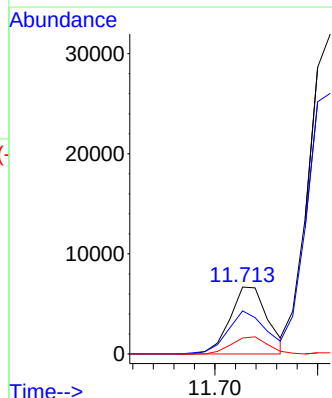
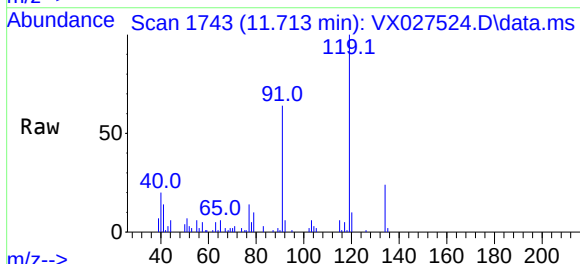




#84
1,2,4-Trimethylbenzene
Concen: 18.327 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 314656
Ion Ratio Lower Upper
105 100
120 45.6 22.6 67.8

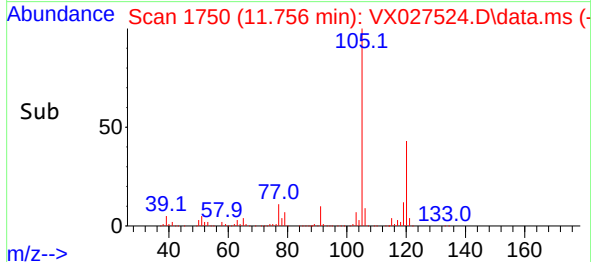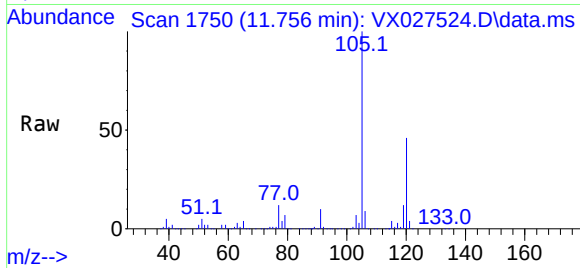

#85
sec-Butylbenzene
Concen: 15.267 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion:105 Resp: 314656
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#


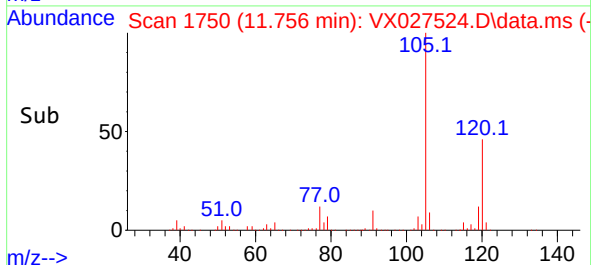

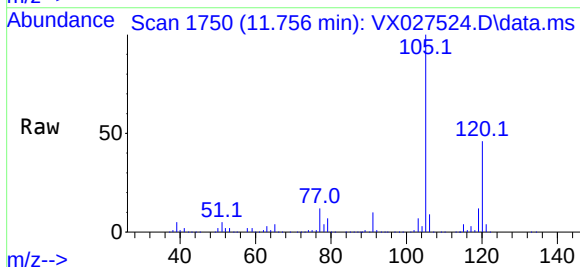




#89
n-Butylbenzene
Concen: 0.806 ug/l
RT: 12.323 min Scan# 11912
Delta R.T. -0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 11912
Ion Ratio Lower Upper
91 100
92 23.3 27.8 83.3#
134 123.8 13.3 39.8#

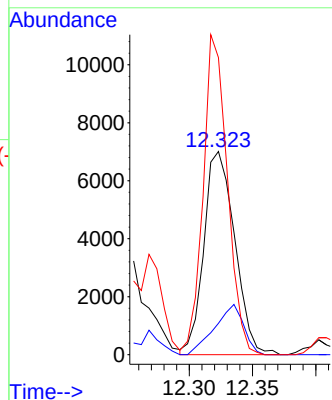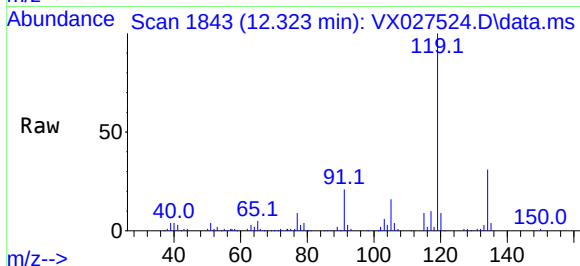

#90
Hexachloroethane
Concen: 0.754 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion: 117 Resp: 2130
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#


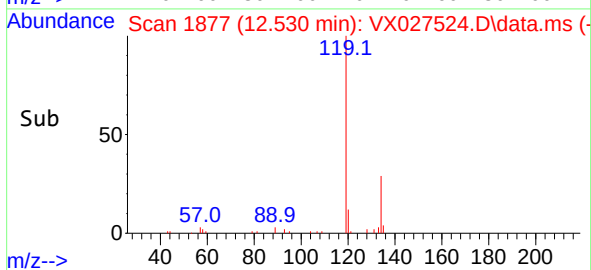
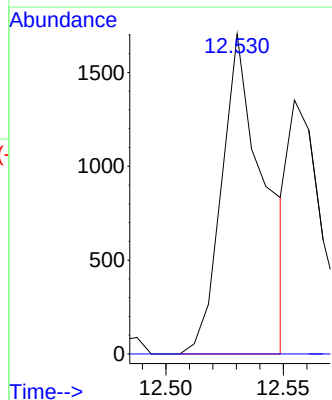
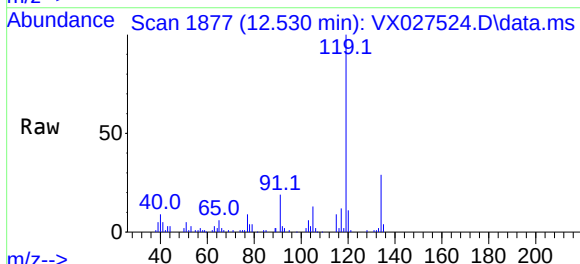




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.227 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.025 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 338
Ion Ratio Lower Upper
75 100
155 0.0 47.0 141.2#
157 0.0 57.9 173.6#

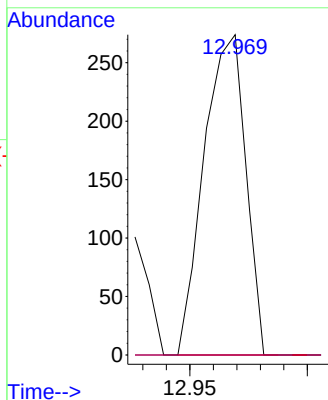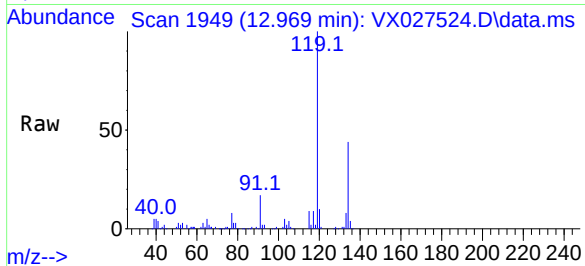

#95
Naphthalene
Concen: 4.815 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX027524.D
Acq: 18 Mar 2022 13:44

Tgt Ion:128 Resp: 93713
Ion Ratio Lower Upper
128 100
127 12.4 10.2 15.4
129 10.9 8.7 13.1

