

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
 Data File : VX027519.D
 Acq On : 18 Mar 2022 11:09
 Operator : JC/MD
 Sample : VX0318WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0318WBL01

Quant Time: Mar 19 03:05:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	329264	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	547008	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	498531	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	236335	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	208962	51.517	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	103.040%
35) Dibromofluoromethane	5.391	113	182277	51.793	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	103.580%
50) Toluene-d8	8.653	98	644044	48.360	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.720%
62) 4-Bromofluorobenzene	11.085	95	233408	47.683	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	95.360%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
Data File : VX027519.D
Acq On : 18 Mar 2022 11:09
Operator : JC/MD
Sample : VX0318WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0318WBL01

Quant Time: Mar 19 03:05:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration




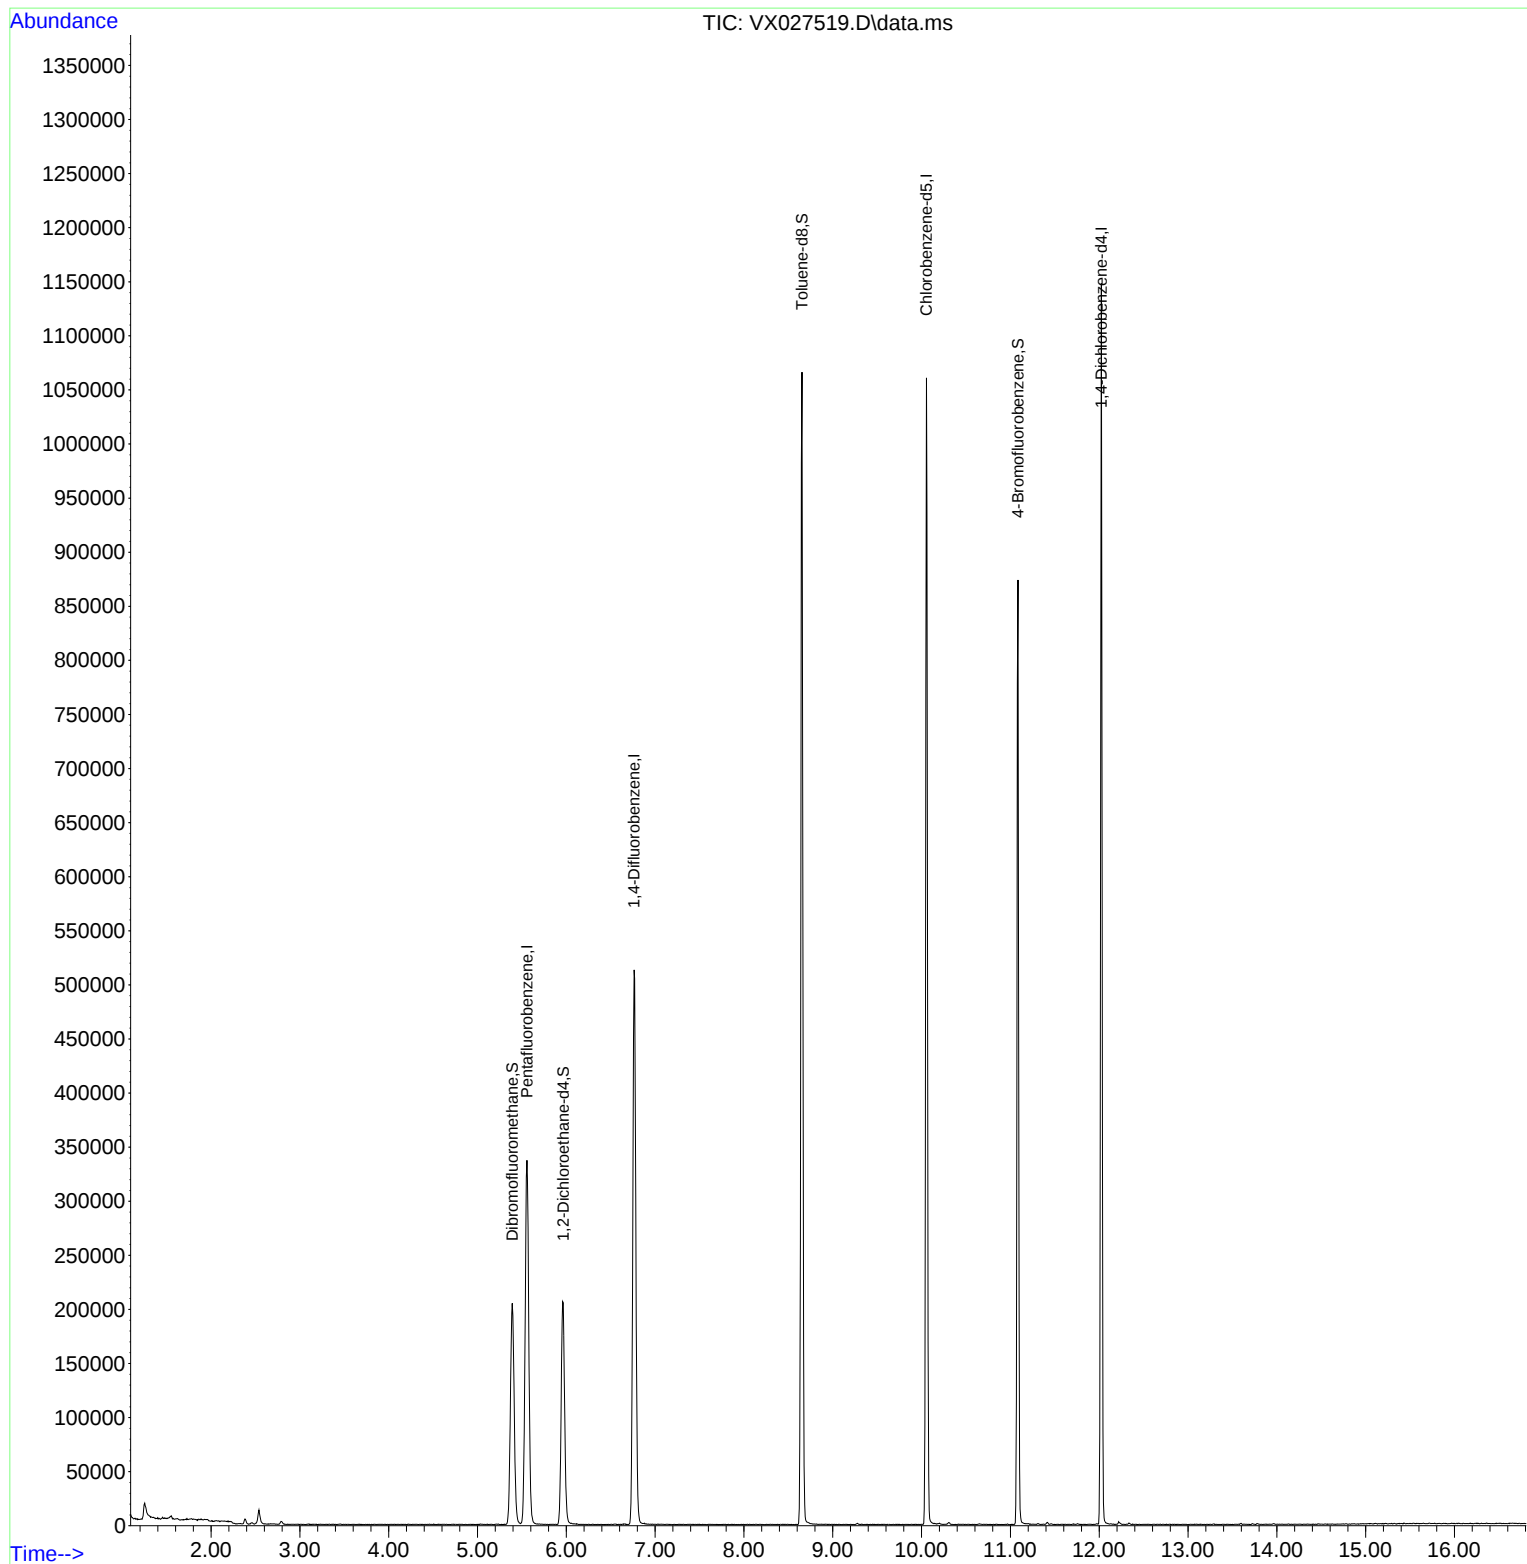




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0318WBL01


Tgt Ion:168 Resp: 329264
Ion Ratio Lower Upper
168 100
99 58.3 41.7 62.5

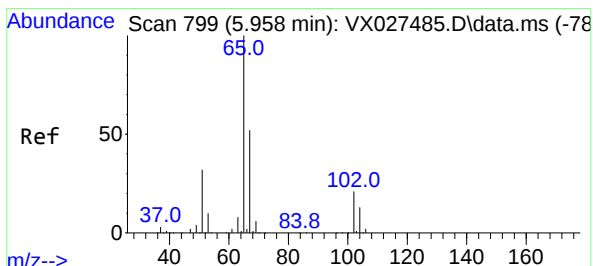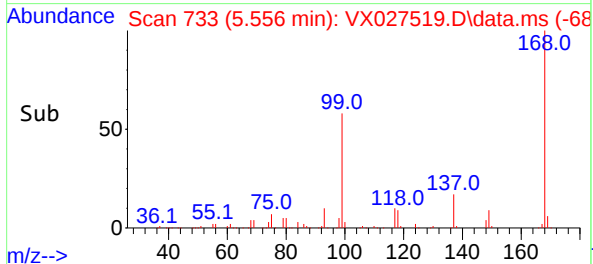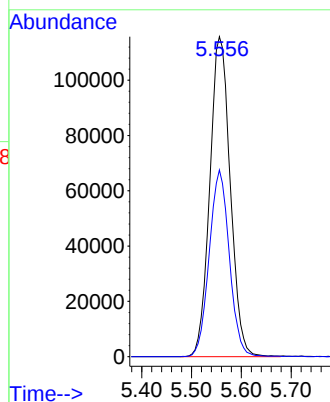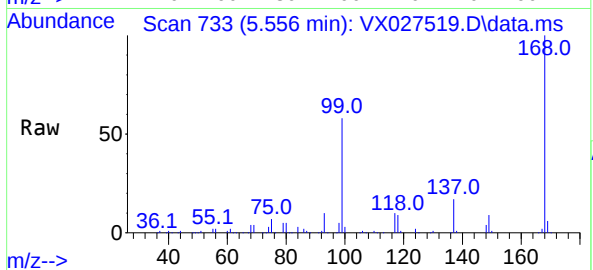

#33
1,2-Dichloroethane-d4
Concen: 51.517 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09

Tgt Ion: 65 Resp: 208962
Ion Ratio Lower Upper
65 100
67 51.6 0.0 107.4


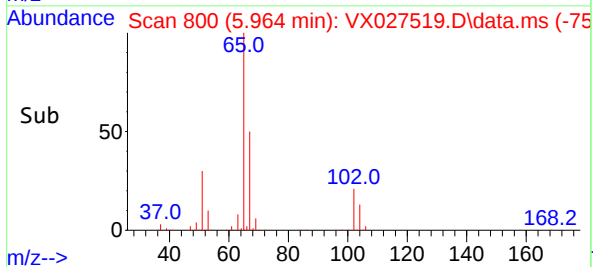
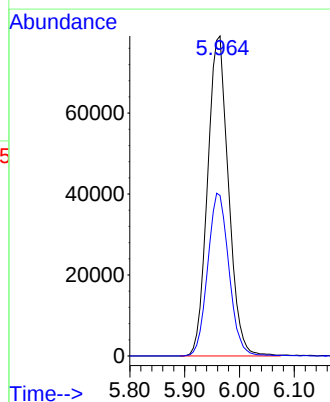
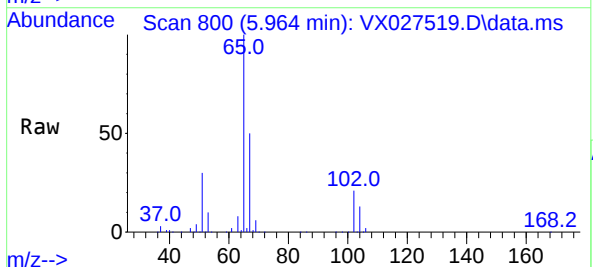


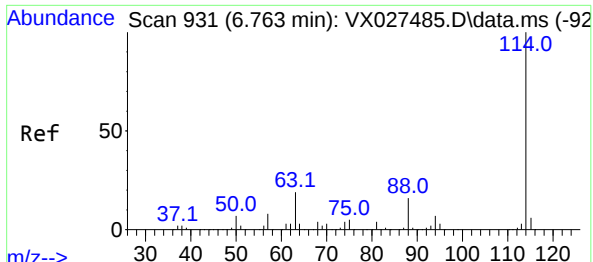

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0318WBL01


Tgt Ion:114 Resp: 547008
Ion Ratio Lower Upper
114 100
63 18.9 0.0 36.8
88 15.9 0.0 32.4

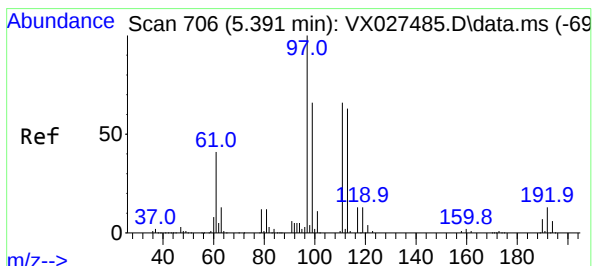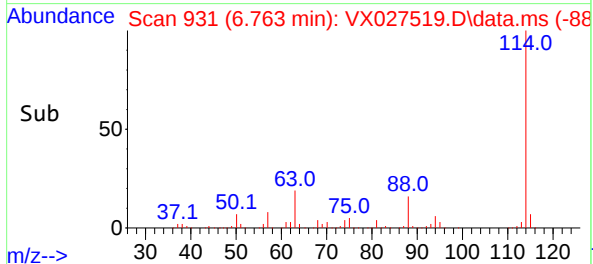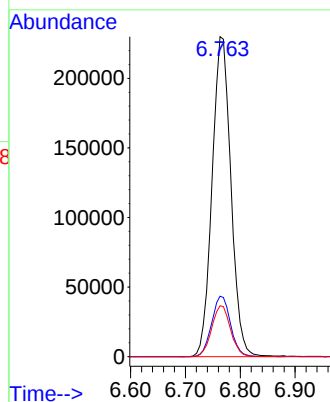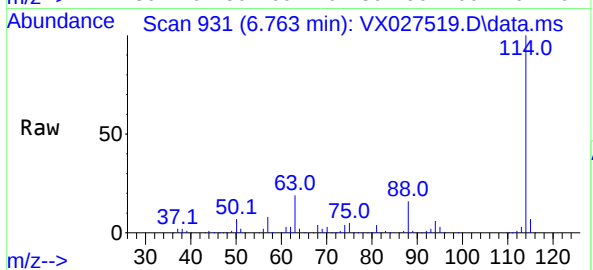

#35
Dibromofluoromethane
Concen: 51.793 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09

Tgt Ion:113 Resp: 182277
Ion Ratio Lower Upper
113 100
111 103.7 82.8 124.2
192 20.1 16.9 25.3


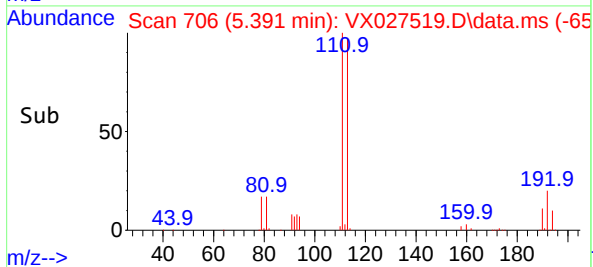
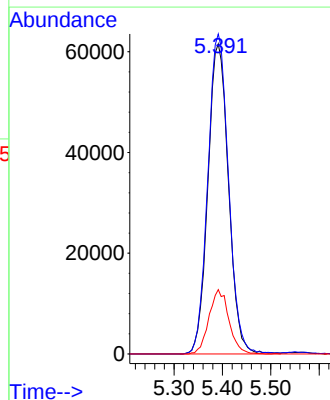
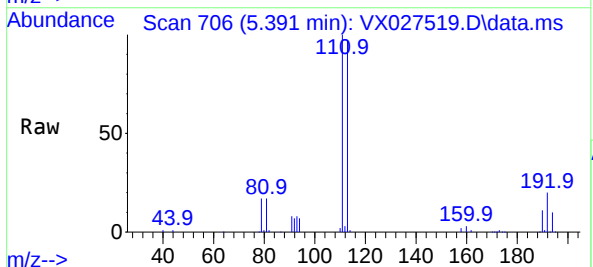


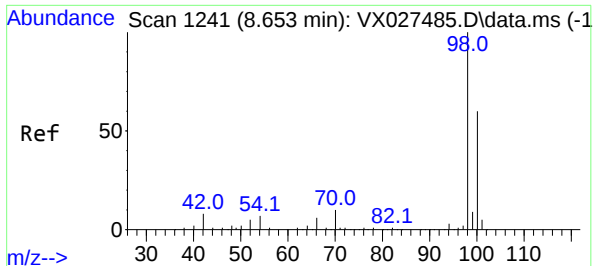

#50
Toluene-d8
Concen: 48.360 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09




Instrument :
MSVOA_X
ClientSampleId :
VX0318WBL01


Tgt Ion: 98 Resp: 644044
Ion Ratio Lower Upper
98 100
100 64.2 52.6 78.8

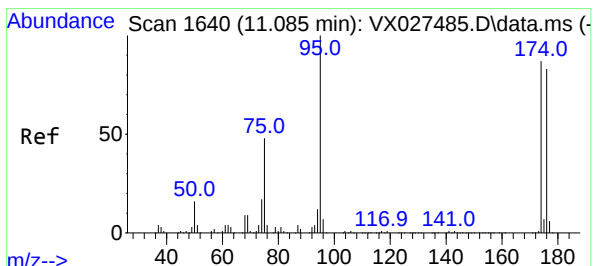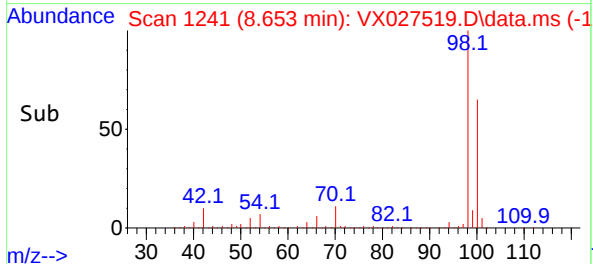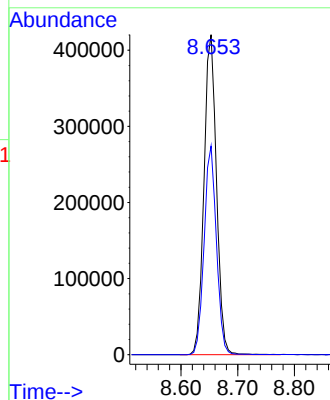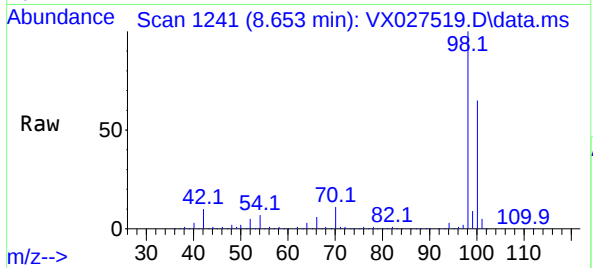

#62
4-Bromofluorobenzene
Concen: 47.683 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09

Tgt Ion: 95 Resp: 233408
Ion Ratio Lower Upper
95 100
174 82.0 0.0 163.0
176 79.9 0.0 155.0


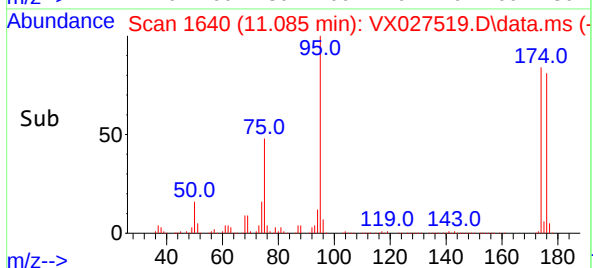
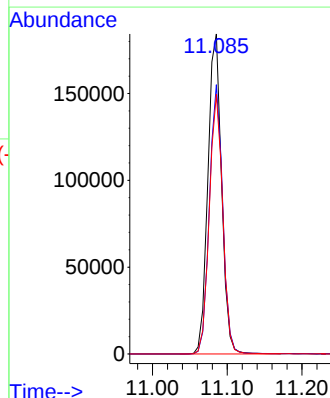
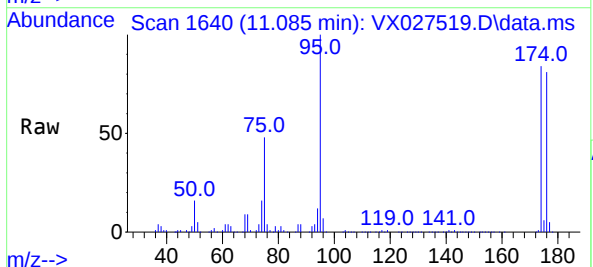


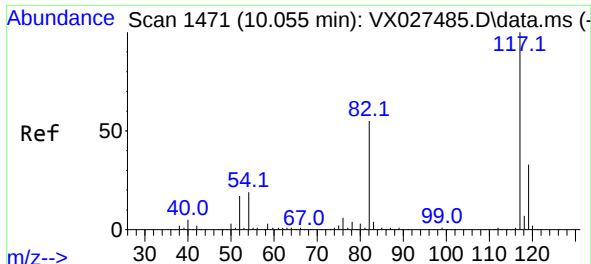

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09

Instrument :
MSVOA_X
ClientSampleId :
VX0318WBL01

Tgt Ion:117 Resp: 498531
Ion Ratio Lower Upper
117 100
82 55.7 41.8 62.8
119 32.6 24.8 37.2

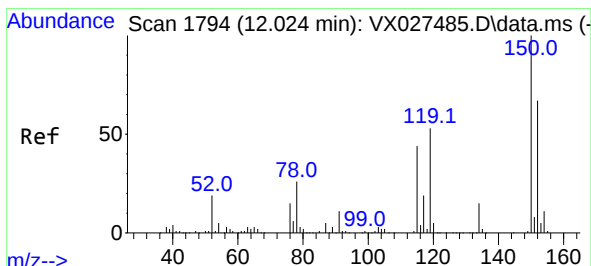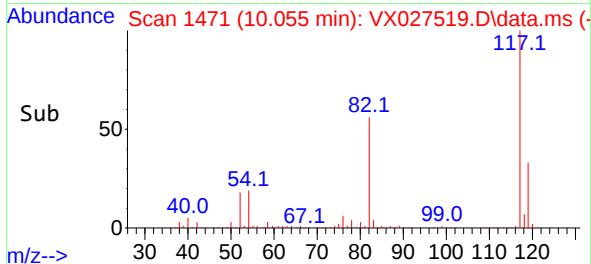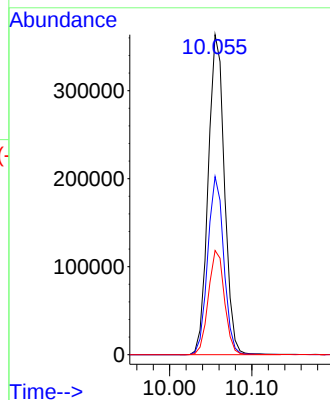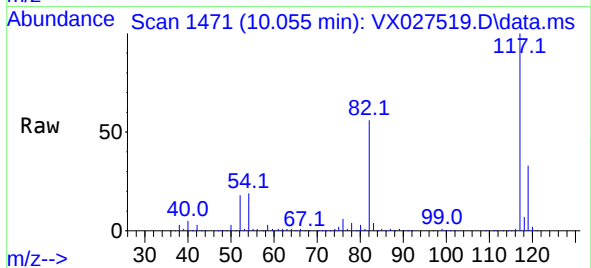

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027519.D
Acq: 18 Mar 2022 11:09

Tgt Ion:152 Resp: 236335
Ion Ratio Lower Upper
152 100
115 59.4 37.5 112.7
150 156.6 0.0 338.2

