

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
 Data File : VX027527.D
 Acq On : 18 Mar 2022 14:55
 Operator : JC/MD
 Sample : N2014-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DEWATERING-EFFLUENT-031722

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	20	27	38	rBV2	15530	39499	2.26%	0.405%
2	2.538	230	238	251	rBV	60111	113851	6.51%	1.166%
3	5.391	692	706	722	rBV3	212258	617945	35.32%	6.330%
4	5.556	722	733	749	rVB	354729	995591	56.91%	10.198%
5	5.958	789	799	814	rBV	203488	540288	30.88%	5.534%
6	6.763	921	931	946	rBV	538155	1277204	73.01%	13.082%
7	8.653	1234	1241	1258	rBV	1142930	1749400	100.00%	17.919%
8	10.055	1465	1471	1483	rBV	1185695	1571180	89.81%	16.094%
9	11.085	1634	1640	1652	rBV	958490	1232528	70.45%	12.625%
10	12.024	1788	1794	1804	rBV	1321359	1625233	92.90%	16.647%




Sum of corrected areas: 9762719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
Data File : VX027527.D
Acq On : 18 Mar 2022 14:55
Operator : JC/MD
Sample : N2014-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEWATERING-EFFLUENT-031722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

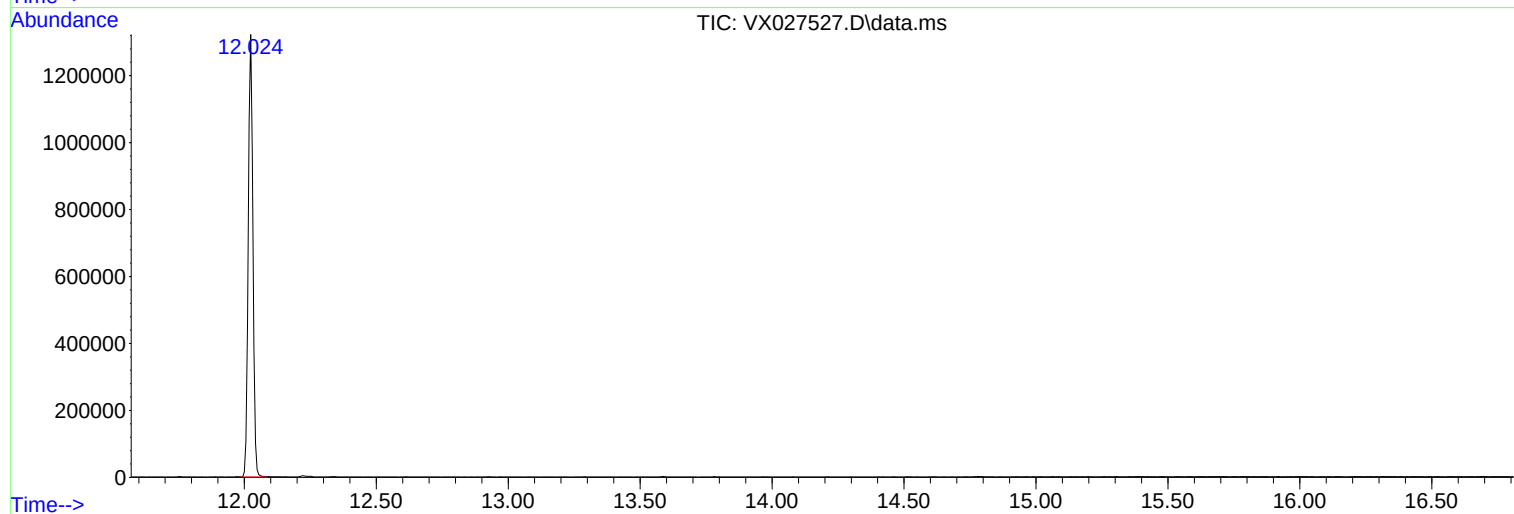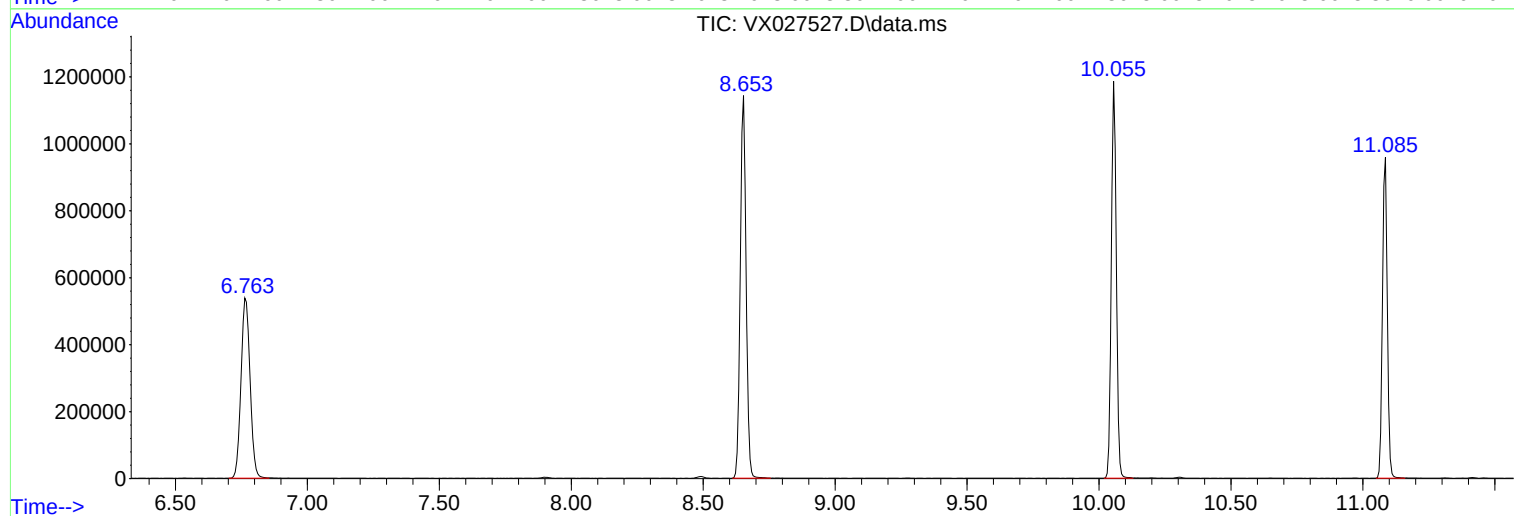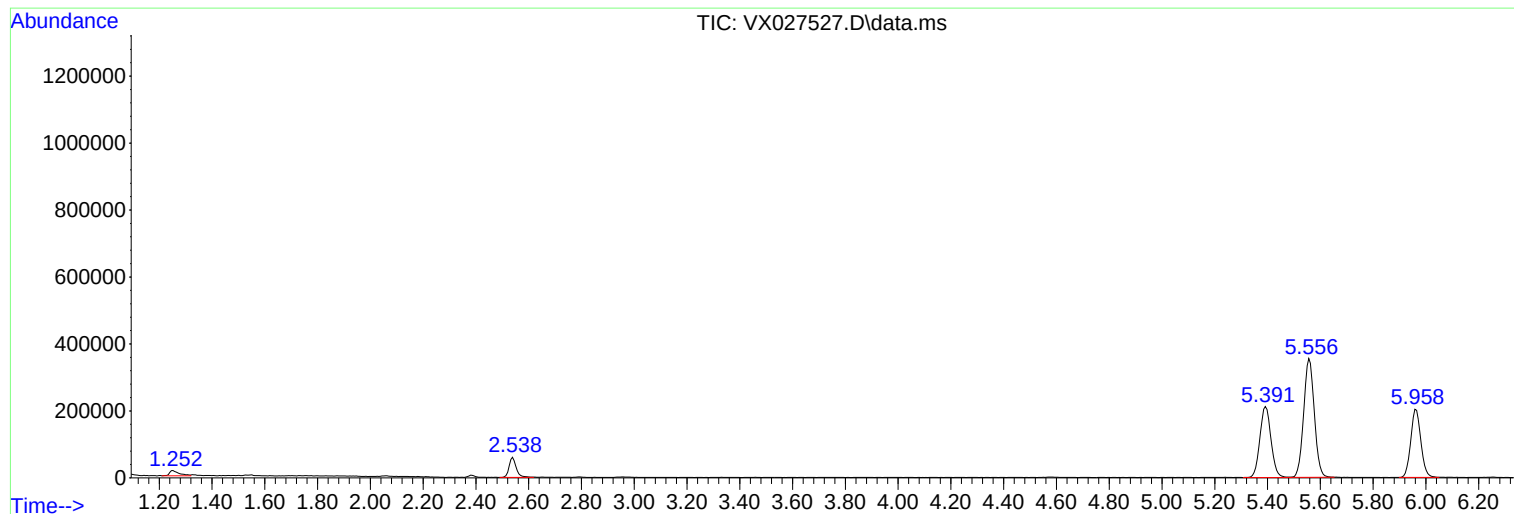

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
Data File : VX027527.D
Acq On : 18 Mar 2022 14:55
Operator : JC/MD
Sample : N2014-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEWATERING-EFFLUENT-031722










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.538	5.72 ug/l	113851	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			4-Penten-2-ol	86	C5H10O	000625-31-0	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

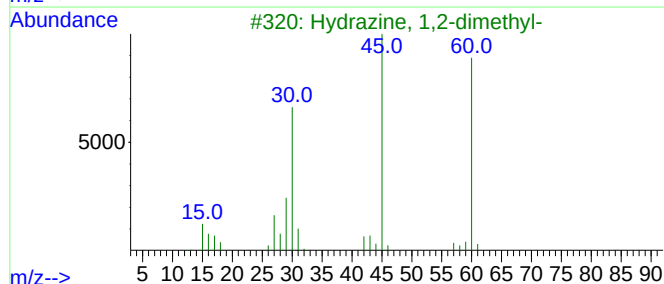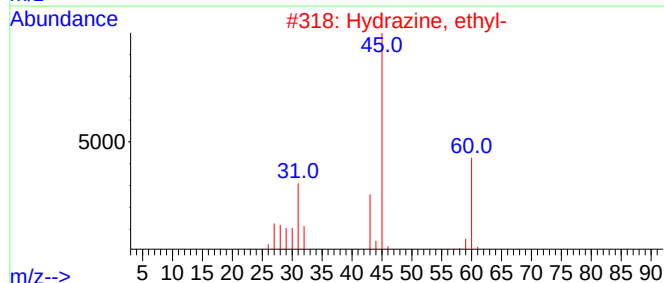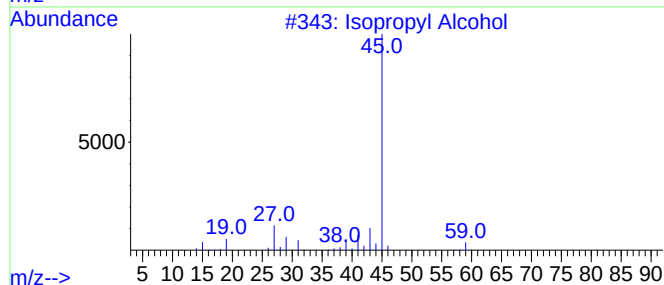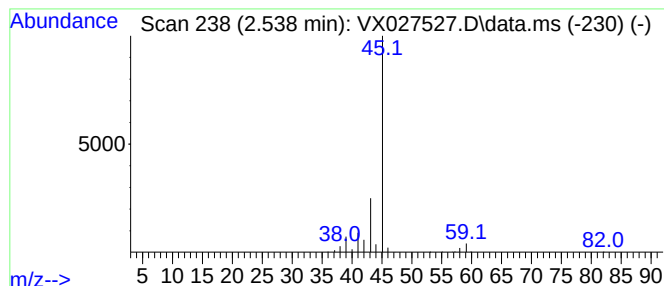

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031822\
Data File : VX027527.D
Acq On : 18 Mar 2022 14:55
Operator : JC/MD
Sample : N2014-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEWATERING-EFFLUENT-031722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.538	5.7	ug/l	113851	1	5.556	995591	50.0