

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031822\  
 Data File : VX027530.D  
 Acq On : 18 Mar 2022 16:06  
 Operator : JC/MD  
 Sample : N1998-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-127

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027530.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.538       | 229           | 238         | 246          | rBV2     | 11934          | 23565         | 1.43%           | 0.247%        |
| 2         | 2.965       | 299           | 308         | 320          | rBV      | 29133          | 66354         | 4.04%           | 0.695%        |
| 3         | 3.117       | 323           | 333         | 345          | rVB      | 169779         | 394626        | 24.02%          | 4.133%        |
| 4         | 4.318       | 520           | 530         | 540          | rBV5     | 5460           | 16892         | 1.03%           | 0.177%        |
| 5         | 5.391       | 693           | 706         | 721          | rBV      | 209001         | 599857        | 36.51%          | 6.283%        |
| 6         | 5.556       | 721           | 733         | 748          | rVB      | 335276         | 949807        | 57.81%          | 9.948%        |
| 7         | 5.964       | 789           | 800         | 817          | rBV      | 202939         | 548819        | 33.40%          | 5.748%        |
| 8         | 6.330       | 851           | 860         | 874          | rVB      | 11165          | 32699         | 1.99%           | 0.342%        |
| 9         | 6.763       | 919           | 931         | 949          | rBV      | 514676         | 1224503       | 74.52%          | 12.825%       |
| 10        | 8.653       | 1234          | 1241        | 1255         | rBV      | 1069167        | 1643111       | 100.00%         | 17.210%       |
| 11        | 10.055      | 1465          | 1471        | 1487         | rBV      | 1092151        | 1454153       | 88.50%          | 15.231%       |
| 12        | 11.085      | 1634          | 1640        | 1652         | rBV      | 895004         | 1138326       | 69.28%          | 11.923%       |
| 13        | 12.024      | 1788          | 1794        | 1804         | rBV      | 1215881        | 1454859       | 88.54%          | 15.238%       |




Sum of corrected areas: 9547571

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031822\  
Data File : VX027530.D  
Acq On : 18 Mar 2022 16:06  
Operator : JC/MD  
Sample : N1998-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

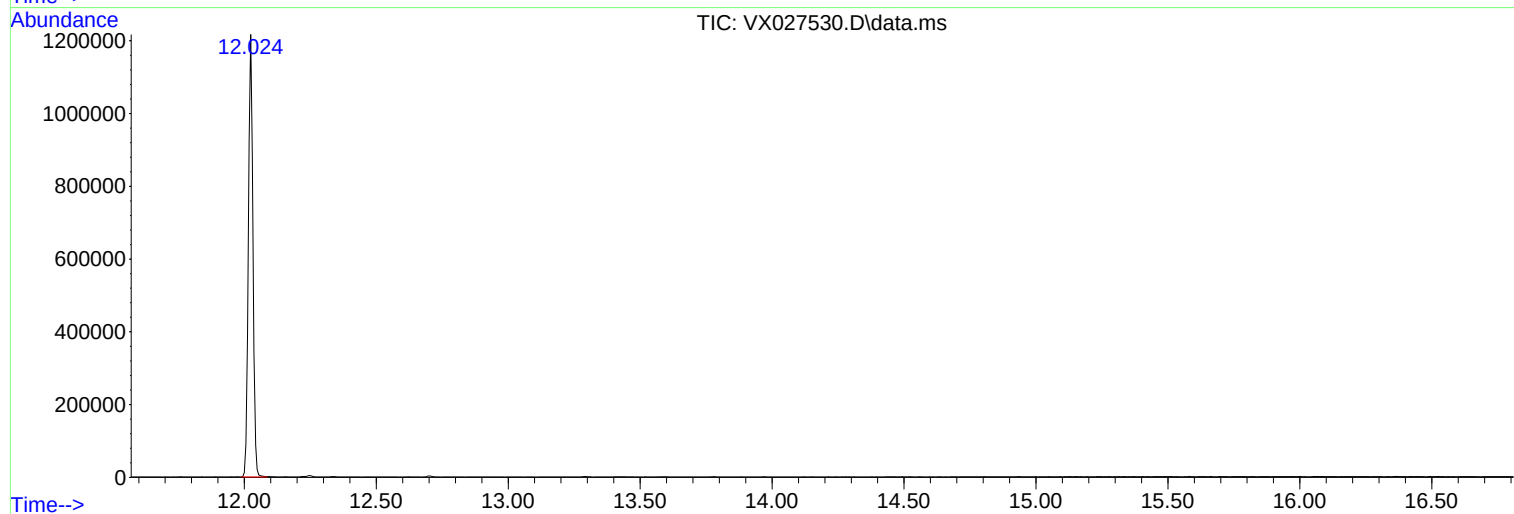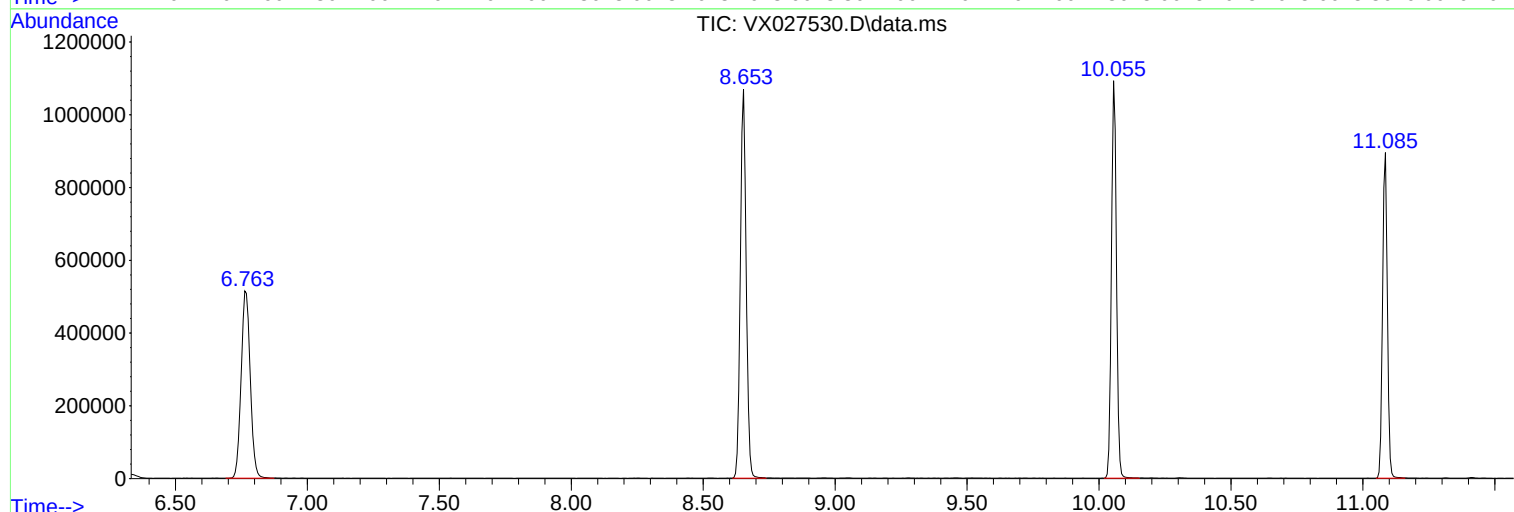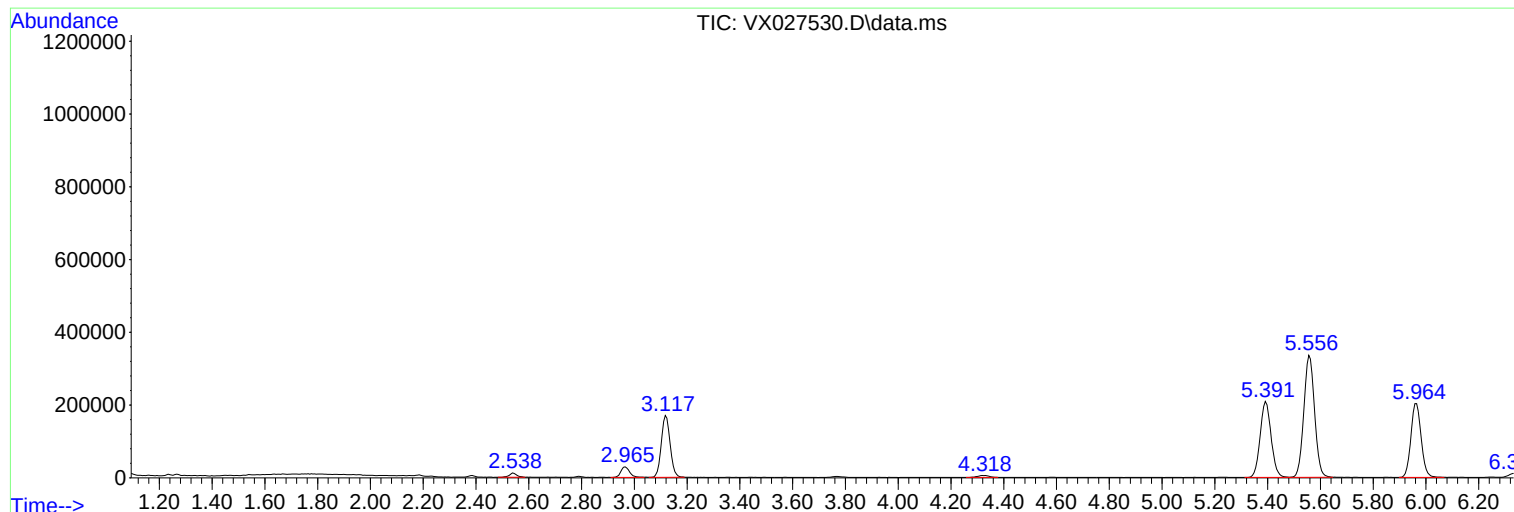

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031822\  
Data File : VX027530.D  
Acq On : 18 Mar 2022 16:06  
Operator : JC/MD  
Sample : N1998-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031822\  
Data File : VX027530.D  
Acq On : 18 Mar 2022 16:06  
Operator : JC/MD  
Sample : N1998-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|