

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040698.D
 Acq On : 18 Mar 2024 14:51
 Operator : JC/MD
 Sample : P1753-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY7DL

Quant Time: Mar 19 01:24:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 19 01:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	137341	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	142151	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	62125	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	50149	41.655	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.320%
7) Chloroethane-d5	1.666	69	42575	44.296	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.600%
11) 1,1-Dichloroethene-d2	2.307	65	23969	43.249	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.500%
21) 2-Butanone-d5	4.452	46	92429	100.048	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.050%
24) Chloroform-d	5.056	84	118352	52.936	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.880%
26) 1,2-Dichloroethane-d4	5.952	65	84752	50.774	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.540%
32) Benzene-d6	5.970	84	208781	47.873	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.740%
36) 1,2-Dichloropropane-d6	7.306	67	65990	48.822	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.640%
41) Toluene-d8	8.647	98	196329	46.713	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.420%
43) trans-1,3-Dichloroprop...	8.952	79	32337	44.951	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.900%
47) 2-Hexanone-d5	9.385	63	68221	91.474	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.470%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	84595	41.802	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.600%
66) 1,2-Dichlorobenzene-d4	12.317	152	73324	56.352	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.700%
Target Compounds						
13) Acetone	2.380	43	103146	156.347	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040698.D
Acq On : 18 Mar 2024 14:51
Operator : JC/MD
Sample : P1753-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY7DL

Quant Time: Mar 19 01:24:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 19 01:22:22 2024
Response via : Initial Calibration

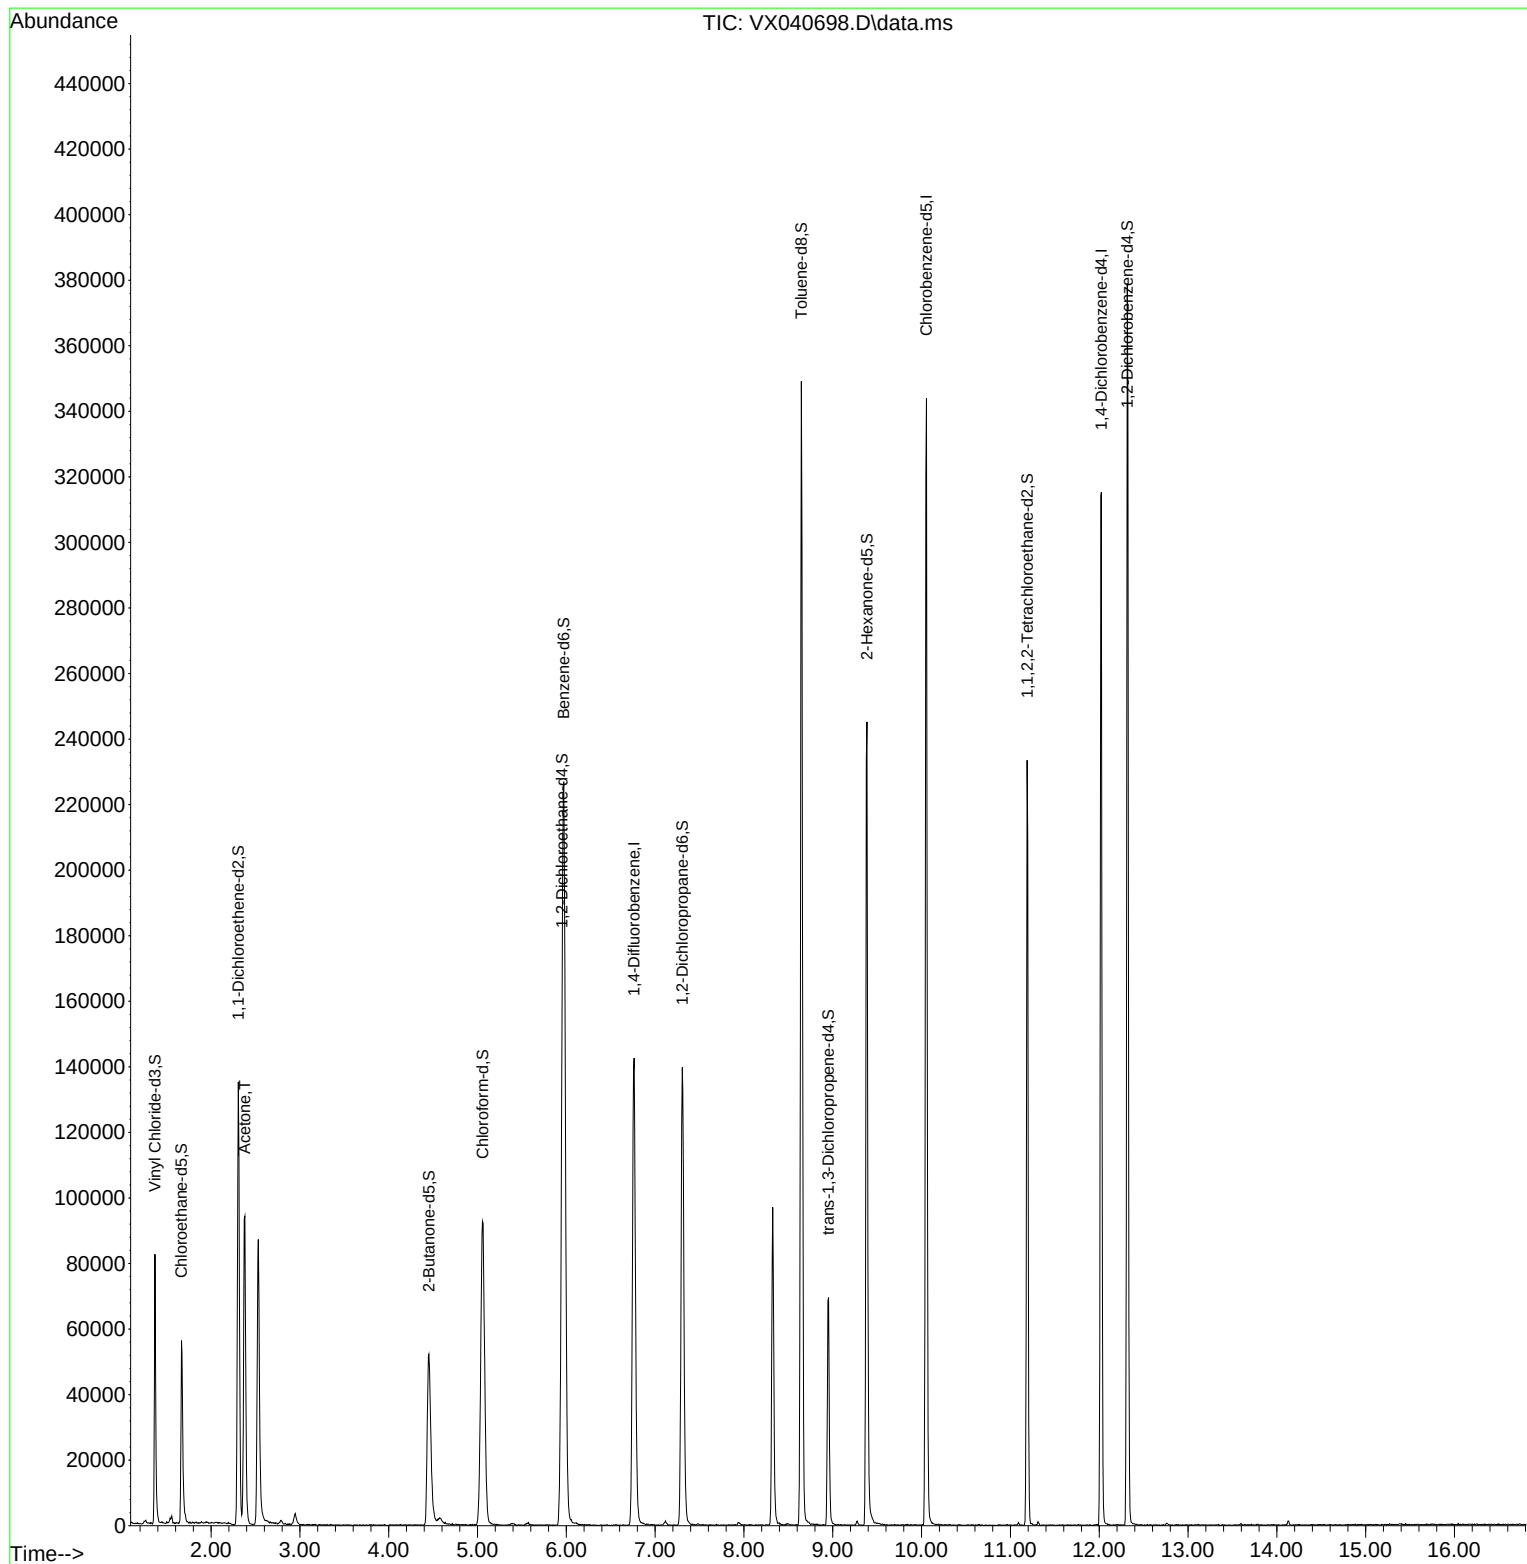

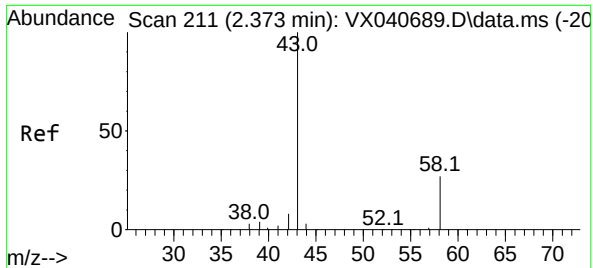

#13
 Acetone
 Concen: 156.347 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX040698.D
 Acq: 18 Mar 2024 14:51

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY7DL

Tgt Ion: 43 Resp: 103146
 Ion Ratio Lower Upper
 43 100
 58 26.9 0.0 54.6

