

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040700.D
 Acq On : 18 Mar 2024 15:37
 Operator : JC/MD
 Sample : P1753-18DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL36DL

Quant Time: Mar 19 01:25:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 19 01:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	145141	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	138174	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	66706	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	63014	49.528	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	99.060%	
7) Chloroethane-d5	1.666	69	52017	51.211	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.420%	
11) 1,1-Dichloroethene-d2	2.307	65	27893	47.625	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.260%	
21) 2-Butanone-d5	4.453	46	92362	94.602	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	94.600%	
24) Chloroform-d	5.056	84	118750	50.260	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.520%	
26) 1,2-Dichloroethane-d4	5.952	65	87173	49.417	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.840%	
32) Benzene-d6	5.971	84	216688	51.116	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.240%	
36) 1,2-Dichloropropane-d6	7.306	67	65978	50.219	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.440%	
41) Toluene-d8	8.647	98	198874	48.681	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.360%	
43) trans-1,3-Dichloroprop...	8.946	79	33552	47.983	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.960%	
47) 2-Hexanone-d5	9.385	63	67632	93.294	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	93.290%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	95419	48.508	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.020%	
66) 1,2-Dichlorobenzene-d4	12.317	152	72933	52.202	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						
13) Acetone	2.374	43	80042	114.806	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040700.D
Acq On : 18 Mar 2024 15:37
Operator : JC/MD
Sample : P1753-18DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL36DL

Quant Time: Mar 19 01:25:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 19 01:22:22 2024
Response via : Initial Calibration

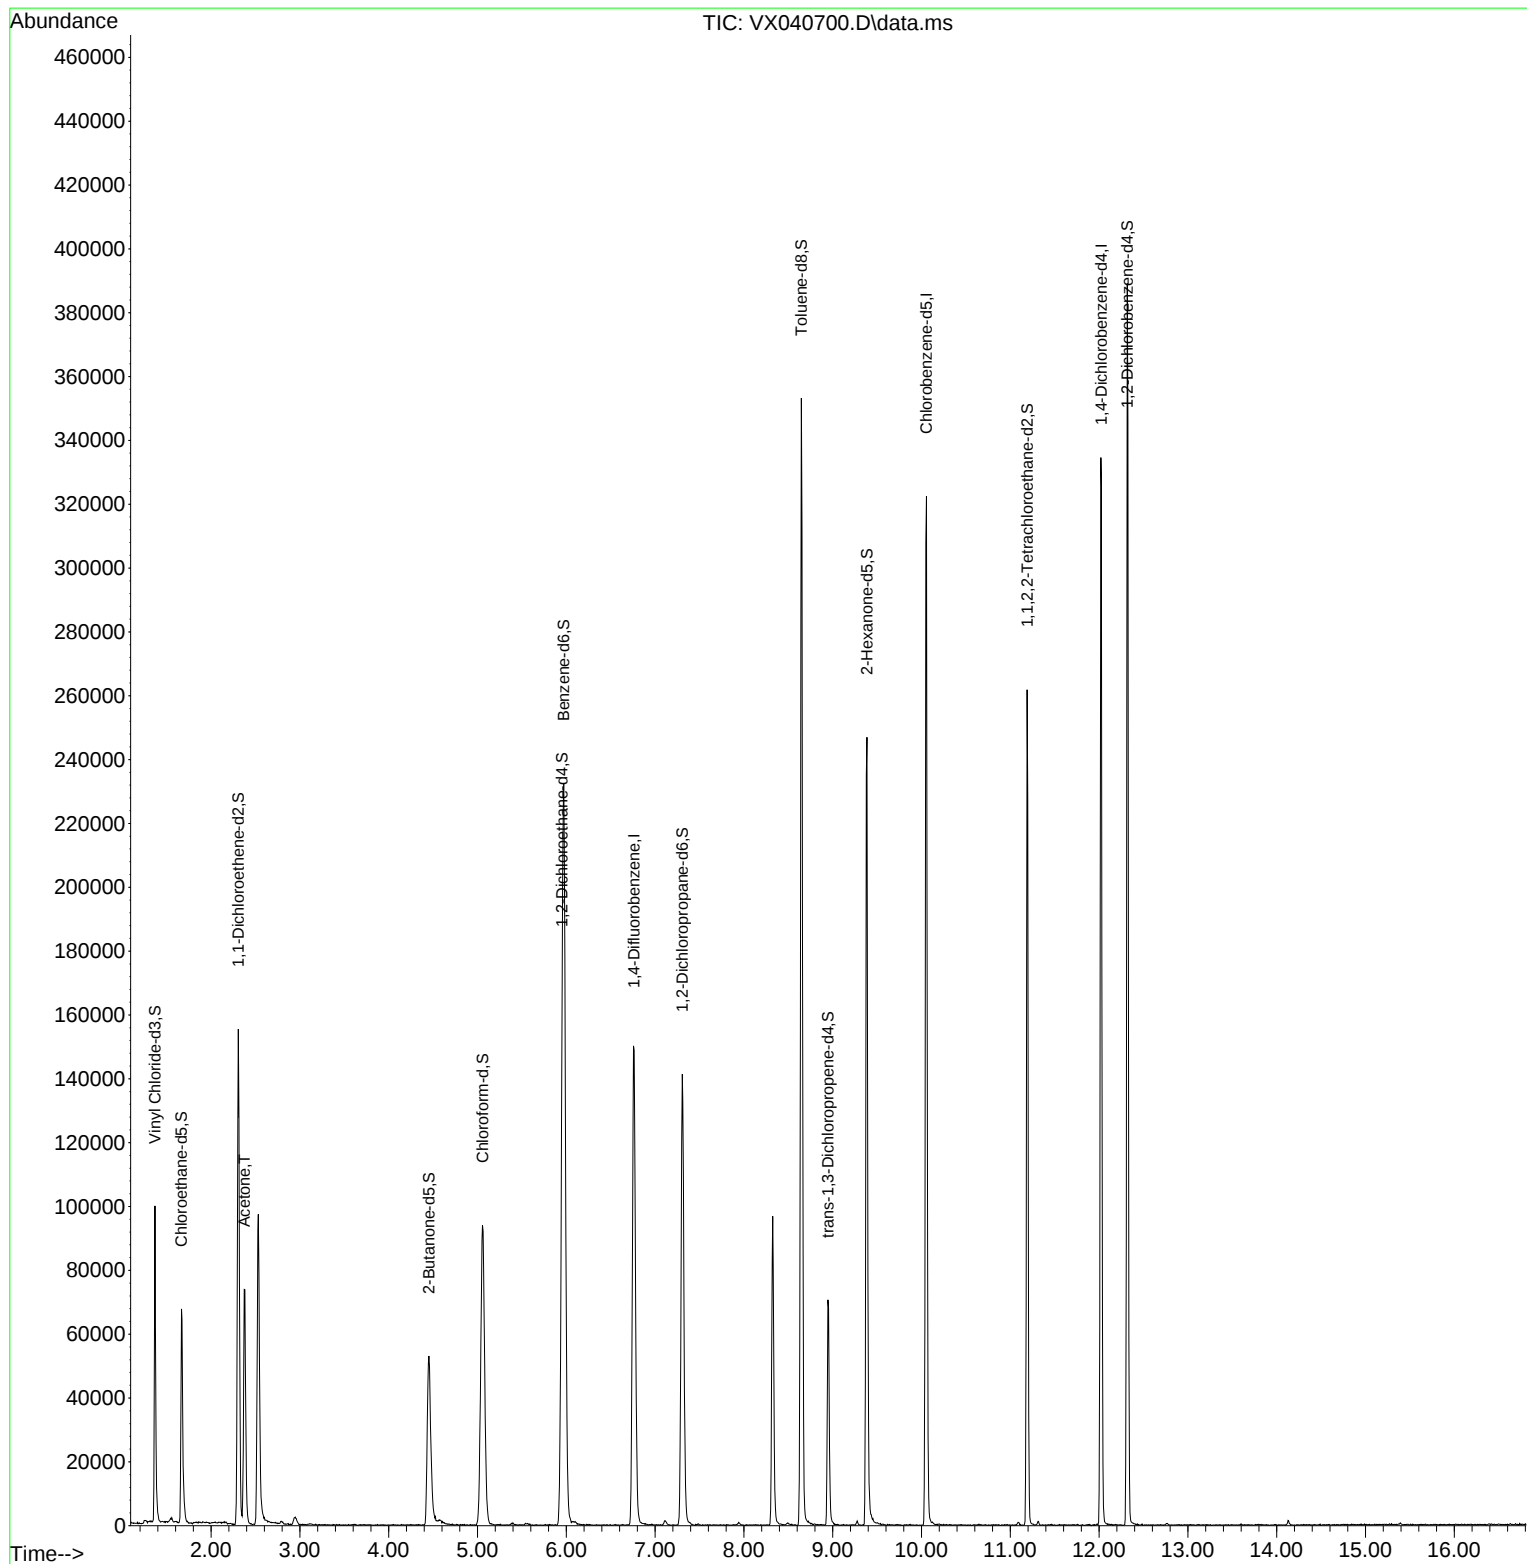

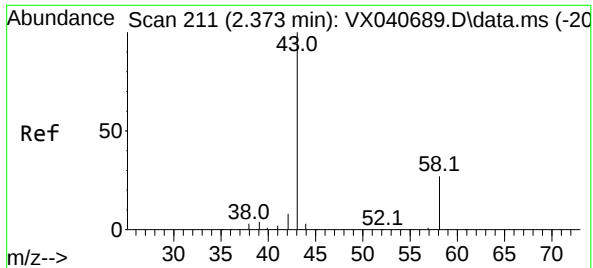

#13
 Acetone
 Concen: 114.806 ug/L
 RT: 2.374 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX040700.D
 Acq: 18 Mar 2024 15:37

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL36DL

Tgt Ion: 43 Resp: 80042
 Ion Ratio Lower Upper
 43 100
 58 26.3 0.0 54.6

