

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040690.D
 Acq On : 18 Mar 2024 11:41
 Operator : JC/MD
 Sample : VX0318WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M

Title : VOC Analysis

Signal : TIC: VX040690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	13	15	17	rBV	547	379	0.05%	0.007%
2	1.368	42	46	58	rVB	105842	110046	15.04%	2.005%
3	1.666	91	95	111	rVB	72056	101556	13.88%	1.850%
4	2.307	193	200	212	rBV	165507	255976	34.98%	4.663%
5	2.514	230	234	240	rVB2	988	1435	0.20%	0.026%
6	2.587	243	246	247	rBV2	300	308	0.04%	0.006%
7	2.782	276	278	285	rVB3	776	1443	0.20%	0.026%
8	3.215	345	349	352	rBV2	216	250	0.03%	0.005%
9	3.325	366	367	370	rBV	143	174	0.02%	0.003%
10	3.532	398	401	402	rBV	245	242	0.03%	0.004%
11	3.556	402	405	408	rBV2	137	213	0.03%	0.004%
12	3.794	442	444	448	rVV2	158	219	0.03%	0.004%
13	3.971	471	473	475	rVB	214	175	0.02%	0.003%
14	4.032	475	483	485	rBV2	283	665	0.09%	0.012%
15	4.068	485	489	491	rVV2	256	281	0.04%	0.005%
16	4.257	518	520	523	rVB2	229	201	0.03%	0.004%
17	4.324	529	531	535	rVV2	176	190	0.03%	0.003%
18	4.446	541	551	566	rBV	57400	159177	21.75%	2.899%
19	5.056	638	651	668	rBV	96495	305041	41.69%	5.556%
20	5.385	701	705	707	rBV2	465	635	0.09%	0.012%
21	5.525	725	728	729	rBV2	301	311	0.04%	0.006%
22	5.544	729	731	734	rVV2	595	662	0.09%	0.012%
23	5.800	769	773	777	rVB	236	354	0.05%	0.006%
24	5.830	777	778	781	rBV2	202	218	0.03%	0.004%
25	5.964	788	800	817	rBV2	244943	731749	100.00%	13.329%
26	6.141	827	829	831	rVB2	335	156	0.02%	0.003%
27	6.294	851	854	862	rBV2	235	528	0.07%	0.010%
28	6.550	894	896	901	rVB	294	301	0.04%	0.005%
29	6.592	901	903	906	rBV	239	257	0.04%	0.005%
30	6.757	921	930	946	rBV	172853	404806	55.32%	7.374%
31	6.903	952	954	957	rVB3	317	249	0.03%	0.005%
32	7.056	976	979	981	rBV2	204	199	0.03%	0.004%
33	7.111	982	988	990	rBV3	1794	2878	0.39%	0.052%
34	7.202	1001	1003	1006	rVV	152	177	0.02%	0.003%
35	7.306	1011	1020	1037	rBV	150419	327249	44.72%	5.961%
36	7.476	1043	1048	1053	rBV4	519	972	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040690.D
 Acq On : 18 Mar 2024 11:41
 Operator : JC/MD
 Sample : VX0318WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.812	1102	1103	1108	rVB2	146	175	0.02%	0.003%
38	7.934	1119	1123	1130	rBV4	772	1573	0.21%	0.029%
39	8.226	1168	1171	1172	rBV	252	286	0.04%	0.005%
40	8.251	1172	1175	1177	rVB	173	180	0.02%	0.003%
41	8.324	1180	1187	1198	rBV	101011	171900	23.49%	3.131%
42	8.494	1210	1215	1217	rBV2	556	792	0.11%	0.014%
43	8.647	1233	1240	1249	rBV	378163	586704	80.18%	10.687%
44	8.946	1283	1289	1299	rBV	76111	115250	15.75%	2.099%
45	9.061	1306	1308	1310	rBV2	192	150	0.02%	0.003%
46	9.305	1347	1348	1352	rVB2	323	246	0.03%	0.004%
47	9.378	1355	1360	1378	rBV	264788	386929	52.88%	7.048%
48	9.610	1395	1398	1400	rBV3	360	435	0.06%	0.008%
49	9.927	1448	1450	1453	rBV	144	174	0.02%	0.003%
50	10.049	1465	1470	1488	rBV	363342	501313	68.51%	9.132%
51	10.262	1501	1505	1506	rBV	230	255	0.03%	0.005%
52	10.305	1511	1512	1516	rVV4	359	443	0.06%	0.008%
53	10.360	1519	1521	1523	rBV	237	234	0.03%	0.004%
54	10.537	1546	1550	1551	rBV2	230	250	0.03%	0.005%
55	10.653	1564	1569	1571	rVV4	492	763	0.10%	0.014%
56	10.799	1590	1593	1595	rBV2	169	170	0.02%	0.003%
57	10.854	1600	1602	1604	rVB	278	184	0.03%	0.003%
58	10.884	1604	1607	1608	rBV	215	226	0.03%	0.004%
59	10.970	1616	1621	1624	rBV3	545	846	0.12%	0.015%
60	11.085	1637	1640	1645	rVB4	771	1178	0.16%	0.021%
61	11.189	1652	1657	1669	rVB	282160	350348	47.88%	6.382%
62	11.311	1674	1677	1682	rVB2	435	545	0.07%	0.010%
63	11.354	1682	1684	1688	rVB2	252	209	0.03%	0.004%
64	11.384	1688	1689	1691	rVB	256	154	0.02%	0.003%
65	11.457	1697	1701	1705	rVB2	570	836	0.11%	0.015%
66	11.677	1734	1737	1740	rVB	219	250	0.03%	0.005%
67	11.707	1740	1742	1745	rBV	160	228	0.03%	0.004%
68	11.756	1747	1750	1755	rVV	898	973	0.13%	0.018%
69	11.975	1783	1786	1788	rVB	795	752	0.10%	0.014%
70	12.018	1788	1793	1804	rBV	351775	453608	61.99%	8.263%
71	12.140	1811	1813	1814	rBV	239	164	0.02%	0.003%
72	12.189	1819	1821	1823	rBV2	191	162	0.02%	0.003%
73	12.232	1823	1828	1830	rBV	245	316	0.04%	0.006%
74	12.317	1837	1842	1853	rBV	371334	482158	65.89%	8.783%
75	12.469	1865	1867	1869	rBV2	211	164	0.02%	0.003%
76	12.768	1911	1916	1921	rVB2	1124	1589	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040690.D
 Acq On : 18 Mar 2024 11:41
 Operator : JC/MD
 Sample : VX0318WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.823	1923	1925	1927	rBV	208	194	0.03%	0.004%
78	12.878	1931	1934	1935	rBV	151	158	0.02%	0.003%
79	12.994	1951	1953	1954	rBV	260	156	0.02%	0.003%
80	13.116	1969	1973	1977	rBV2	1351	1663	0.23%	0.030%
81	13.359	2010	2013	2015	rVB2	191	240	0.03%	0.004%
82	13.384	2015	2017	2022	rBV2	214	383	0.05%	0.007%
83	13.445	2026	2027	2030	rBV2	145	180	0.02%	0.003%
84	13.591	2048	2051	2057	rVB4	1486	2352	0.32%	0.043%
85	13.646	2058	2060	2064	rVV	215	184	0.03%	0.003%
86	13.725	2072	2073	2075	rBV	188	154	0.02%	0.003%
87	13.780	2078	2082	2086	rVV	2900	4063	0.56%	0.074%
88	13.963	2108	2112	2118	rVB4	1842	2739	0.37%	0.050%
89	14.030	2121	2123	2126	rVB2	195	192	0.03%	0.003%
90	14.128	2135	2139	2146	rBV2	1346	1997	0.27%	0.036%
91	14.231	2154	2156	2157	rBV	286	236	0.03%	0.004%
92	14.573	2210	2212	2213	rBV	167	152	0.02%	0.003%
93	14.609	2216	2218	2221	rVB	329	369	0.05%	0.007%
94	14.664	2225	2227	2228	rBV	206	163	0.02%	0.003%
95	14.890	2262	2264	2265	rBV	273	250	0.03%	0.005%
96	15.048	2286	2290	2293	rBV2	294	393	0.05%	0.007%
97	15.371	2341	2343	2344	rBV	295	211	0.03%	0.004%
98	15.749	2404	2405	2408	rBV	275	185	0.03%	0.003%
99	15.828	2417	2418	2420	rBV	250	210	0.03%	0.004%
100	16.615	2545	2547	2550	rBV2	253	233	0.03%	0.004%




Sum of corrected areas: 5489841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040690.D
Acq On : 18 Mar 2024 11:41
Operator : JC/MD
Sample : VX0318WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

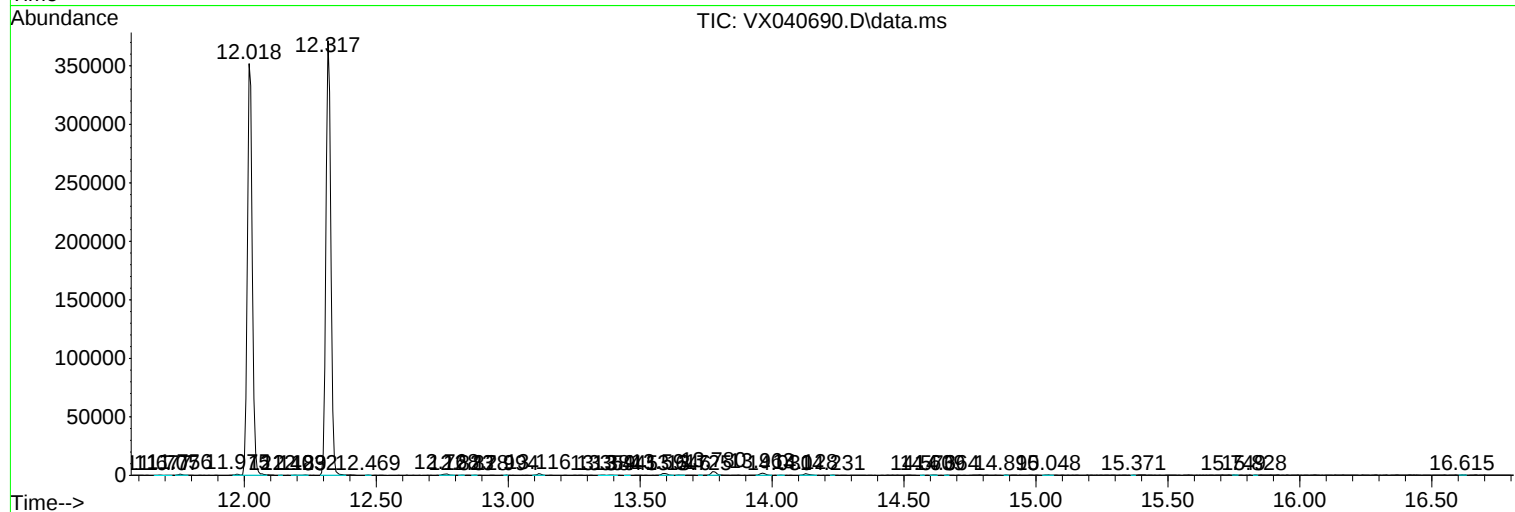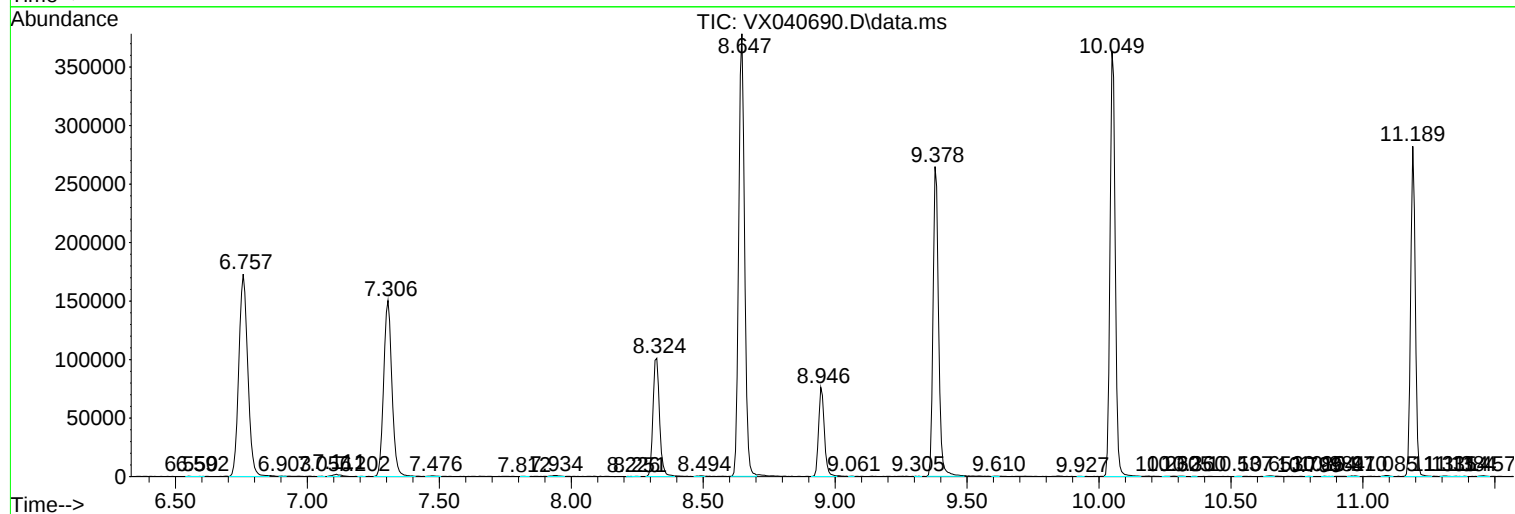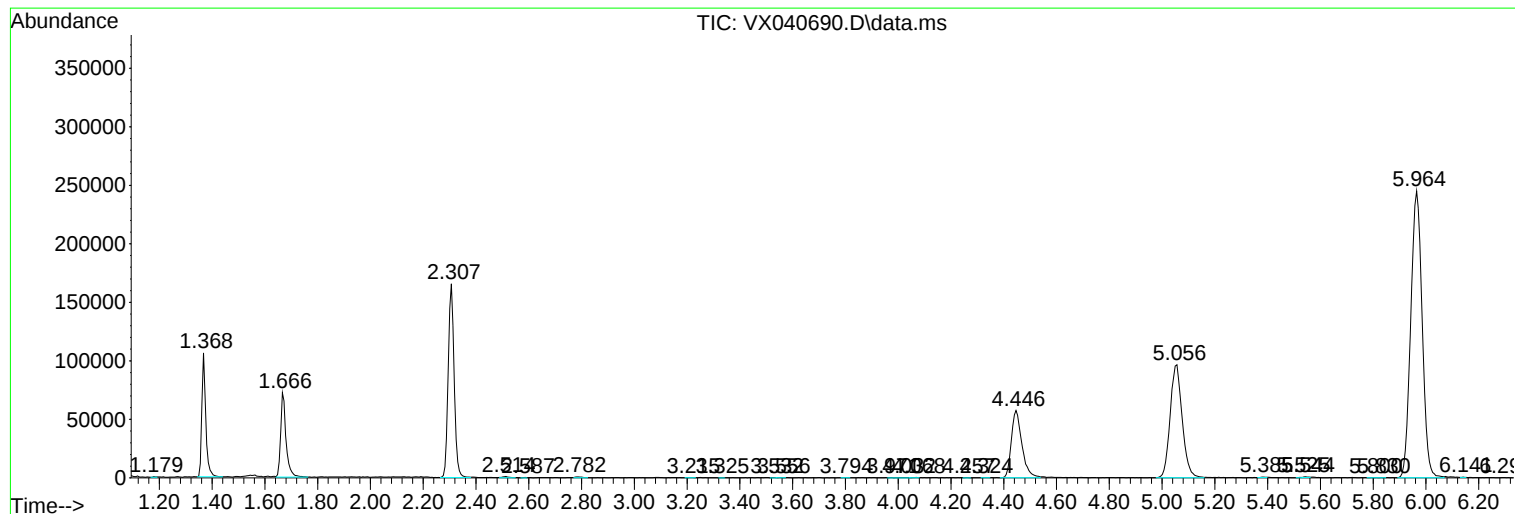

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040690.D
Acq On : 18 Mar 2024 11:41
Operator : JC/MD
Sample : VX0318WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040690.D
Acq On : 18 Mar 2024 11:41
Operator : JC/MD
Sample : VX0318WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc