

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040693.D
 Acq On : 18 Mar 2024 12:57
 Operator : JC/MD
 Sample : P1753-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M

Title : VOC Analysis

Signal : TIC: VX040693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	103570	107866	15.26%	1.997%
2	1.532	71	73	74	rBV	1130	751	0.11%	0.014%
3	1.666	91	95	109	rVB	68228	98031	13.87%	1.815%
4	2.209	183	184	186	rVB	456	217	0.03%	0.004%
5	2.306	194	200	217	rVB2	182792	346012	48.94%	6.405%
6	2.532	230	237	247	rBV3	6081	12522	1.77%	0.232%
7	2.709	264	266	271	rBV3	162	200	0.03%	0.004%
8	2.794	275	280	283	rVB4	1060	1588	0.22%	0.029%
9	2.946	297	305	311	rBV2	1972	4774	0.68%	0.088%
10	3.062	321	324	325	rBV	217	270	0.04%	0.005%
11	3.099	329	330	332	rBV	371	231	0.03%	0.004%
12	3.117	332	333	338	rVB2	276	291	0.04%	0.005%
13	3.355	368	372	373	rBV	224	288	0.04%	0.005%
14	3.404	378	380	381	rBV	196	199	0.03%	0.004%
15	3.422	381	383	385	rVB	239	189	0.03%	0.003%
16	3.617	408	415	419	rBV4	1939	4181	0.59%	0.077%
17	3.977	471	474	477	rVB2	200	263	0.04%	0.005%
18	4.105	493	495	497	rBV2	185	197	0.03%	0.004%
19	4.324	529	531	533	rBV2	222	211	0.03%	0.004%
20	4.446	543	551	567	rBV	53609	163654	23.15%	3.029%
21	4.836	614	615	619	rVB	342	287	0.04%	0.005%
22	4.971	635	637	639	rBV	244	272	0.04%	0.005%
23	5.056	639	651	668	rVV2	94685	295263	41.76%	5.466%
24	5.172	668	670	671	rVV	320	224	0.03%	0.004%
25	5.385	698	705	715	rVB5	3402	9437	1.33%	0.175%
26	5.556	728	733	739	rBB3	835	1799	0.25%	0.033%
27	5.672	748	752	754	rVB2	203	255	0.04%	0.005%
28	5.964	789	800	817	rBV2	233879	706967	100.00%	13.087%
29	6.202	838	839	842	rBV2	232	195	0.03%	0.004%
30	6.428	871	876	878	rBV2	124	213	0.03%	0.004%
31	6.458	878	881	885	rBV2	224	244	0.03%	0.005%
32	6.537	891	894	895	rBV	199	225	0.03%	0.004%
33	6.757	921	930	949	rBV	150779	362644	51.30%	6.713%
34	6.940	956	960	964	rBV2	319	477	0.07%	0.009%
35	6.988	966	968	970	rBV2	247	284	0.04%	0.005%
36	7.049	977	978	980	rBV	305	233	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040693.D
 Acq On : 18 Mar 2024 12:57
 Operator : JC/MD
 Sample : P1753-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.123	983	990	999	rVB7	5082	11858	1.68%	0.220%
38	7.305	1011	1020	1039	rVB	143152	317241	44.87%	5.873%
39	7.446	1039	1043	1046	rBV2	375	538	0.08%	0.010%
40	7.482	1046	1049	1054	rBV2	384	559	0.08%	0.010%
41	7.574	1062	1064	1066	rBV	164	210	0.03%	0.004%
42	7.848	1107	1109	1112	rVB	235	230	0.03%	0.004%
43	7.879	1112	1114	1116	rBV	214	229	0.03%	0.004%
44	7.927	1119	1122	1123	rBV2	729	613	0.09%	0.011%
45	8.226	1168	1171	1172	rBV	210	204	0.03%	0.004%
46	8.324	1179	1187	1200	rBV	102506	165716	23.44%	3.068%
47	8.488	1210	1214	1218	rBV3	551	1044	0.15%	0.019%
48	8.647	1234	1240	1256	rVV	358170	563340	79.68%	10.428%
49	8.945	1284	1289	1299	rBV	71214	110845	15.68%	2.052%
50	9.214	1332	1333	1335	rBV	201	189	0.03%	0.003%
51	9.281	1339	1344	1346	rBV2	842	1018	0.14%	0.019%
52	9.384	1355	1361	1381	rVV	246800	368021	52.06%	6.813%
53	9.518	1381	1383	1384	rVV2	535	412	0.06%	0.008%
54	9.561	1388	1390	1396	rVB2	329	400	0.06%	0.007%
55	9.610	1396	1398	1401	rVB2	188	216	0.03%	0.004%
56	9.903	1442	1446	1449	rVB	199	271	0.04%	0.005%
57	10.055	1465	1471	1485	rBV	318520	445811	63.06%	8.253%
58	10.195	1492	1494	1496	rBV2	332	237	0.03%	0.004%
59	10.311	1509	1513	1516	rBV	535	610	0.09%	0.011%
60	10.640	1565	1567	1570	rVB	304	292	0.04%	0.005%
61	10.677	1570	1573	1576	rBV3	242	431	0.06%	0.008%
62	10.732	1580	1582	1586	rBV	347	334	0.05%	0.006%
63	10.768	1586	1588	1589	rBV	239	189	0.03%	0.003%
64	10.963	1618	1620	1624	rVB	376	469	0.07%	0.009%
65	11.055	1630	1635	1637	rBV2	198	306	0.04%	0.006%
66	11.091	1637	1641	1646	rVB4	1129	1681	0.24%	0.031%
67	11.189	1652	1657	1671	rVV	264581	336574	47.61%	6.230%
68	11.311	1675	1677	1681	rVV2	329	357	0.05%	0.007%
69	11.457	1698	1701	1703	rBV2	351	353	0.05%	0.007%
70	11.512	1709	1710	1714	rBV2	191	230	0.03%	0.004%
71	11.756	1747	1750	1754	rBV2	356	501	0.07%	0.009%
72	11.847	1761	1765	1768	rVB2	228	388	0.05%	0.007%
73	11.969	1782	1785	1788	rBV3	650	659	0.09%	0.012%
74	12.018	1788	1793	1807	rBV	333356	436507	61.74%	8.080%
75	12.317	1837	1842	1850	rBV	399519	502553	71.09%	9.303%
76	12.542	1878	1879	1881	rBV	226	188	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040693.D
 Acq On : 18 Mar 2024 12:57
 Operator : JC/MD
 Sample : P1753-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.762	1911	1915	1919	rBV2	792	1004	0.14%	0.019%
78	12.920	1937	1941	1943	rVB2	133	215	0.03%	0.004%
79	13.036	1958	1960	1963	rBV	244	264	0.04%	0.005%
80	13.121	1972	1974	1976	rVB3	316	317	0.04%	0.006%
81	13.463	2029	2030	2034	rVV2	176	186	0.03%	0.003%
82	13.512	2036	2038	2043	rVB2	226	323	0.05%	0.006%
83	13.591	2048	2051	2052	rBV2	254	255	0.04%	0.005%
84	13.786	2079	2083	2088	rBV2	466	849	0.12%	0.016%
85	13.969	2110	2113	2118	rVB3	385	407	0.06%	0.008%
86	14.018	2118	2121	2124	rBV2	152	255	0.04%	0.005%
87	14.127	2135	2139	2143	rBV2	1221	1573	0.22%	0.029%
88	14.243	2155	2158	2161	rBV2	191	248	0.04%	0.005%
89	14.274	2161	2163	2166	rVV2	193	196	0.03%	0.004%
90	14.396	2181	2183	2185	rBV	214	191	0.03%	0.004%
91	14.444	2189	2191	2193	rVB	274	209	0.03%	0.004%
92	14.469	2193	2195	2198	rBV2	179	215	0.03%	0.004%
93	14.603	2215	2217	2218	rVB	327	203	0.03%	0.004%
94	14.627	2218	2221	2224	rBV2	357	470	0.07%	0.009%
95	14.652	2224	2225	2228	rBV2	219	192	0.03%	0.004%
96	14.743	2239	2240	2243	rVB2	235	198	0.03%	0.004%
97	15.213	2314	2317	2318	rBV	248	252	0.04%	0.005%
98	15.389	2343	2346	2350	rVB2	619	771	0.11%	0.014%
99	16.103	2459	2463	2465	rBV	324	301	0.04%	0.006%
100	16.694	2559	2560	2562	rBV2	341	237	0.03%	0.004%


Sum of corrected areas: 5402109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040693.D
Acq On : 18 Mar 2024 12:57
Operator : JC/MD
Sample : P1753-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

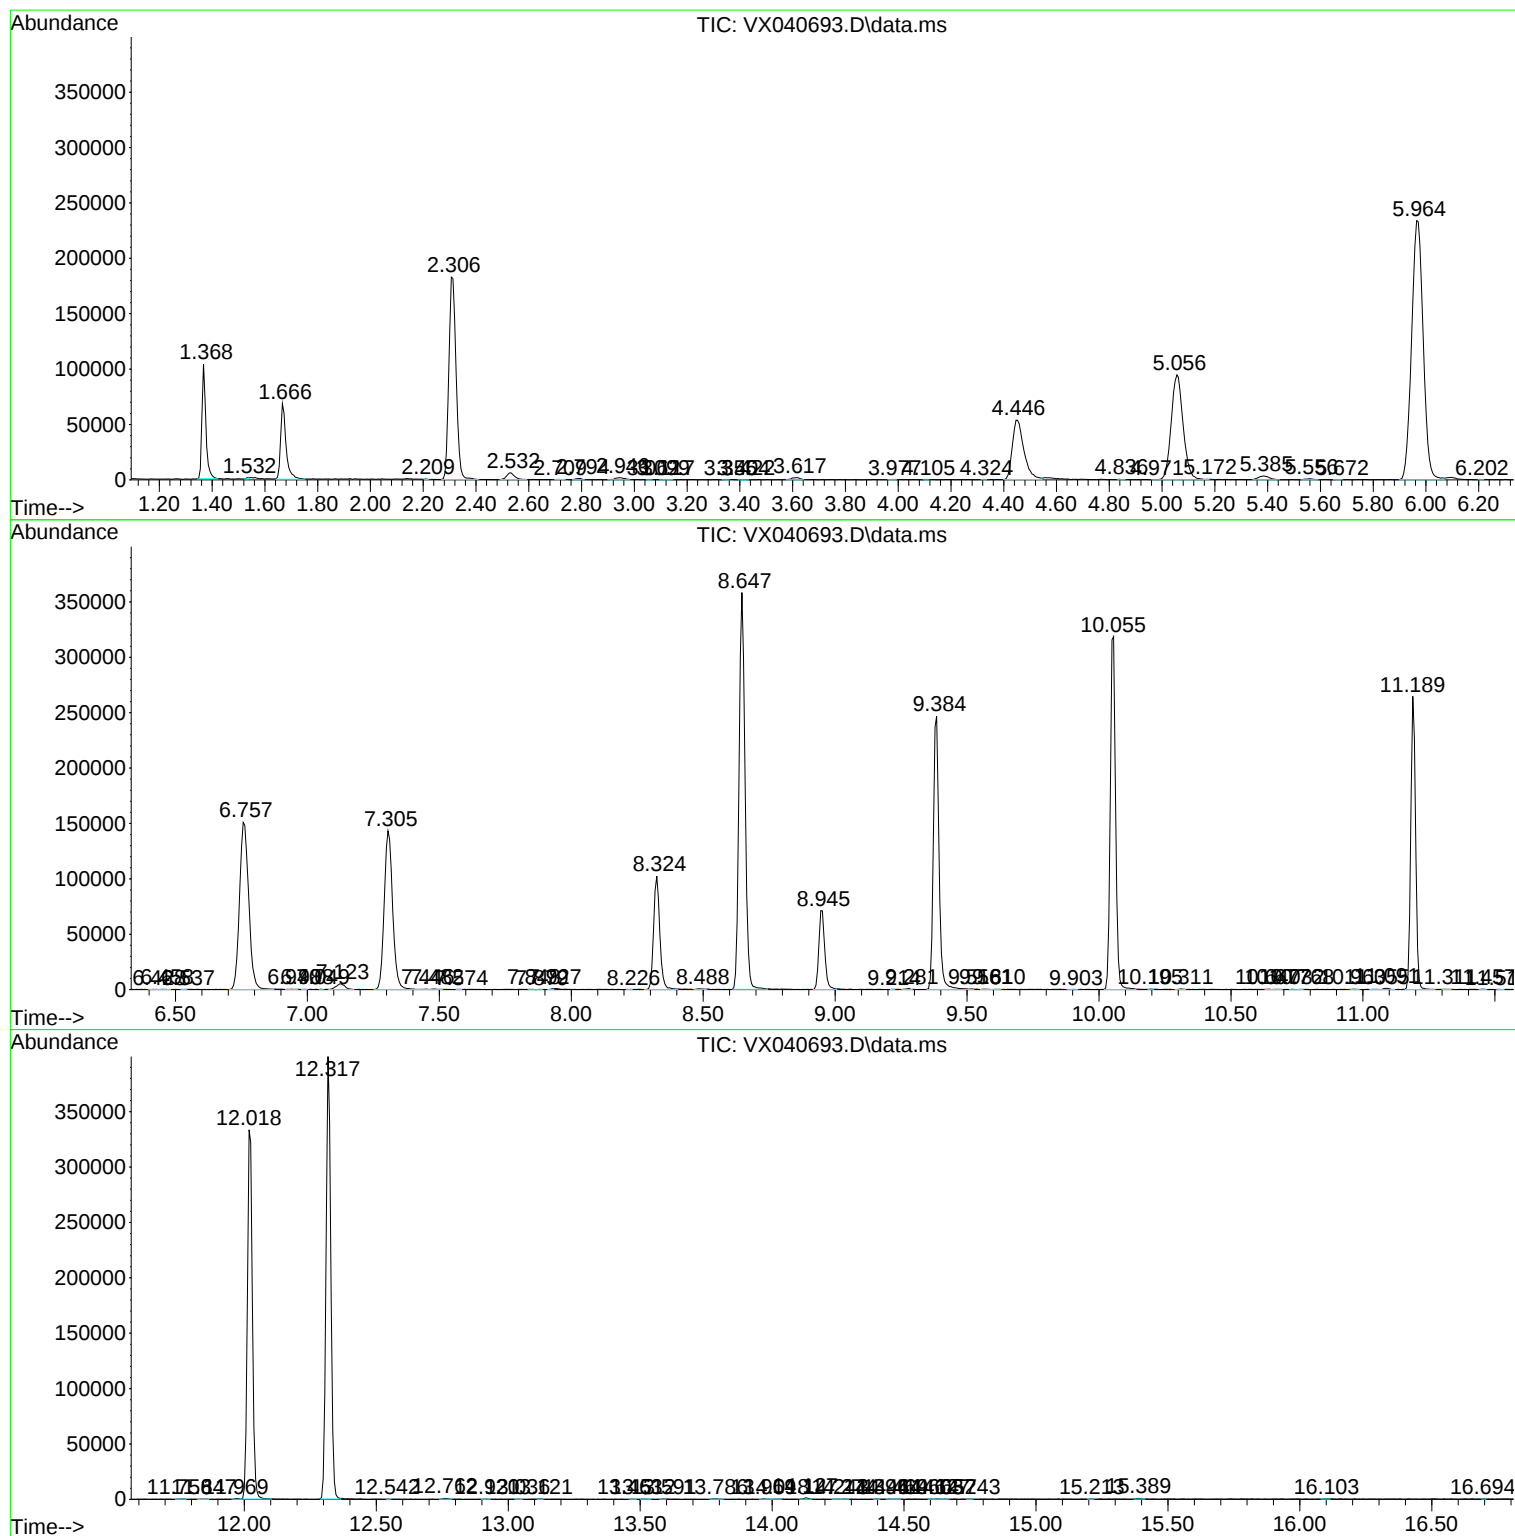

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040693.D
Acq On : 18 Mar 2024 12:57
Operator : JC/MD
Sample : P1753-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040693.D
Acq On : 18 Mar 2024 12:57
Operator : JC/MD
Sample : P1753-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc