

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040703.D
 Acq On : 18 Mar 2024 16:45
 Operator : JC/MD
 Sample : P1753-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rBV	100886	103762	15.28%	2.073%
2	1.666	91	95	108	rBV	64806	93600	13.79%	1.870%
3	2.258	190	192	194	rBV2	217	199	0.03%	0.004%
4	2.306	194	200	209	rBV	155844	239095	35.22%	4.777%
5	2.532	230	237	245	rBV3	1972	4334	0.64%	0.087%
6	2.587	245	246	248	rVB2	434	281	0.04%	0.006%
7	2.788	276	279	286	rVB3	1314	2320	0.34%	0.046%
8	2.953	303	306	309	rBV2	240	356	0.05%	0.007%
9	3.264	354	357	358	rBV	263	267	0.04%	0.005%
10	3.373	373	375	378	rVB	264	218	0.03%	0.004%
11	3.453	385	388	391	rBV2	218	264	0.04%	0.005%
12	3.940	466	468	472	rBV2	221	334	0.05%	0.007%
13	4.452	543	552	567	rVV	51501	146173	21.53%	2.920%
14	4.940	629	632	635	rBV2	155	218	0.03%	0.004%
15	5.056	639	651	668	rVV	90522	281192	41.42%	5.618%
16	5.275	685	687	690	rBV	199	262	0.04%	0.005%
17	5.336	694	697	700	rBV2	175	265	0.04%	0.005%
18	5.391	700	706	709	rBV3	415	885	0.13%	0.018%
19	5.617	739	743	744	rVB	165	179	0.03%	0.004%
20	5.647	744	748	749	rBV2	260	195	0.03%	0.004%
21	5.769	767	768	771	rBV2	189	198	0.03%	0.004%
22	5.970	789	801	816	rBV2	227494	678869	100.00%	13.563%
23	6.214	840	841	843	rVB	283	162	0.02%	0.003%
24	6.239	843	845	847	rBV	237	228	0.03%	0.005%
25	6.330	858	860	863	rBV	217	236	0.03%	0.005%
26	6.385	866	869	870	rVB	277	182	0.03%	0.004%
27	6.458	878	881	884	rBV2	128	212	0.03%	0.004%
28	6.531	890	893	897	rBV2	236	432	0.06%	0.009%
29	6.763	922	931	941	rBV	143473	339099	49.95%	6.775%
30	7.104	983	987	995	rVB5	1598	3652	0.54%	0.073%
31	7.178	995	999	1000	rBV	176	198	0.03%	0.004%
32	7.306	1011	1020	1036	rVV	137857	302011	44.49%	6.034%
33	7.482	1045	1049	1054	rBV4	323	613	0.09%	0.012%
34	7.940	1121	1124	1127	rVV4	857	1175	0.17%	0.023%
35	8.001	1131	1134	1136	rBV2	231	207	0.03%	0.004%
36	8.043	1138	1141	1143	rBV	138	192	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040703.D
 Acq On : 18 Mar 2024 16:45
 Operator : JC/MD
 Sample : P1753-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	8.190	1164	1165	1169	rBV	178	168	0.02%	0.003%
38	8.257	1174	1176	1177	rBV2	209	186	0.03%	0.004%
39	8.324	1181	1187	1199	rBV	95102	154690	22.79%	3.091%
40	8.494	1209	1215	1220	rBV4	591	1183	0.17%	0.024%
41	8.647	1233	1240	1251	rBV	342585	538770	79.36%	10.764%
42	8.769	1258	1260	1262	rBV2	260	167	0.02%	0.003%
43	8.872	1274	1277	1278	rBV2	252	207	0.03%	0.004%
44	8.952	1284	1290	1298	rBV	67331	103561	15.25%	2.069%
45	9.061	1306	1308	1310	rVB	192	162	0.02%	0.003%
46	9.269	1338	1342	1349	rVB3	944	1690	0.25%	0.034%
47	9.384	1355	1361	1377	rBV	241927	352009	51.85%	7.033%
48	9.513	1380	1382	1385	rVV2	365	321	0.05%	0.006%
49	9.848	1433	1437	1439	rBV	339	350	0.05%	0.007%
50	10.055	1465	1471	1481	rBV	299005	419028	61.72%	8.372%
51	10.195	1492	1494	1495	rBV2	339	265	0.04%	0.005%
52	10.275	1506	1507	1510	rBV2	117	164	0.02%	0.003%
53	10.445	1532	1535	1538	rBV	220	247	0.04%	0.005%
54	10.482	1538	1541	1542	rBV	172	162	0.02%	0.003%
55	10.616	1561	1563	1566	rVV2	202	200	0.03%	0.004%
56	10.640	1566	1567	1571	rVB2	358	249	0.04%	0.005%
57	10.927	1613	1614	1617	rBV2	183	187	0.03%	0.004%
58	10.976	1619	1622	1624	rBV3	258	283	0.04%	0.006%
59	11.092	1636	1641	1646	rVB3	1188	1499	0.22%	0.030%
60	11.140	1646	1649	1652	rBV	206	340	0.05%	0.007%
61	11.189	1652	1657	1667	rVV	258272	324200	47.76%	6.477%
62	11.287	1669	1673	1674	rVV	249	320	0.05%	0.006%
63	11.317	1674	1678	1681	rVV	1488	1863	0.27%	0.037%
64	11.409	1691	1693	1694	rBV	224	182	0.03%	0.004%
65	11.445	1698	1699	1704	rVB3	269	255	0.04%	0.005%
66	11.530	1709	1713	1717	rBV2	131	260	0.04%	0.005%
67	11.750	1747	1749	1752	rVB2	307	266	0.04%	0.005%
68	11.963	1781	1784	1788	rBV3	225	402	0.06%	0.008%
69	12.018	1788	1793	1805	rBV	315239	408798	60.22%	8.167%
70	12.225	1826	1827	1831	rVB2	292	314	0.05%	0.006%
71	12.268	1831	1834	1837	rBV2	229	369	0.05%	0.007%
72	12.317	1837	1842	1854	rBV	373096	481005	70.85%	9.610%
73	12.451	1862	1864	1868	rVB2	373	488	0.07%	0.010%
74	12.664	1893	1899	1901	rBV2	169	319	0.05%	0.006%
75	12.768	1911	1916	1921	rBV3	551	929	0.14%	0.019%
76	12.866	1931	1932	1935	rVB	256	166	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040703.D
 Acq On : 18 Mar 2024 16:45
 Operator : JC/MD
 Sample : P1753-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.988	1947	1952	1955	rVB2	233	369	0.05%	0.007%
78	13.036	1955	1960	1961	rBV2	153	223	0.03%	0.004%
79	13.109	1970	1972	1974	rBV	241	230	0.03%	0.005%
80	13.292	2000	2002	2004	rVV	241	164	0.02%	0.003%
81	13.457	2027	2029	2032	rBV	175	175	0.03%	0.003%
82	13.567	2045	2047	2050	rVV2	160	198	0.03%	0.004%
83	13.591	2050	2051	2057	rVB3	389	593	0.09%	0.012%
84	13.634	2057	2058	2061	rBV	150	186	0.03%	0.004%
85	13.853	2091	2094	2095	rBV	180	188	0.03%	0.004%
86	13.945	2106	2109	2111	rBV2	168	195	0.03%	0.004%
87	14.128	2135	2139	2142	rVV	915	1207	0.18%	0.024%
88	14.445	2189	2191	2194	rBV2	182	262	0.04%	0.005%
89	14.475	2194	2196	2199	rVB	221	196	0.03%	0.004%
90	14.658	2224	2226	2229	rBV	294	224	0.03%	0.004%
91	14.725	2235	2237	2239	rBV	170	207	0.03%	0.004%
92	15.274	2326	2327	2329	rBV2	338	338	0.05%	0.007%
93	15.450	2352	2356	2361	rBV3	288	556	0.08%	0.011%
94	15.524	2365	2368	2371	rBV2	224	289	0.04%	0.006%
95	15.554	2371	2373	2376	rVB	195	179	0.03%	0.004%
96	15.889	2425	2428	2430	rBV2	183	238	0.04%	0.005%
97	15.981	2442	2443	2445	rBV	335	225	0.03%	0.004%
98	16.109	2462	2464	2465	rBV2	175	164	0.02%	0.003%
99	16.731	2564	2566	2568	rBV2	291	197	0.03%	0.004%
100	16.773	2571	2573	2574	rBV3	252	213	0.03%	0.004%




Sum of corrected areas: 5005305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040703.D
Acq On : 18 Mar 2024 16:45
Operator : JC/MD
Sample : P1753-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

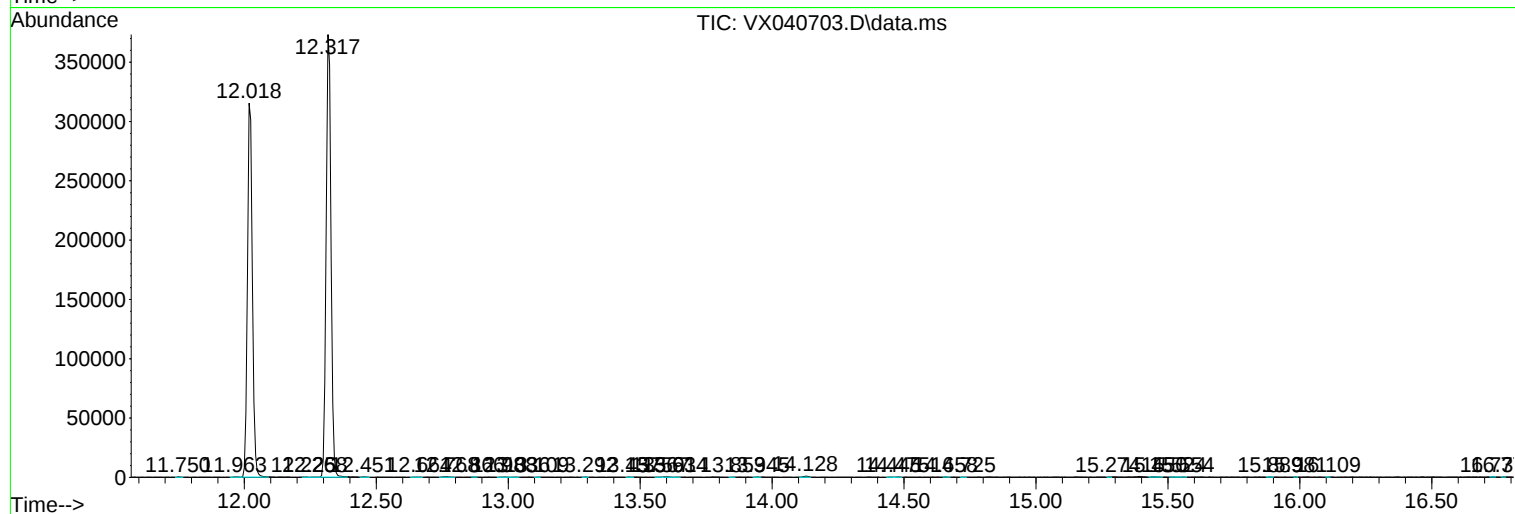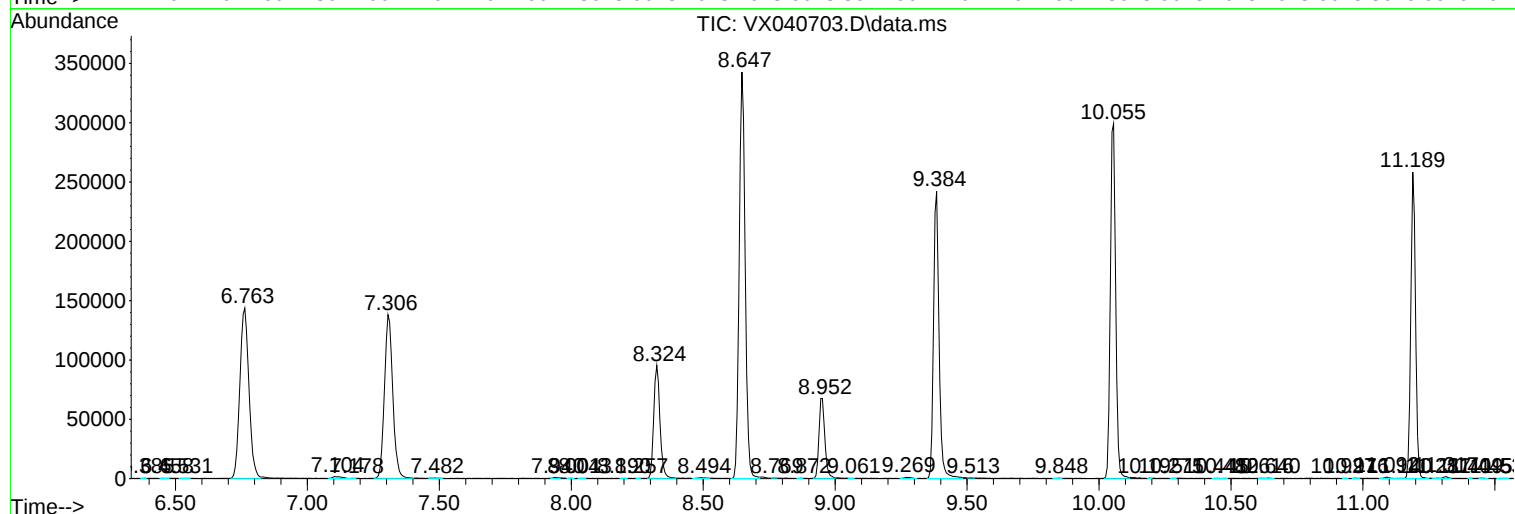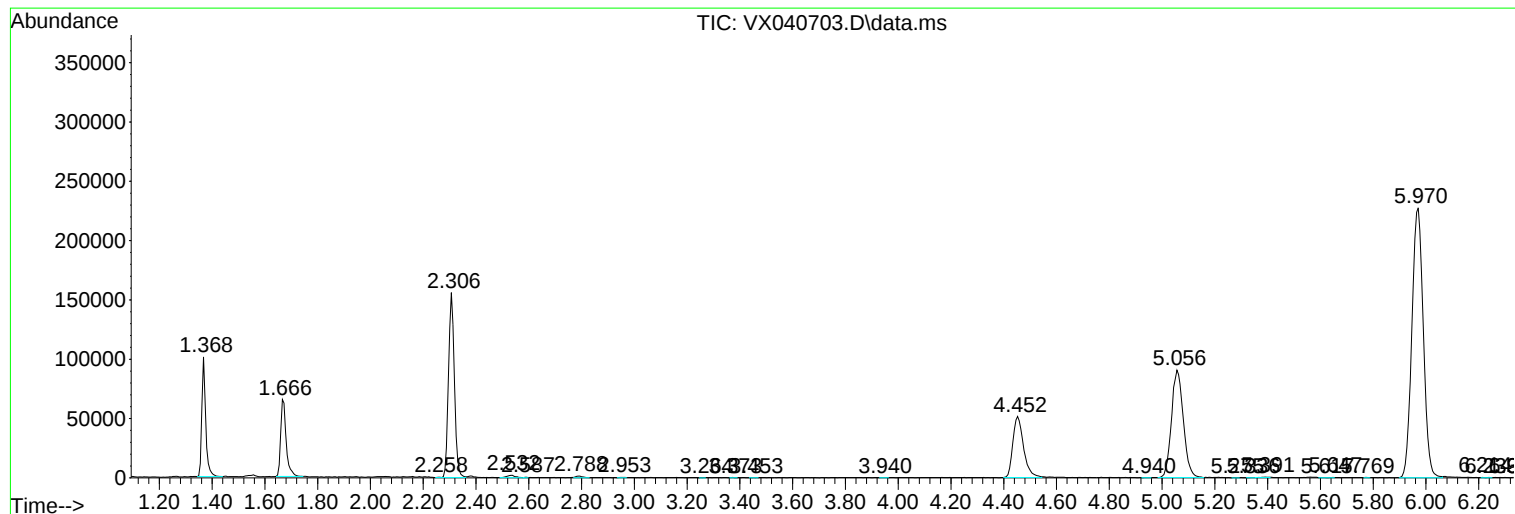

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040703.D
Acq On : 18 Mar 2024 16:45
Operator : JC/MD
Sample : P1753-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040703.D
Acq On : 18 Mar 2024 16:45
Operator : JC/MD
Sample : P1753-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc