

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040706.D
 Acq On : 18 Mar 2024 17:54
 Operator : JC/MD
 Sample : P1754-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	97532	102737	15.08%	2.028%
2	1.666	91	95	110	rBV	57626	87670	12.87%	1.731%
3	2.093	163	165	168	rBV2	458	373	0.05%	0.007%
4	2.306	193	200	209	rBV	154538	241119	35.38%	4.760%
5	2.745	269	272	273	rBV2	157	208	0.03%	0.004%
6	2.788	277	279	283	rVB2	491	589	0.09%	0.012%
7	2.940	302	304	309	rVB2	554	614	0.09%	0.012%
8	3.300	361	363	366	rBV2	145	194	0.03%	0.004%
9	3.337	367	369	372	rVB	202	170	0.02%	0.003%
10	3.751	435	437	440	rBV2	157	168	0.02%	0.003%
11	3.879	456	458	462	rBV2	190	233	0.03%	0.005%
12	4.038	480	484	485	rBV	204	168	0.02%	0.003%
13	4.074	488	490	493	rVB2	168	195	0.03%	0.004%
14	4.111	493	496	497	rBV2	171	220	0.03%	0.004%
15	4.190	508	509	512	rVB	261	213	0.03%	0.004%
16	4.318	527	530	531	rBV2	224	241	0.04%	0.005%
17	4.452	544	552	572	rBV	54835	152628	22.40%	3.013%
18	4.678	587	589	591	rBV2	197	227	0.03%	0.004%
19	4.775	601	605	607	rBV	196	251	0.04%	0.005%
20	5.056	639	651	669	rBV	90269	286326	42.02%	5.652%
21	5.239	679	681	684	rVB	391	299	0.04%	0.006%
22	5.342	696	698	700	rBV	197	166	0.02%	0.003%
23	5.379	702	704	705	rBV2	337	305	0.04%	0.006%
24	5.440	713	714	717	rBV	274	230	0.03%	0.005%
25	5.745	762	764	767	rBV2	167	218	0.03%	0.004%
26	5.970	788	801	815	rBV2	226998	681443	100.00%	13.451%
27	6.165	830	833	835	rBV2	270	257	0.04%	0.005%
28	6.184	835	836	841	rVB2	288	242	0.04%	0.005%
29	6.275	850	851	854	rBV	259	263	0.04%	0.005%
30	6.367	862	866	867	rBV2	146	169	0.02%	0.003%
31	6.452	878	880	883	rVB	203	174	0.03%	0.003%
32	6.482	883	885	888	rBV2	145	217	0.03%	0.004%
33	6.543	892	895	897	rBV	278	289	0.04%	0.006%
34	6.690	918	919	921	rBV2	174	179	0.03%	0.004%
35	6.757	921	930	948	rVV	141662	346223	50.81%	6.834%
36	7.116	983	989	995	rVB3	2084	4570	0.67%	0.090%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040706.D
 Acq On : 18 Mar 2024 17:54
 Operator : JC/MD
 Sample : P1754-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.220	1005	1006	1010	rBV2	169	174	0.03%	0.003%
38	7.305	1012	1020	1034	rBV	138005	304855	44.74%	6.018%
39	7.440	1039	1042	1043	rBV2	206	225	0.03%	0.004%
40	7.653	1075	1077	1079	rVB	285	184	0.03%	0.004%
41	7.677	1079	1081	1084	rBV2	223	302	0.04%	0.006%
42	7.738	1090	1091	1094	rBV	200	225	0.03%	0.004%
43	7.830	1102	1106	1107	rBV	157	214	0.03%	0.004%
44	7.939	1119	1124	1131	rVB4	878	1891	0.28%	0.037%
45	8.019	1135	1137	1141	rVB2	163	199	0.03%	0.004%
46	8.324	1180	1187	1200	rVV	94418	156406	22.95%	3.087%
47	8.488	1210	1214	1218	rBV3	549	869	0.13%	0.017%
48	8.647	1233	1240	1251	rBV	351227	541797	79.51%	10.695%
49	8.884	1278	1279	1281	rBV	307	175	0.03%	0.003%
50	8.951	1284	1290	1302	rBV	70670	105131	15.43%	2.075%
51	9.037	1302	1304	1306	rVB	423	270	0.04%	0.005%
52	9.110	1314	1316	1319	rVB	210	191	0.03%	0.004%
53	9.140	1319	1321	1322	rBV	166	165	0.02%	0.003%
54	9.281	1342	1344	1347	rVB2	275	235	0.03%	0.005%
55	9.323	1347	1351	1352	rBV2	229	305	0.04%	0.006%
56	9.384	1356	1361	1379	rBV	249366	361819	53.10%	7.142%
57	9.665	1404	1407	1408	rBV2	202	237	0.03%	0.005%
58	9.823	1429	1433	1435	rBV2	207	246	0.04%	0.005%
59	9.890	1442	1444	1446	rBV2	150	180	0.03%	0.004%
60	10.055	1465	1471	1485	rBV	309080	432517	63.47%	8.538%
61	10.305	1509	1512	1513	rBV	248	223	0.03%	0.004%
62	10.445	1531	1535	1536	rBV	186	196	0.03%	0.004%
63	10.518	1545	1547	1550	rBV	335	317	0.05%	0.006%
64	10.652	1566	1569	1572	rVB	315	368	0.05%	0.007%
65	10.939	1612	1616	1617	rBV	179	200	0.03%	0.004%
66	11.018	1626	1629	1632	rBV2	254	365	0.05%	0.007%
67	11.085	1637	1640	1646	rBV4	790	1228	0.18%	0.024%
68	11.189	1652	1657	1670	rBV	253951	325964	47.83%	6.434%
69	11.311	1675	1677	1682	rBV3	141	166	0.02%	0.003%
70	11.427	1693	1696	1697	rBV	168	197	0.03%	0.004%
71	11.451	1698	1700	1701	rVV	357	263	0.04%	0.005%
72	11.561	1713	1718	1722	rBV2	224	556	0.08%	0.011%
73	11.847	1763	1765	1767	rBV	169	199	0.03%	0.004%
74	11.963	1781	1784	1785	rBV2	285	231	0.03%	0.005%
75	12.018	1788	1793	1805	rBV	314309	415008	60.90%	8.192%
76	12.201	1821	1823	1826	rVB2	197	193	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
 Data File : VX040706.D
 Acq On : 18 Mar 2024 17:54
 Operator : JC/MD
 Sample : P1754-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1851	rBV	384778	492323	72.25%	9.718%
78	12.737	1905	1911	1912	rBV2	291	362	0.05%	0.007%
79	12.762	1912	1915	1923	rVV3	1257	1779	0.26%	0.035%
80	12.945	1944	1945	1952	rBV2	179	320	0.05%	0.006%
81	13.085	1967	1968	1970	rBV	216	185	0.03%	0.004%
82	13.146	1976	1978	1982	rBV2	134	188	0.03%	0.004%
83	13.365	2012	2014	2018	rVB	207	251	0.04%	0.005%
84	13.725	2071	2073	2076	rVB	351	245	0.04%	0.005%
85	13.786	2079	2083	2085	rBV2	295	404	0.06%	0.008%
86	13.865	2092	2096	2097	rBV2	205	185	0.03%	0.004%
87	13.969	2108	2113	2114	rBV2	352	363	0.05%	0.007%
88	14.133	2136	2140	2144	rVB2	921	1374	0.20%	0.027%
89	14.201	2148	2151	2153	rBV	257	289	0.04%	0.006%
90	14.572	2210	2212	2215	rVB	308	274	0.04%	0.005%
91	14.603	2215	2217	2220	rBV2	149	208	0.03%	0.004%
92	14.761	2241	2243	2246	rBV2	163	181	0.03%	0.004%
93	14.853	2256	2258	2262	rBV3	335	660	0.10%	0.013%
94	14.963	2275	2276	2280	rVV2	175	244	0.04%	0.005%
95	15.048	2287	2290	2292	rBV3	196	215	0.03%	0.004%
96	15.097	2297	2298	2302	rBV2	302	483	0.07%	0.010%
97	15.261	2323	2325	2329	rBV2	221	295	0.04%	0.006%
98	15.377	2342	2344	2345	rBV	426	334	0.05%	0.007%
99	15.462	2355	2358	2361	rBV2	216	305	0.04%	0.006%
100	15.755	2404	2406	2408	rBV	283	191	0.03%	0.004%

Sum of corrected areas: 5065932




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040706.D
Acq On : 18 Mar 2024 17:54
Operator : JC/MD
Sample : P1754-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

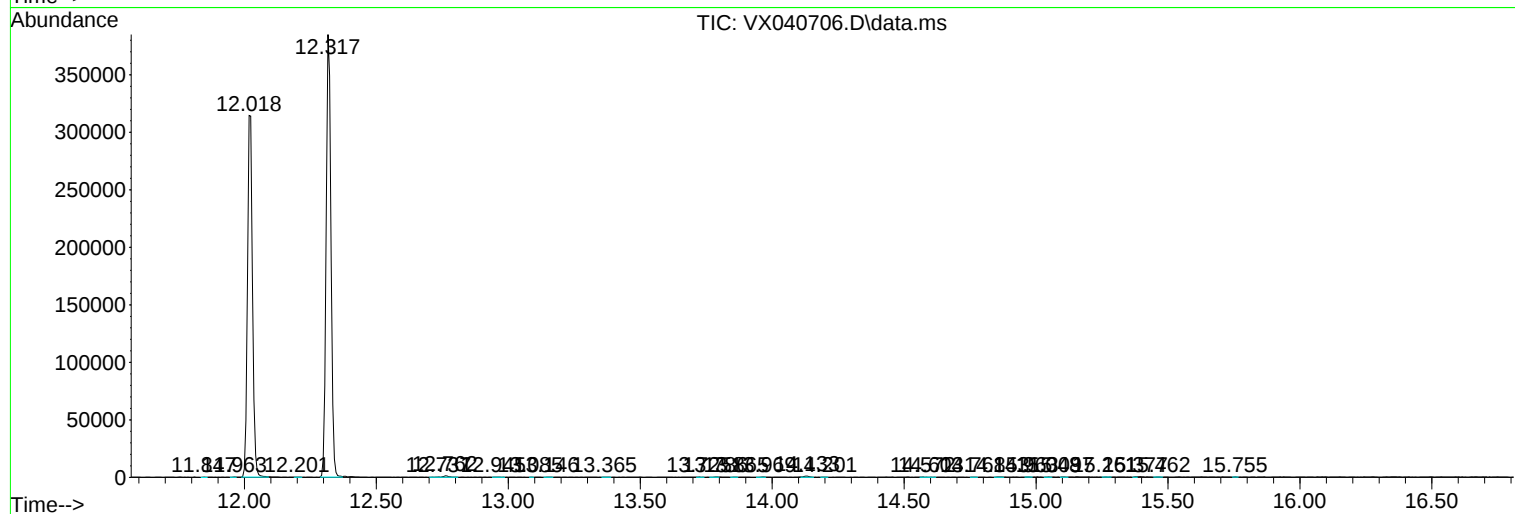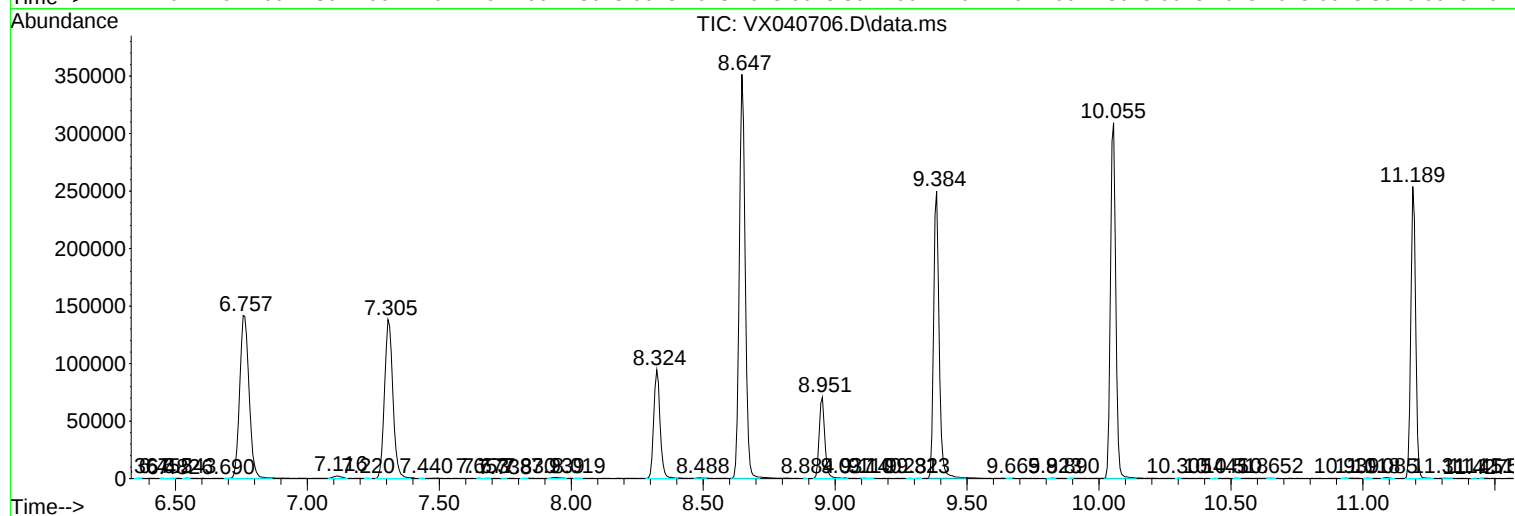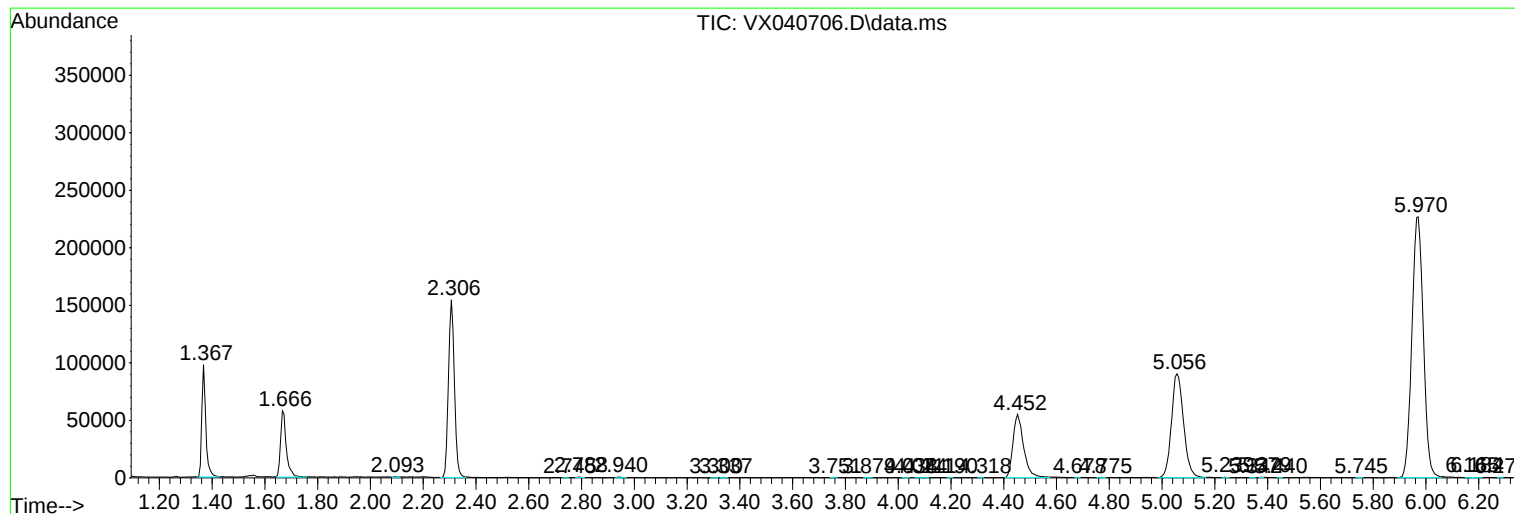

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040706.D
Acq On : 18 Mar 2024 17:54
Operator : JC/MD
Sample : P1754-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040706.D
Acq On : 18 Mar 2024 17:54
Operator : JC/MD
Sample : P1754-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------