
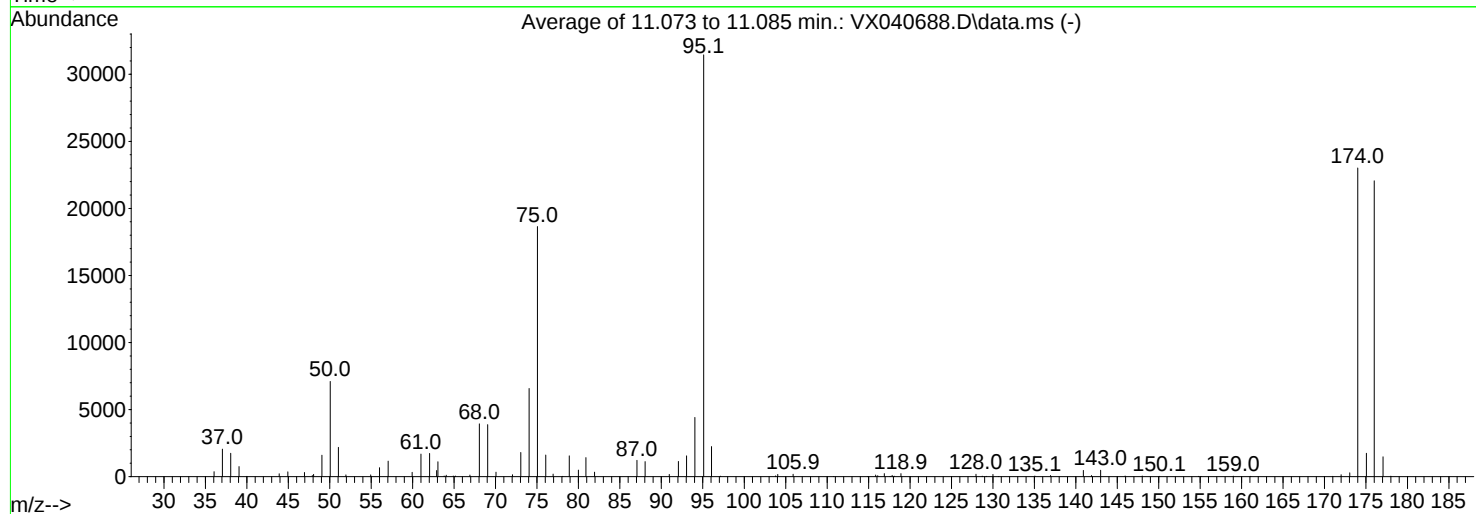


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031824\
Data File : VX040688.D
Acq On : 18 Mar 2024 10:42
Operator : JC/MD
Sample : BFB668
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB668

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM030724WMA.M
Title : VOC Analysis
Last Update : Tue Mar 19 01:22:22 2024

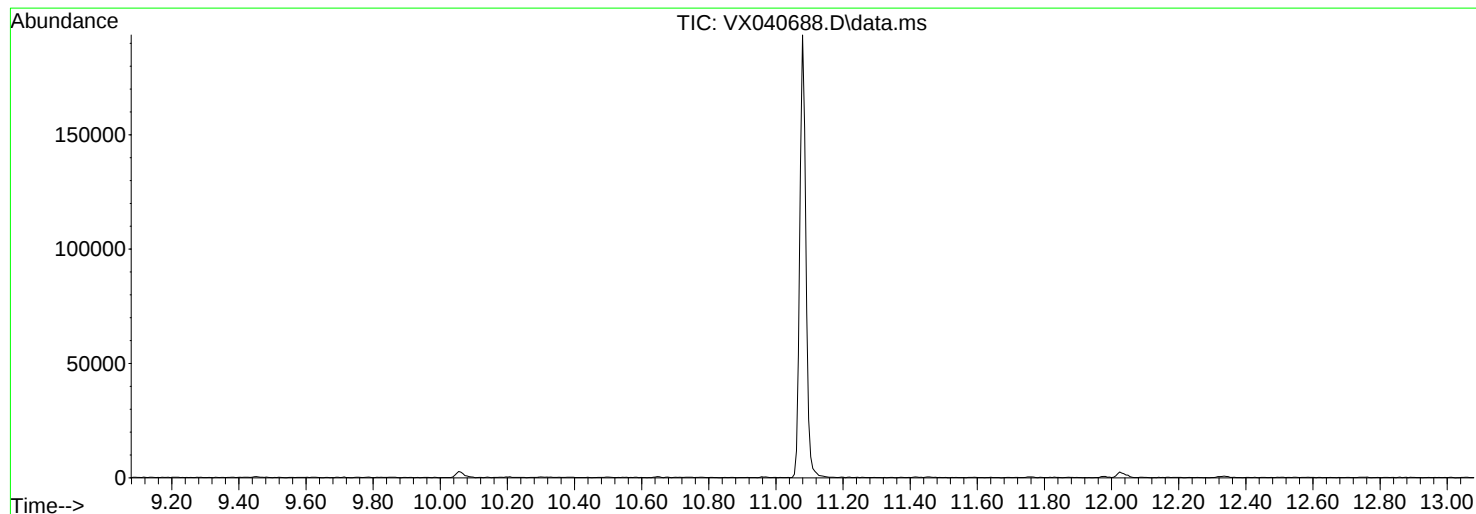

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.6	7101	PASS
75	95	30	80	59.3	18645	PASS
95	95	100	100	100.0	31451	PASS
96	95	5	9	7.1	2240	PASS
173	174	0.00	2	1.3	291	PASS
174	95	50	120	73.2	23016	PASS
175	174	5	9	7.6	1740	PASS
176	174	95	101	95.9	22067	PASS
177	176	5	9	6.7	1477	PASS

m/z	Abundance
40.10	138.0
43.80	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB668

m/z	Abundance
36.10	407.0
37.10	2067.0
38.00	1910.0
39.00	722.0
40.00	196.0
44.10	243.0
45.00	350.0
46.90	357.0
47.90	236.0
49.10	1594.0
50.00	6683.0
51.00	2260.0
51.90	124.0
55.00	186.0
55.90	678.0
57.10	1118.0
60.00	249.0
61.00	1460.0
62.00	1567.0
62.90	1364.0
63.80	138.0
65.20	78.0
66.90	93.0
68.10	3438.0
69.10	3491.0
70.20	327.0
72.10	79.0
73.10	1412.0
74.00	5938.0
75.10	17152.0
76.00	1677.0
77.00	161.0
78.90	1489.0
80.10	477.0
80.90	1441.0
82.00	337.0
87.00	1078.0
88.10	881.0
90.90	157.0
92.10	1104.0
93.10	1501.0
94.10	3517.0
95.10	27192.0
96.10	1985.0
104.10	187.0
105.90	157.0
115.80	203.0
117.00	217.0
118.00	107.0
118.90	235.0
128.00	134.0
130.00	142.0
136.90	74.0
140.90	355.0
142.00	55.0
143.00	374.0
145.90	60.0
154.80	61.0
172.10	102.0
173.10	147.0
174.00	16464.0
175.00	1246.0
176.00	16360.0
177.00	1012.0
178.00	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB668

m/z	Abundance
36.00	344.0
37.00	2379.0
38.00	1975.0
39.10	904.0
40.00	129.0
43.90	259.0
44.90	413.0
47.00	305.0
48.10	294.0
49.00	1889.0
50.10	8354.0
51.10	2325.0
52.00	144.0
54.90	103.0
56.00	875.0
57.00	1287.0
60.00	470.0
61.00	2101.0
62.00	2125.0
63.10	2049.0
64.10	224.0
64.90	158.0
66.90	130.0
68.10	4828.0
69.10	4752.0
70.00	372.0
72.10	207.0
73.00	2438.0
74.00	8141.0
75.10	22256.0
76.10	1927.0
77.00	169.0
78.10	87.0
78.90	1757.0
79.90	582.0
80.90	1788.0
81.90	422.0
87.10	1412.0
88.10	1302.0
91.00	205.0
92.00	1331.0
93.10	1858.0
94.10	5468.0
95.10	38264.0
96.00	2745.0
97.20	51.0
104.00	300.0
105.80	226.0
110.80	50.0
114.90	53.0
116.10	200.0
116.90	218.0
117.80	189.0
118.90	277.0
128.00	184.0
129.20	68.0
130.00	202.0
130.70	52.0
135.00	88.0
137.00	117.0
140.90	539.0
141.90	116.0
143.00	489.0
146.00	105.0
148.00	65.0
155.10	92.0
159.00	97.0
171.90	212.0
173.10	445.0
174.00	27264.0
175.10	2131.0
176.00	26368.0
177.10	1862.0

Instrument :
MSVOA_X
ClientSampleId :
BFB668

m/z	Abundance
36.00	369.0
37.10	1723.0
38.10	1359.0
39.00	620.0
40.00	175.0
43.90	300.0
44.90	310.0
47.00	271.0
48.00	199.0
49.00	1324.0
50.10	6266.0
51.00	1966.0
52.00	126.0
54.90	106.0
56.10	442.0
57.00	1085.0
59.80	239.0
61.00	1497.0
62.10	1506.0
63.00	1284.0
64.00	104.0
65.10	82.0
66.90	140.0
68.00	3561.0
69.00	3398.0
70.00	304.0
71.90	130.0
73.10	1562.0
74.10	5638.0
75.00	16528.0
76.00	1232.0
76.90	256.0
78.90	1413.0
80.00	395.0
80.90	1049.0
81.90	257.0
87.00	1150.0
88.00	1181.0
91.00	134.0
92.10	973.0
93.00	1289.0
94.00	4257.0
95.10	28896.0
96.10	1990.0
97.10	53.0
103.80	191.0
106.00	138.0
115.90	151.0
116.80	232.0
117.60	89.0
118.10	116.0
118.90	184.0
127.90	229.0
128.70	100.0
130.00	143.0
135.10	55.0
137.00	67.0
140.90	492.0
141.80	66.0
143.00	586.0
148.00	81.0
150.10	71.0
161.10	61.0
171.00	62.0
172.10	134.0
173.00	282.0
174.00	25320.0
175.00	1844.0
176.00	23472.0
177.00	1558.0
178.00	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB668