


Acrolein

Response Ratio

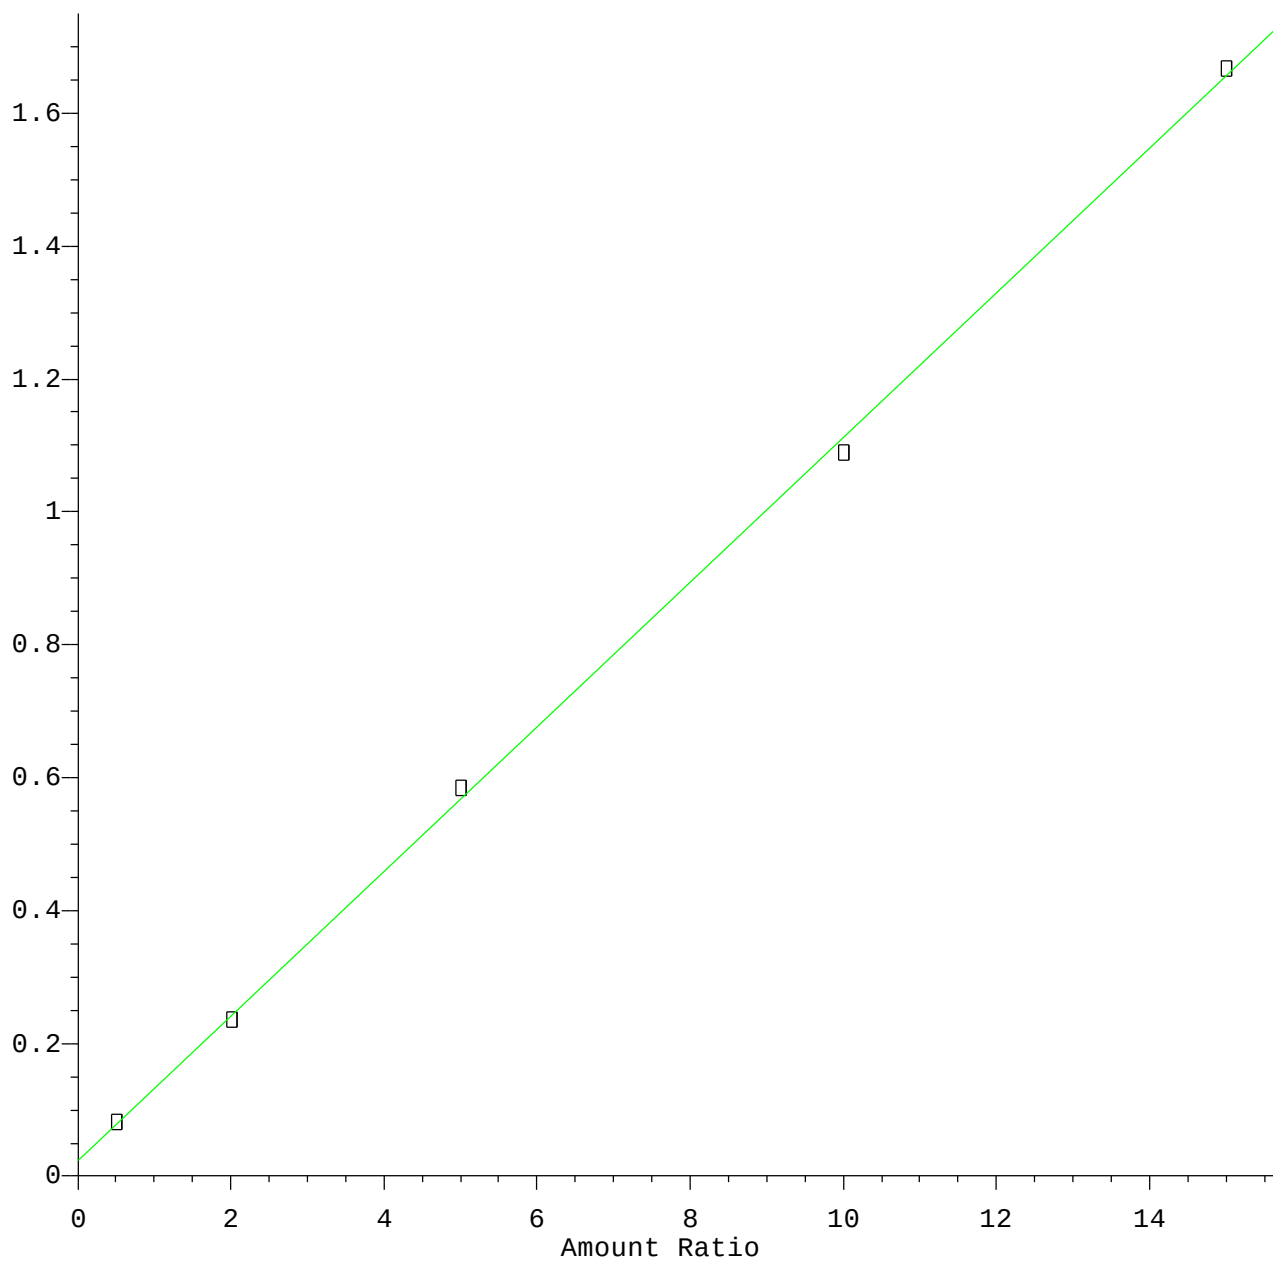


Resp Ratio = 1.09e-001 * Amt + 2.37e-002
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019


trans-1,4-Dichloro-2-butene

Response Ratio

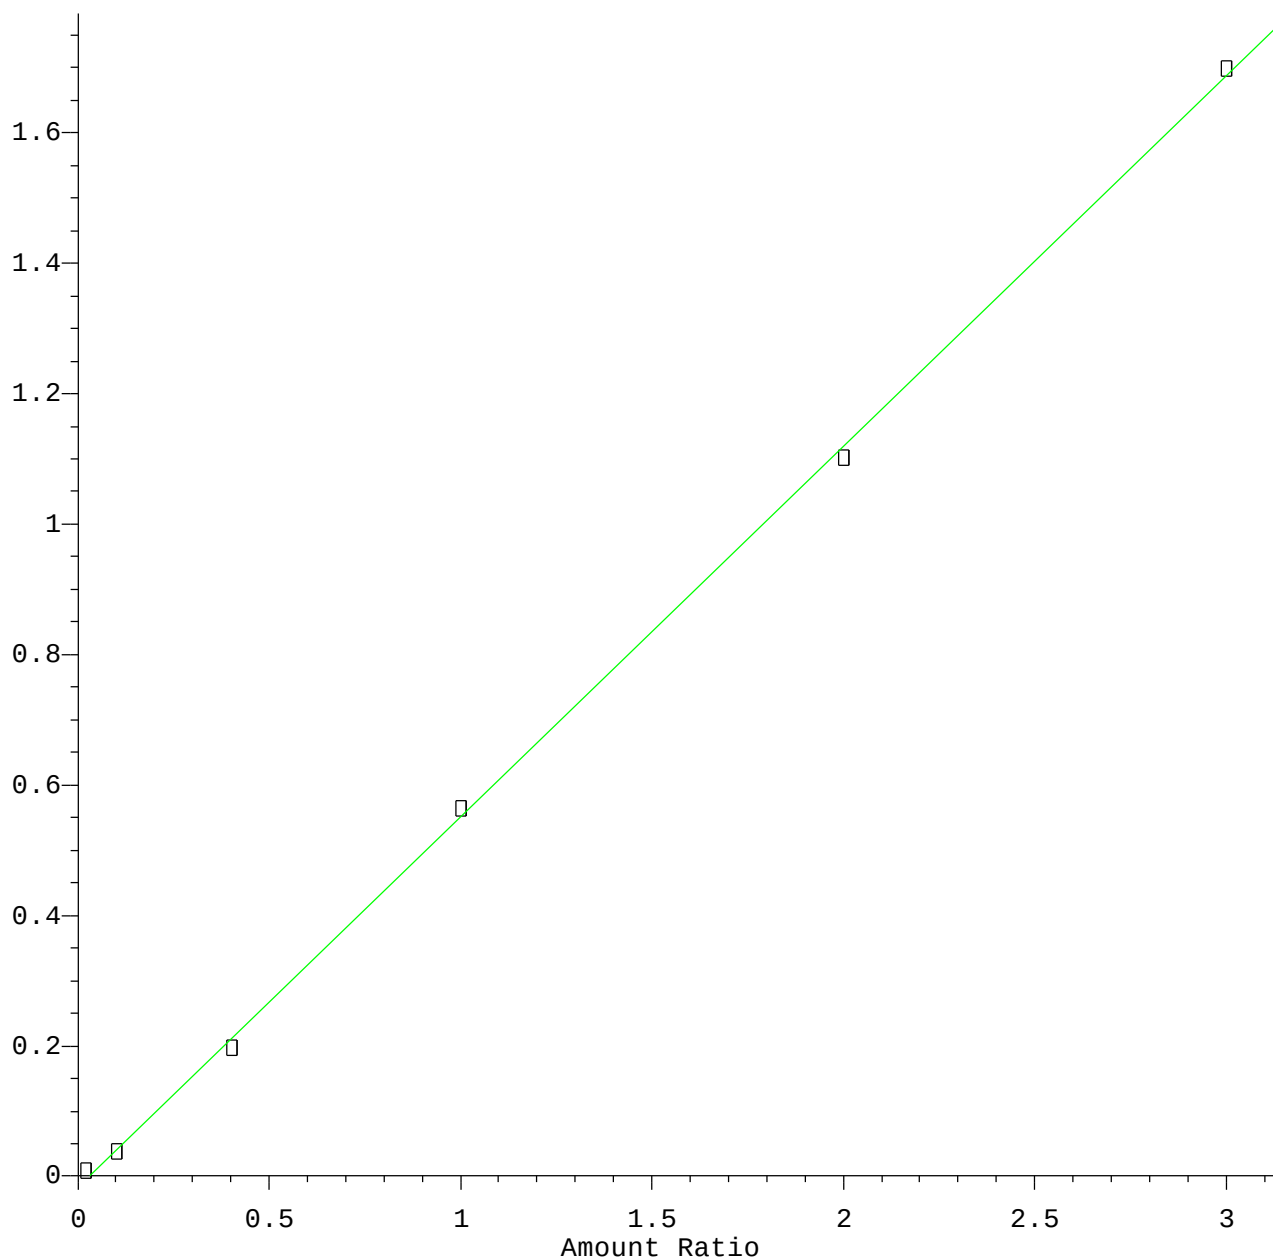


Resp Ratio = 5.68e-001 * Amt - 1.63e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019

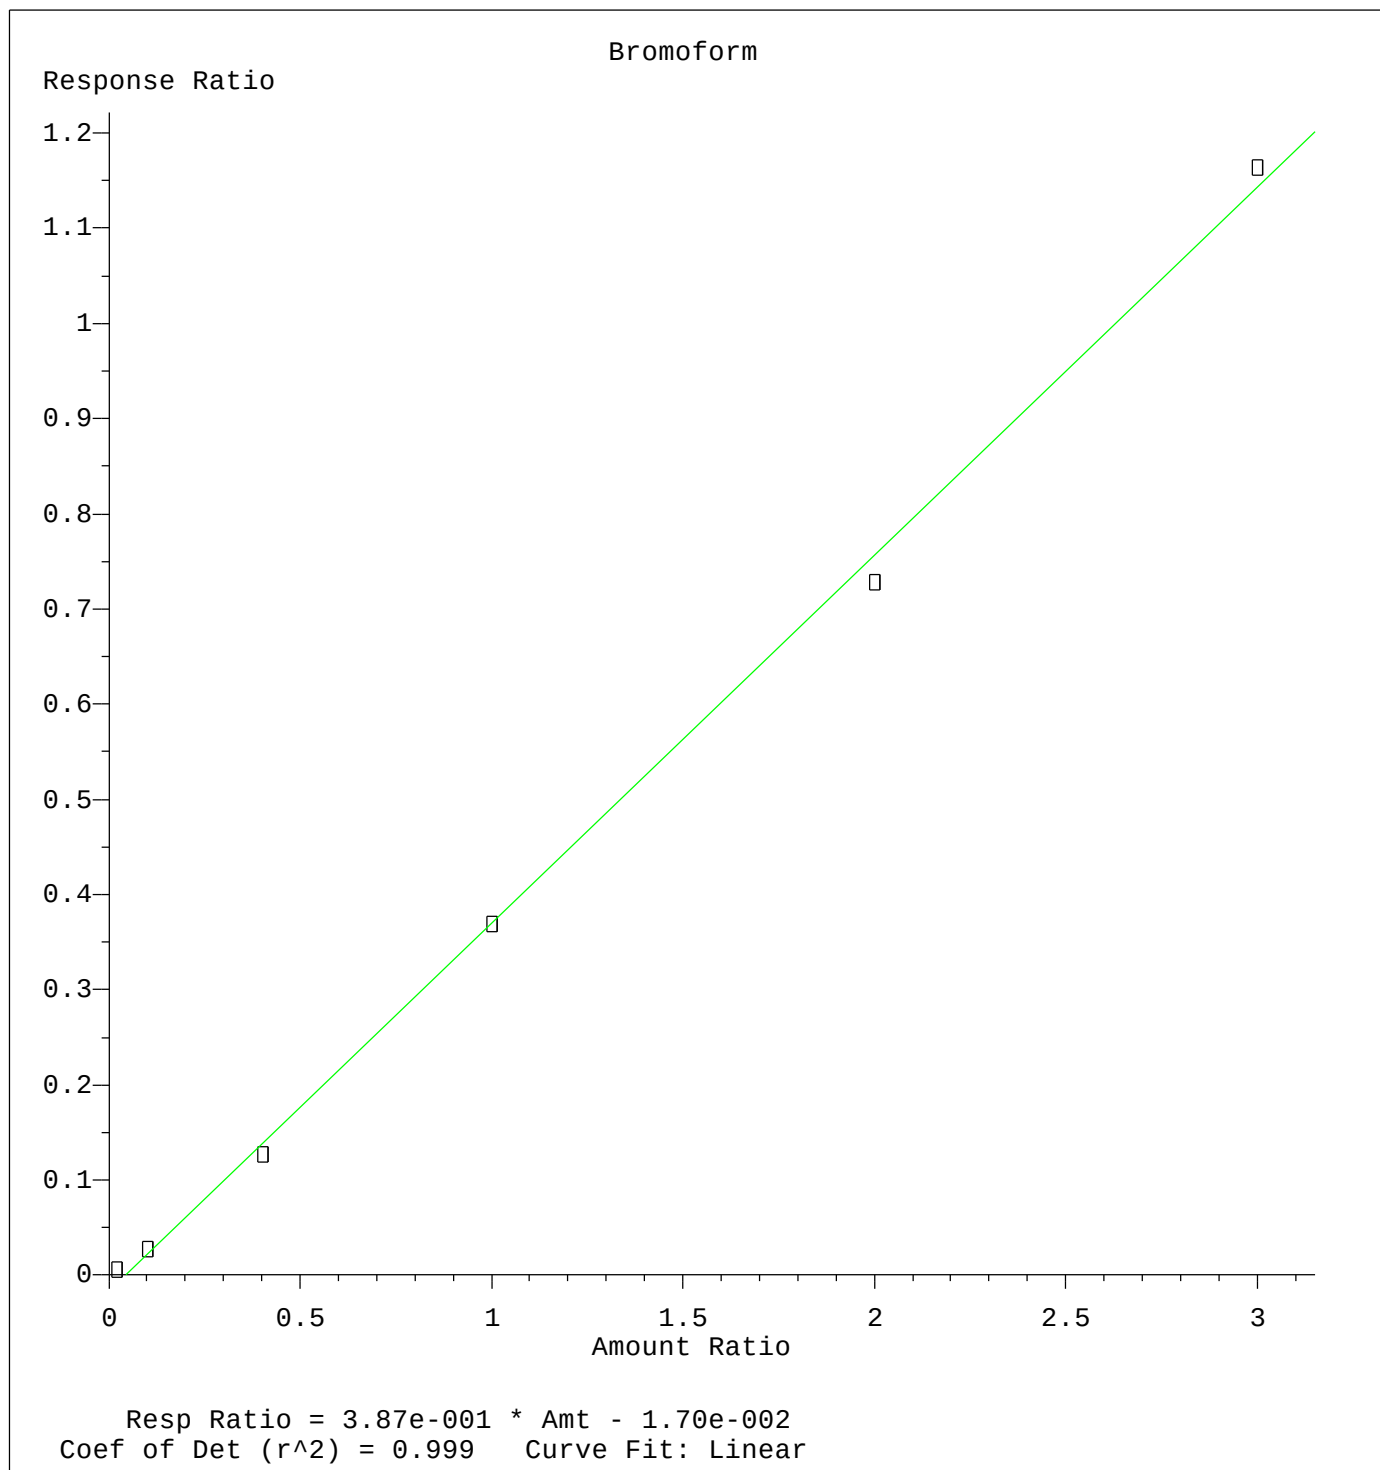


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019

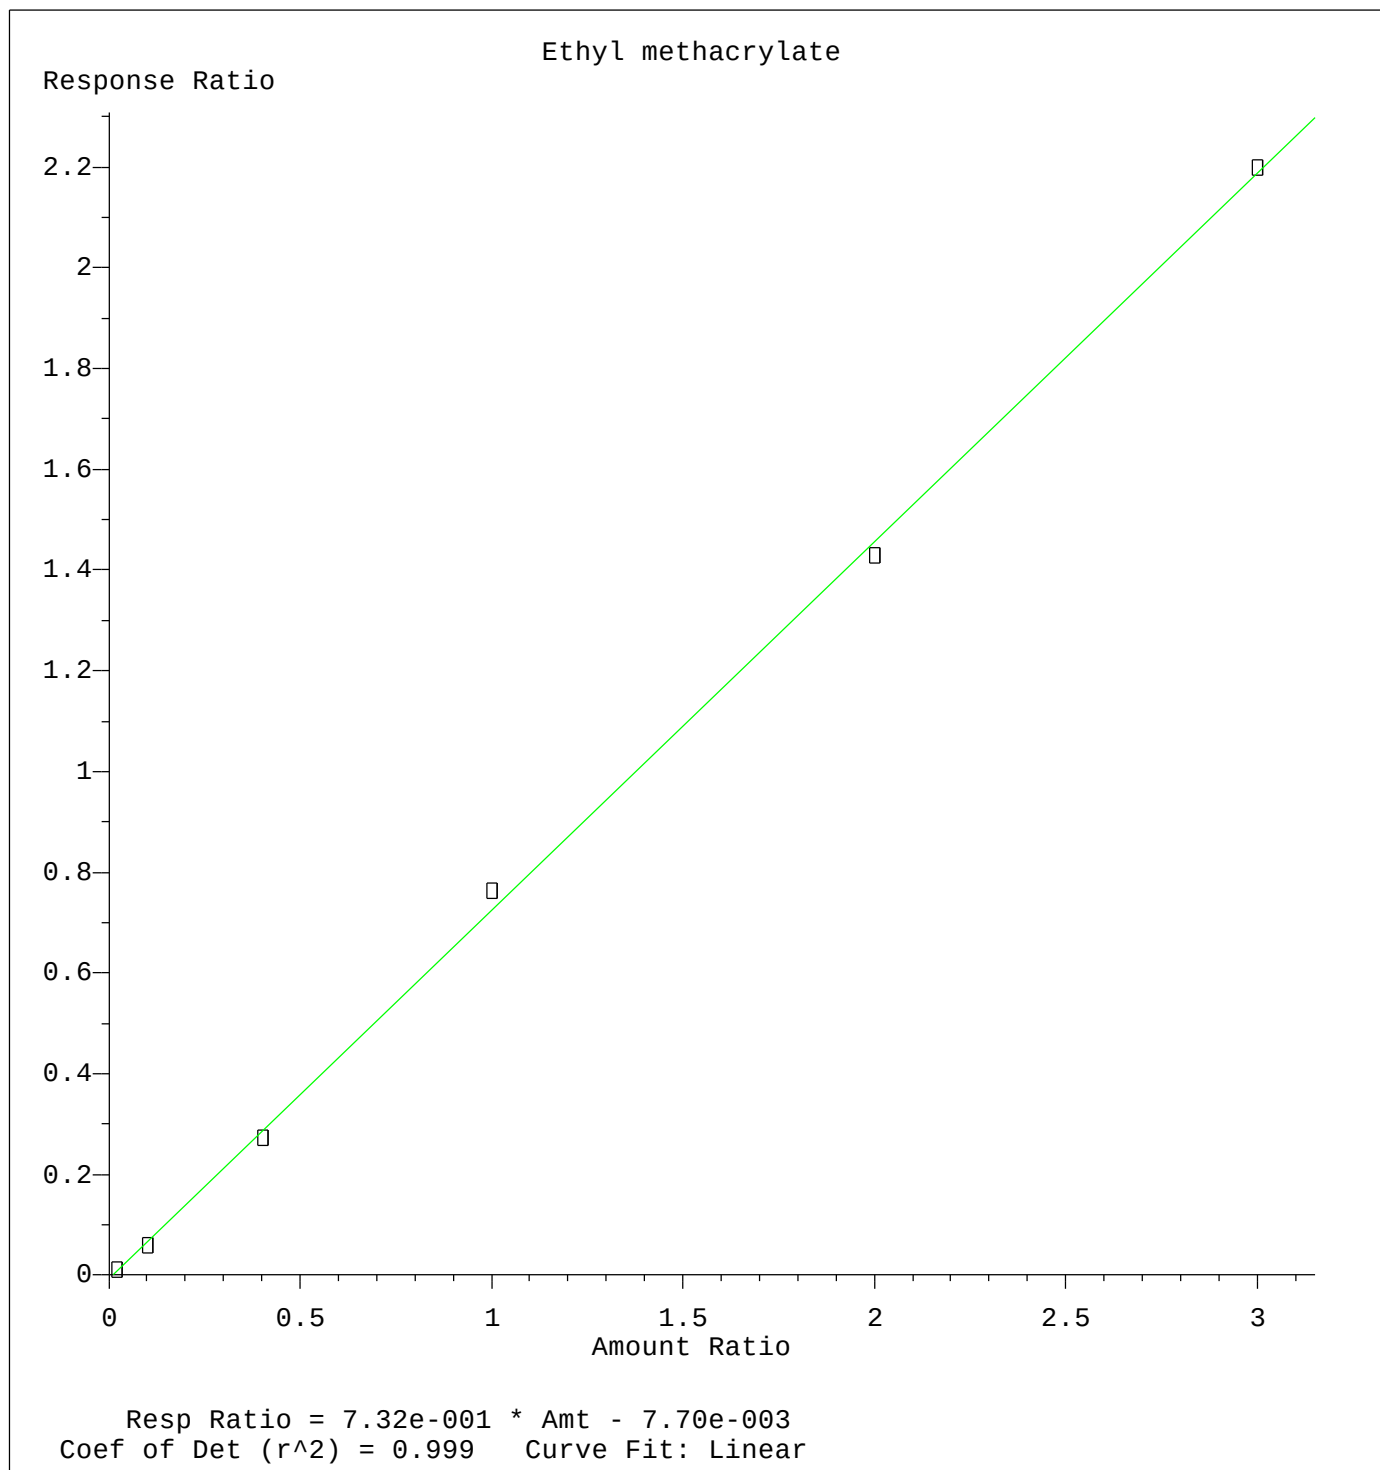

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019


t-1,3-Dichloropropene

Response Ratio

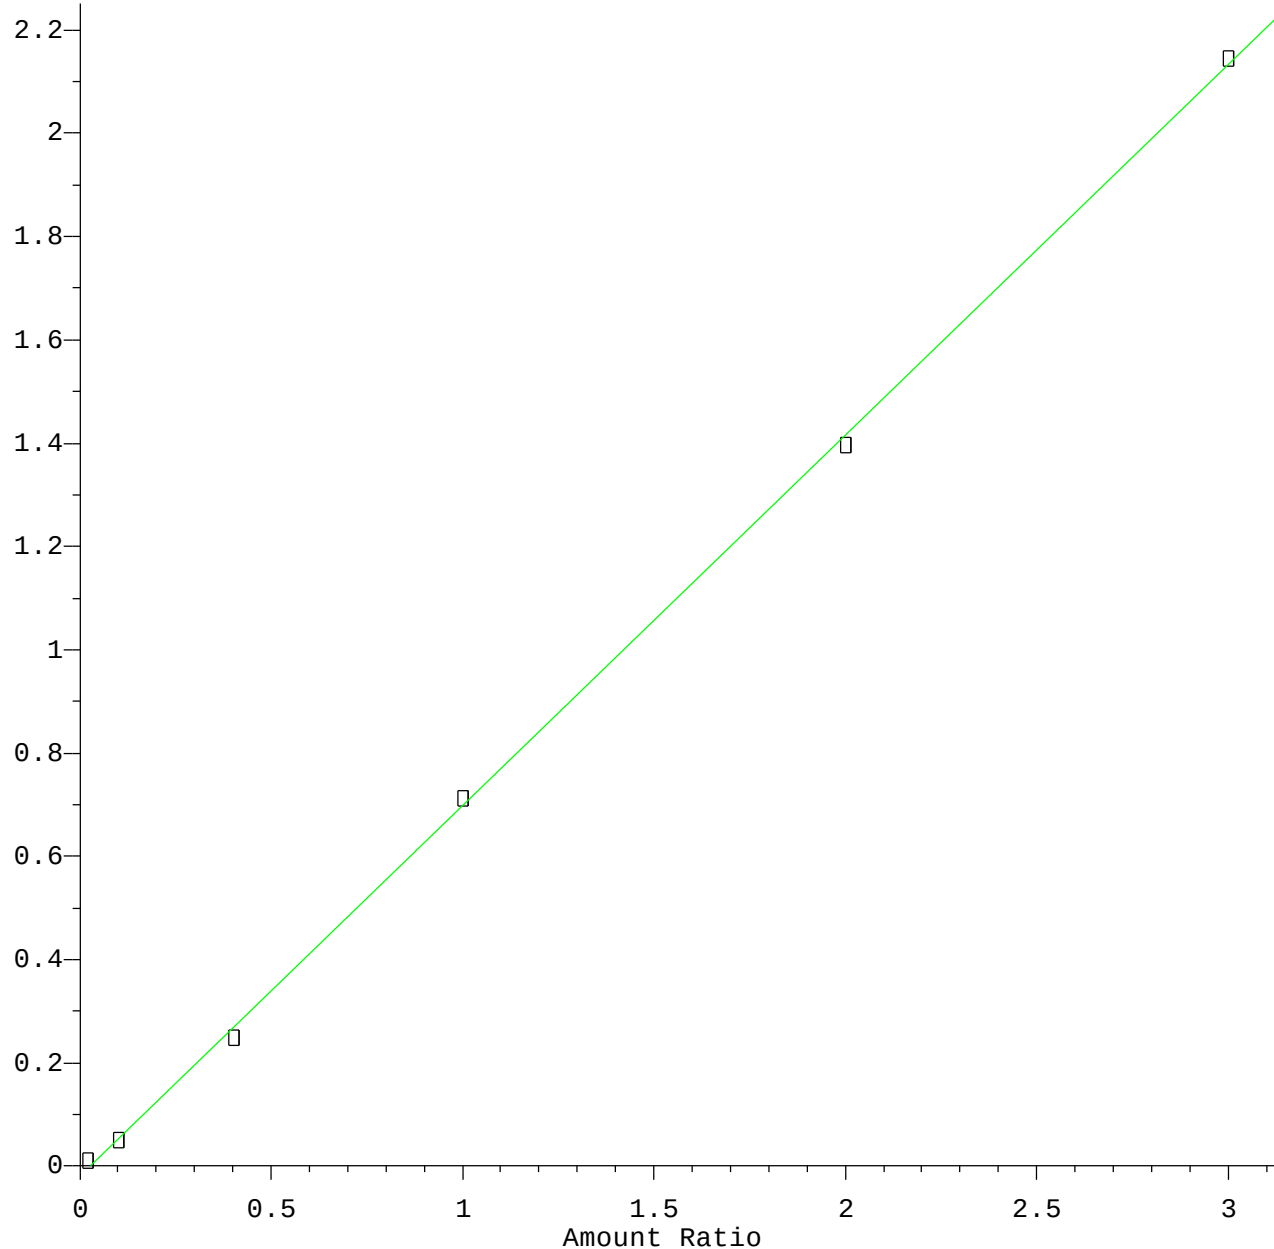

Resp Ratio = $7.17 \times 10^{-1} \times \text{Amt} - 2.04 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019

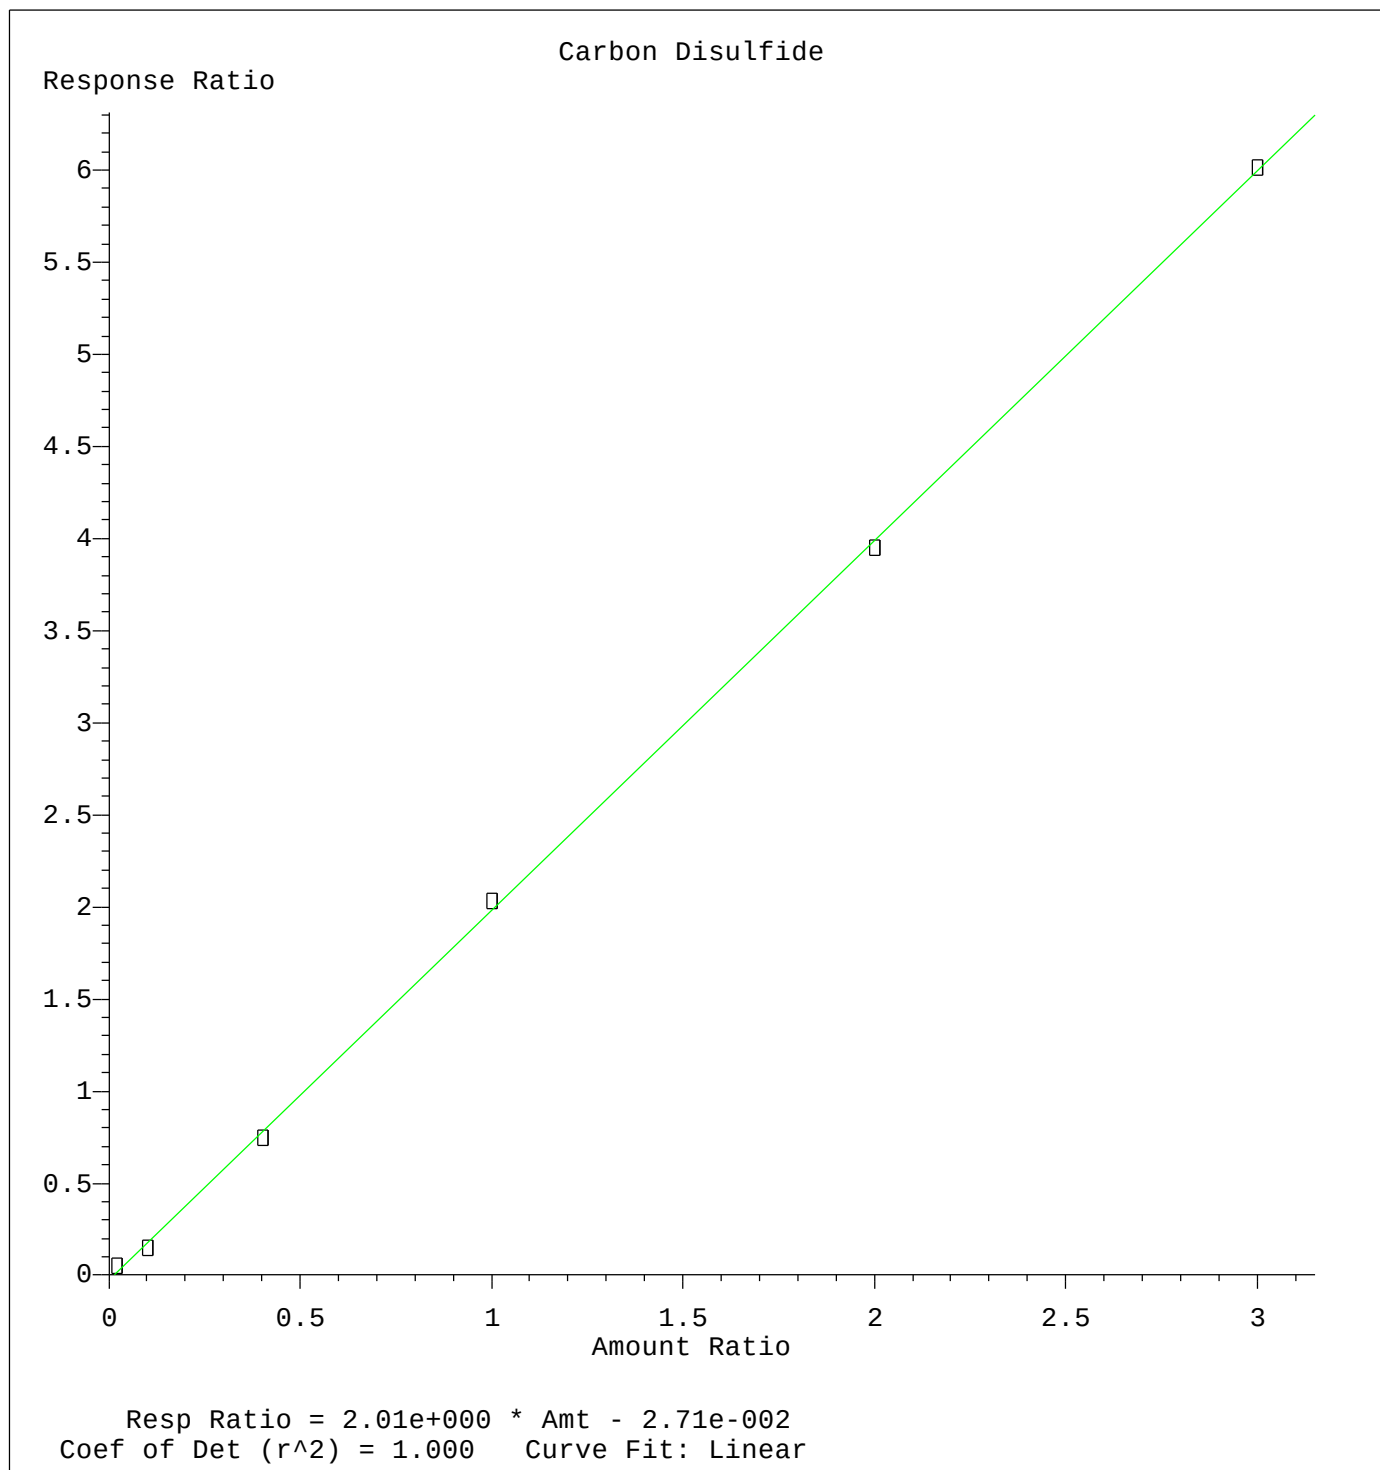

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Calibration Table Last Updated: Tue Mar 19 13:15:13 2019