

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031919\  
Data File : VX008216.D  
Acq On : 20 Mar 2019 02:47  
Operator : JC/SP  
Sample : K1900-03  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW30411-20190312

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X031919W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.611       | 67            | 75          | 79           | rVB3     | 21177          | 44528         | 2.54%           | 0.503%        |
| 2         | 5.501       | 700           | 713         | 727          | rBV      | 198371         | 562591        | 32.15%          | 6.360%        |
| 3         | 5.665       | 728           | 740         | 753          | rVB      | 349424         | 975209        | 55.73%          | 11.025%       |
| 4         | 6.061       | 795           | 805         | 822          | rBV      | 238604         | 631373        | 36.08%          | 7.138%        |
| 5         | 6.860       | 925           | 936         | 948          | rBV      | 553894         | 1290948       | 73.77%          | 14.594%       |
| 6         | 8.713       | 1233          | 1240        | 1249         | rBV      | 1139697        | 1749934       | 100.00%         | 19.783%       |
| 7         | 10.110      | 1463          | 1469        | 1481         | rBV      | 1029077        | 1421298       | 81.22%          | 16.068%       |
| 8         | 11.134      | 1630          | 1637        | 1648         | rBV      | 791036         | 1025169       | 58.58%          | 11.589%       |
| 9         | 12.079      | 1785          | 1792        | 1800         | rBV      | 901058         | 1144684       | 65.41%          | 12.941%       |


Sum of corrected areas: 8845734

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031919\  
Data File : VX008216.D  
Acq On : 20 Mar 2019 02:47  
Operator : JC/SP  
Sample : K1900-03  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW30411-20190312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X031919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

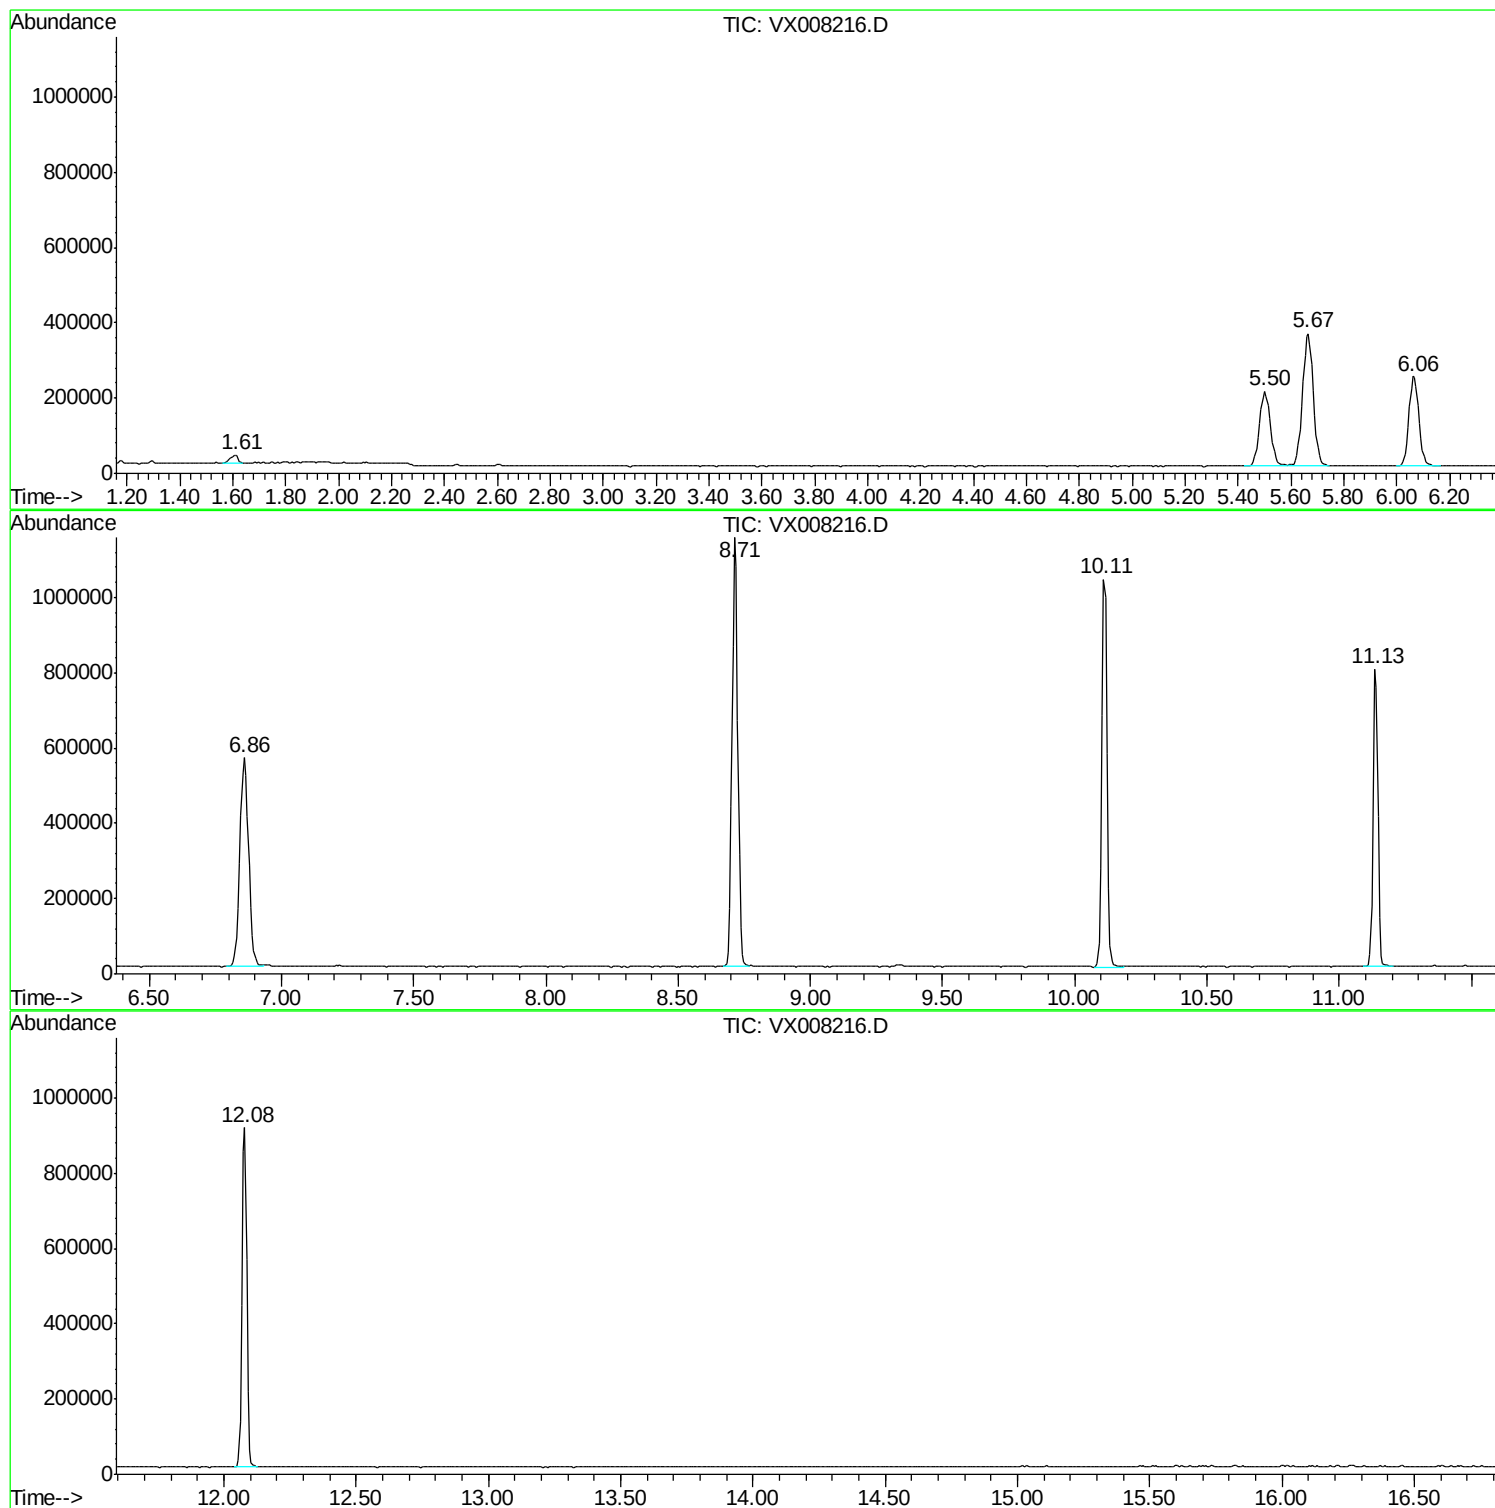

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX031919\  
Data File : VX008216.D  
Acq On : 20 Mar 2019 02:47  
Operator : JC/SP  
Sample : K1900-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW30411-20190312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X031919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX031919\  
Data File : VX008216.D  
Acq On : 20 Mar 2019 02:47  
Operator : JC/SP  
Sample : K1900-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW30411-20190312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X031919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |