


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX031919\
Data File : VX008178.D
Acq On : 19 Mar 2019 09:14
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Title : SW846 8260
Last Update : Tue Mar 19 13:15:13 2019

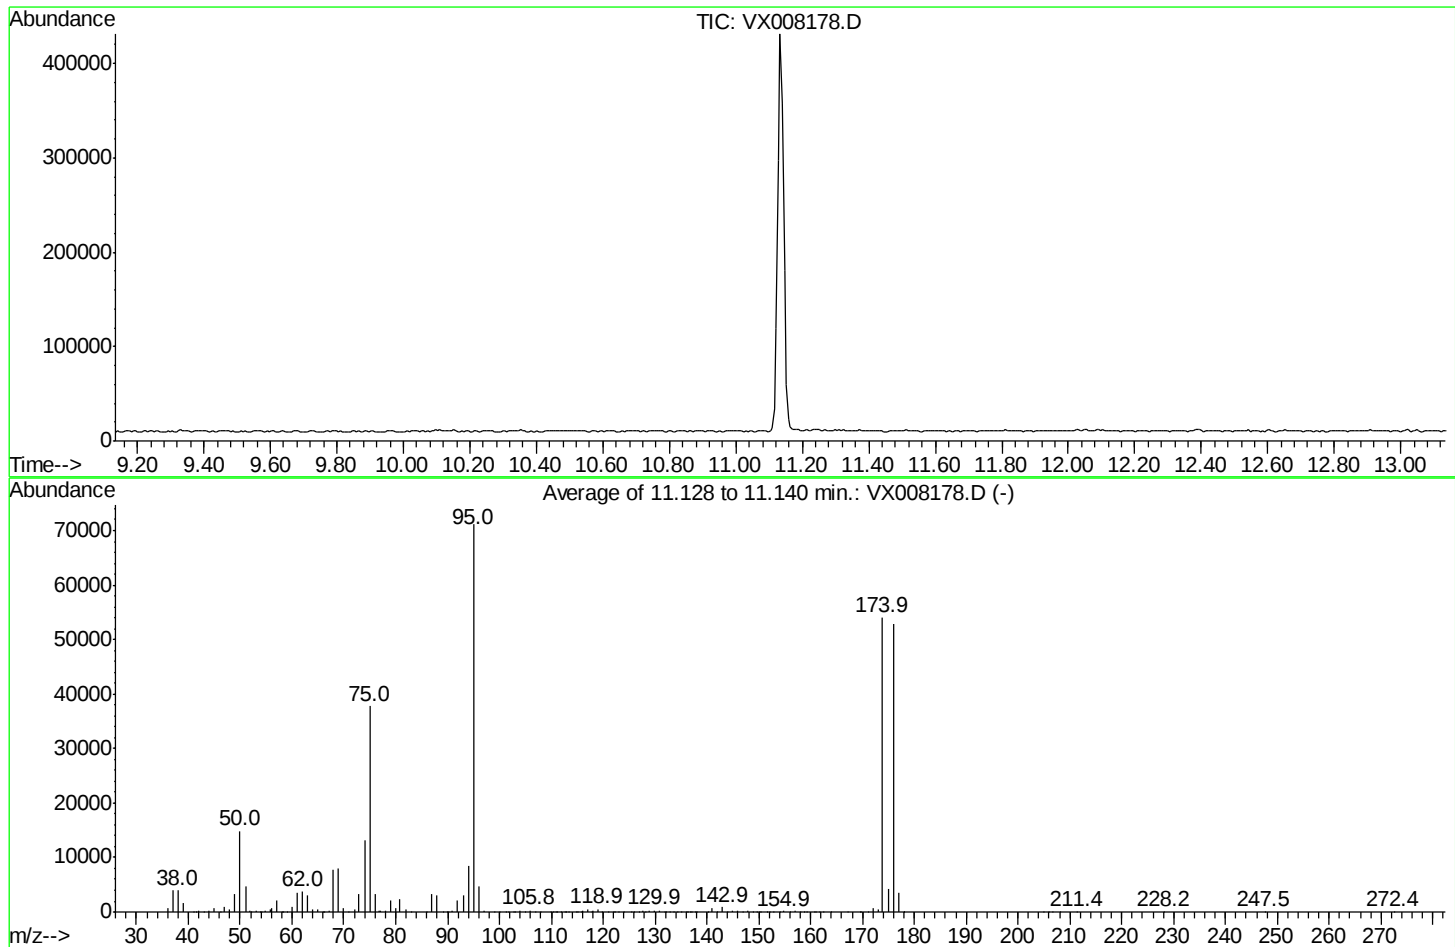

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	14879	PASS
75	95	30	60	53.0	37725	PASS
95	95	100	100	100.0	71136	PASS
96	95	5	9	6.6	4679	PASS
173	174	0.00	2	0.9	496	PASS
174	95	50	100	75.9	54005	PASS
175	174	5	9	7.8	4236	PASS
176	174	95	101	97.9	52846	PASS
177	176	5	9	6.6	3511	PASS