

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021287.D
 Acq On : 18 Mar 2021 19:17
 Operator : JC/MD
 Sample : M1715-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210317058-01-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX021287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.581	80	84	86	rBV	4050	5739	1.99%	0.199%
2	1.870	130	133	139	rVB	2995	3945	1.37%	0.137%
3	2.170	178	184	192	rBV	13163	19873	6.89%	0.688%
4	2.428	220	228	233	rBV2	19086	36542	12.67%	1.265%
5	2.464	233	234	244	rVV2	7859	17098	5.93%	0.592%
6	3.011	317	327	340	rBV	55649	124486	43.17%	4.308%
7	3.170	346	354	362	rVB3	2493	6847	2.37%	0.237%
8	4.658	593	607	621	rBV2	68902	227895	79.03%	7.887%
9	4.982	651	662	672	rBV2	38634	117457	40.73%	4.065%
10	5.093	672	681	696	rVB	87115	263669	91.43%	9.125%
11	6.029	830	840	849	rBV	43275	113783	39.46%	3.938%
12	6.111	849	854	864	rVB2	7819	19879	6.89%	0.688%
13	6.305	875	887	898	rBV3	3334	9473	3.28%	0.328%
14	6.423	898	907	919	rVB9	2726	9735	3.38%	0.337%
15	6.829	967	976	991	rBV	91209	215761	74.82%	7.467%
16	7.511	1084	1092	1098	rVB	5882	12023	4.17%	0.416%
17	7.711	1117	1126	1135	rBV	7643	16135	5.60%	0.558%
18	7.953	1161	1167	1175	rBV4	4797	9388	3.26%	0.325%
19	8.470	1249	1255	1261	rVB4	1331	3071	1.06%	0.106%
20	8.547	1261	1268	1271	rBV5	1760	3059	1.06%	0.106%
21	8.594	1272	1276	1286	rVV3	3329	8117	2.81%	0.281%
22	8.694	1286	1293	1300	rVV	184220	288377	100.00%	9.980%
23	8.765	1300	1305	1314	rVV3	9445	20033	6.95%	0.693%
24	8.847	1314	1319	1328	rVV	7988	14683	5.09%	0.508%
25	8.941	1328	1335	1342	rVB3	2572	4433	1.54%	0.153%
26	9.282	1388	1393	1397	rBV2	4077	6453	2.24%	0.223%
27	9.418	1408	1416	1422	rBV	9859	15786	5.47%	0.546%
28	9.476	1422	1426	1430	rVV3	1978	3518	1.22%	0.122%
29	9.529	1430	1435	1442	rVV	12947	20254	7.02%	0.701%
30	9.600	1442	1447	1452	rVB5	2883	5135	1.78%	0.178%
31	9.835	1481	1487	1491	rBV5	2288	3610	1.25%	0.125%
32	9.982	1507	1512	1519	rBV	3643	5410	1.88%	0.187%
33	10.094	1519	1531	1534	rBV	187956	285279	98.93%	9.873%
34	10.235	1550	1555	1561	rBV2	8911	17310	6.00%	0.599%
35	10.341	1568	1573	1580	rBV	28149	40836	14.16%	1.413%
36	10.412	1580	1585	1597	rVB3	3413	6550	2.27%	0.227%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021287.D
 Acq On : 18 Mar 2021 19:17
 Operator : JC/MD
 Sample : M1715-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210317058-01-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

37	10.682	1626	1631	1637	rBV	23989	31952	11.08%	1.106%
38	10.806	1650	1652	1656	rVB3	2720	3310	1.15%	0.115%
39	10.912	1663	1670	1672	rBV7	1473	3334	1.16%	0.115%
40	11.000	1679	1685	1690	rVB2	11226	16189	5.61%	0.560%
41	11.118	1700	1705	1711	rBV	157240	206201	71.50%	7.136%
42	11.212	1719	1721	1727	rVB7	2318	3008	1.04%	0.104%
43	11.271	1727	1731	1735	rBV4	2267	2913	1.01%	0.101%
44	11.341	1739	1743	1746	rVV2	5605	7265	2.52%	0.251%
45	11.412	1750	1755	1763	rVB3	6916	13745	4.77%	0.476%
46	11.488	1763	1768	1773	rVB2	4243	5903	2.05%	0.204%
47	11.541	1773	1777	1784	rVB4	2023	3069	1.06%	0.106%
48	11.606	1784	1788	1792	rBV4	3311	4977	1.73%	0.172%
49	11.653	1792	1796	1805	rVB	14121	19536	6.77%	0.676%
50	11.788	1807	1819	1824	rBV	19953	27664	9.59%	0.957%
51	11.841	1824	1828	1835	rBV6	1541	3425	1.19%	0.119%
52	11.924	1837	1842	1850	rVB	19242	25908	8.98%	0.897%
53	12.006	1850	1856	1858	rBV6	2715	3936	1.36%	0.136%
54	12.047	1858	1863	1865	rVV3	9995	14620	5.07%	0.506%
55	12.083	1865	1869	1873	rVB	67234	85745	29.73%	2.968%
56	12.130	1873	1877	1882	rBV2	11276	17987	6.24%	0.623%
57	12.177	1882	1885	1889	rVB6	1888	3147	1.09%	0.109%
58	12.283	1896	1903	1907	rBV2	35629	47655	16.53%	1.649%
59	12.371	1912	1918	1927	rVB5	7138	13671	4.74%	0.473%
60	12.447	1927	1931	1937	rBV5	6500	12135	4.21%	0.420%
61	12.577	1948	1953	1961	rVB3	4939	11090	3.85%	0.384%
62	12.653	1961	1966	1970	rVB	6924	8369	2.90%	0.290%
63	12.712	1970	1976	1978	rBV4	3989	6289	2.18%	0.218%
64	12.742	1978	1981	1988	rVB5	3827	6011	2.08%	0.208%
65	12.800	1988	1991	1995	rVB4	3807	5635	1.95%	0.195%
66	12.947	2011	2016	2021	rVV2	37727	51266	17.78%	1.774%
67	13.000	2021	2025	2029	rVB6	8338	12797	4.44%	0.443%
68	13.165	2049	2053	2056	rVV4	3112	4367	1.51%	0.151%
69	13.200	2056	2059	2065	rVV5	3384	6578	2.28%	0.228%
70	13.271	2065	2071	2074	rVV6	2925	4080	1.41%	0.141%
71	13.324	2076	2080	2085	rVV3	15299	20637	7.16%	0.714%
72	13.371	2085	2088	2092	rVV4	5301	7367	2.55%	0.255%
73	13.465	2099	2104	2107	rVB2	9063	10884	3.77%	0.377%
74	13.512	2107	2112	2116	rBV2	19547	28545	9.90%	0.988%
75	13.553	2116	2119	2127	rVB3	10100	13590	4.71%	0.470%
76	13.630	2127	2132	2135	rBV4	3638	5687	1.97%	0.197%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021287.D
 Acq On : 18 Mar 2021 19:17
 Operator : JC/MD
 Sample : M1715-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210317058-01-VOA

Integration Parameters: RTEINT3.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

77	13.700	2142	2144	2151	rVB7	1928	3906	1.35%	0.135%
78	13.818	2158	2164	2169	rVB	38284	49472	17.16%	1.712%
79	13.906	2173	2179	2184	rVB2	3919	7650	2.65%	0.265%
80	13.965	2184	2189	2197	rBV6	6554	14311	4.96%	0.495%
81	14.136	2211	2218	2222	rBV6	2238	4310	1.49%	0.149%
82	14.271	2236	2241	2245	rBV5	2040	3193	1.11%	0.111%
83	14.683	2306	2311	2312	rVV3	9927	13375	4.64%	0.463%
84	14.701	2312	2314	2321	rVB3	10440	14946	5.18%	0.517%
85	14.824	2330	2335	2342	rVB2	11085	16118	5.59%	0.558%


Sum of corrected areas: 2889410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021287.D
Acq On : 18 Mar 2021 19:17
Operator : JC/MD
Sample : M1715-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317058-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

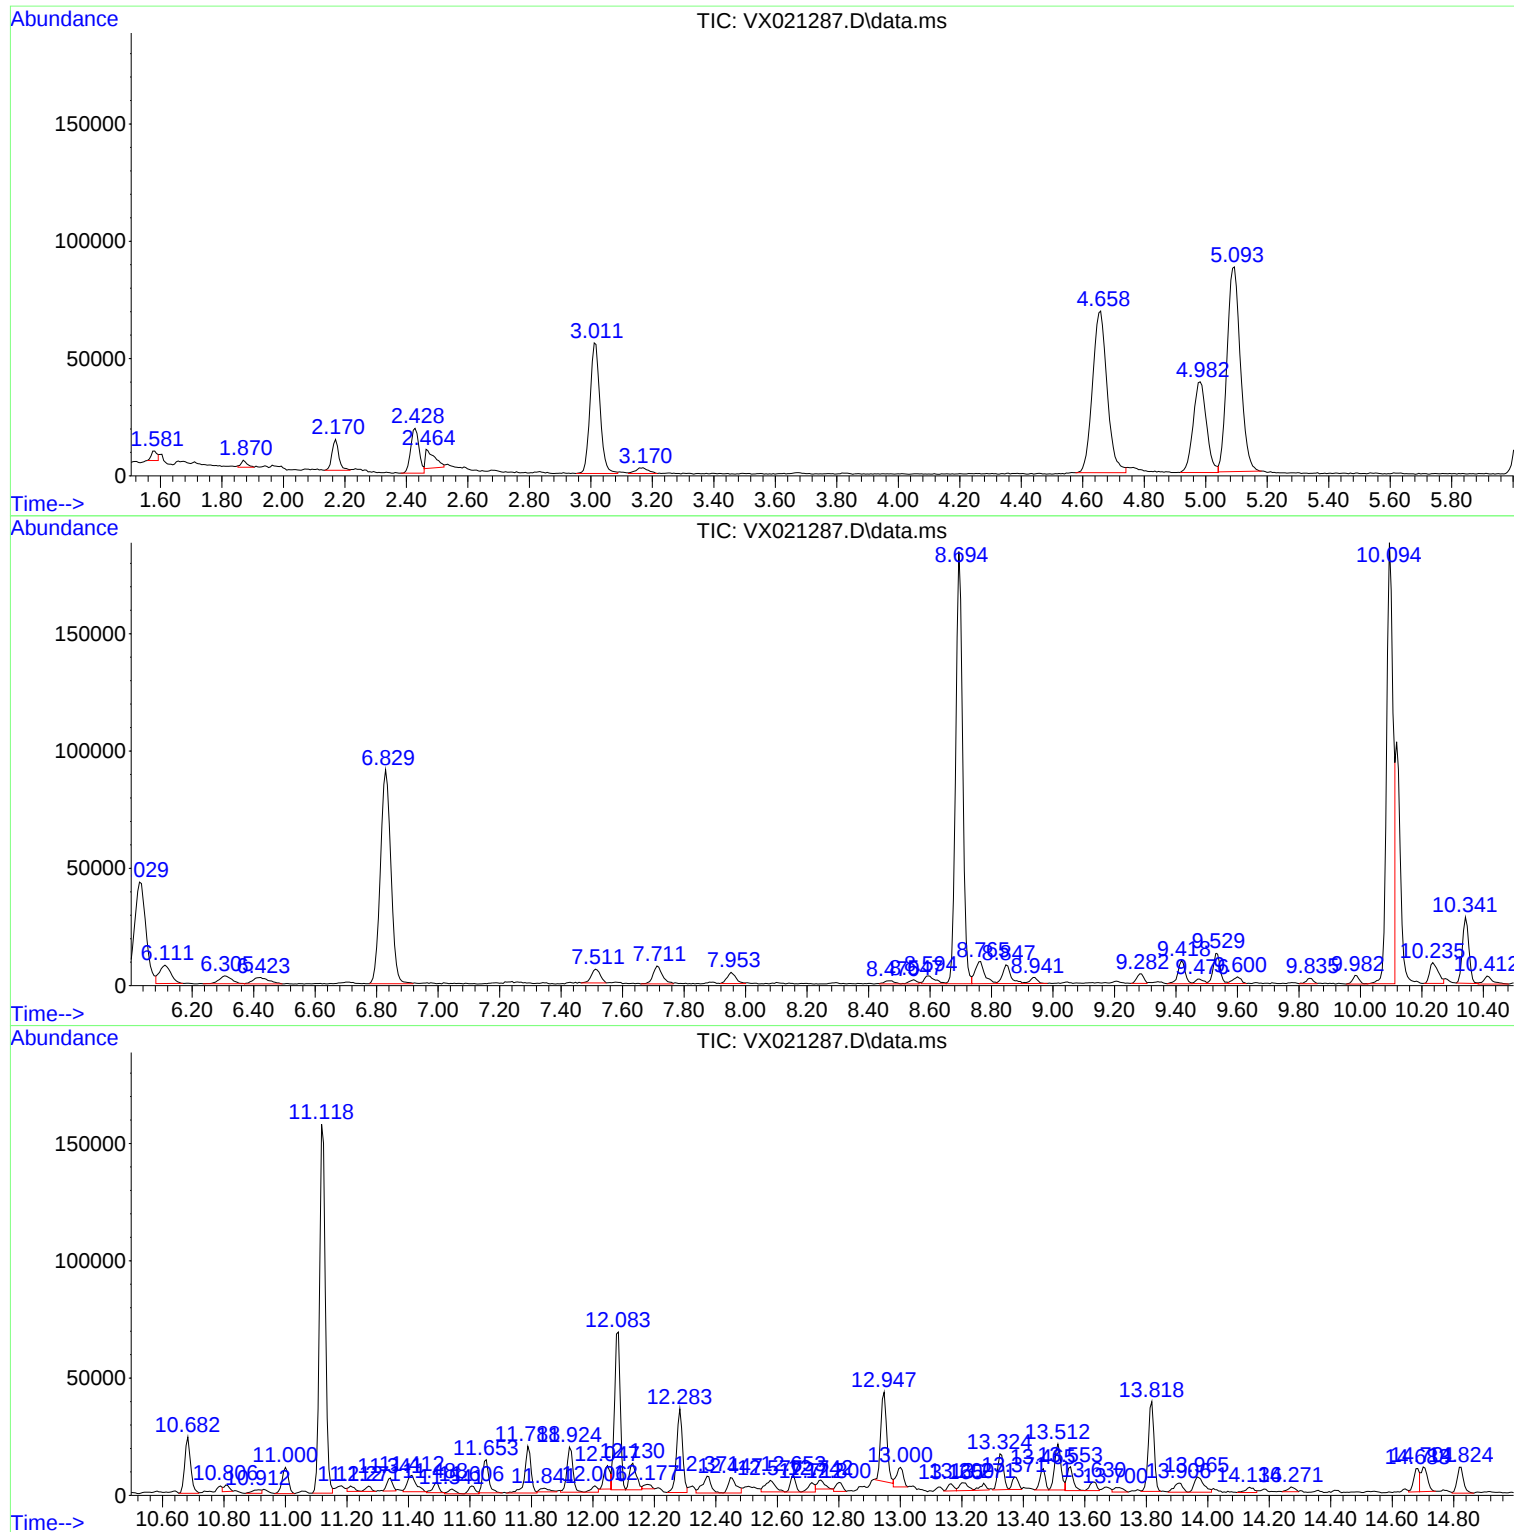

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021287.D
Acq On : 18 Mar 2021 19:17
Operator : JC/MD
Sample : M1715-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317058-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021287.D
Acq On : 18 Mar 2021 19:17
Operator : JC/MD
Sample : M1715-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317058-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
