

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021288.D
 Acq On : 18 Mar 2021 19:40
 Operator : JC/MD
 Sample : M1716-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210317059-01-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX021288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.564	78	81	86	rBV	40480	41741	1.38%	0.277%
2	2.093	165	171	180	rBV	48386	74708	2.48%	0.495%
3	2.417	219	226	240	rBV	148764	261696	8.68%	1.734%
4	2.582	244	254	263	rBV	53304	106846	3.54%	0.708%
5	3.017	316	328	346	rBV	1315914	2846591	94.43%	18.863%
6	4.664	591	608	621	rBV2	865164	3014419	100.00%	19.975%
7	4.982	651	662	670	rBV2	38021	112226	3.72%	0.744%
8	5.088	670	680	698	rVB	309967	915968	30.39%	6.070%
9	6.029	830	840	848	rBV2	42800	113953	3.78%	0.755%
10	6.147	848	860	872	rVV6	33182	134251	4.45%	0.890%
11	6.306	879	887	898	rVB	21850	57913	1.92%	0.384%
12	6.829	966	976	988	rBV	91107	217995	7.23%	1.445%
13	8.618	1272	1280	1286	rBV3	14418	32955	1.09%	0.218%
14	8.694	1286	1293	1299	rBV	190776	297919	9.88%	1.974%
15	8.759	1299	1304	1314	rVB2	48539	83570	2.77%	0.554%
16	8.847	1314	1319	1324	rBV	33644	51416	1.71%	0.341%
17	9.418	1407	1416	1422	rBV	128999	187235	6.21%	1.241%
18	9.529	1430	1435	1441	rVB	22314	30841	1.02%	0.204%
19	10.094	1519	1531	1543	rBV	214996	346870	11.51%	2.299%
20	10.235	1550	1555	1564	rBV2	102978	161226	5.35%	1.068%
21	10.341	1568	1573	1579	rVV	95923	140268	4.65%	0.929%
22	10.683	1626	1631	1644	rVB	63006	95143	3.16%	0.630%
23	11.000	1678	1685	1690	rVB2	18579	33896	1.12%	0.225%
24	11.118	1699	1705	1711	rBV	167407	230277	7.64%	1.526%
25	11.418	1749	1756	1762	rVB3	20607	39407	1.31%	0.261%
26	11.542	1774	1777	1784	rVB	32368	41287	1.37%	0.274%
27	11.789	1815	1819	1823	rVB	42349	52725	1.75%	0.349%
28	11.924	1838	1842	1850	rVB	58806	72686	2.41%	0.482%
29	12.047	1859	1863	1866	rBV2	42245	57194	1.90%	0.379%
30	12.077	1866	1868	1872	rVB	34692	38430	1.27%	0.255%
31	12.142	1872	1879	1883	rBV4	89235	137747	4.57%	0.913%
32	12.283	1895	1903	1913	rBV2	42848	89640	2.97%	0.594%
33	12.453	1927	1932	1937	rBV3	25736	44110	1.46%	0.292%
34	12.559	1946	1950	1953	rBV2	27802	44269	1.47%	0.293%
35	12.612	1956	1959	1964	rVB	57964	70600	2.34%	0.468%
36	12.800	1985	1991	1996	rVV2	131939	183445	6.09%	1.216%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021288.D
 Acq On : 18 Mar 2021 19:40
 Operator : JC/MD
 Sample : M1716-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210317059-01-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

37	12.942	2003	2015	2021	rBV	763056	1042788	34.59%	6.910%
38	13.001	2021	2025	2029	rVB3	42602	63079	2.09%	0.418%
39	13.206	2055	2060	2063	rBV3	20018	31294	1.04%	0.207%
40	13.253	2063	2068	2074	rVB3	33792	59691	1.98%	0.396%
41	13.324	2077	2080	2084	rVB3	24922	33399	1.11%	0.221%
42	13.377	2084	2089	2092	rBV	94601	130014	4.31%	0.862%
43	13.465	2099	2104	2107	rVB2	34625	47536	1.58%	0.315%
44	13.512	2107	2112	2114	rBV2	139257	185046	6.14%	1.226%
45	13.554	2114	2119	2126	rVB	1085363	1484556	49.25%	9.837%
46	13.630	2126	2132	2141	rBV3	278250	396630	13.16%	2.628%
47	13.771	2151	2156	2159	rBV	156689	190778	6.33%	1.264%
48	13.818	2159	2164	2170	rVB	368126	468755	15.55%	3.106%
49	13.959	2183	2188	2189	rBV2	26516	38149	1.27%	0.253%
50	14.136	2211	2218	2230	rBV	206057	298084	9.89%	1.975%
51	14.483	2273	2277	2293	rVB2	19912	35952	1.19%	0.238%
52	14.677	2306	2310	2314	rVV	53246	62895	2.09%	0.417%
53	14.818	2331	2334	2343	rVB	48843	61001	2.02%	0.404%




Sum of corrected areas: 15091110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021288.D
Acq On : 18 Mar 2021 19:40
Operator : JC/MD
Sample : M1716-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317059-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

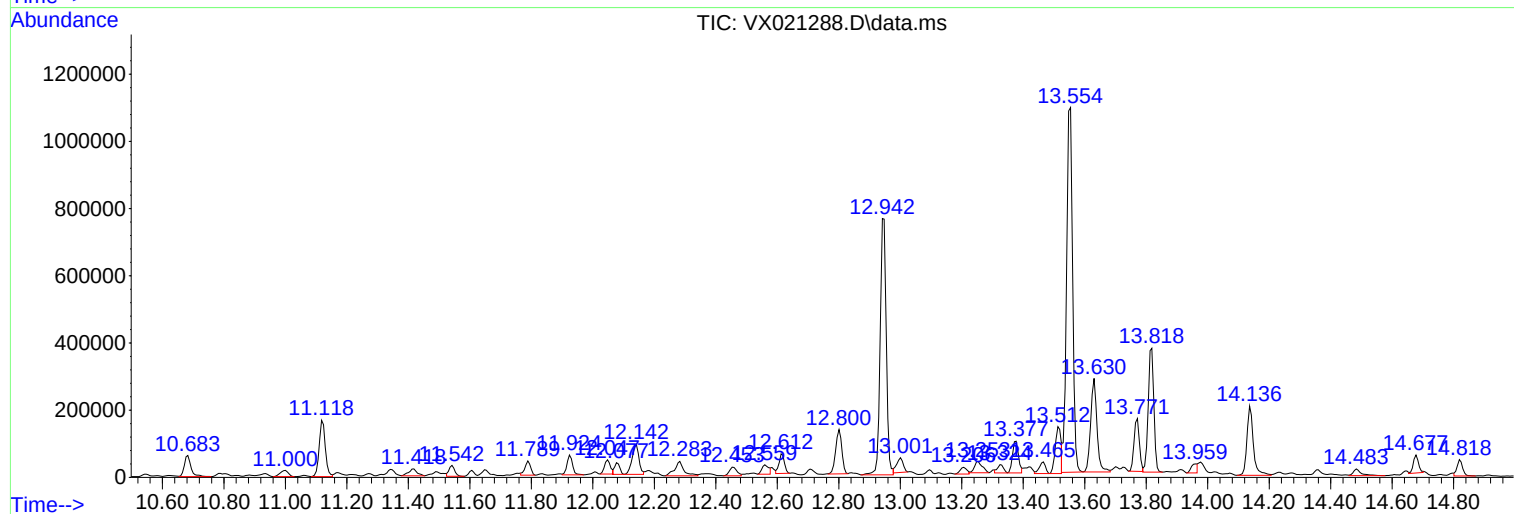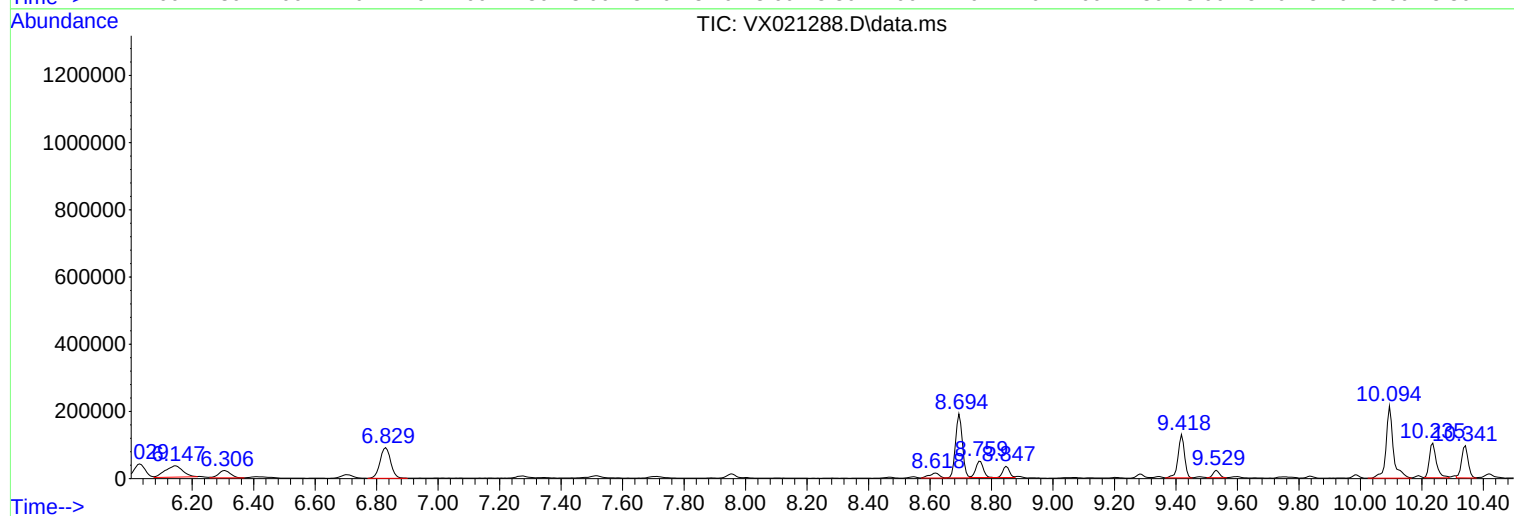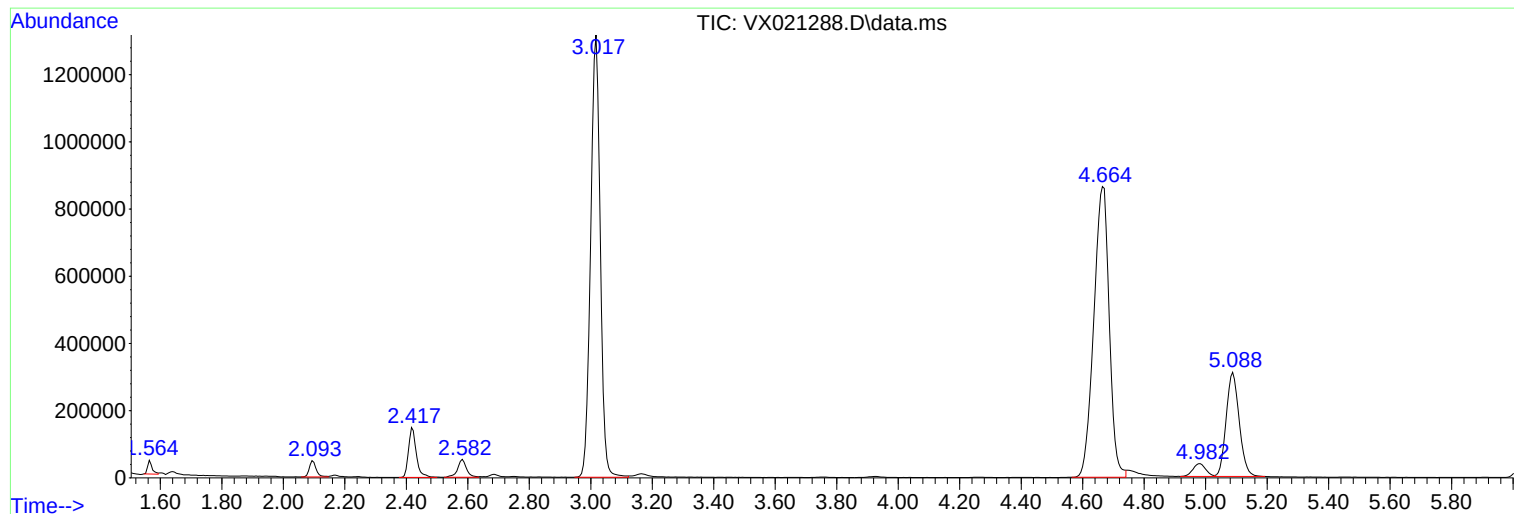

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021288.D
Acq On : 18 Mar 2021 19:40
Operator : JC/MD
Sample : M1716-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317059-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
Data File : VX021288.D
Acq On : 18 Mar 2021 19:40
Operator : JC/MD
Sample : M1716-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210317059-01-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------