
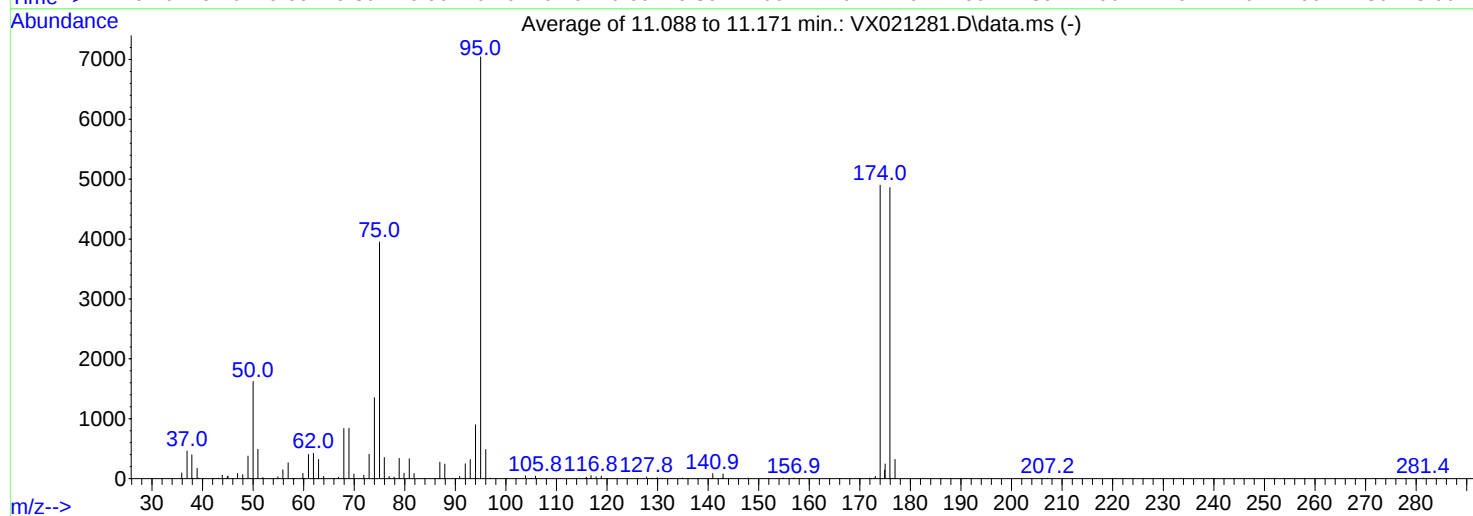


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031921\
 Data File : VX021281.D
 Acq On : 18 Mar 2021 15:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X031221W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Mar 12 12:55:27 2021

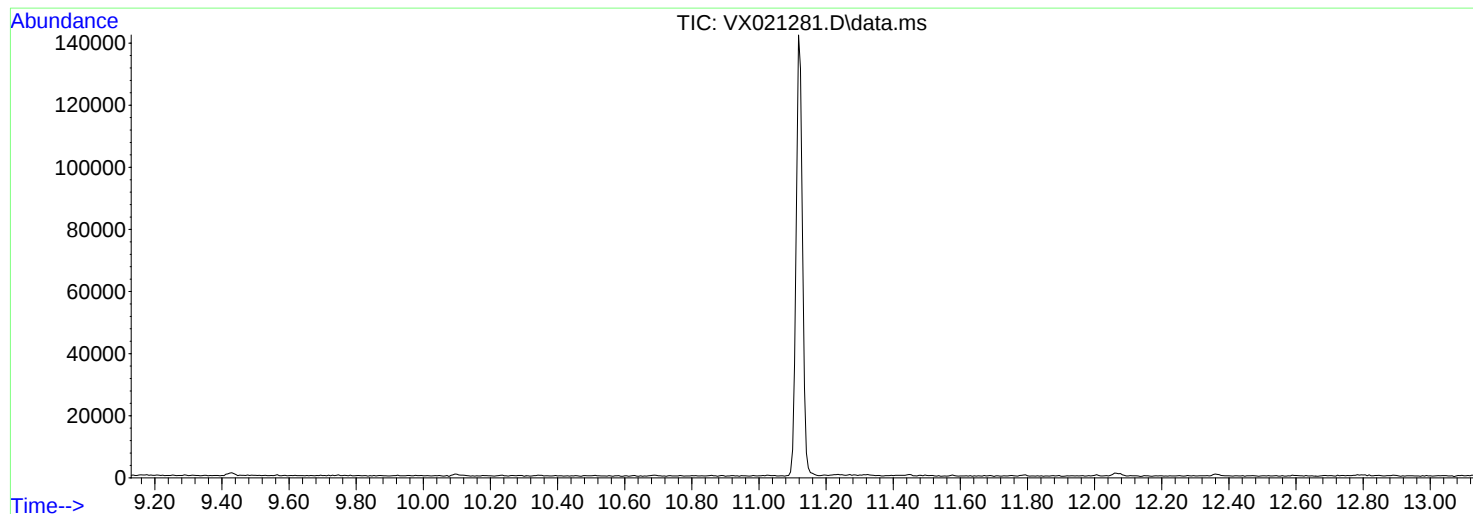

AutoFind: Averaged scan 1700 to 1714; Bkg corrected with scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	1622	PASS
75	95	30	60	56.1	3952	PASS
95	95	100	100	100.0	7043	PASS
96	95	5	9	6.9	485	PASS
173	174	0.00	2	0.8	37	PASS
174	95	50	100	69.6	4899	PASS
175	174	5	9	5.0	247	PASS
176	174	95	101	99.2	4860	PASS
177	176	5	9	6.6	322	PASS