

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
 Data File : VX027557.D
 Acq On : 19 Mar 2022 13:59
 Operator : JC/MD
 Sample : N2000-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE-132D3-20220315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	36	rBV	34303	66767	3.87%	0.668%
2	2.325	196	203	210	rBV2	28885	56491	3.27%	0.565%
3	2.544	230	239	249	rVB	10972	20812	1.21%	0.208%
4	5.391	695	706	722	rBV	196155	567321	32.87%	5.673%
5	5.556	722	733	748	rVV	330106	921136	53.37%	9.212%
6	5.958	789	799	817	rBV	180444	478341	27.71%	4.784%
7	6.763	922	931	947	rBV	492372	1179709	68.35%	11.797%
8	7.129	979	991	1007	rBV	793403	1726005	100.00%	17.260%
9	8.653	1234	1241	1259	rBV	1029125	1587880	92.00%	15.879%
10	9.275	1336	1343	1350	rBV	54904	81513	4.72%	0.815%
11	10.055	1465	1471	1480	rBV	998653	1322932	76.65%	13.230%
12	11.085	1634	1640	1652	rBV	724053	926229	53.66%	9.263%
13	12.024	1788	1794	1804	rBV	879020	1064623	61.68%	10.646%




Sum of corrected areas: 9999759

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027557.D
Acq On : 19 Mar 2022 13:59
Operator : JC/MD
Sample : N2000-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-132D3-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

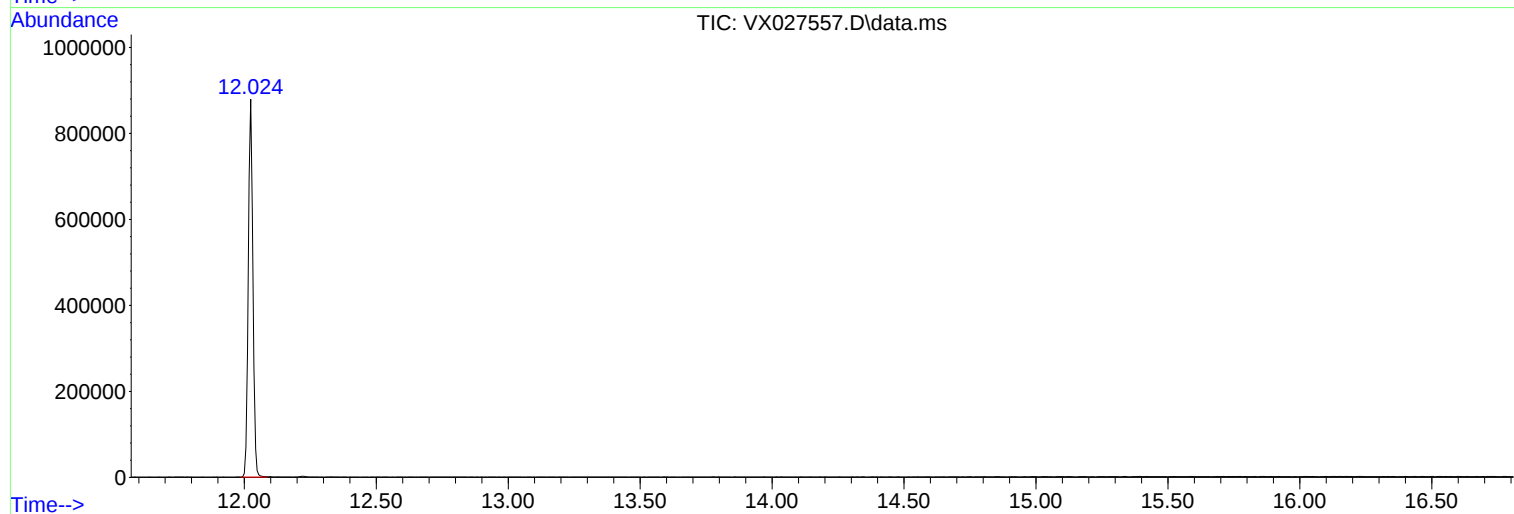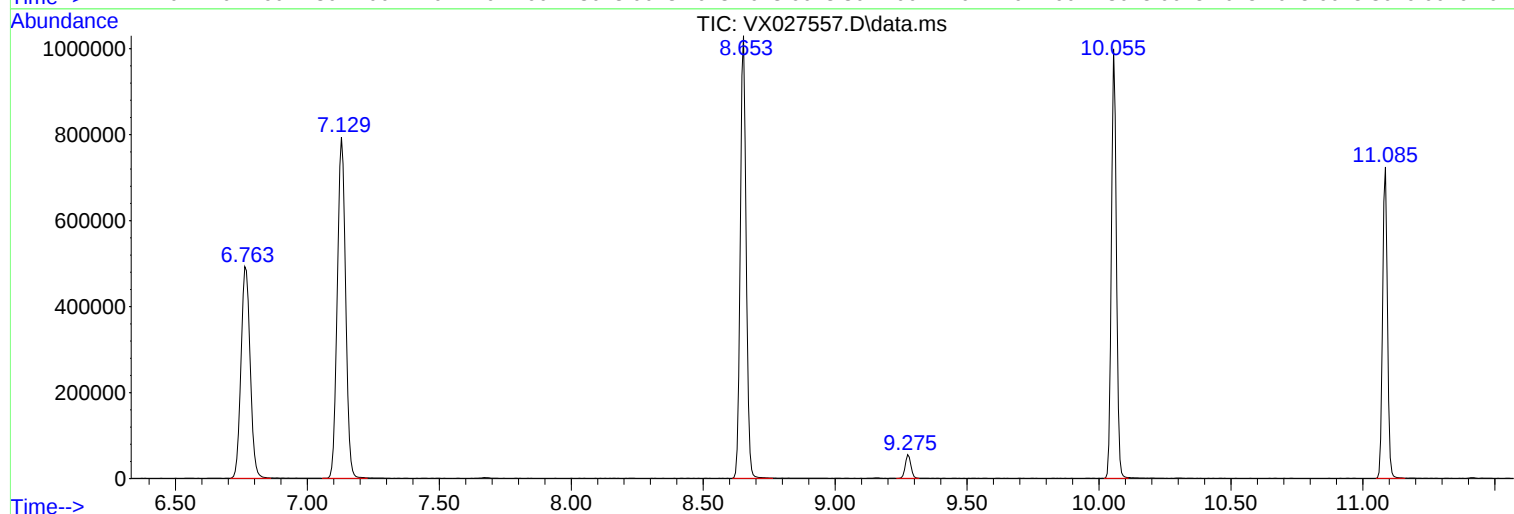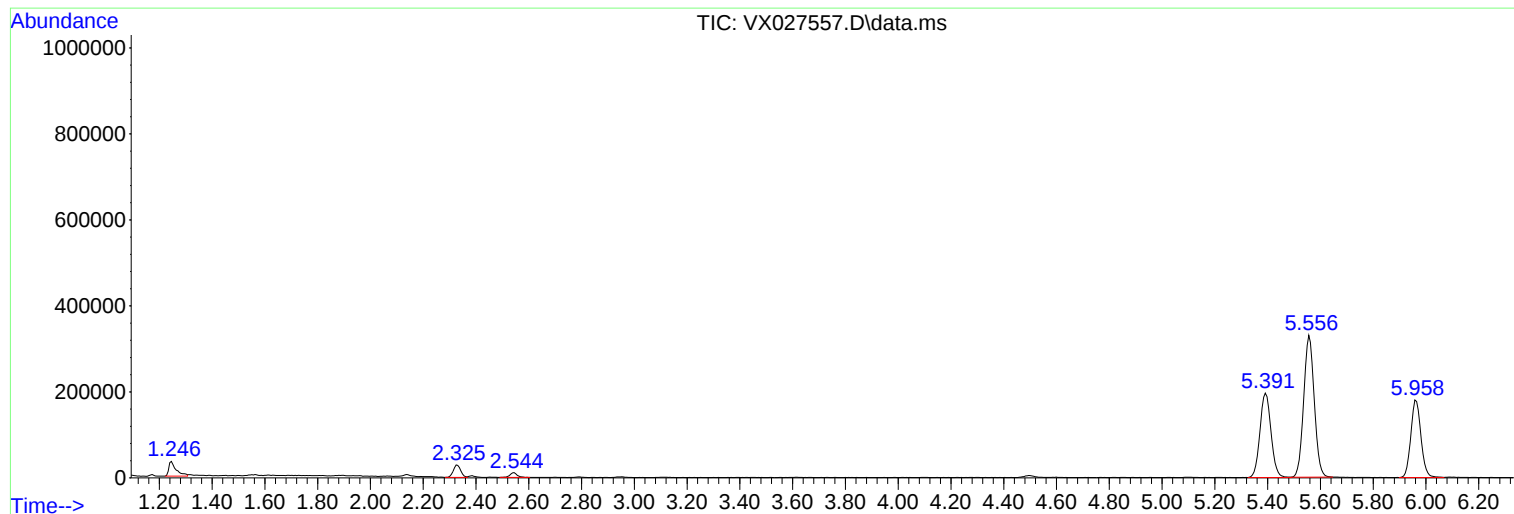

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027557.D
Acq On : 19 Mar 2022 13:59
Operator : JC/MD
Sample : N2000-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-132D3-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027557.D
Acq On : 19 Mar 2022 13:59
Operator : JC/MD
Sample : N2000-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-132D3-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
