

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
 Data File : VX027571.D
 Acq On : 19 Mar 2022 19:30
 Operator : JC/MD
 Sample : N2000-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP06-20220316

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	39	rBV	37419	71547	2.01%	0.580%
2	2.325	197	203	210	rBV3	60756	116097	3.25%	0.942%
3	5.391	694	706	721	rBV	204221	589470	16.52%	4.781%
4	5.556	721	733	747	rVV	334429	940802	26.37%	7.630%
5	5.964	788	800	817	rBV	196475	528770	14.82%	4.288%
6	6.769	921	932	949	rBV	498735	1204353	33.76%	9.768%
7	7.129	981	991	1008	rBV	1683209	3567234	100.00%	28.931%
8	8.653	1234	1241	1251	rBV	1028575	1604021	44.97%	13.009%
9	10.055	1465	1471	1487	rBV	1048390	1392248	39.03%	11.291%
10	11.085	1634	1640	1653	rBV	809530	1049237	29.41%	8.510%
11	12.024	1789	1794	1805	rBV	1058226	1266338	35.50%	10.270%




Sum of corrected areas: 12330117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027571.D
Acq On : 19 Mar 2022 19:30
Operator : JC/MD
Sample : N2000-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

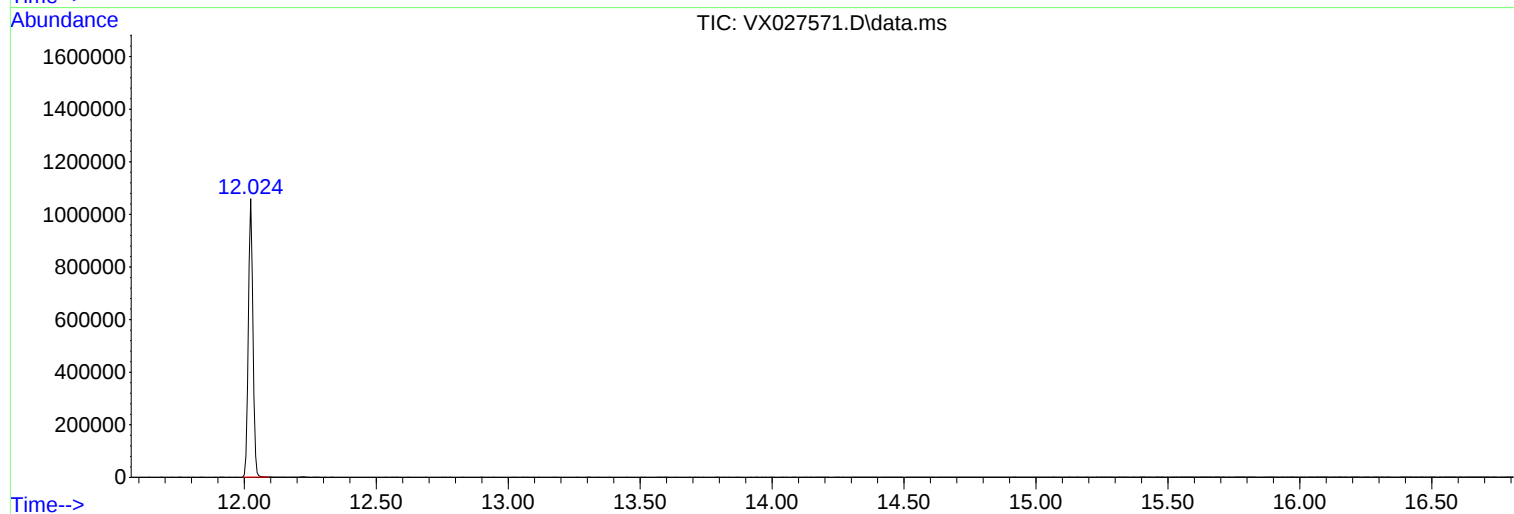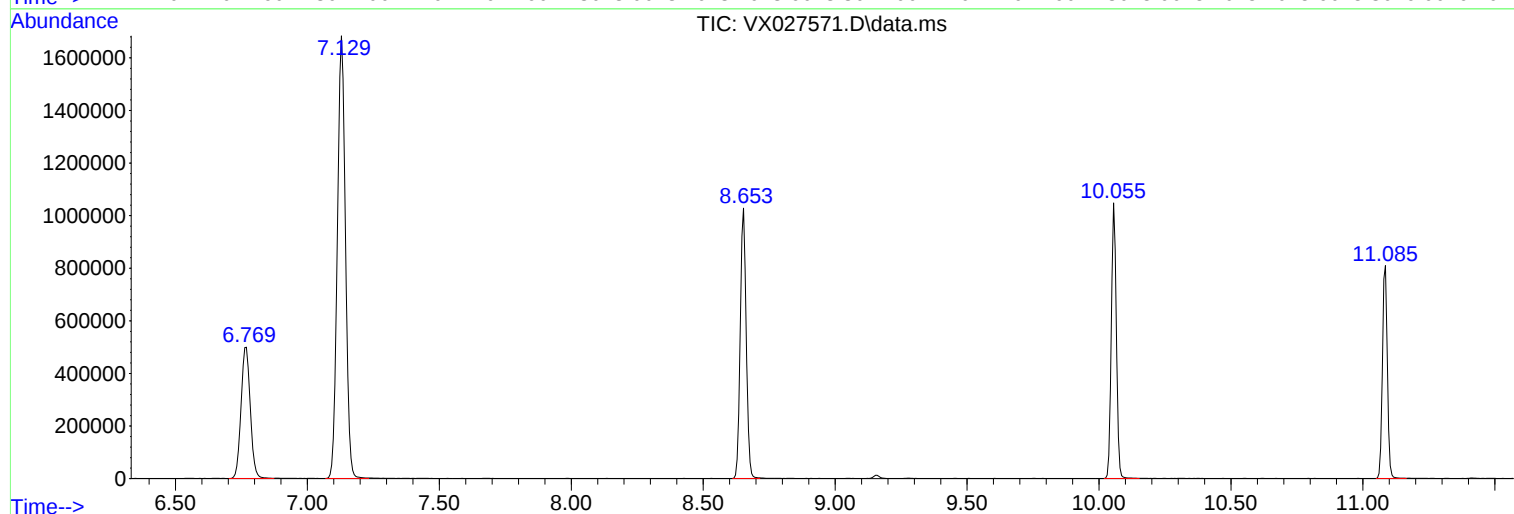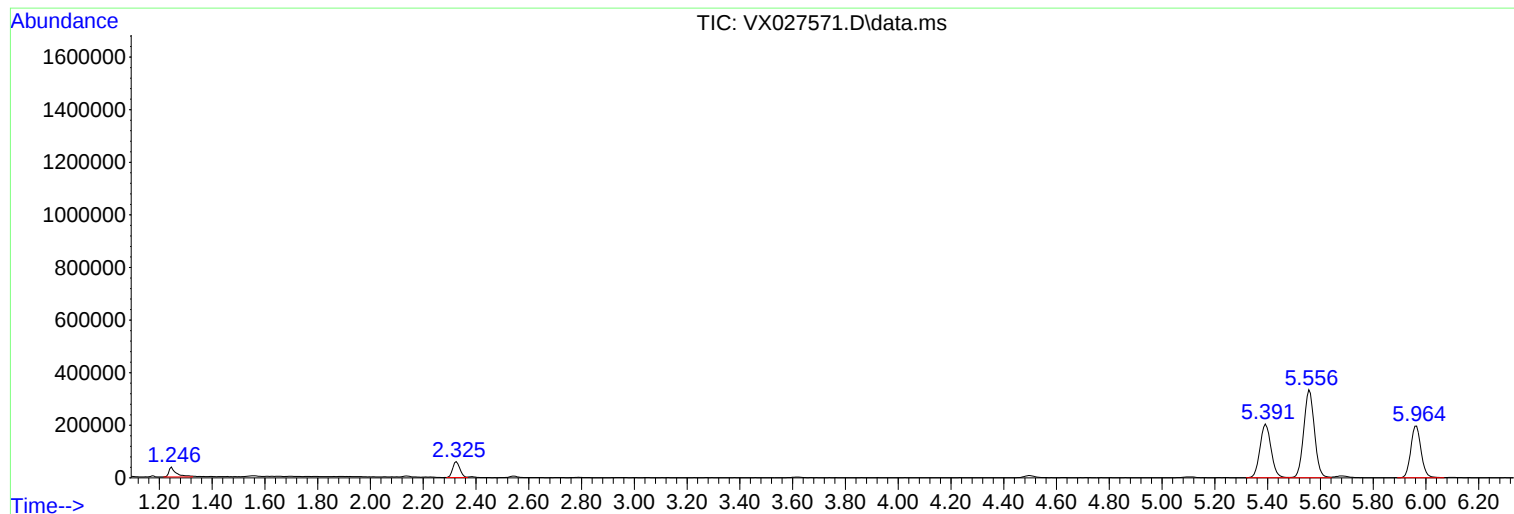

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027571.D
Acq On : 19 Mar 2022 19:30
Operator : JC/MD
Sample : N2000-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031922\
Data File : VX027571.D
Acq On : 19 Mar 2022 19:30
Operator : JC/MD
Sample : N2000-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------