

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031924\
 Data File : VX040713.D
 Acq On : 19 Mar 2024 11:22
 Operator : JC/MD
 Sample : P1788-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PEZOMETER-200

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX040713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.373	206	211	221	rVB3	2476	4380	1.45%	0.294%
2	4.897	614	625	639	rBV	40403	121347	40.04%	8.131%
3	5.952	786	798	810	rBV2	46861	126013	41.58%	8.444%
4	6.756	921	930	943	rBV	94944	229996	75.88%	15.412%
5	8.646	1234	1240	1250	rBV	196367	303089	100.00%	20.310%
6	9.518	1378	1383	1393	rBV3	7580	11409	3.76%	0.765%
7	10.049	1465	1470	1490	rBV	201050	286125	94.40%	19.173%
8	11.079	1634	1639	1651	rBV	175640	222033	73.26%	14.878%
9	12.268	1832	1834	1838	rVV2	2795	3129	1.03%	0.210%
10	12.316	1838	1842	1850	rVB4	6345	10196	3.36%	0.683%
11	12.530	1873	1877	1879	rVV2	5018	6374	2.10%	0.427%
12	12.554	1879	1881	1886	rVV	5661	6293	2.08%	0.422%
13	12.615	1886	1891	1896	rVV	12389	15215	5.02%	1.020%
14	12.719	1899	1908	1913	rBV6	3935	7594	2.51%	0.509%
15	12.853	1925	1930	1935	rBV2	6189	8912	2.94%	0.597%
16	12.920	1935	1941	1945	rVV	13039	17577	5.80%	1.178%
17	12.963	1945	1948	1954	rVB	22264	25606	8.45%	1.716%
18	13.024	1954	1958	1960	rBV3	3187	4609	1.52%	0.309%
19	13.066	1963	1965	1970	rVV2	4518	5788	1.91%	0.388%
20	13.121	1970	1974	1977	rVV4	3415	5142	1.70%	0.345%
21	13.164	1977	1981	1986	rVB3	9454	13299	4.39%	0.891%
22	13.255	1992	1996	1998	rBV3	5050	7649	2.52%	0.513%
23	13.292	1998	2002	2012	rVV3	19695	31753	10.48%	2.128%
24	13.371	2012	2015	2021	rVB2	3596	4494	1.48%	0.301%
25	13.578	2044	2049	2055	rBV3	3012	6291	2.08%	0.422%
26	13.780	2077	2082	2086	rVB2	3562	4949	1.63%	0.332%
27	14.036	2121	2124	2128	rBV2	2491	3050	1.01%	0.204%




Sum of corrected areas: 1492312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031924\
Data File : VX040713.D
Acq On : 19 Mar 2024 11:22
Operator : JC/MD
Sample : P1788-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PEZOMETER-200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

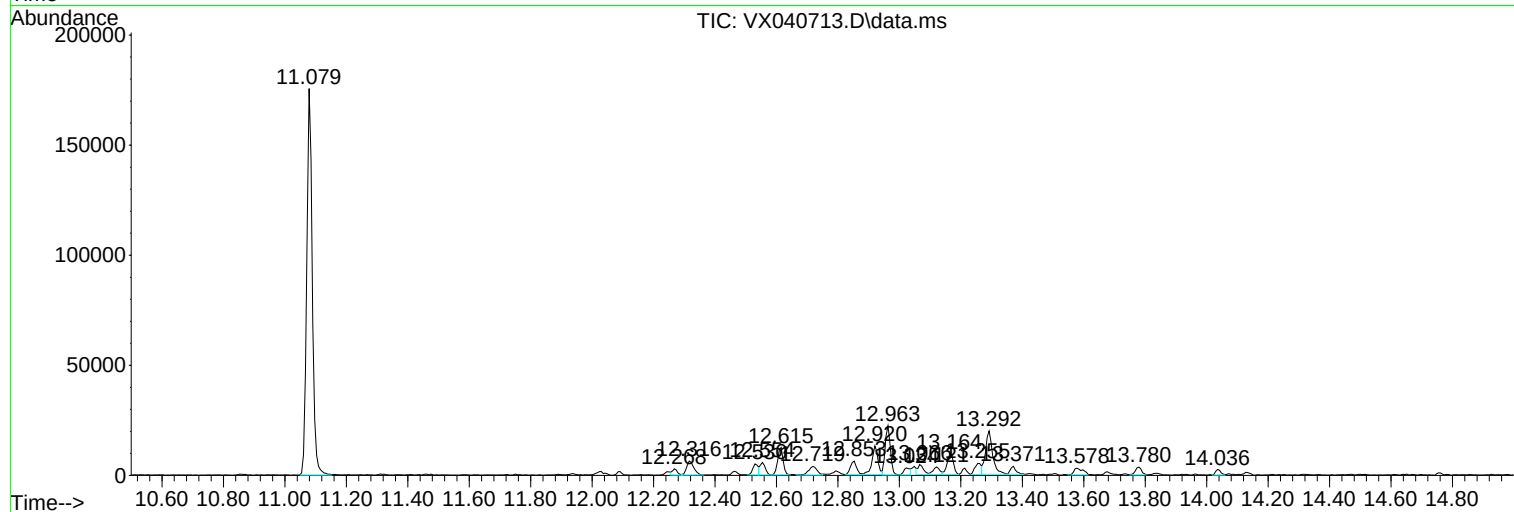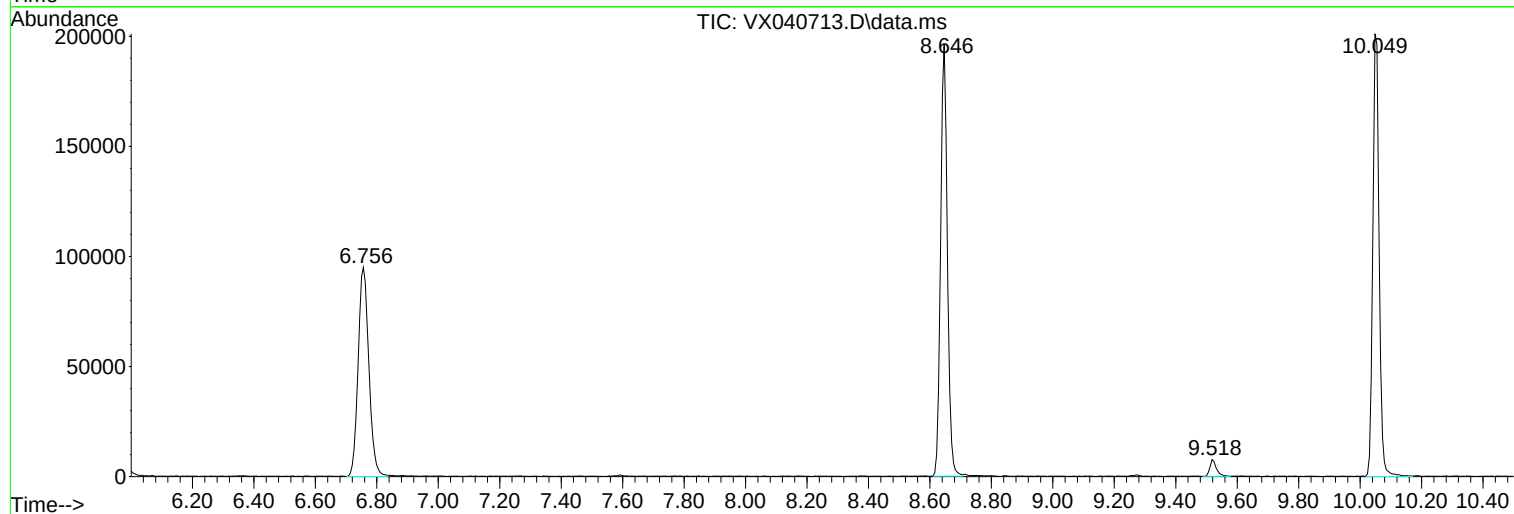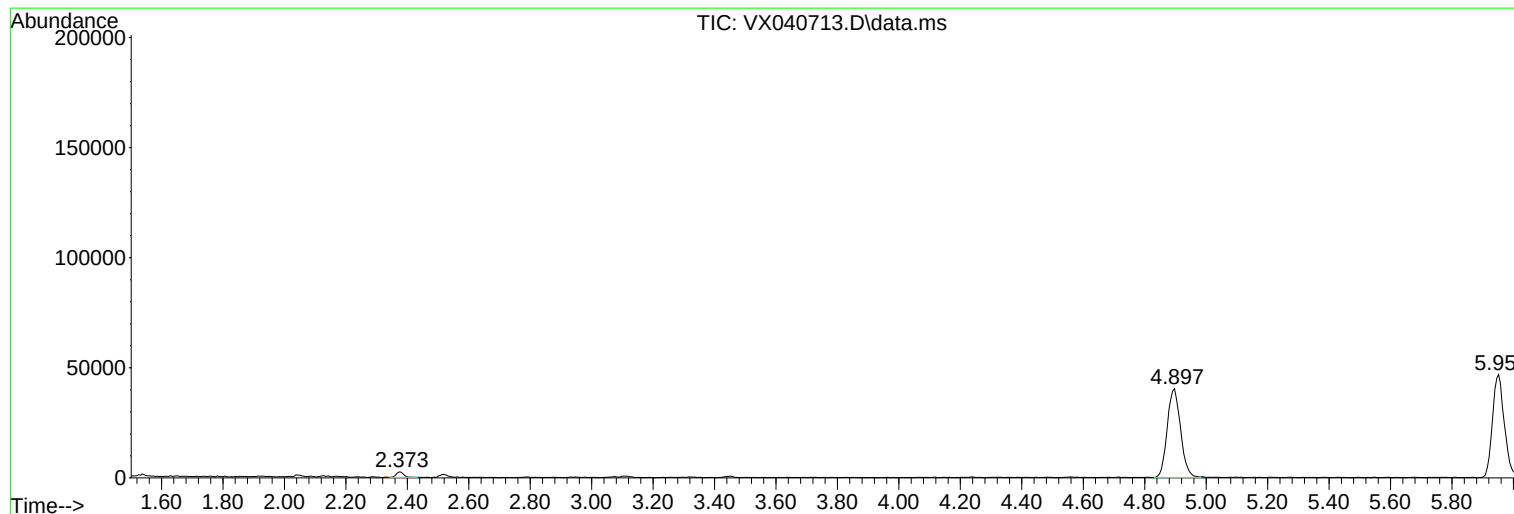

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031924\
Data File : VX040713.D
Acq On : 19 Mar 2024 11:22
Operator : JC/MD
Sample : P1788-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PEZOMETER-200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031924\
Data File : VX040713.D
Acq On : 19 Mar 2024 11:22
Operator : JC/MD
Sample : P1788-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PEZOMETER-200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------