
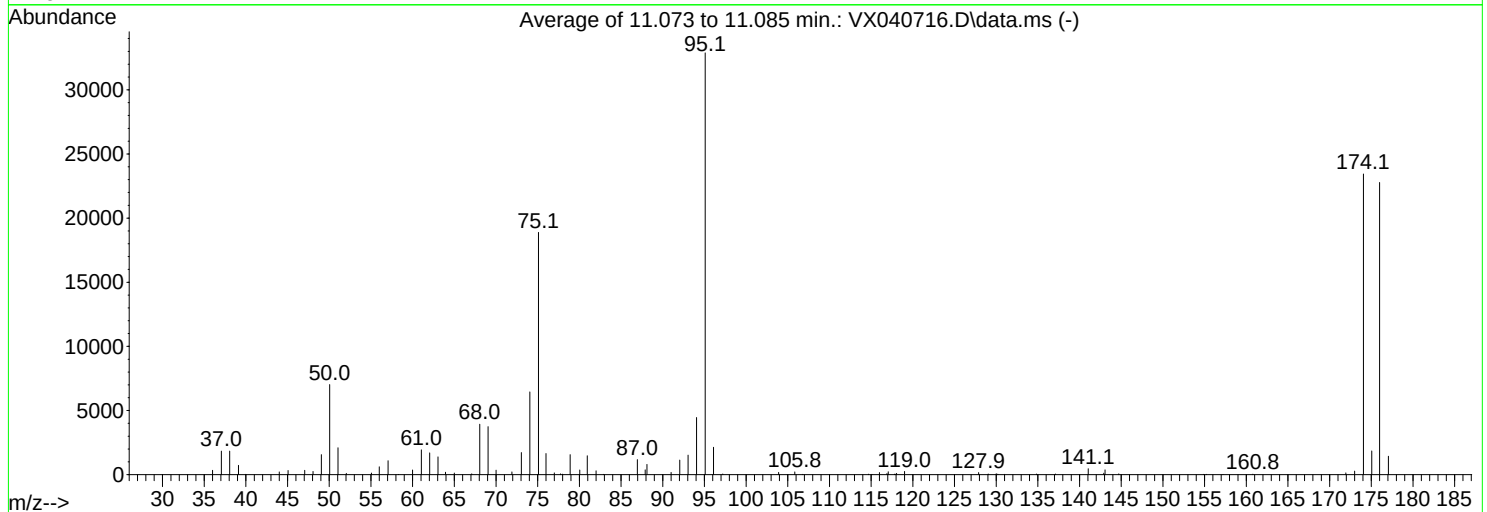


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031924\  
Data File : VX040716.D  
Acq On : 19 Mar 2024 15:36  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X030524W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Tue Mar 05 13:21:29 2024

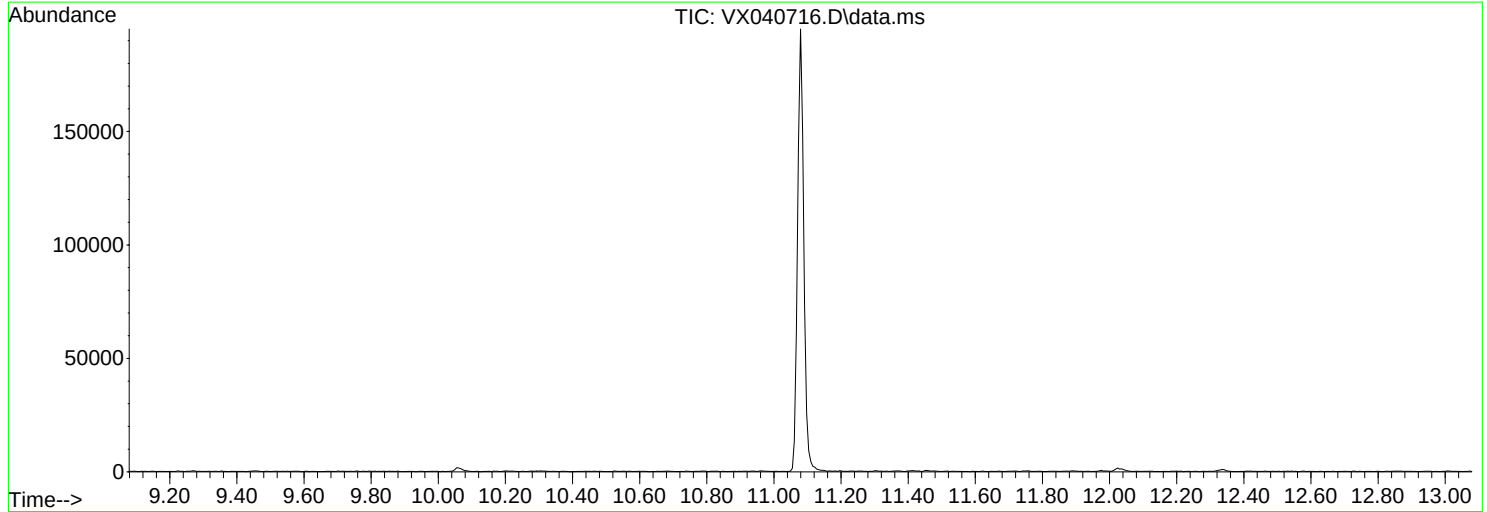

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 21.4         | 7022       | PASS                |
| 75             | 95              | 30              | 60              | 57.4         | 18883      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 32885      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 2137       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 281        | PASS                |
| 174            | 95              | 50              | 100             | 71.3         | 23437      | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 1842       | PASS                |
| 176            | 174             | 95              | 101             | 97.2         | 22773      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 1437       | PASS                |