


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031925\
 Data File : VX045339.D
 Acq On : 19 Mar 2025 10:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022125W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Feb 22 01:06:36 2025

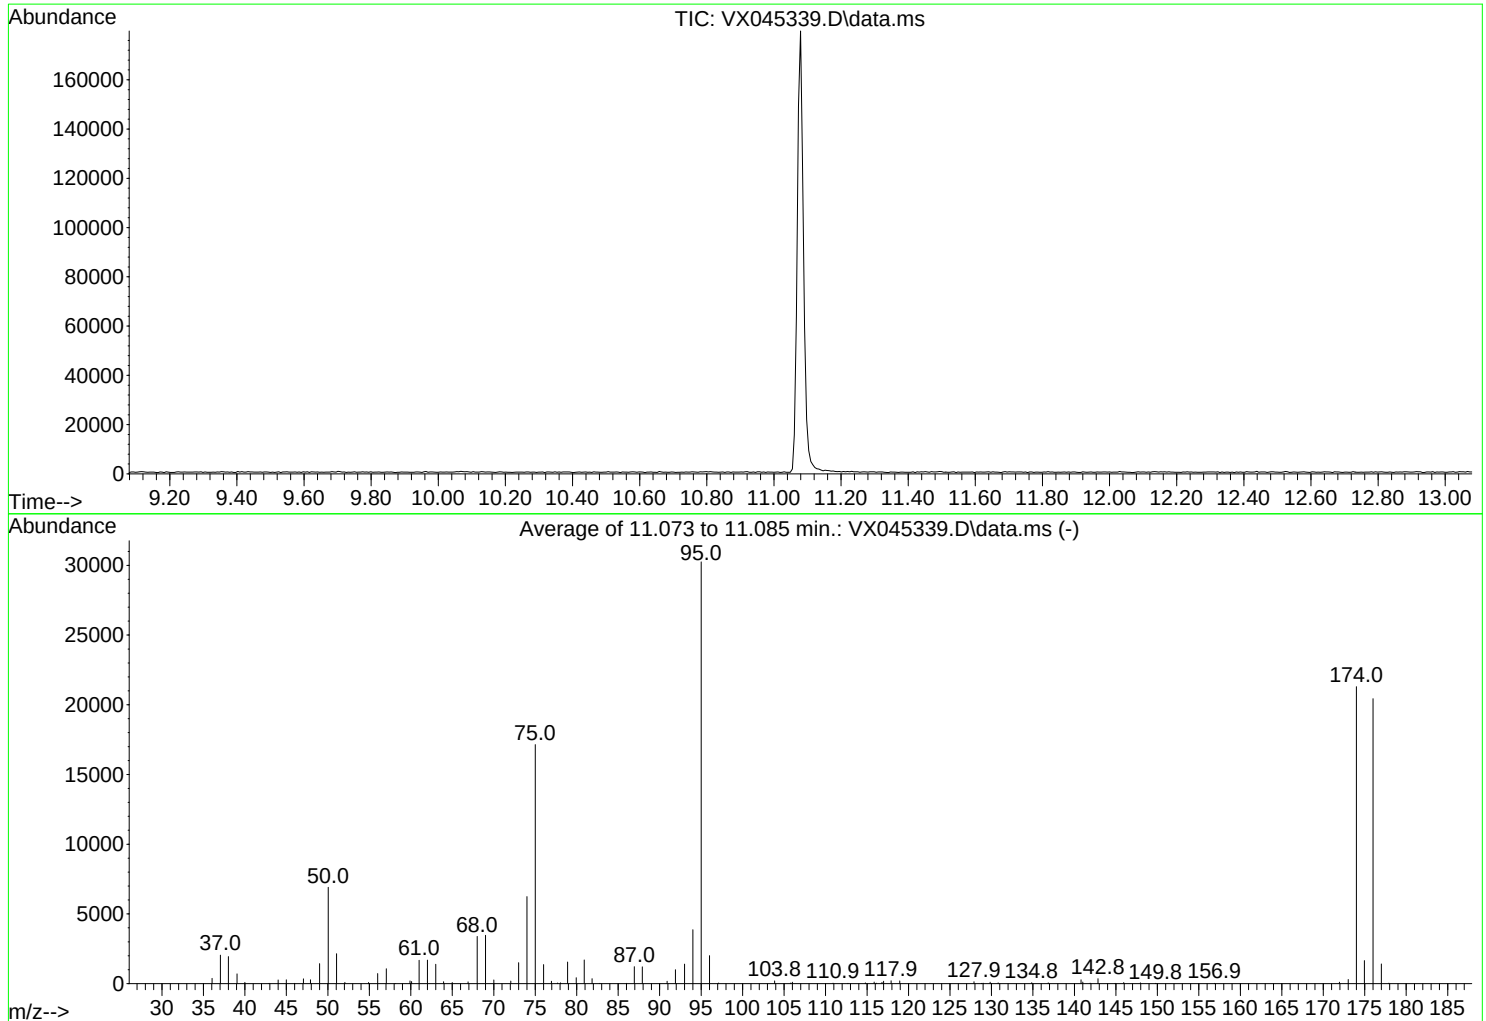

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	6907	PASS
75	95	30	60	56.7	17149	PASS
95	95	100	100	100.0	30251	PASS
96	95	5	9	6.6	2004	PASS
173	174	0.00	2	1.4	297	PASS
174	95	50	100	70.4	21304	PASS
175	174	5	9	7.8	1655	PASS
176	174	95	101	95.9	20440	PASS
177	176	5	9	6.9	1413	PASS