


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032019\
 Data File : VX008229.D
 Acq On : 20 Mar 2019 09:07
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
 Title : SW846 8260
 Last Update : Tue Mar 19 13:15:13 2019

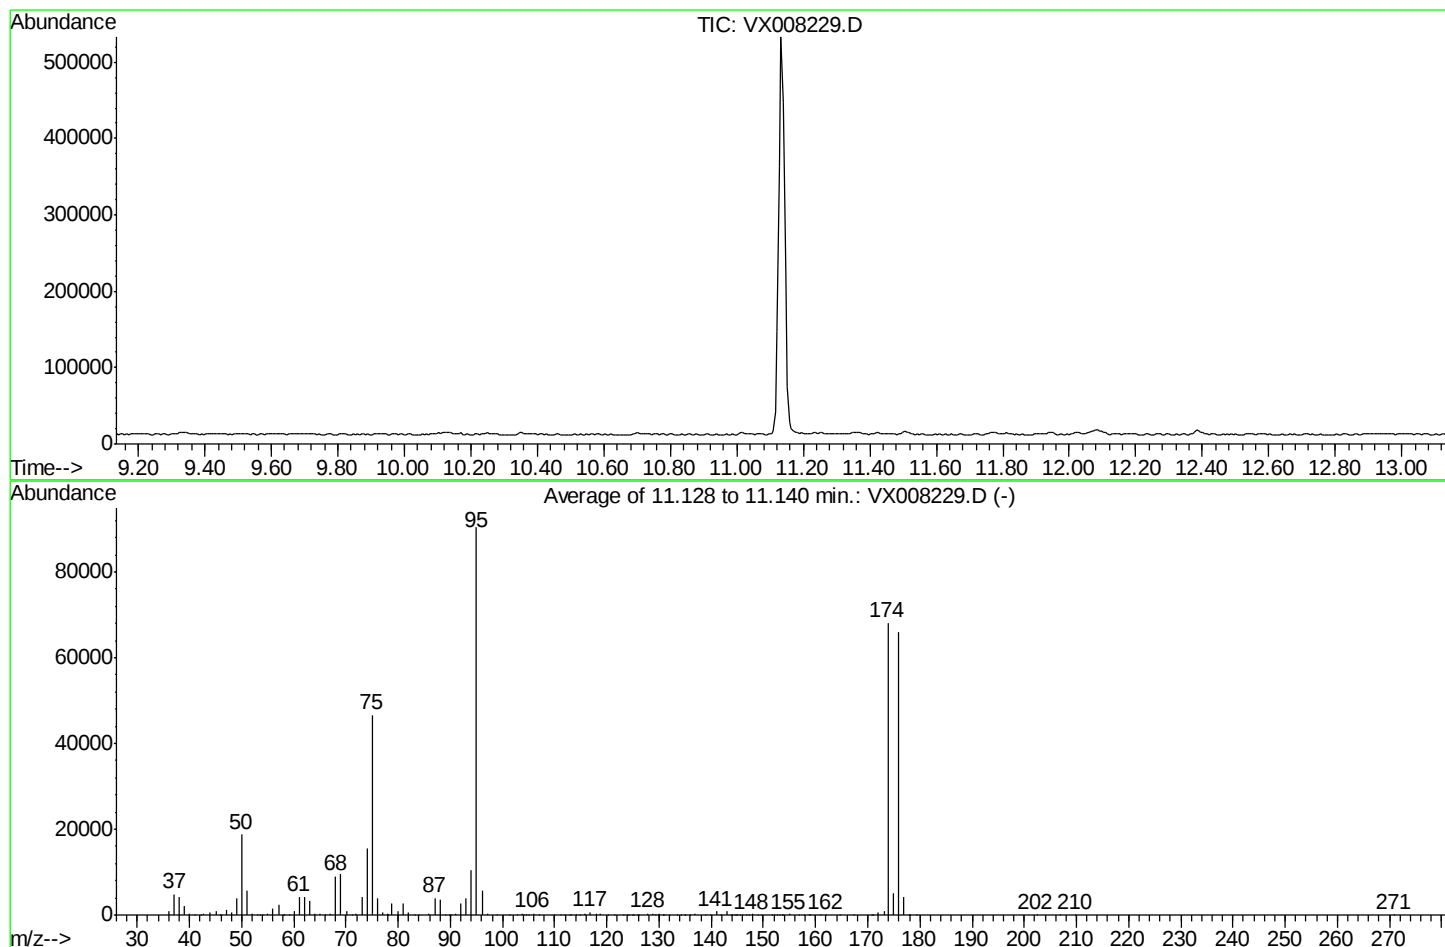

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	18800	PASS
75	95	30	60	51.6	46656	PASS
95	95	100	100	100.0	90405	PASS
96	95	5	9	6.4	5785	PASS
173	174	0.00	2	1.5	1031	PASS
174	95	50	100	75.3	68090	PASS
175	174	5	9	7.6	5176	PASS
176	174	95	101	97.0	66032	PASS
177	176	5	9	6.6	4330	PASS