

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
 Data File : VX021294.D
 Acq On : 19 Mar 2021 10:12
 Operator : JC/MD
 Sample : VX0320WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK307

Quant Time: Mar 20 00:00:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 19 23:59:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.823	114	60462	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.094	117	54212	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.059	152	25145	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.387	65	17344	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.693	69	14034	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.340	63	30473	3.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.00%
20) 2-Butanone-d5	4.523	46	50285	48.37	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.74%
24) Chloroform-d	5.135	84	38381	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	6.023	65	22352	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
32) Benzene-d6	6.047	84	70911	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	7.364	67	22302	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	8.694	98	66144	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
43) trans-1,3-Dichloroprop...	8.994	79	9673	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	9.424	63	38230	47.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.20%
56) 1,1,2,2-Tetrachloroeth...	11.230	84	16191	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
66) 1,2-Dichlorobenzene-d4	12.359	152	21875	4.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.60%
Target Compounds						Qvalue
16) Methylene chloride	2.829	84	2425	0.45	ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
Data File : VX021294.D
Acq On : 19 Mar 2021 10:12
Operator : JC/MD
Sample : VX0320WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Quant Time: Mar 20 00:00:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 19 23:59:09 2021
Response via : Initial Calibration

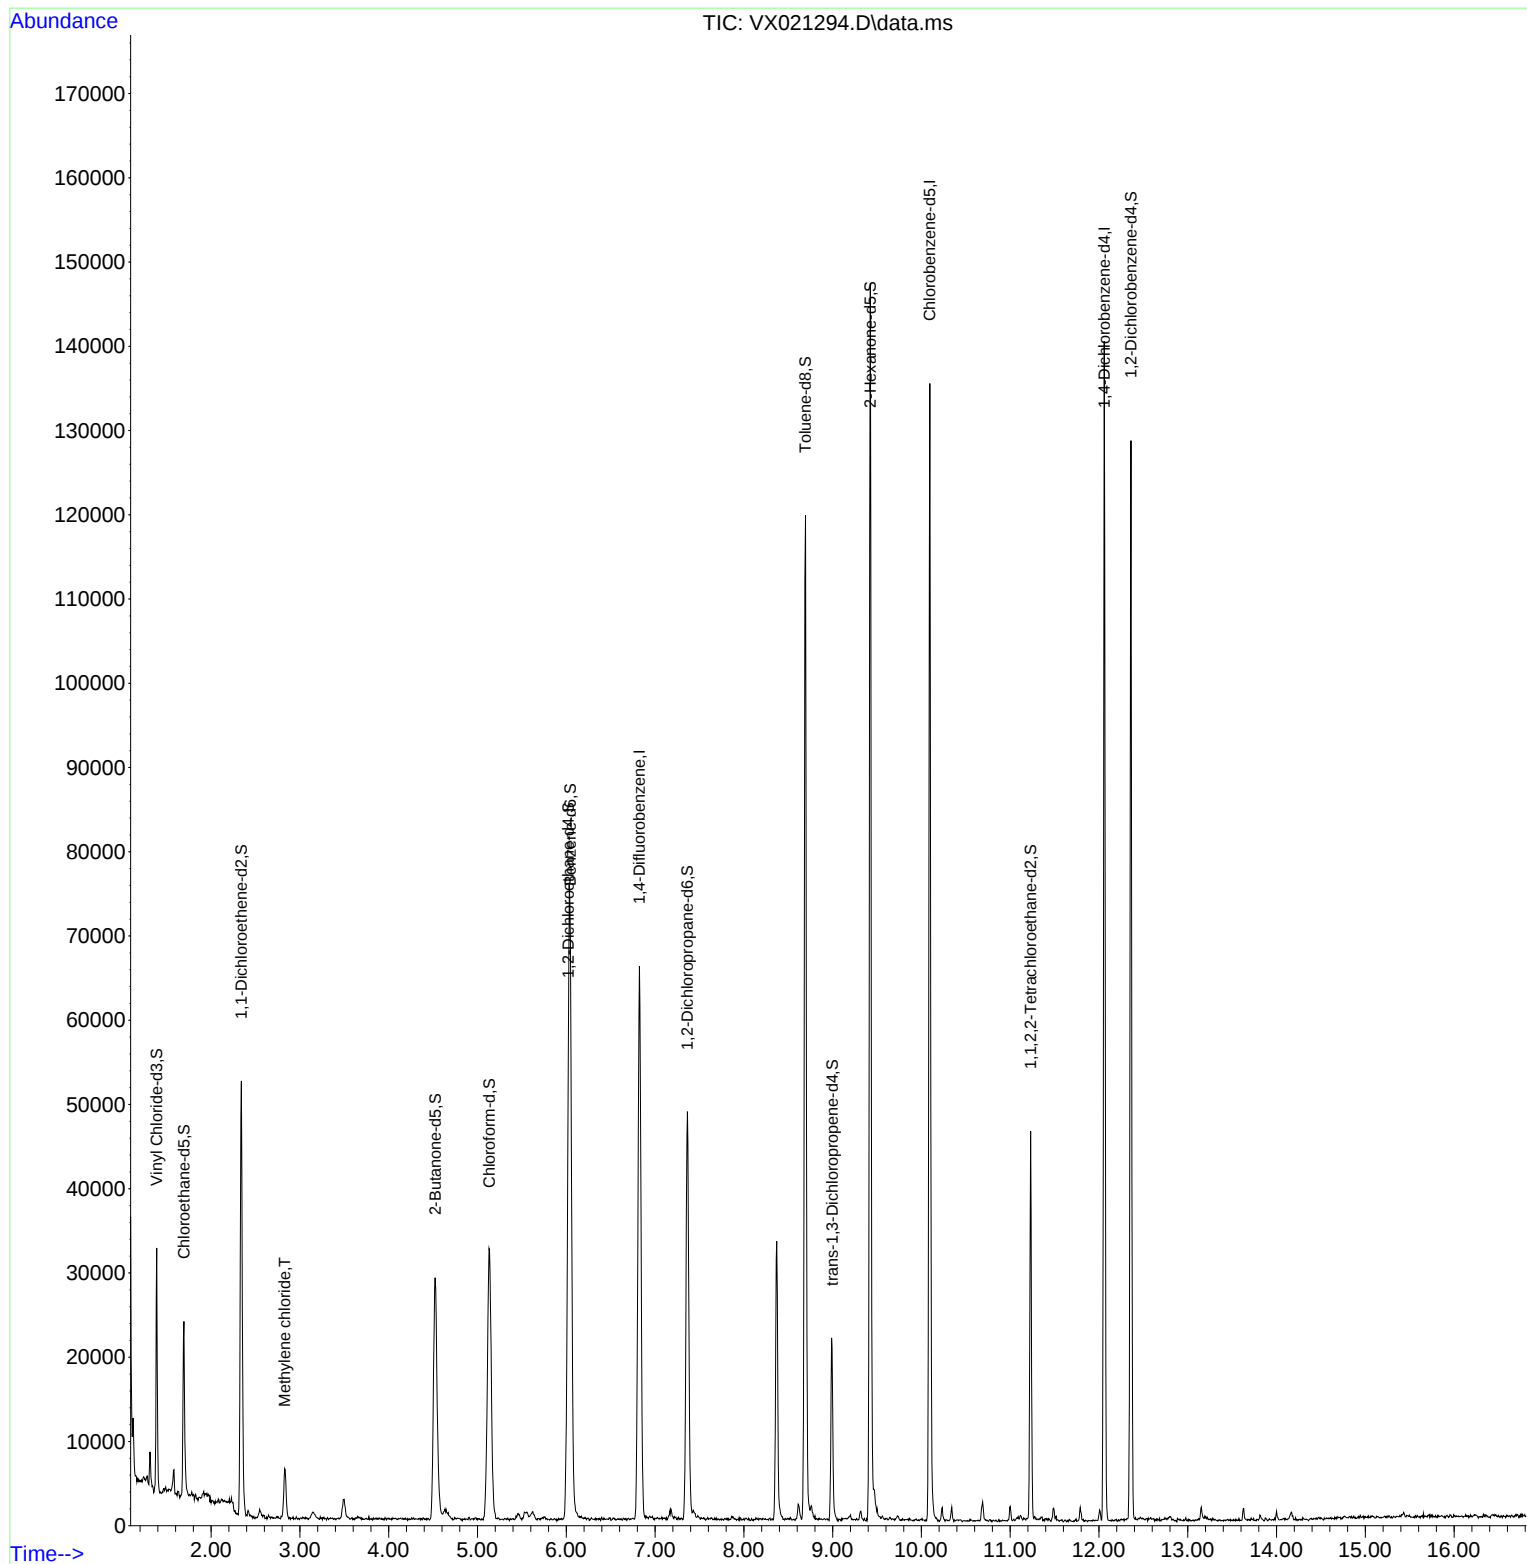

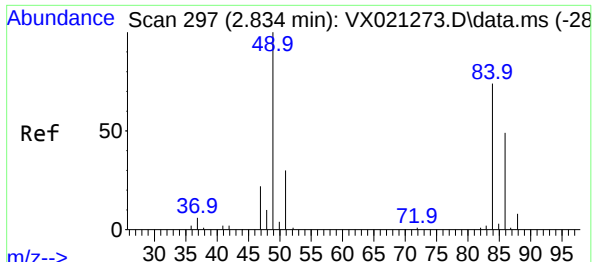

#16
Methylene chloride
Concen: 0.45 ug/L
RT: 2.829 min Scan# 296
Delta R.T. -0.000 min
Lab File: VX021294.D
Acq: 19 Mar 2021 10:12

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Tgt Ion: 84 Resp: 2425

Ion	Ratio	Lower	Upper
84	100		
86	63.9	44.6	82.8
49	143.2	79.5	147.6

