

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
 Data File : VX021294.D
 Acq On : 19 Mar 2021 10:12
 Operator : JC/MD
 Sample : VX0320WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK307

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VX021294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.122	4	6	10	rVB	6864	6275	2.83%	0.330%
2	1.311	36	38	42	rVB	4150	4059	1.83%	0.213%
3	1.387	47	51	57	rVB	29092	29560	13.35%	1.554%
4	1.581	81	84	86	rVB2	2881	2927	1.32%	0.154%
5	1.693	98	103	112	rVB	20676	27368	12.36%	1.438%
6	2.340	207	213	222	rVB	51639	83539	37.74%	4.391%
7	2.829	290	296	304	rVB	5958	11420	5.16%	0.600%
8	3.146	341	350	360	rBV7	882	2955	1.33%	0.155%
9	3.499	400	410	416	rBV4	2352	5611	2.53%	0.295%
10	4.523	573	584	598	rBV2	28780	83203	37.59%	4.373%
11	5.129	676	687	701	rBV	32225	98097	44.31%	5.156%
12	5.623	764	771	779	rVB3	1003	2762	1.25%	0.145%
13	6.035	828	841	860	rBV2	75326	221372	100.00%	11.635%
14	6.823	966	975	987	rBV	65636	153925	69.53%	8.090%
15	7.176	1028	1035	1041	rBV6	1323	2635	1.19%	0.138%
16	7.364	1058	1067	1076	rBV	48452	105753	47.77%	5.558%
17	8.370	1231	1238	1250	rBV	33084	56074	25.33%	2.947%
18	8.612	1275	1279	1285	rVB	1805	2869	1.30%	0.151%
19	8.694	1285	1293	1302	rBV	119151	186979	84.46%	9.827%
20	8.988	1338	1343	1354	rVB	21687	33486	15.13%	1.760%
21	9.424	1411	1417	1423	rBV	146816	201499	91.02%	10.590%
22	10.094	1525	1531	1546	rVB	135047	184247	83.23%	9.683%
23	10.235	1549	1555	1560	rBV3	1665	2240	1.01%	0.118%
24	10.688	1627	1632	1639	rBV5	2278	3646	1.65%	0.192%
25	11.230	1718	1724	1730	rBV	46002	57048	25.77%	2.998%
26	11.488	1763	1768	1771	rBV4	1576	2319	1.05%	0.122%
27	12.059	1859	1865	1875	rVB	139979	172702	78.01%	9.077%
28	12.359	1910	1916	1924	rVB	128020	158149	71.44%	8.312%




Sum of corrected areas: 1902719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
Data File : VX021294.D
Acq On : 19 Mar 2021 10:12
Operator : JC/MD
Sample : VX0320WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

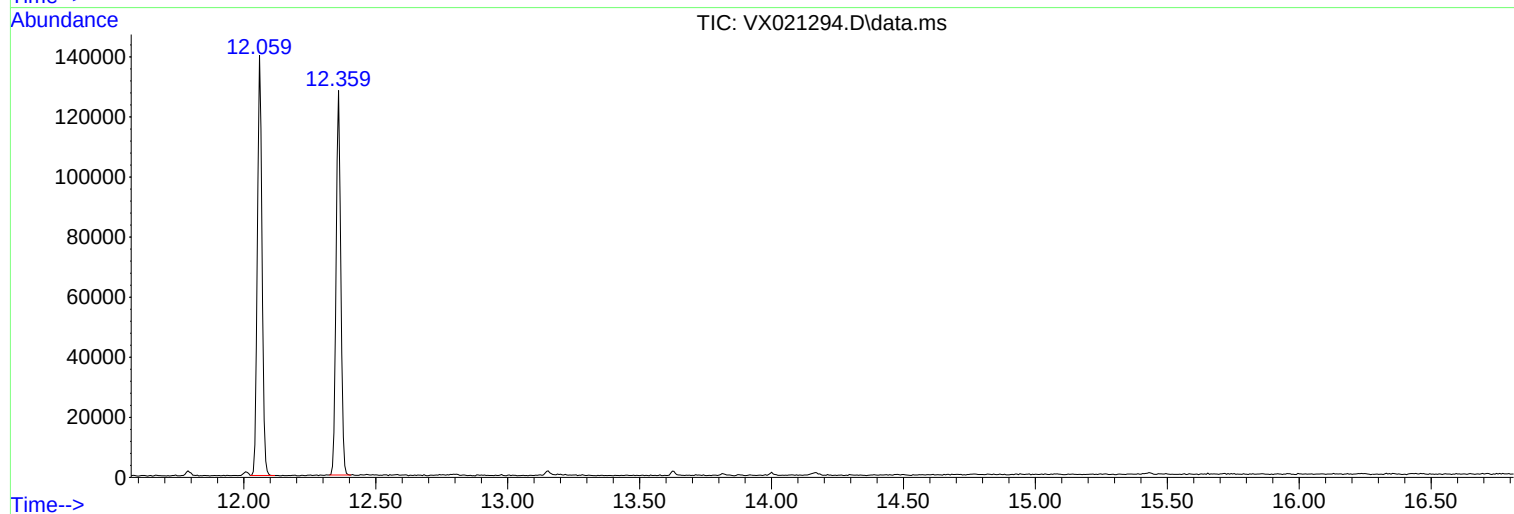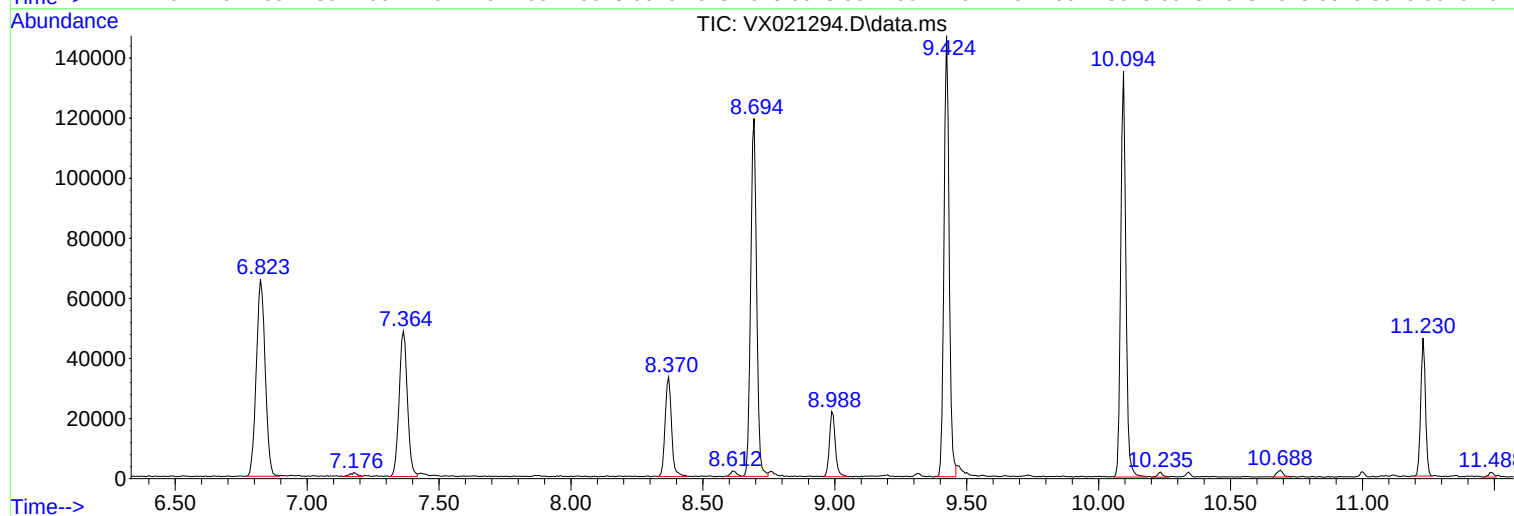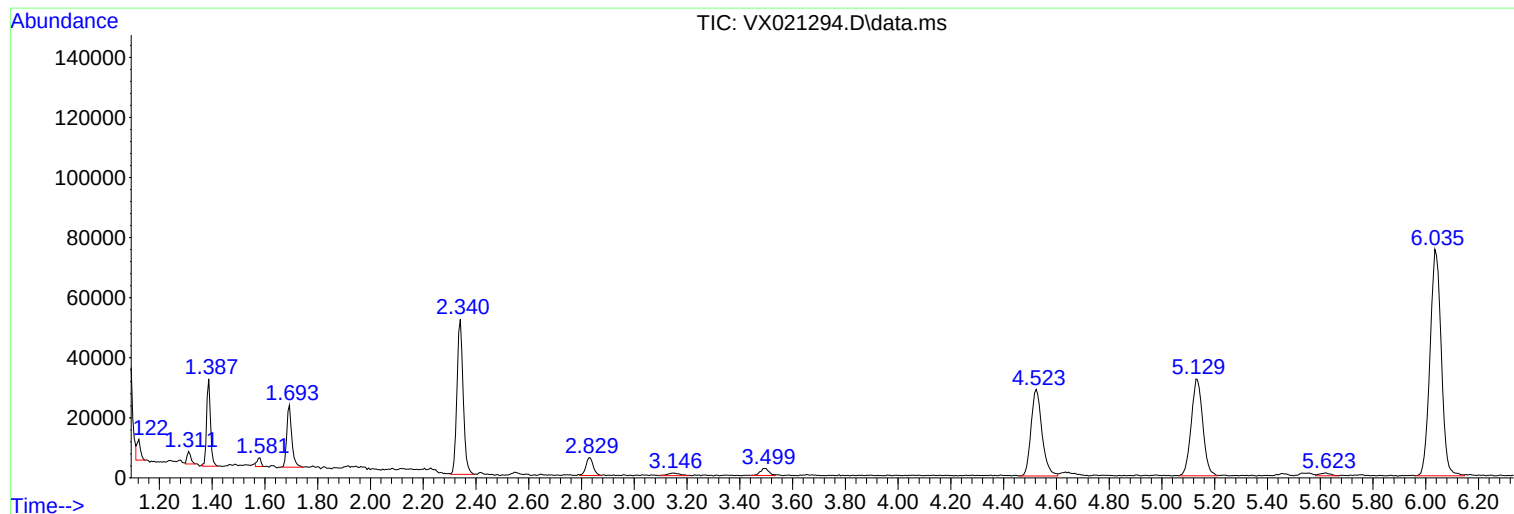

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
Data File : VX021294.D
Acq On : 19 Mar 2021 10:12
Operator : JC/MD
Sample : VX0320WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
Data File : VX021294.D
Acq On : 19 Mar 2021 10:12
Operator : JC/MD
Sample : VX0320WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
