


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032021\
 Data File : VX021292.D
 Acq On : 19 Mar 2021 08:28
 Operator : JC/MD
 Sample : BFB69
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB069

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR031821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 25 18:01:48 2021

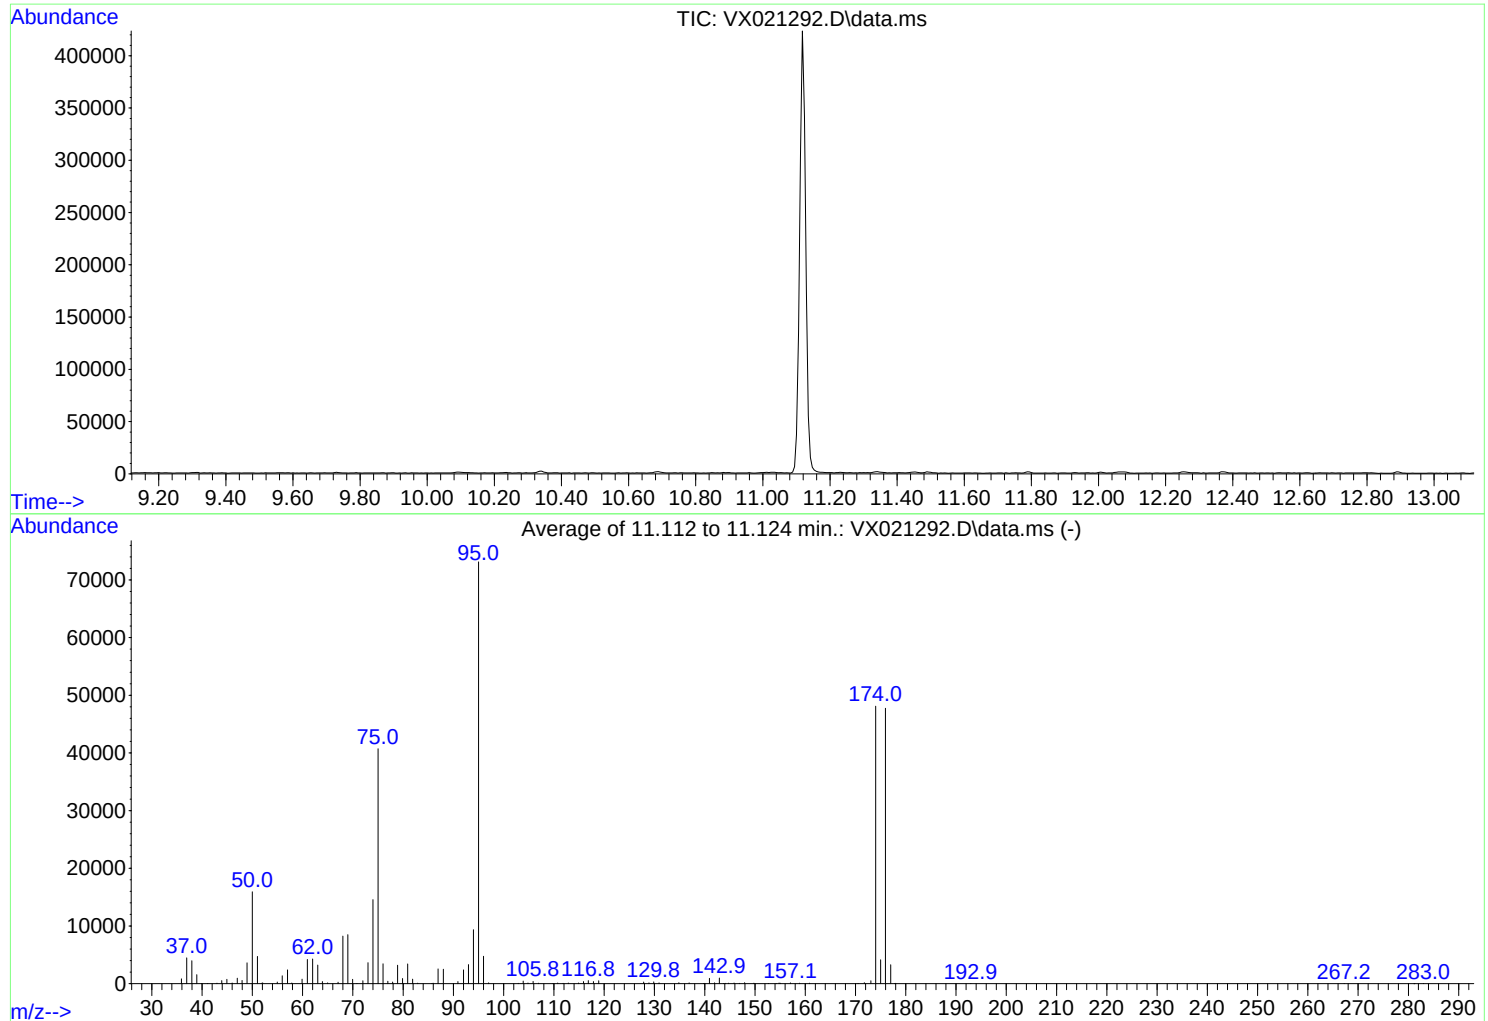

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1697

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	15913	PASS
75	95	30	80	55.7	40723	PASS
95	95	100	100	100.0	73136	PASS
96	95	5	9	6.5	4758	PASS
173	174	0.00	2	1.1	509	PASS
174	95	50	120	65.8	48115	PASS
175	174	5	9	8.6	4137	PASS
176	174	95	105	99.3	47763	PASS
177	176	5	10	6.9	3284	PASS

m/z	Abundance
39.90	237.0
43.90	330.0
73.00	178.0
207.10	63.0
281.10	166.0
282.10	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069

m/z	Abundance
35.90	839.0
37.00	4447.0
37.90	3961.0
39.00	1407.0
40.00	250.0
43.00	83.0
43.90	857.0
45.00	615.0
46.10	119.0
47.00	962.0
48.00	487.0
49.00	3547.0
50.00	14854.0
51.00	4492.0
51.90	228.0
54.90	286.0
56.00	1302.0
57.00	2208.0
57.90	119.0
59.90	691.0
61.00	3758.0
62.00	3806.0
63.00	3155.0
64.00	306.0
65.00	153.0
67.00	188.0
68.00	7943.0
69.00	8128.0
70.00	705.0
72.00	457.0
73.00	3612.0
74.00	13501.0
75.00	37016.0
76.00	3335.0
77.00	393.0
77.90	274.0
78.90	2985.0
79.90	685.0
80.90	3049.0
81.90	665.0
83.00	94.0
86.00	147.0
87.00	2095.0
88.00	2253.0
90.90	286.0
92.00	2056.0
93.00	3012.0
94.00	8640.0
95.00	63816.0
96.00	4252.0
97.10	126.0
103.00	56.0
103.90	346.0
104.80	84.0
105.90	380.0
106.90	92.0
109.80	61.0
110.80	104.0
112.90	110.0
114.90	81.0
115.90	368.0
116.80	442.0
117.80	287.0
118.90	434.0
127.90	281.0
129.00	100.0
129.90	240.0
130.80	114.0
134.90	149.0
136.90	110.0
139.80	59.0
140.90	743.0
142.00	112.0
142.90	843.0
144.70	73.0
145.80	88.0
146.80	52.0
148.00	130.0
150.00	53.0
154.80	142.0
157.00	97.0
159.00	100.0
160.90	90.0
171.90	172.0
174.00	34432.0
175.00	3335.0
175.90	34808.0
177.00	2474.0
177.80	107.0
193.00	55.0
207.00	94.0
281.10	168.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069

m/z	Abundance
35.90	879.0
37.00	5174.0
38.00	4552.0
38.90	1962.0
40.00	234.0
42.90	63.0
43.90	938.0
44.90	1020.0
45.90	103.0
47.00	1050.0
47.90	750.0
48.90	4324.0
50.00	18960.0
51.00	5714.0
52.10	246.0
54.90	297.0
56.00	1662.0
57.00	2988.0
57.80	99.0
59.90	948.0
61.00	5135.0
62.00	5451.0
63.00	3799.0
63.90	445.0
65.00	150.0
67.00	330.0
68.00	9275.0
69.00	10012.0
69.90	942.0
70.80	66.0
72.00	699.0
73.00	4628.0
74.00	16768.0
75.00	49104.0
76.00	4105.0
76.90	471.0
77.90	334.0
78.90	3643.0
79.90	1023.0
80.90	4014.0
81.90	974.0
82.80	111.0
85.90	139.0
86.90	2968.0
88.00	3036.0
90.90	475.0
92.00	2924.0
93.00	4031.0
94.00	11313.0
95.00	87520.0
96.00	5942.0
96.90	157.0
102.90	56.0
103.90	489.0
104.90	148.0
105.80	428.0
106.90	107.0
109.80	56.0
110.70	94.0
111.80	133.0
112.80	136.0
114.90	127.0
115.90	492.0
116.90	670.0
117.90	503.0
118.90	546.0
127.80	295.0
128.90	188.0
129.80	370.0
130.90	183.0
134.90	206.0
136.90	168.0
140.00	89.0
141.00	1008.0
141.90	145.0
142.90	1123.0
143.70	64.0
144.10	72.0
144.80	102.0
145.90	105.0
146.90	75.0
147.90	202.0
149.80	117.0
154.20	72.0
154.80	206.0
157.10	137.0
158.90	97.0
160.80	104.0
170.50	53.0
171.70	187.0
173.00	719.0
174.00	57848.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069

175.00	4619.0
176.00	55088.0
177.00	3792.0
178.00	86.0
267.20	53.0
281.20	123.0
283.00	50.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069

m/z	Abundance
35.90	798.0
36.90	3805.0
38.00	3393.0
38.90	1289.0
40.00	334.0
41.10	87.0
43.00	93.0
43.90	820.0
45.00	650.0
46.00	95.0
47.00	793.0
47.90	426.0
49.00	2946.0
50.00	13926.0
51.00	3949.0
52.00	185.0
55.00	245.0
55.90	1130.0
57.00	1946.0
57.90	132.0
59.90	677.0
60.90	3700.0
62.00	3574.0
63.00	2671.0
64.00	313.0
65.00	82.0
67.10	201.0
68.00	7484.0
69.00	7301.0
70.00	574.0
70.80	57.0
71.90	356.0
73.00	3239.0
74.00	13406.0
75.00	36048.0
76.00	2876.0
77.00	424.0
77.90	265.0
78.90	2925.0
79.90	925.0
80.90	3190.0
81.90	654.0
82.90	62.0
85.70	63.0
86.90	2567.0
88.00	2233.0
90.90	299.0
92.00	2168.0
93.00	2915.0
94.00	8131.0
95.00	68072.0
96.00	4080.0
97.00	108.0
102.80	52.0
103.90	521.0
104.90	124.0
105.90	389.0
107.00	96.0
110.80	161.0
111.80	72.0
112.80	72.0
114.90	119.0
115.90	266.0
116.90	453.0
117.90	327.0
118.90	522.0
127.80	302.0
128.80	141.0
129.90	302.0
131.00	140.0
134.80	191.0
136.90	146.0
140.00	68.0
140.90	1022.0
141.90	143.0
142.90	969.0
143.80	56.0
144.10	64.0
144.70	100.0
145.90	109.0
147.00	61.0
148.00	190.0
149.70	73.0
152.70	53.0
155.00	216.0
157.10	167.0
158.80	85.0
160.80	94.0
171.70	162.0
173.10	809.0
174.00	52064.0
175.00	4458.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069

176.00	53392.0
177.00	3585.0
178.00	124.0
192.90	62.0
207.10	73.0
281.00	239.0
282.10	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB069