

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
 Data File : VX034621.D
 Acq On : 20 Mar 2023 12:35
 Operator : JC/MD
 Sample : VX0320MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0320MBL01

Quant Time: Mar 21 01:39:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	271678	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	460058	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	412979	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	194230	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	198467	50.215	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.420%
35) Dibromofluoromethane	5.385	113	148497	48.888	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.780%
50) Toluene-d8	8.647	98	550555	48.553	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.100%
62) 4-Bromofluorobenzene	11.079	95	218637	47.735	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
Data File : VX034621.D
Acq On : 20 Mar 2023 12:35
Operator : JC/MD
Sample : VX0320MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0320MBL01

Quant Time: Mar 21 01:39:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




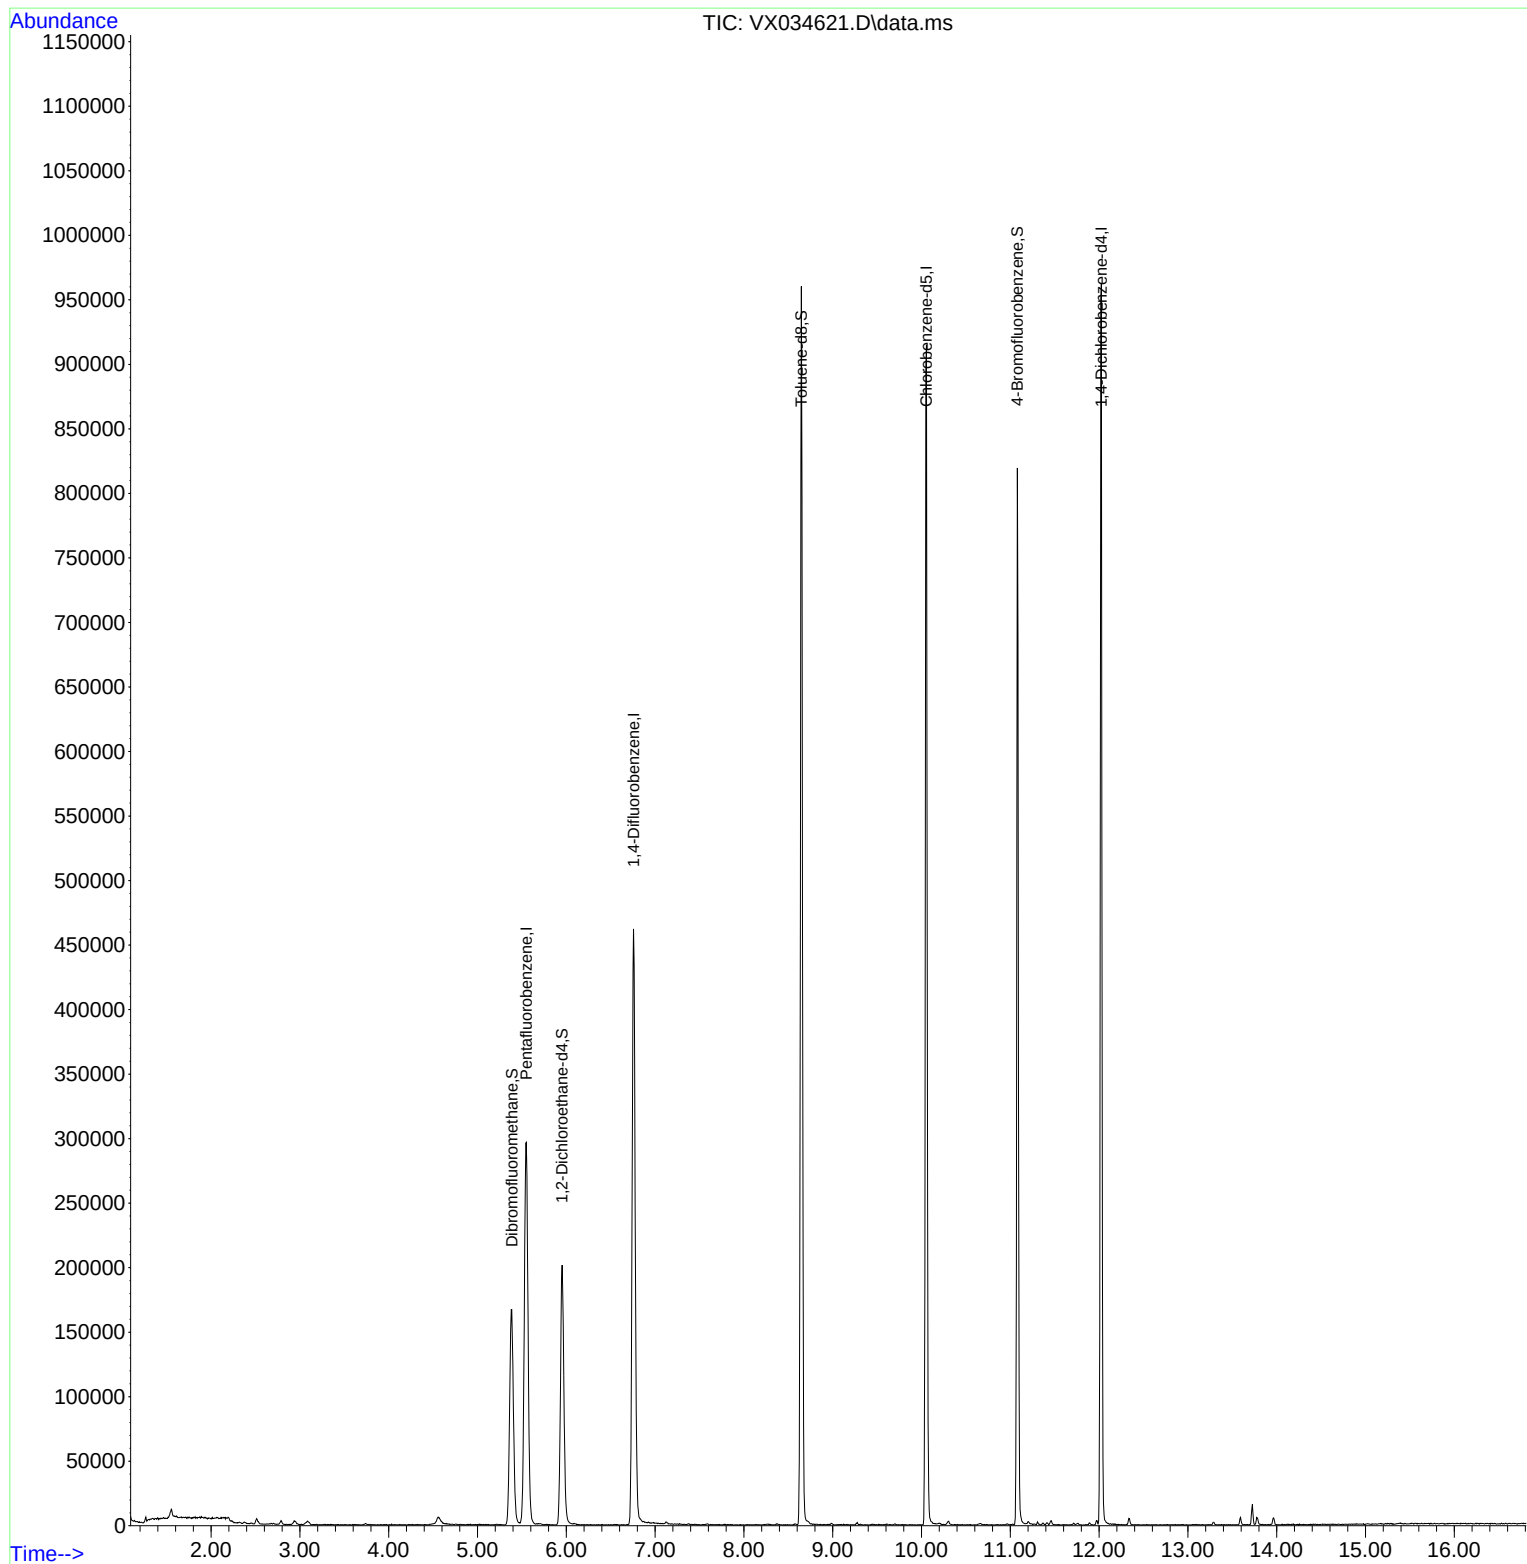


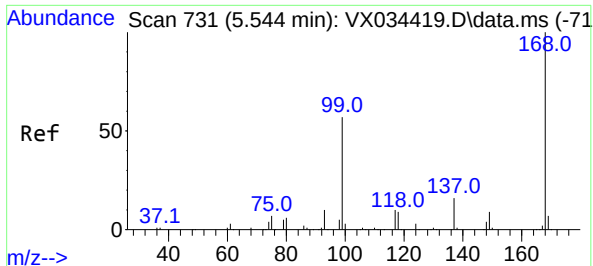

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35




Instrument :
MSVOA_X
ClientSampleId :
VX0320MBL01


Tgt Ion:168 Resp: 271678
Ion Ratio Lower Upper
168 100
99 61.6 45.7 68.5

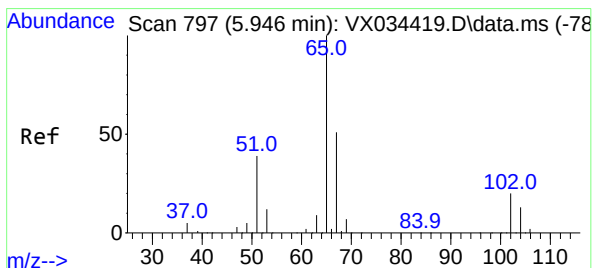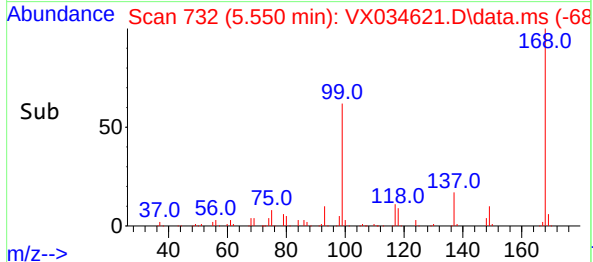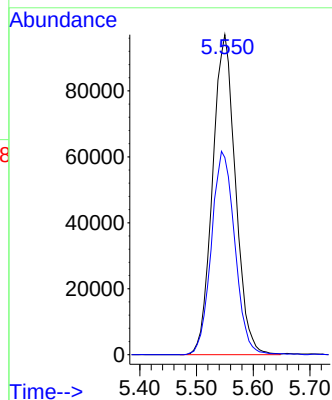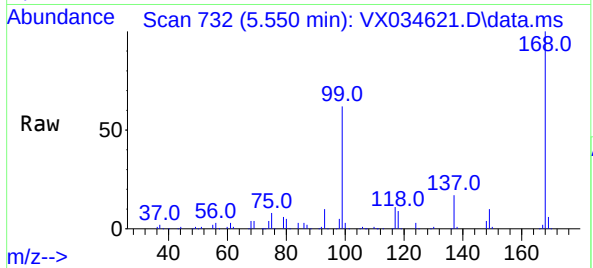

#33
1,2-Dichloroethane-d4
Concen: 50.215 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35

Tgt Ion: 65 Resp: 198467
Ion Ratio Lower Upper
65 100
67 50.1 0.0 104.0

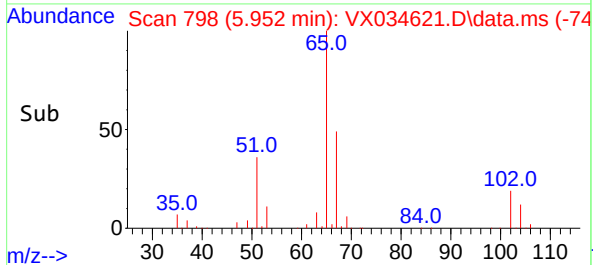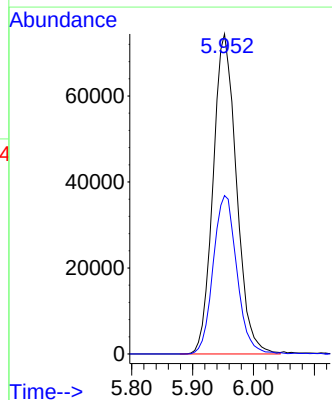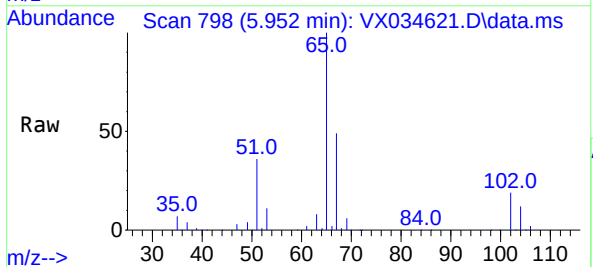

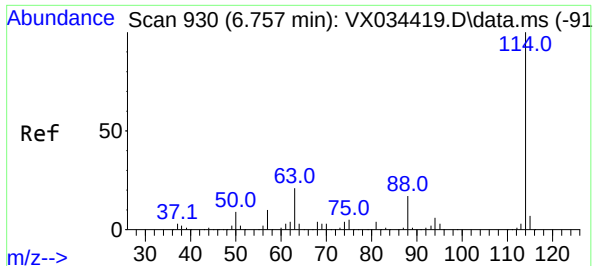

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 91

Delta R.T. 0.000 min

Lab File: VX034621.D

Acq: 20 Mar 2023 12:35

Instrument :

MSVOA_X

ClientSampleId :

VX0320MBL01





Tgt Ion:114 Resp: 460058

Ion Ratio Lower Upper

114 100

63 22.6 0.0 42.2

88 16.7 0.0 33.2

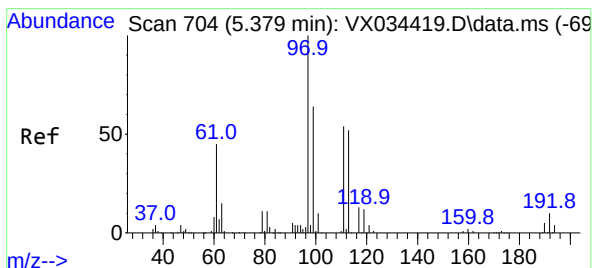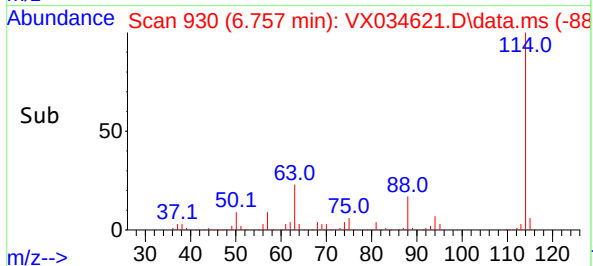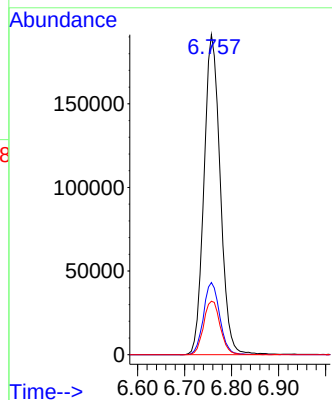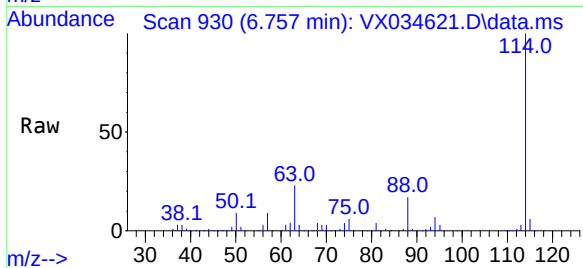

#35

Dibromofluoromethane

Concen: 48.888 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX034621.D

Acq: 20 Mar 2023 12:35




Tgt Ion:113 Resp: 148497


Ion Ratio Lower Upper

113 100

111 102.4 83.7 125.5

192 18.7 15.4 23.2


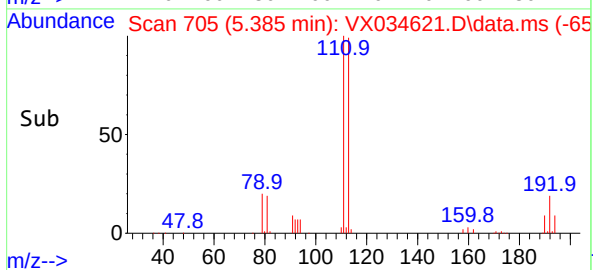
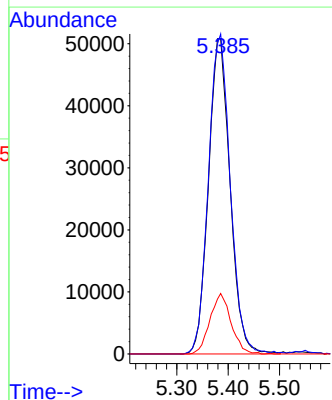
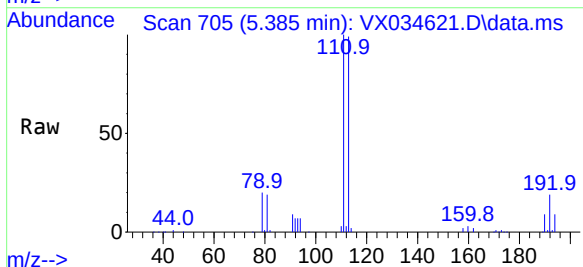


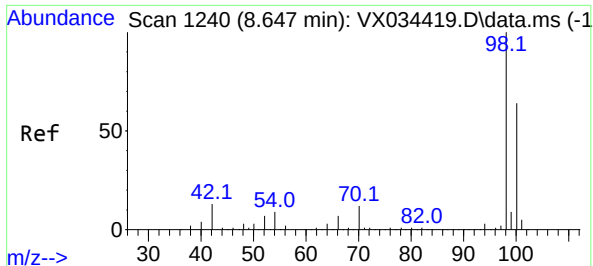

#50
Toluene-d8
Concen: 48.553 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35




Instrument :
MSVOA_X
ClientSampleId :
VX0320MBL01


Tgt Ion: 98 Resp: 550555
Ion Ratio Lower Upper
98 100
100 66.8 52.5 78.7

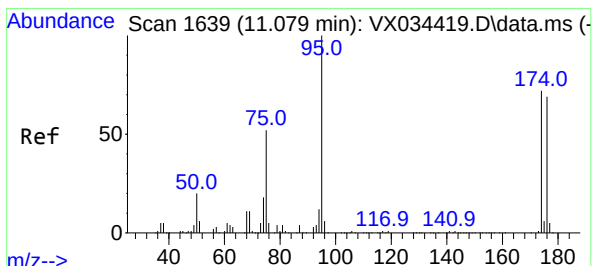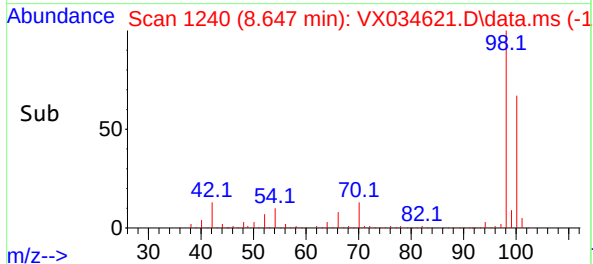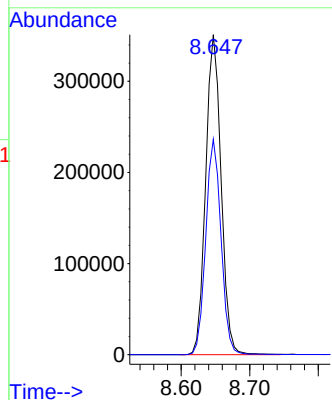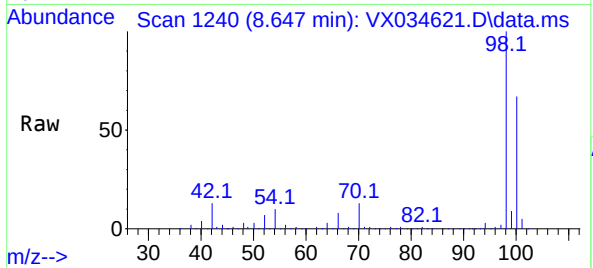

#62
4-Bromofluorobenzene
Concen: 47.735 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35

Tgt Ion: 95 Resp: 218637
Ion Ratio Lower Upper
95 100
174 69.8 0.0 147.4
176 68.3 0.0 140.6


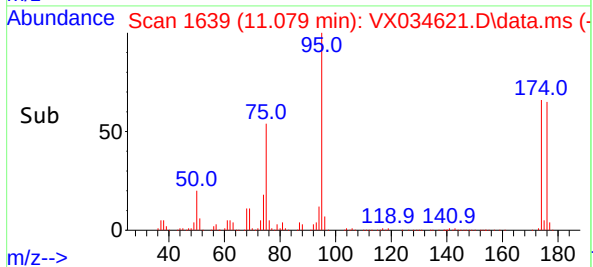
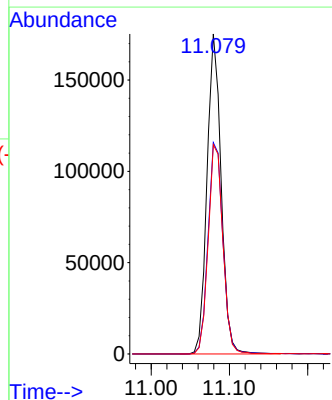
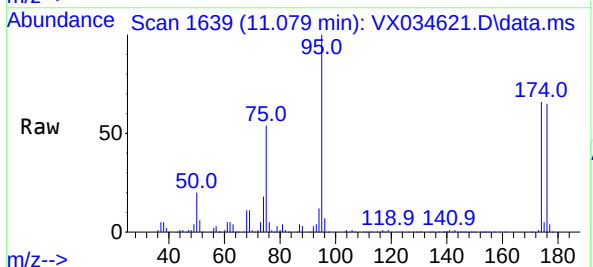


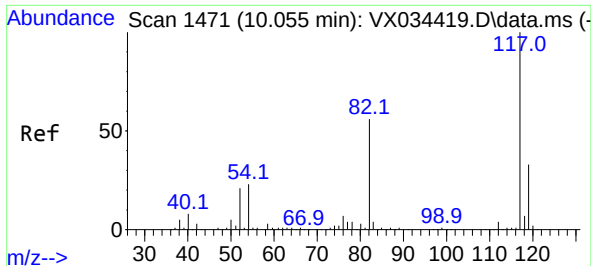

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35

Instrument :
MSVOA_X
ClientSampleId :
VX0320MBL01

Tgt Ion:117 Resp: 412979
Ion Ratio Lower Upper
117 100
82 57.5 45.0 67.4
119 32.4 26.0 39.0

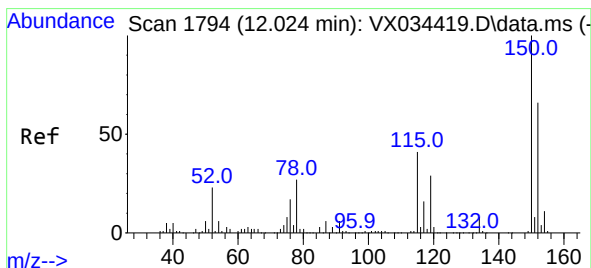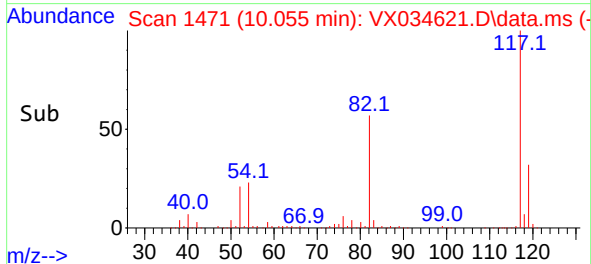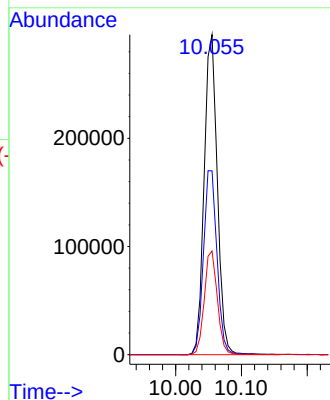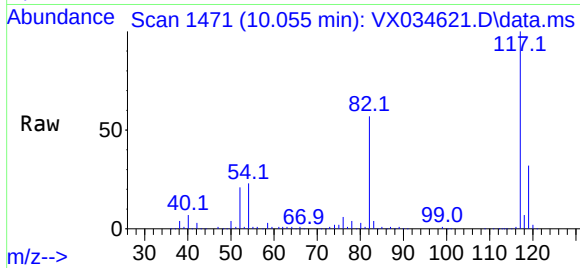

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034621.D
Acq: 20 Mar 2023 12:35

Tgt Ion:152 Resp: 194230
Ion Ratio Lower Upper
152 100
115 64.4 45.0 135.0
150 158.4 0.0 352.4

