

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
 Data File : VX034633.D
 Acq On : 20 Mar 2023 17:19
 Operator : JC/MD
 Sample : 02015-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Mar 21 01:45:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	255434	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	428634	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	372165	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4</						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
Data File : VX034633.D
Acq On : 20 Mar 2023 17:19
Operator : JC/MD
Sample : 02015-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Mar 21 01:45:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration



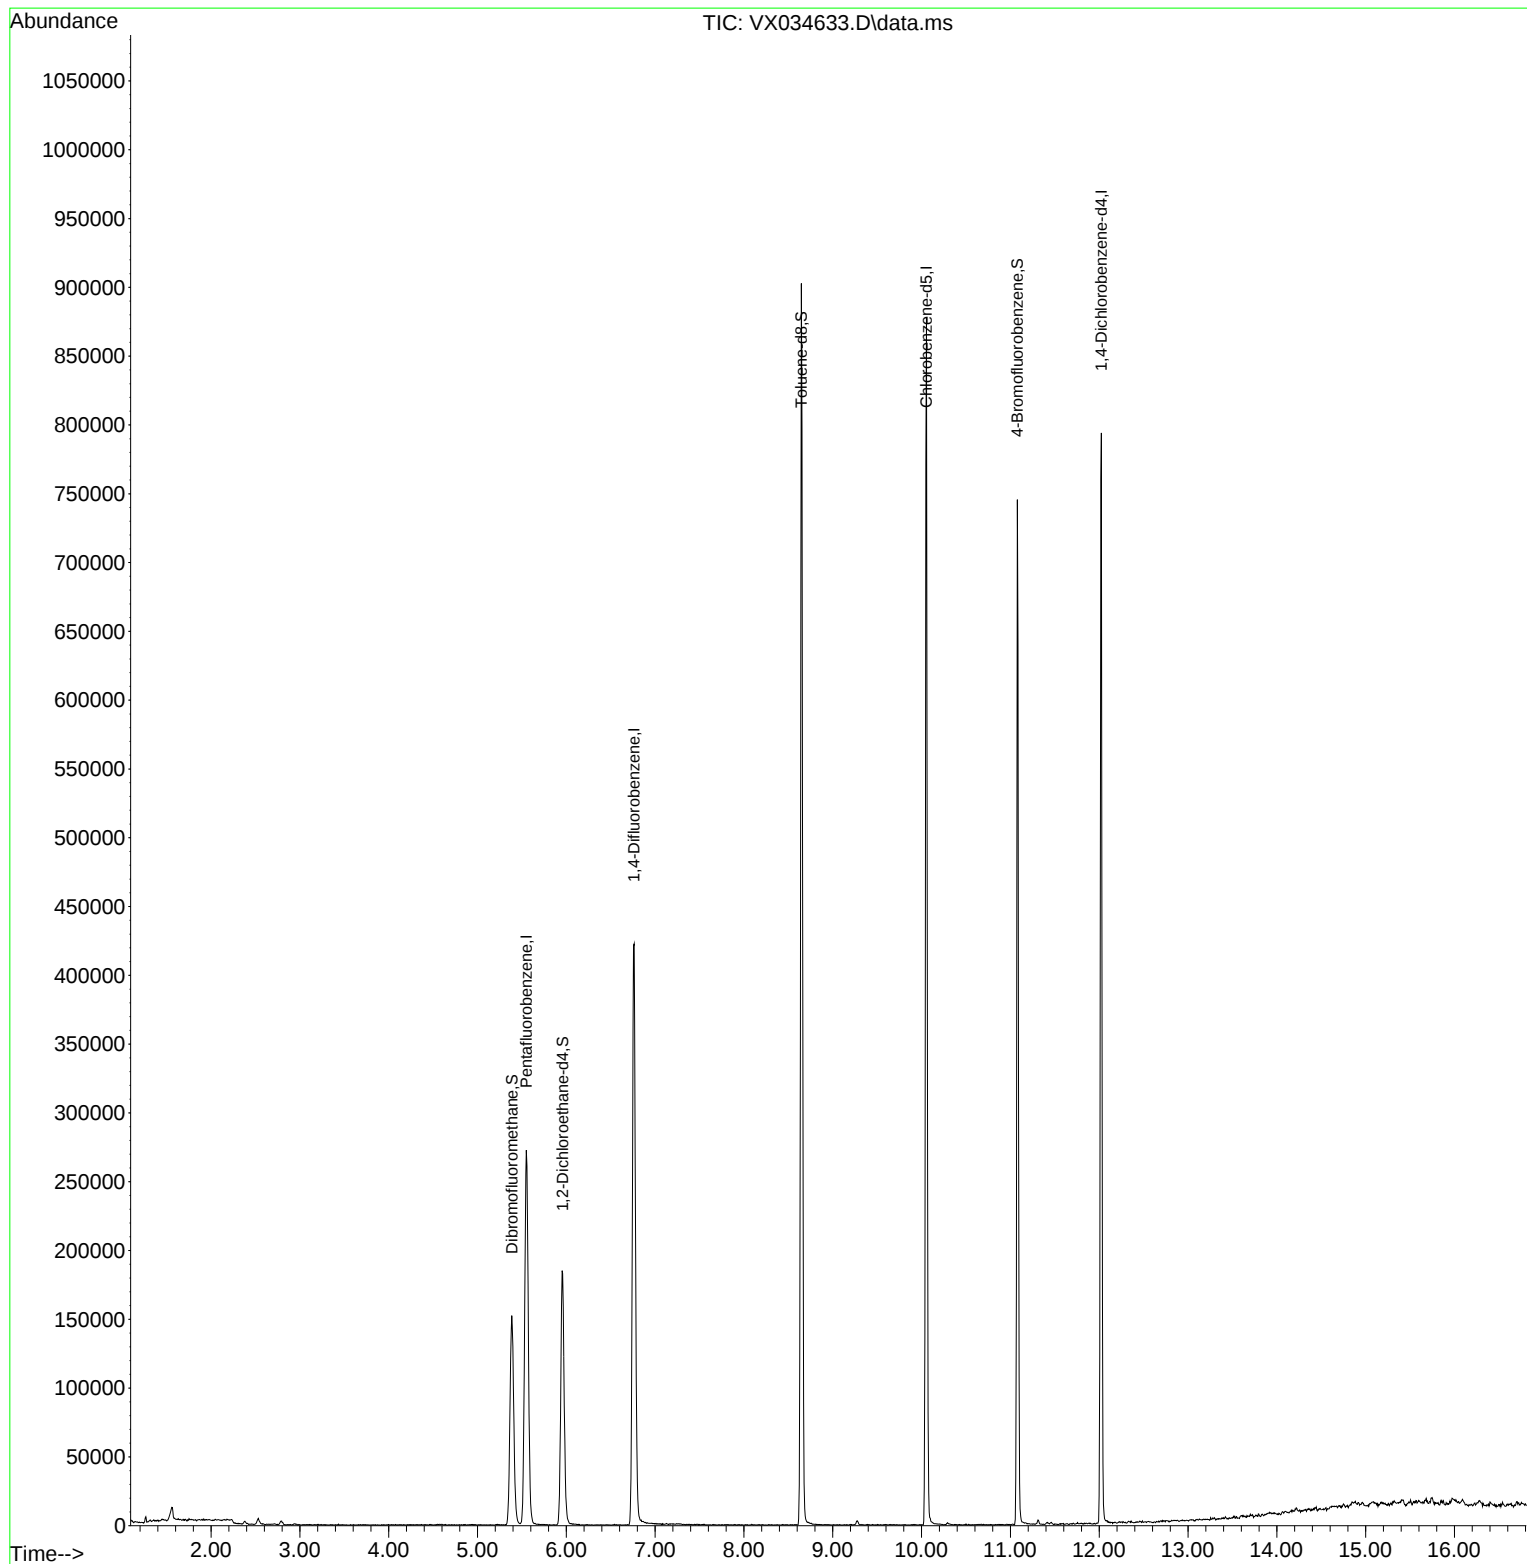





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034633.D
Acq: 20 Mar 2023 17:19

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:168 Resp: 255434
Ion Ratio Lower Upper
168 100
99 58.2 45.7 68.5

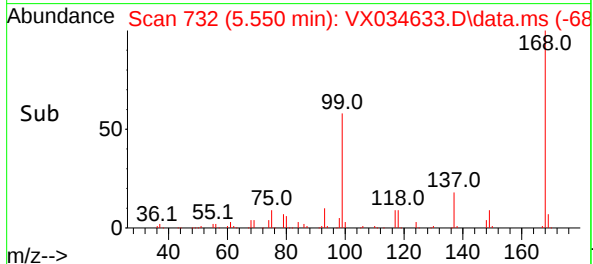
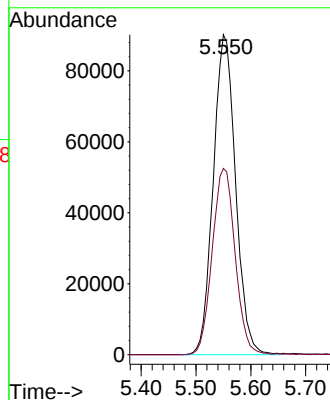
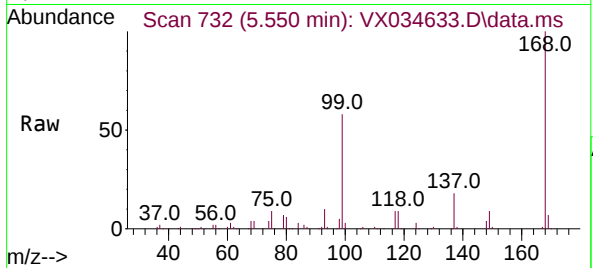


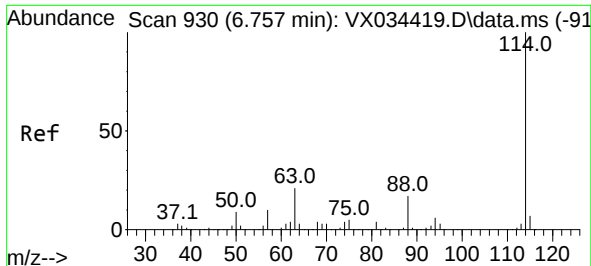


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034633.D
Acq: 20 Mar 2023 17:19

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:114 Resp: 428634
Ion Ratio Lower Upper
114 100
63 21.2 0.0 42.2
88 16.0 0.0 33.2


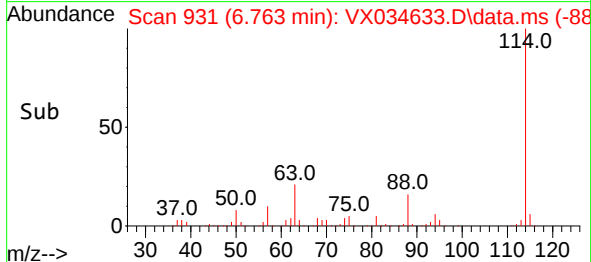
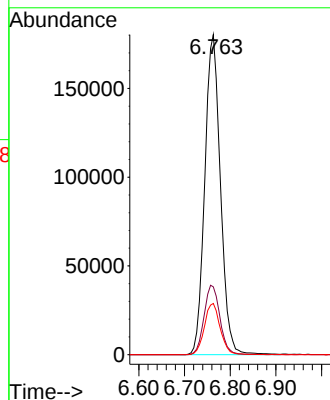
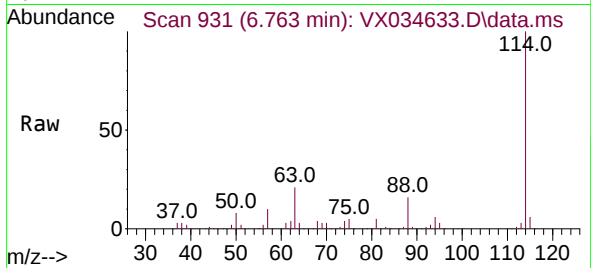


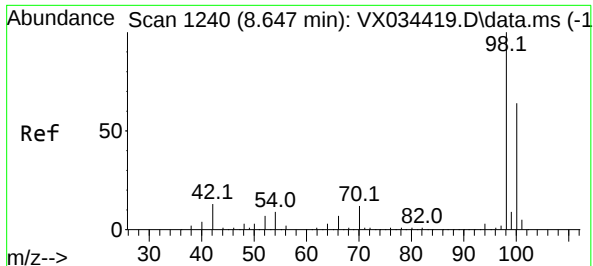


#50
Toluene-d8
Concen: 48.278 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034633.D
Acq: 20 Mar 2023 17:19

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion: 98 Resp: 510044
Ion Ratio Lower Upper
98 100
100 65.9 52.5 78.7

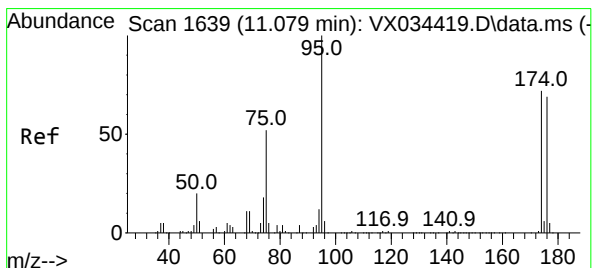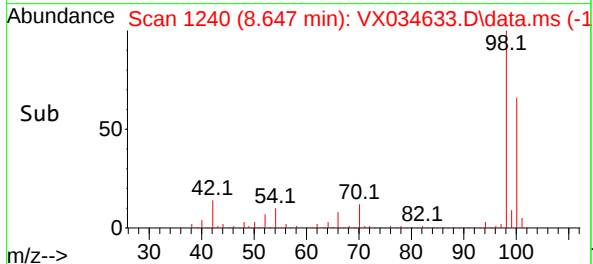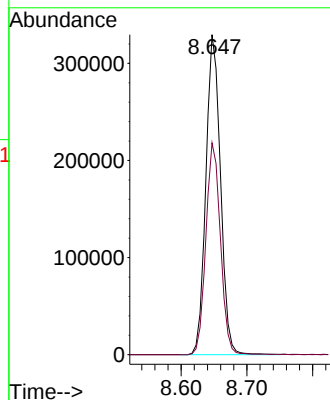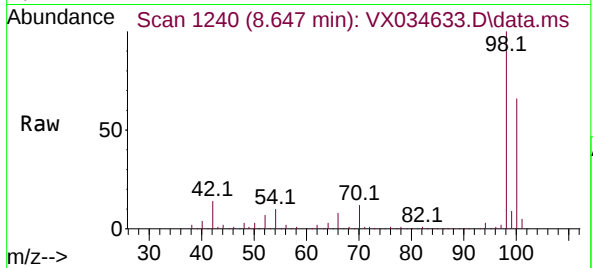

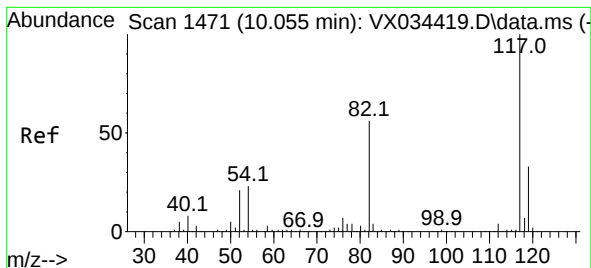

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX034633.D

Acq: 20 Mar 2023 17:19

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 372165

Ion Ratio Lower Upper

117 100

82 56.2 45.0 67.4