

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
 Data File : VX034640.D
 Acq On : 20 Mar 2023 20:04
 Operator : JC/MD
 Sample : 02012-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-23-GW01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV2	170574	498831	32.33%	5.746%
2	5.550	721	732	748	rVB	310054	881127	57.12%	10.150%
3	5.952	787	798	821	rBV	205705	554320	35.93%	6.385%
4	6.763	920	931	946	rBV	474886	1164239	75.47%	13.411%
5	8.647	1233	1240	1247	rBV	975062	1542715	100.00%	17.770%
6	8.720	1247	1252	1263	rVB	305491	480445	31.14%	5.534%
7	10.055	1465	1471	1486	rBV	964978	1315425	85.27%	15.152%
8	11.079	1634	1639	1653	rBV	828635	1059481	68.68%	12.204%
9	12.024	1788	1794	1803	rBV	862724	1150520	74.58%	13.253%
10	12.225	1821	1827	1838	rBV5	6647	17372	1.13%	0.200%
11	13.780	2078	2082	2091	rVB	10594	16987	1.10%	0.196%




Sum of corrected areas: 8681462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
Data File : VX034640.D
Acq On : 20 Mar 2023 20:04
Operator : JC/MD
Sample : 02012-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-23-GW01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

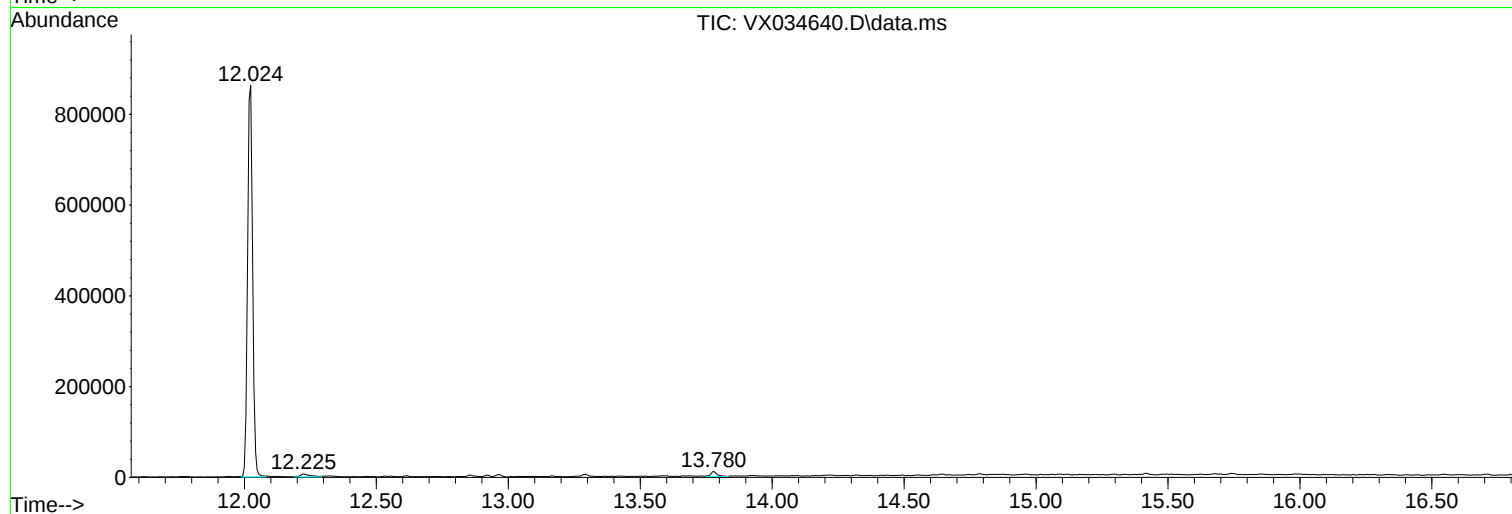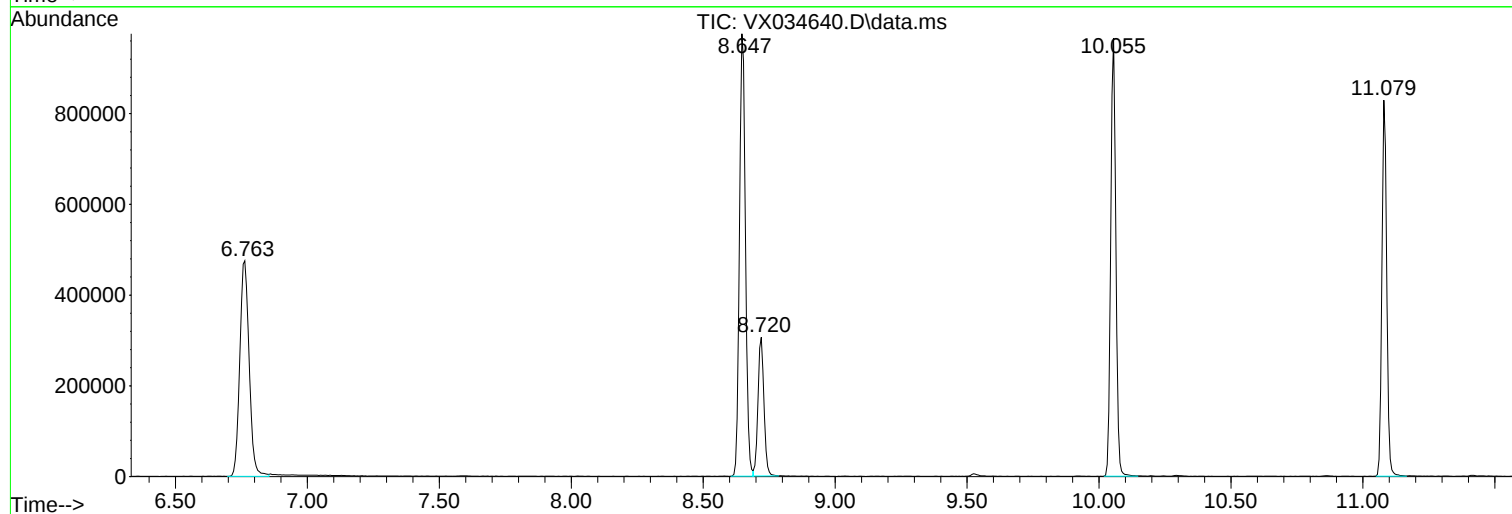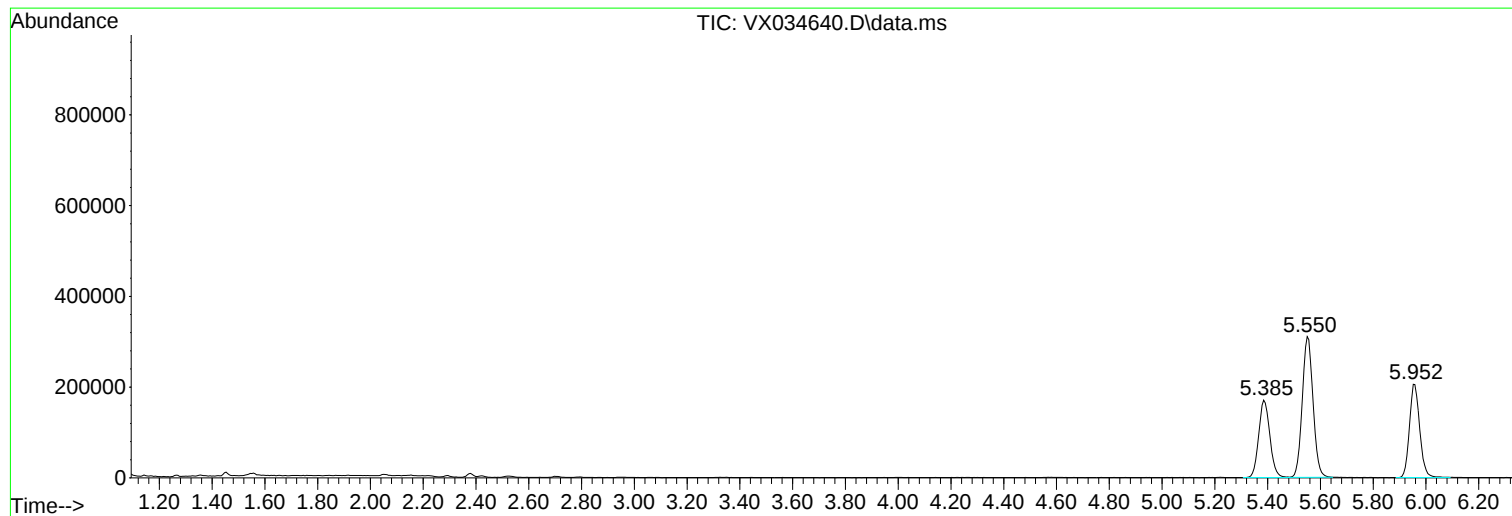

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
Data File : VX034640.D
Acq On : 20 Mar 2023 20:04
Operator : JC/MD
Sample : 02012-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-23-GW01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032023\
Data File : VX034640.D
Acq On : 20 Mar 2023 20:04
Operator : JC/MD
Sample : 02012-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-23-GW01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------