

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032119\
 Data File : VX008301.D
 Acq On : 21 Mar 2019 19:32
 Operator : JC/SP
 Sample : K1937-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB04-20190313

Quant Time: Mar 22 09:57:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 19 13:15:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	228320	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	375799	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	322795	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	136406	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	153390	44.61	ug/l	0.00
Spiked Amount			Recovery	=	89.22%	
35) Dibromofluoromethane	5.50	113	115030	45.72	ug/l	0.00
Spiked Amount			Recovery	=	91.44%	
50) Toluene-d8	8.71	98	457665	47.98	ug/l	0.00
Spiked Amount			Recovery	=	95.96%	
62) 4-Bromofluorobenzene	11.13	95	146567	44.63	ug/l	0.00
Spiked Amount			Recovery	=	89.26%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032119\
Data File : VX008301.D
Acq On : 21 Mar 2019 19:32
Operator : JC/SP
Sample : K1937-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB04-20190313

Quant Time: Mar 22 09:57:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 19 13:15:13 2019
Response via : Initial Calibration

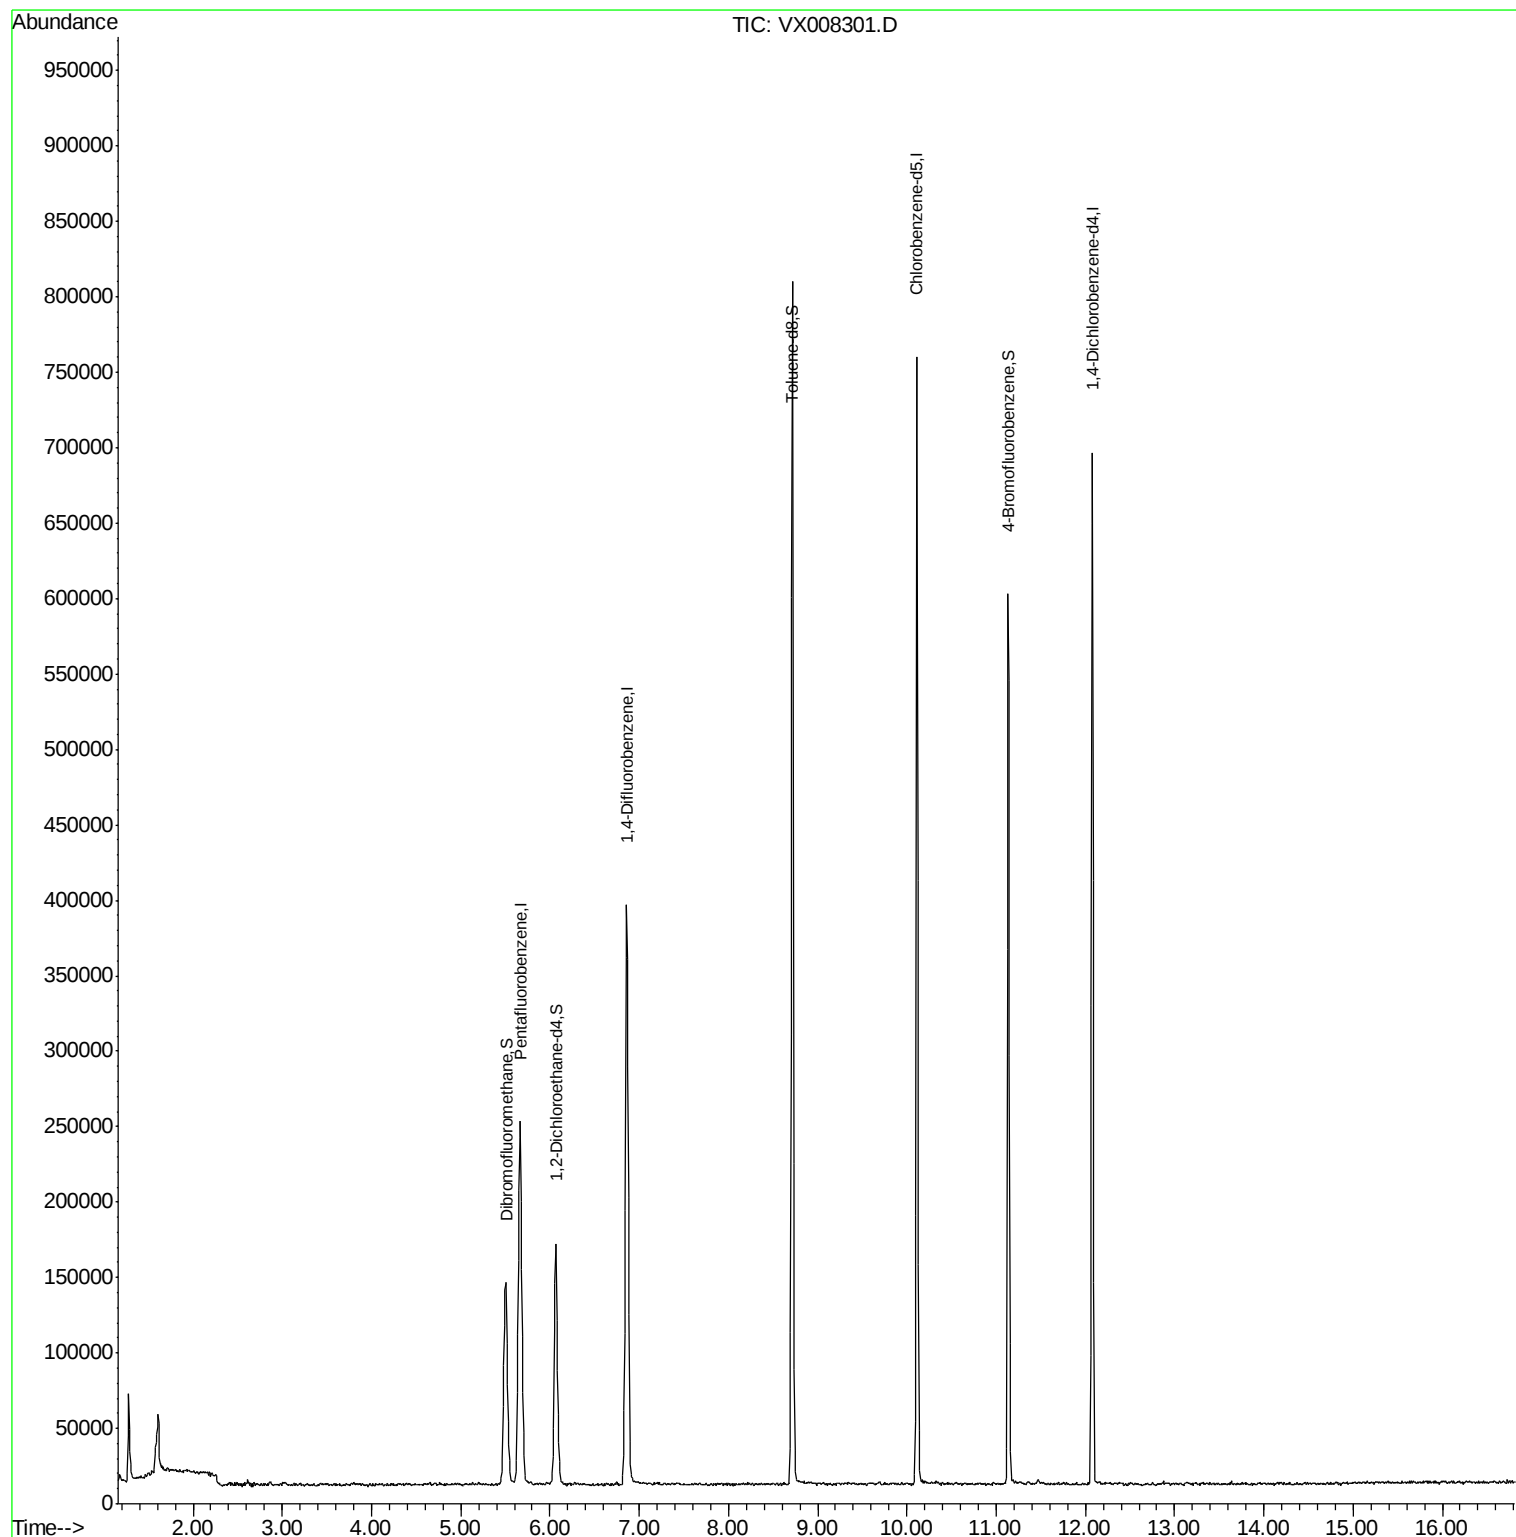

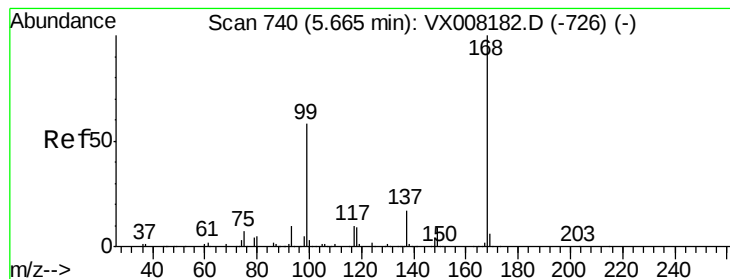

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX008301.D

Acq: 21 Mar 2019 19:32

Instrument :

MSVOA_X

ClientSampleId :


BP-TB04-20190313

Tot Ion:168 Resp: 228320

Ion Ratio Lower Upper

168 100

99 53.1 37.6 56.4


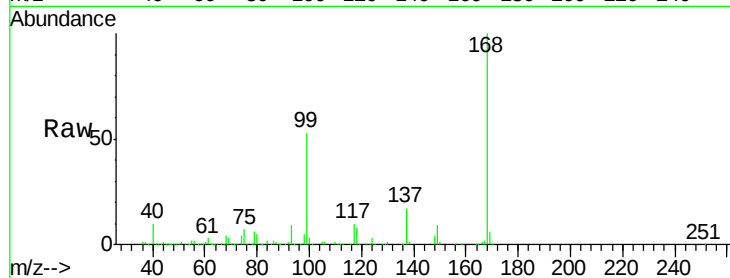


Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

Time--> 5.50 5.60 5.70 5.80

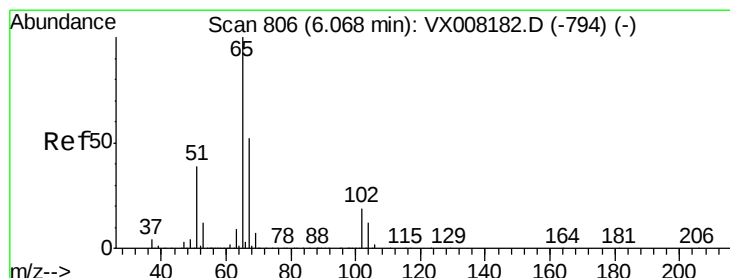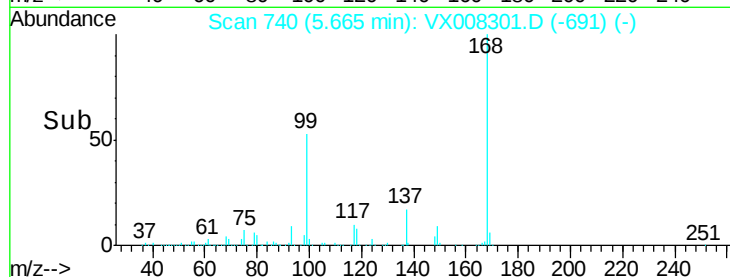

#33

1,2-Dichloroethane-d4

Concen: 44.607 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX008301.D


Acq: 21 Mar 2019 19:32

Tgt Ion: 65 Resp: 153390

Ion Ratio Lower Upper

65 100

67 50.5 0.0 110.0

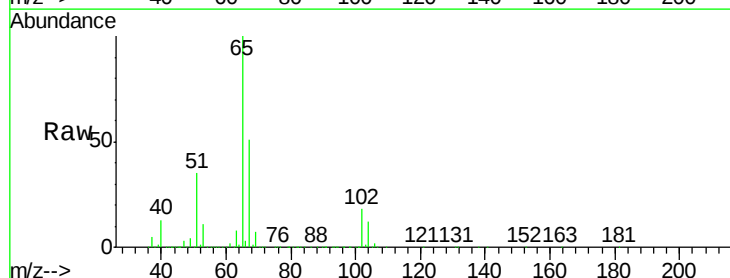



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

Time--> 5.90 6.00 6.10 6.20

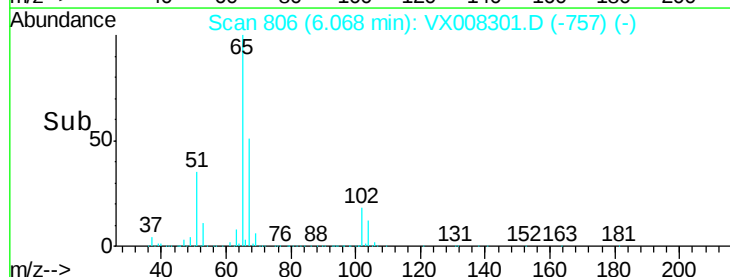

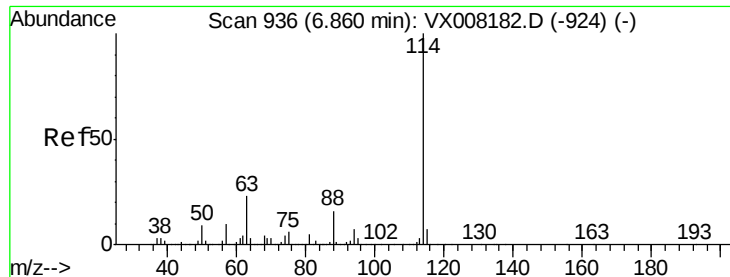

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX008301.D

Acq: 21 Mar 2019 19:32

Instrument :

MSVOA_X

ClientSampleId :

BP-TB04-20190313


Tot Ion:114 Resp: 375799

Ion Ratio Lower Upper

114 100

63 21.8 0.0 39.8




88 16.5 0.0 31.4

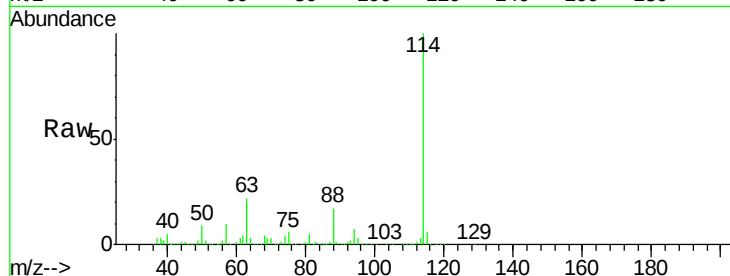

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

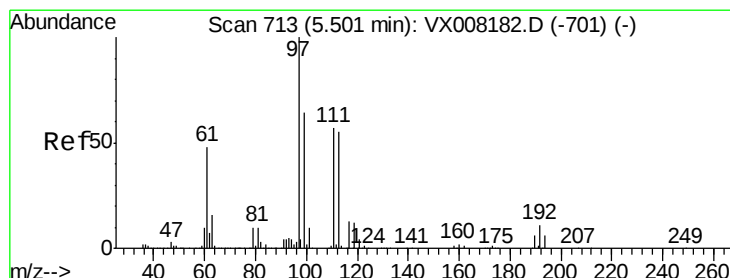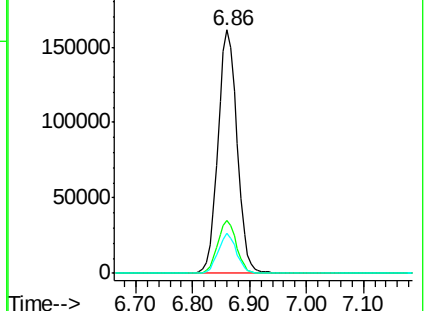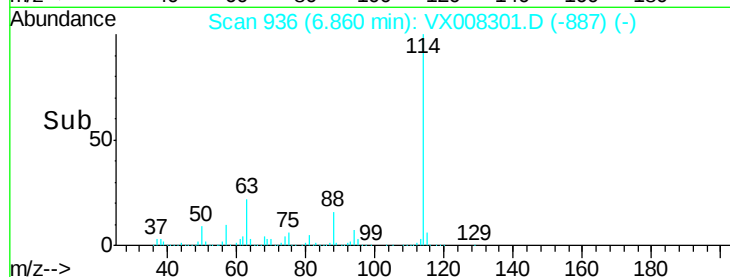

#35

Dibromofluoromethane

Concen: 45.724 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX008301.D

Acq: 21 Mar 2019 19:32


Tgt Ion:113 Resp: 115030

Ion Ratio Lower Upper

113 100

111 101.6 81.4 122.0



192 21.9 19.4 29.0

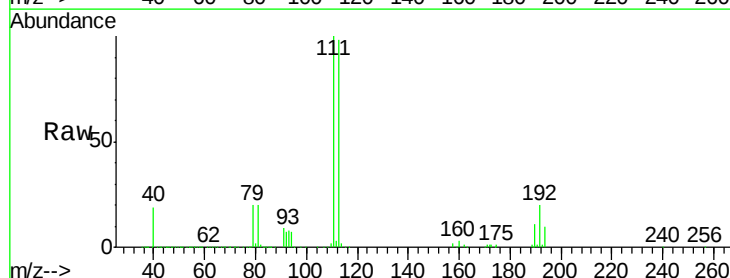


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

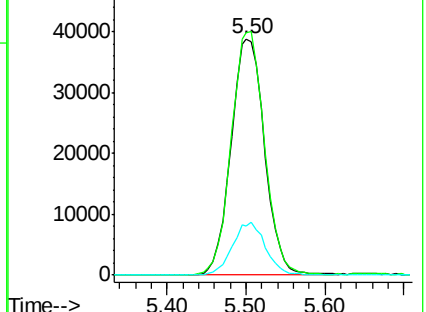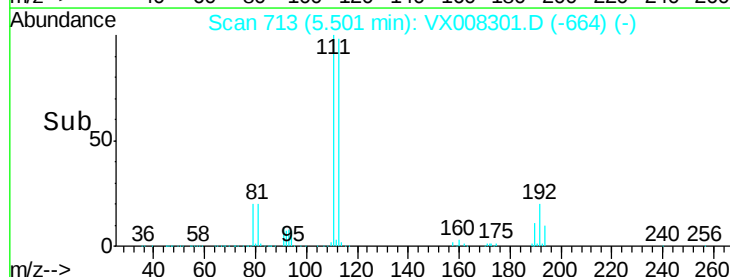

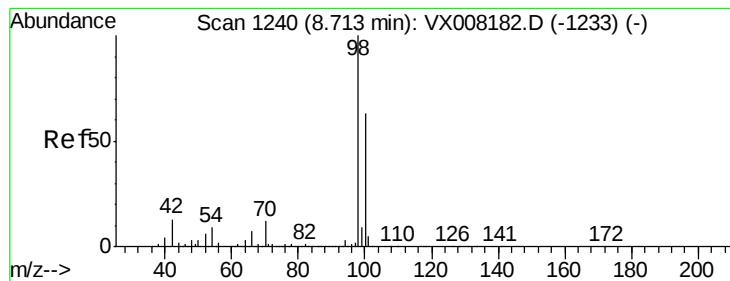

#50

Toluene-d8

Concen: 47.983 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX008301.D

Acq: 21 Mar 2019 19:32

Instrument :

MSVOA_X

ClientSampleId :


BP-TB04-20190313

Tot Ion: 98 Resp: 457665

Ion Ratio Lower Upper

98 100

100 63.2 51.7 77.5

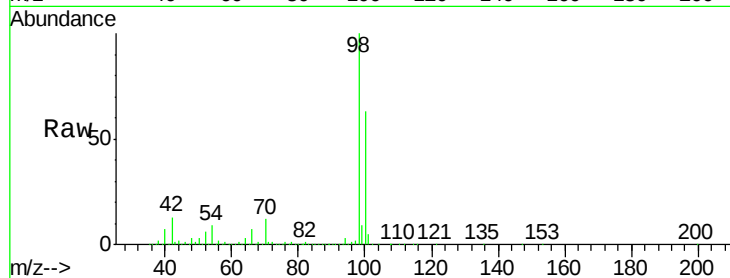

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71



300000

200000

100000

0

Time--> 8.60 8.70 8.80

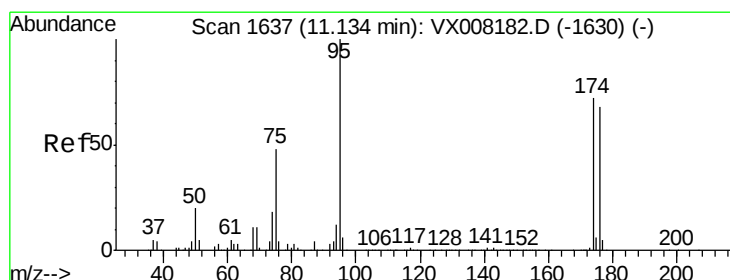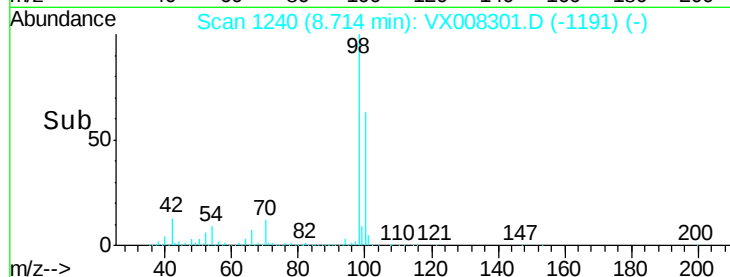

#62

4-Bromofluorobenzene

Concen: 44.629 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX008301.D

Acq: 21 Mar 2019 19:32


Tgt Ion: 95 Resp: 146567

Ion Ratio Lower Upper

95 100

174 84.8 0.0 182.8

176 81.4 0.0 178.0

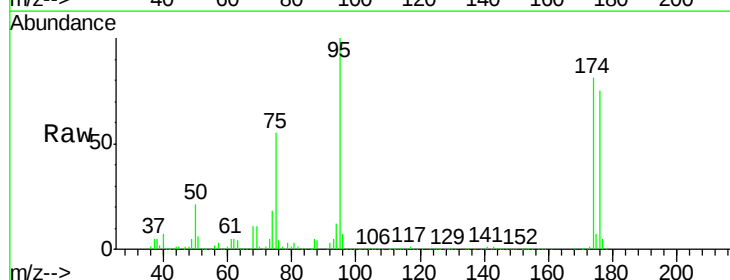

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.13


150000


100000

50000

0

Time--> 11.10 11.20 11.30




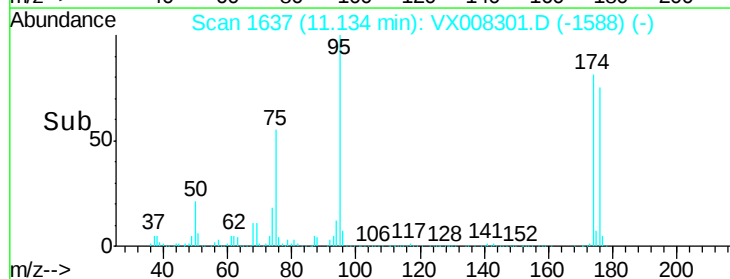


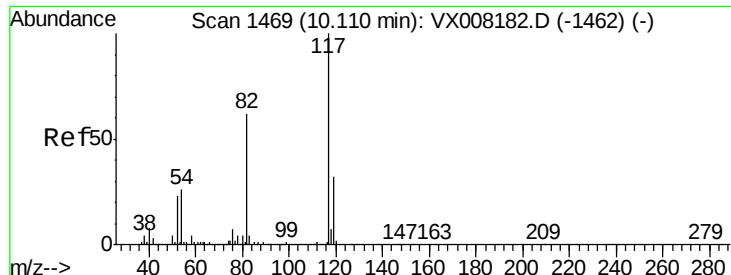

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX008301.D
Acq: 21 Mar 2019 19:32

Instrument :
MSVOA_X
ClientSampleId :
BP-TB04-20190313

Tot Ion:117 Resp: 322795
Ion Ratio Lower Upper
117 100
82 57.2 44.3 66.5
119 31.5 25.3 37.9

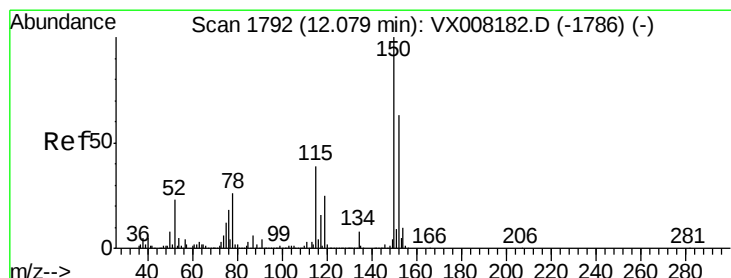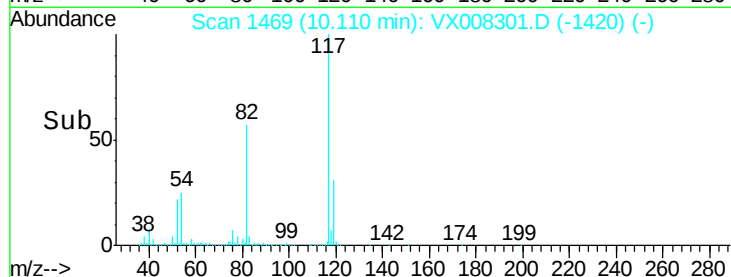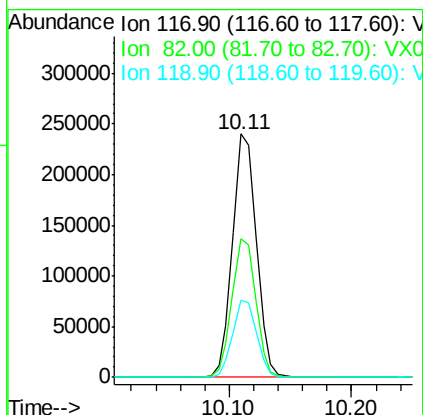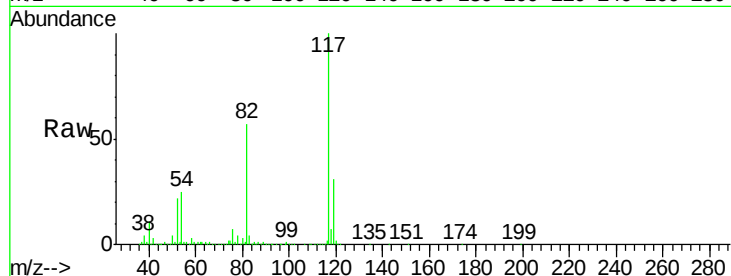

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX008301.D
Acq: 21 Mar 2019 19:32

Tgt Ion:152 Resp: 136406
Ion Ratio Lower Upper
152 100
115 58.3 38.6 115.7
150 154.9 0.0 348.4

