

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032119\
 Data File : VX008292.D
 Acq On : 21 Mar 2019 15:48
 Operator : JC/SP
 Sample : K1963-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPS1-TT-MW307I-20190314

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	27	rBV	100016	123997	8.24%	1.584%
2	1.611	66	75	81	rBV	34060	79967	5.32%	1.022%
3	2.245	177	179	184	rVB	9618	15623	1.04%	0.200%
4	5.501	702	713	725	rBV	171571	490431	32.61%	6.266%
5	5.665	730	740	753	rVB	291722	816110	54.26%	10.427%
6	6.068	795	806	819	rBV	204340	543259	36.12%	6.941%
7	6.860	925	936	946	rBV	479516	1099338	73.09%	14.046%
8	7.220	989	995	1002	rBV3	8335	18893	1.26%	0.241%
9	8.713	1231	1240	1256	rBV	982242	1503988	100.00%	19.216%
10	10.110	1463	1469	1478	rBV	899685	1222744	81.30%	15.623%
11	11.134	1627	1637	1648	rBV	708243	906426	60.27%	11.581%
12	12.079	1785	1792	1800	rBV	800001	1005782	66.87%	12.851%


Sum of corrected areas: 7826558

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032119\
Data File : VX008292.D
Acq On : 21 Mar 2019 15:48
Operator : JC/SP
Sample : K1963-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW307I-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

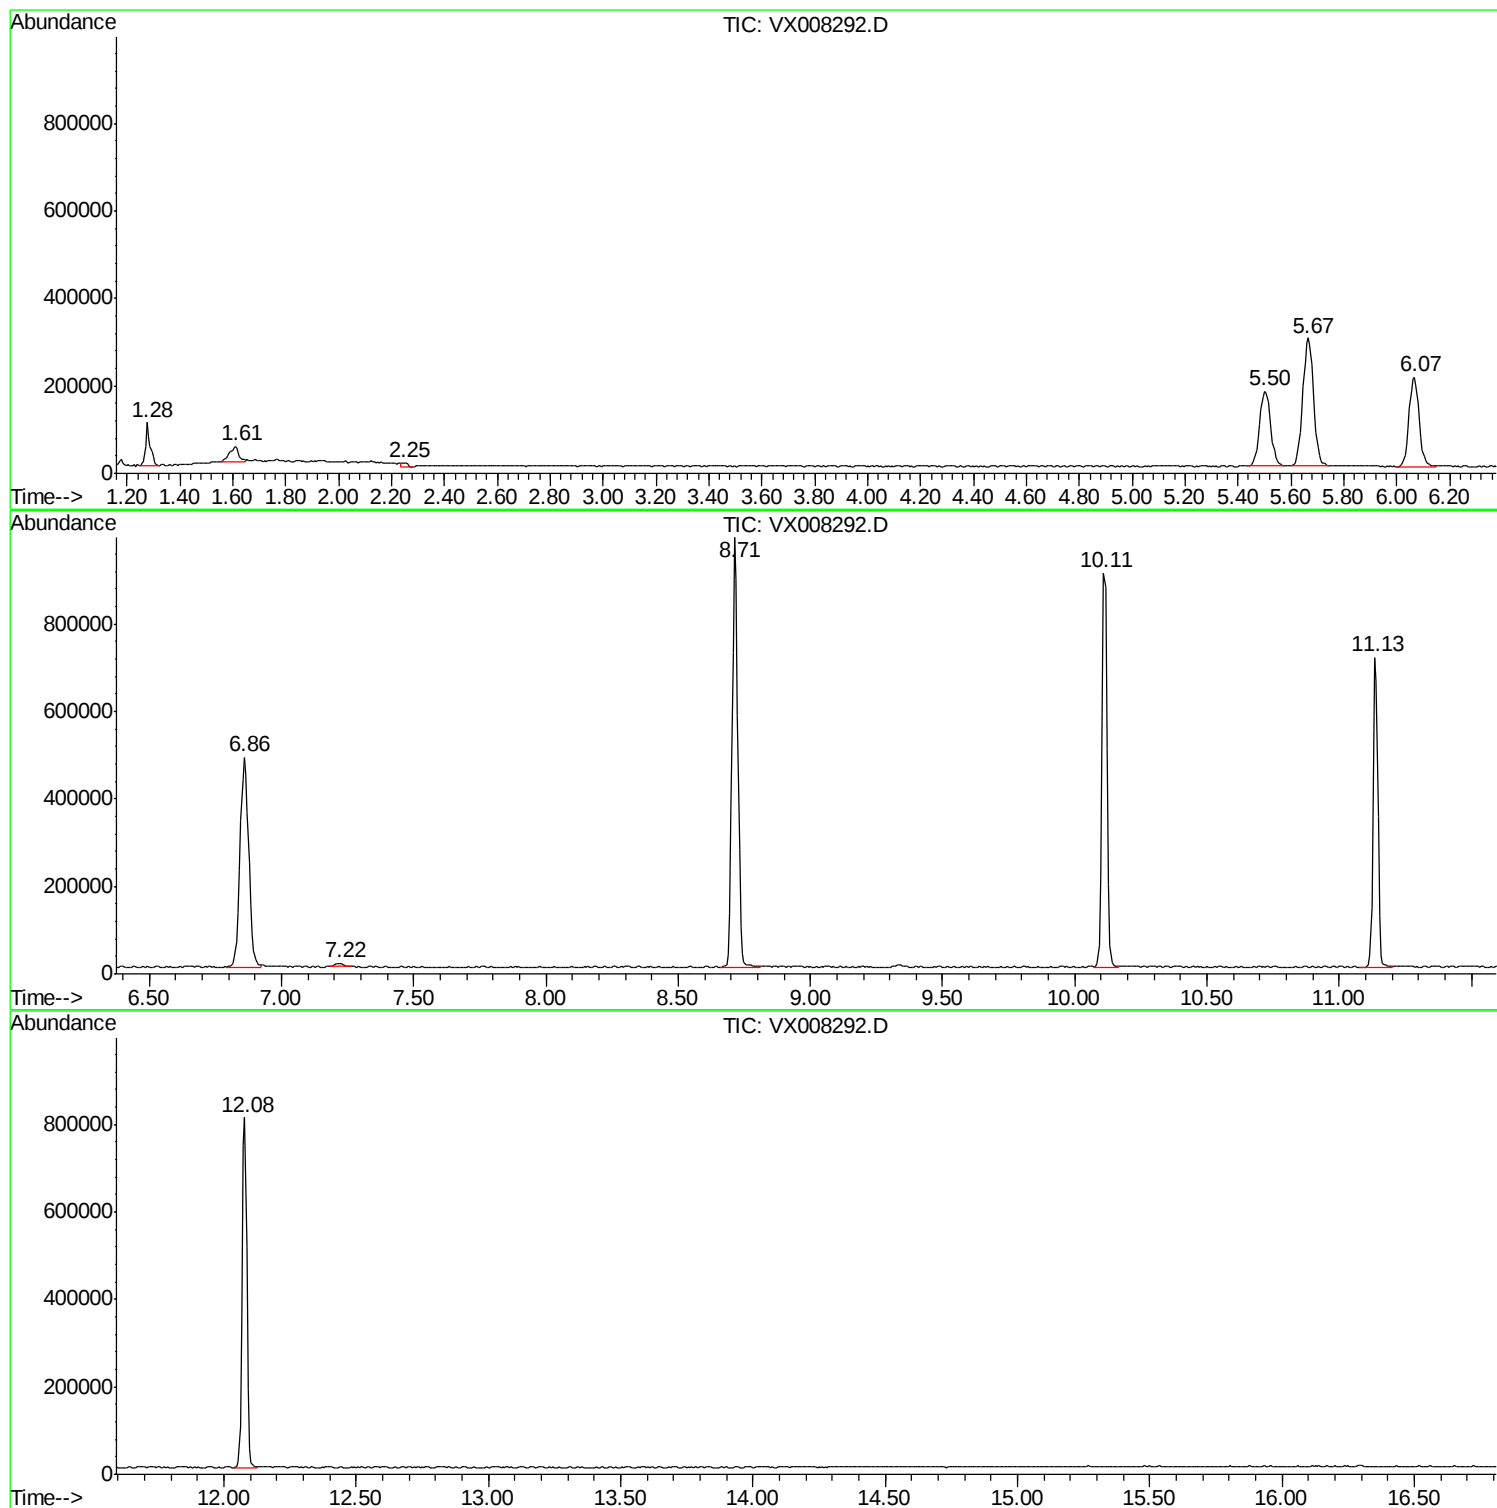

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX032119\
Data File : VX008292.D
Acq On : 21 Mar 2019 15:48
Operator : JC/SP
Sample : K1963-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW307I-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX032119\
Data File : VX008292.D
Acq On : 21 Mar 2019 15:48
Operator : JC/SP
Sample : K1963-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW307I-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc