


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032119\
Data File : VX008282.D
Acq On : 21 Mar 2019 09:09
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031919W.M
Title : SW846 8260
Last Update : Tue Mar 19 13:15:13 2019

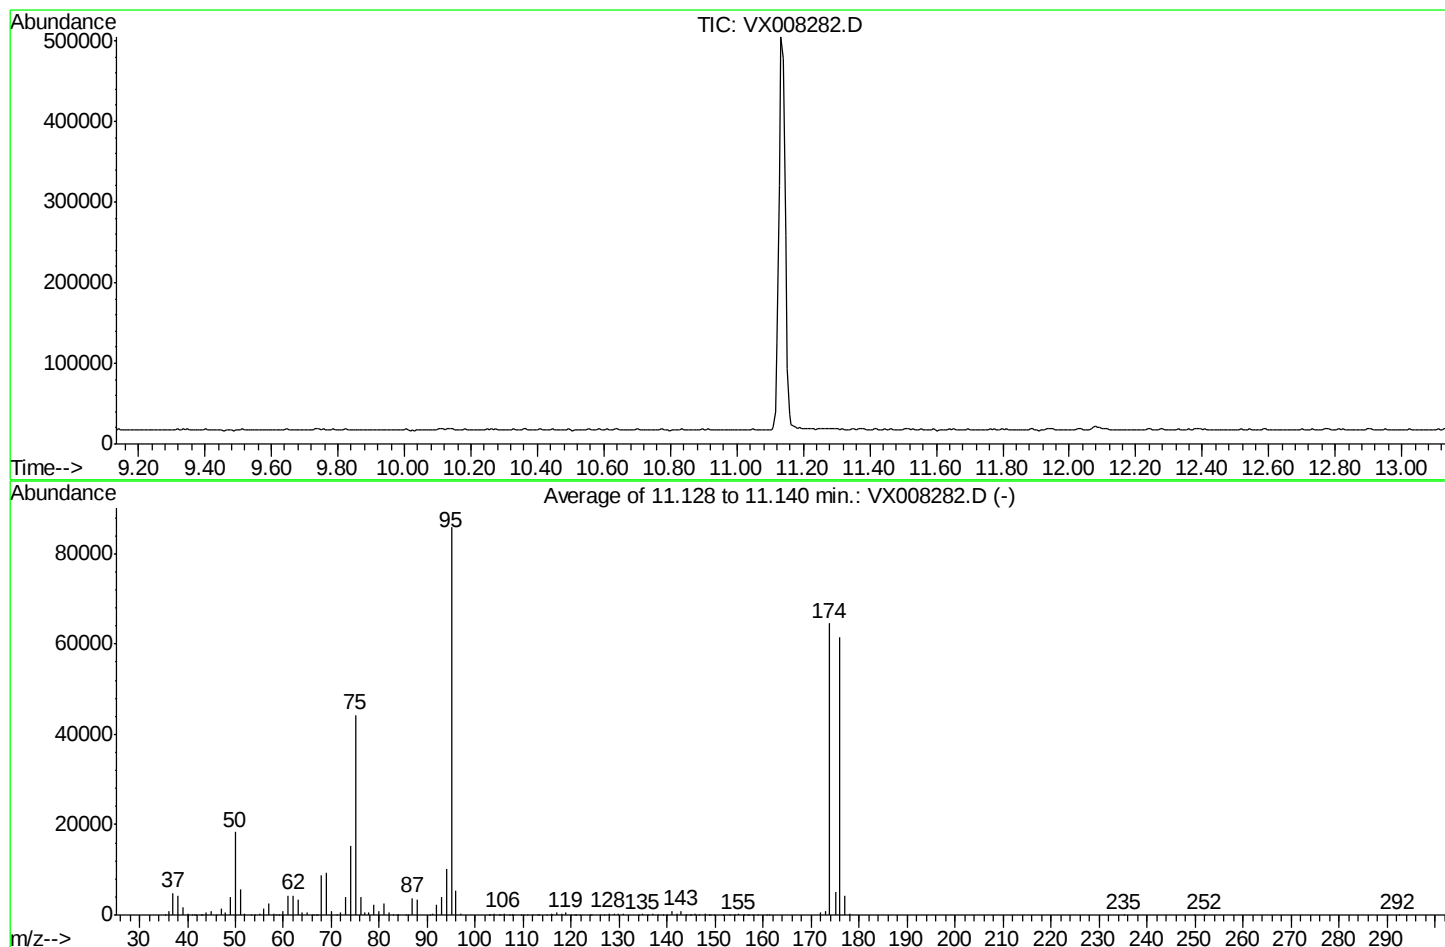

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	18321	PASS
75	95	30	60	51.7	44359	PASS
95	95	100	100	100.0	85861	PASS
96	95	5	9	6.4	5459	PASS
173	174	0.00	2	1.3	815	PASS
174	95	50	100	75.2	64608	PASS
175	174	5	9	7.8	5067	PASS
176	174	95	101	95.4	61656	PASS
177	176	5	9	6.8	4187	PASS