

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021312.D
 Acq On : 19 Mar 2021 19:10
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Mar 20 06:36:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 16 14:00:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.623	168	79431	50.00	ug/l	-0.01
34) 1,4-Difluorobenzene	6.829	114	127463	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	110478	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	46966	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	60358	46.33	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.66%
35) Dibromofluoromethane	5.464	113	43762	50.46	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.92%
50) Toluene-d8	8.694	98	157315	49.99	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.98%
62) 4-Bromofluorobenzene	11.118	95	54843	44.87	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.74%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021312.D
Acq On : 19 Mar 2021 19:10
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Mar 20 06:36:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 16 14:00:21 2021
Response via : Initial Calibration




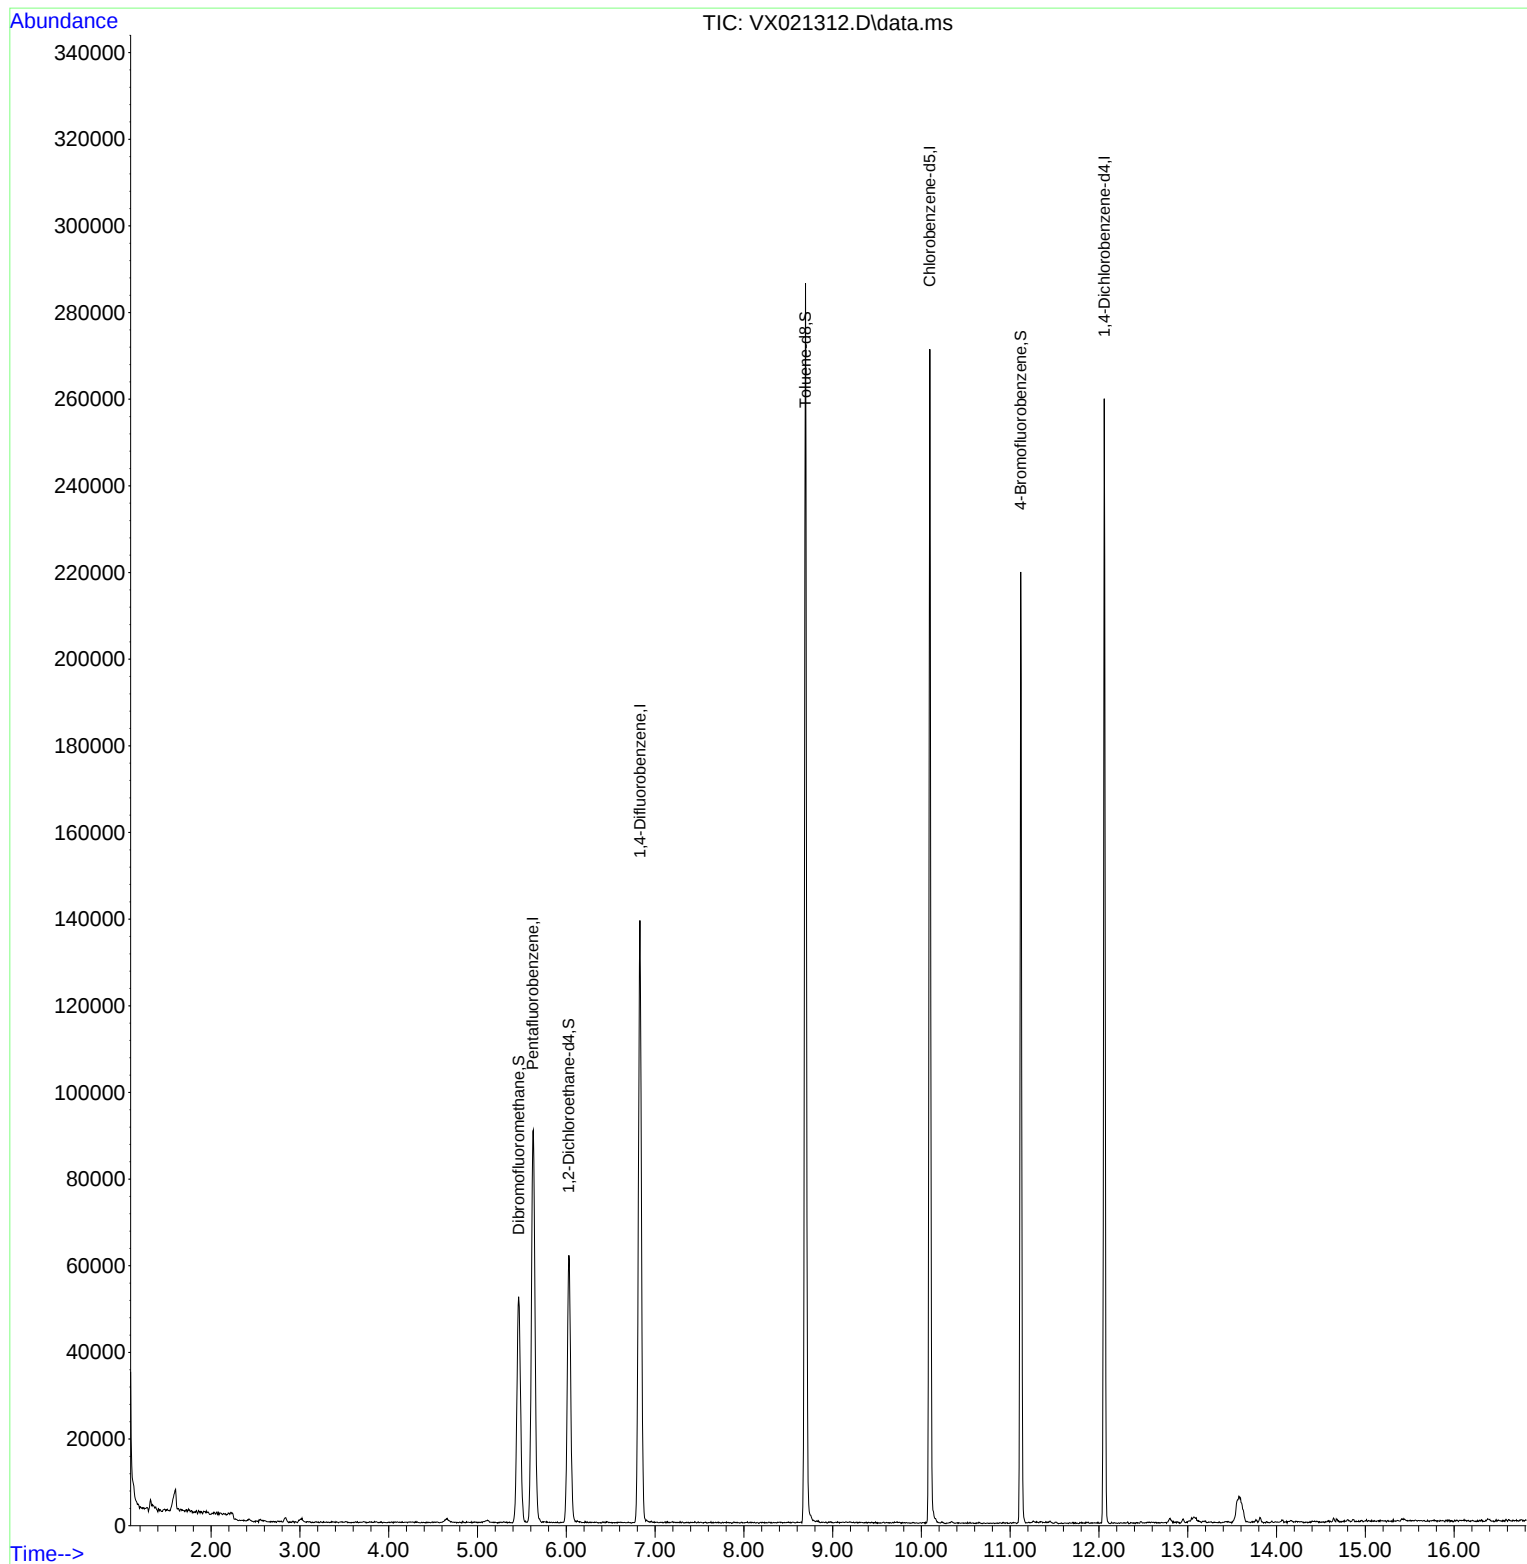


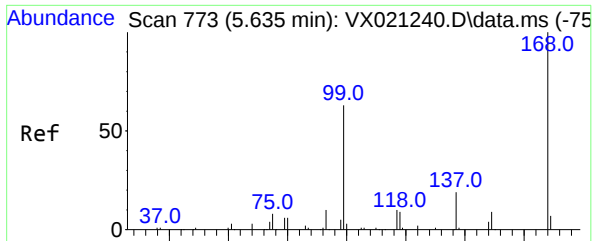

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.012 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 79431
Ion Ratio Lower Upper
168 100
99 62.4 45.8 68.6

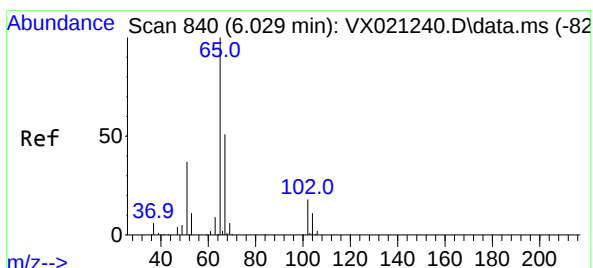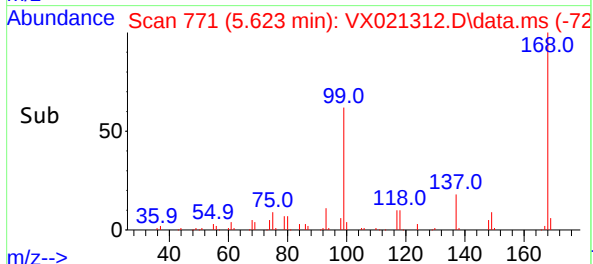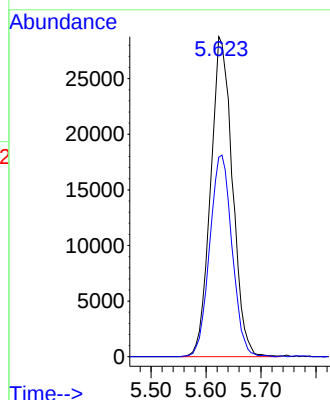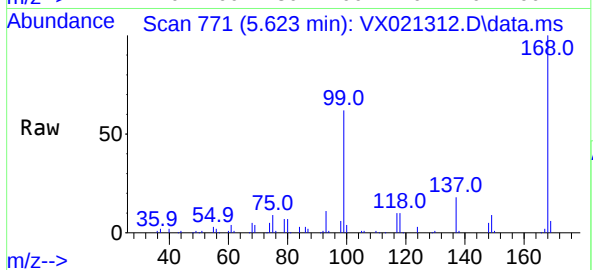

#33
1,2-Dichloroethane-d4
Concen: 46.33 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10


Tgt Ion: 65 Resp: 60358
Ion Ratio Lower Upper
65 100
67 50.9 0.0 105.4

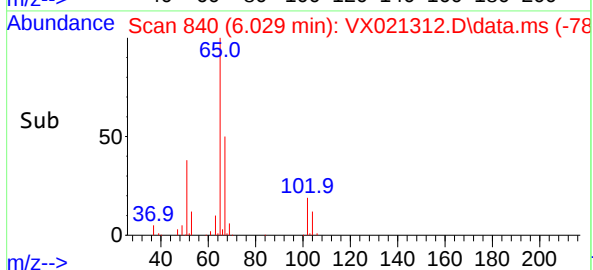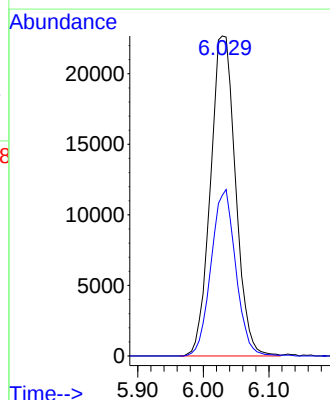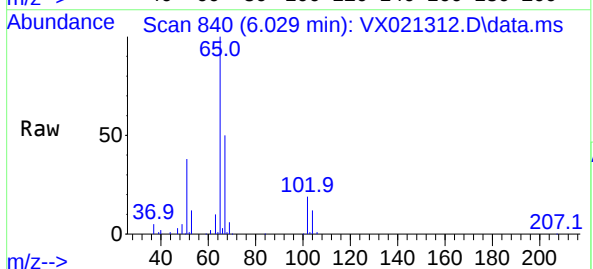



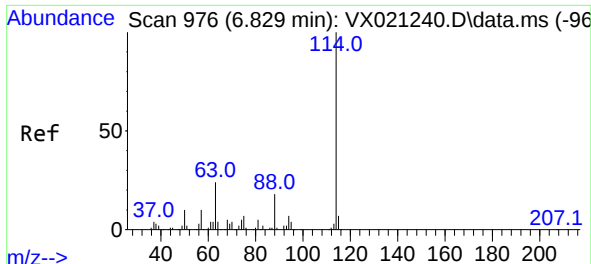


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. 0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10


Instrument :
MSVOA_X
ClientSampled :
IBLK

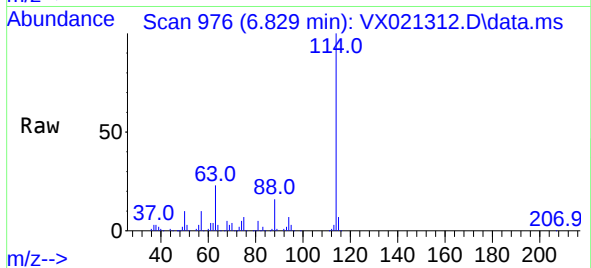



Tgt Ion:114 Resp: 127463
Ion Ratio Lower Upper
114 100
63 23.2 0.0 40.8
88 15.8 0.0 32.8

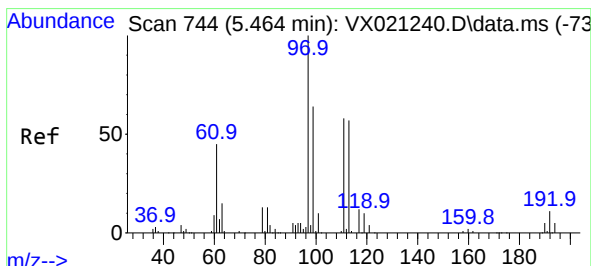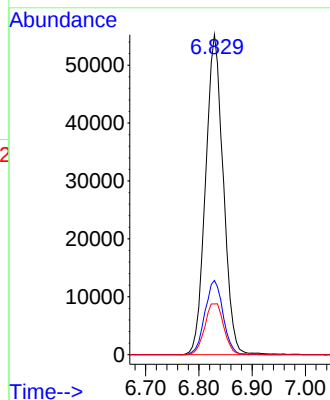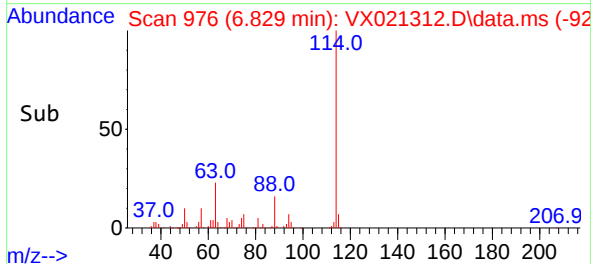


#35
Dibromofluoromethane
Concen: 50.46 ug/l
RT: 5.464 min Scan# 744
Delta R.T. 0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10

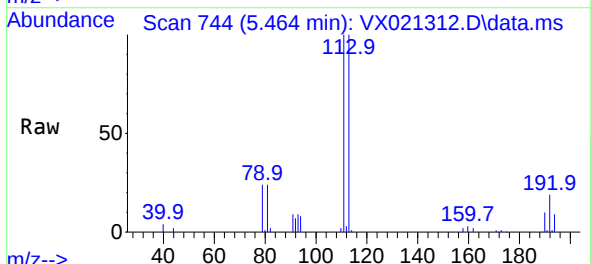

Tgt Ion:113 Resp: 43762
Ion Ratio Lower Upper
113 100
111 102.3 81.9 122.9
192 18.2 16.7 25.1



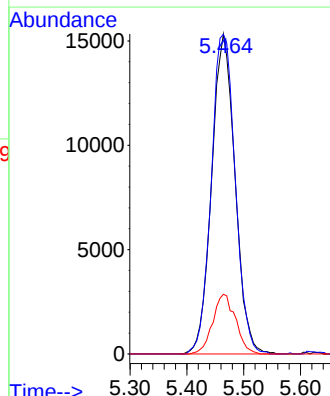
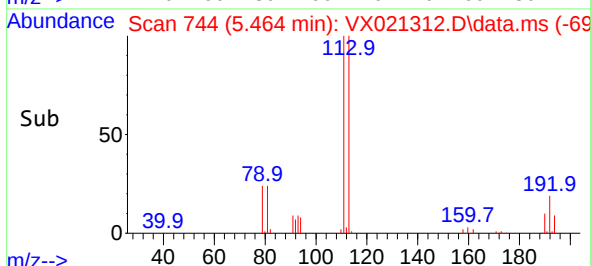


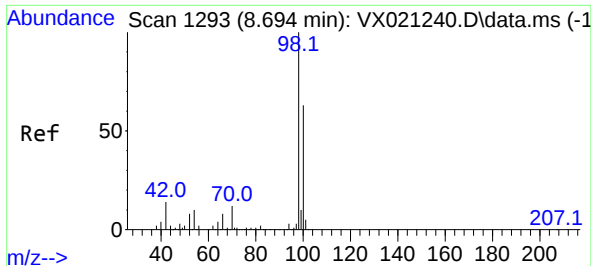

#50
Toluene-d8
Concen: 49.99 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10




Instrument :
MSVOA_X
ClientSampled :
IBLK


Tgt Ion: 98 Resp: 157315
Ion Ratio Lower Upper
98 100
100 63.3 51.9 77.9

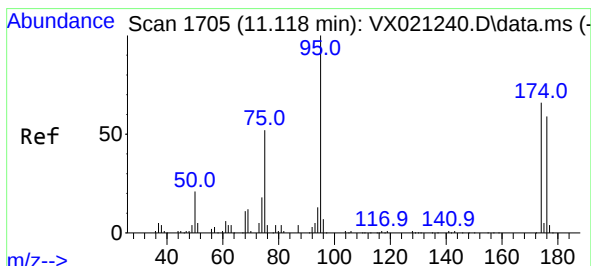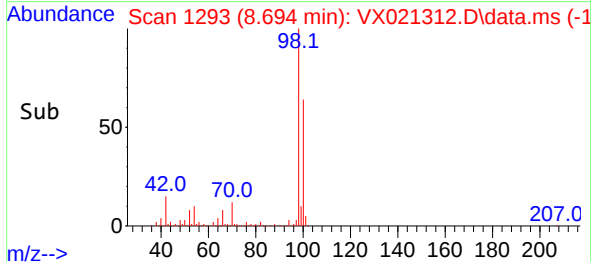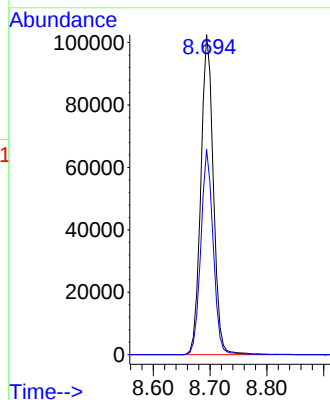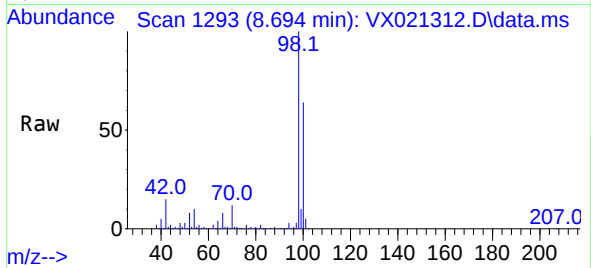

#62
4-Bromofluorobenzene
Concen: 44.87 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10

Tgt Ion: 95 Resp: 54843
Ion Ratio Lower Upper
95 100
174 73.2 0.0 154.6
176 68.6 0.0 155.8


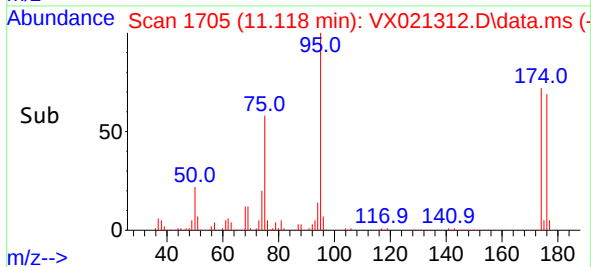
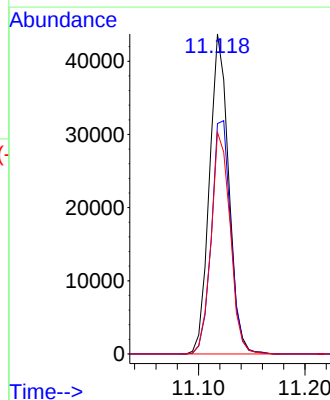
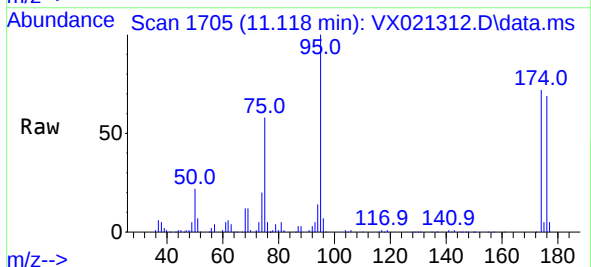


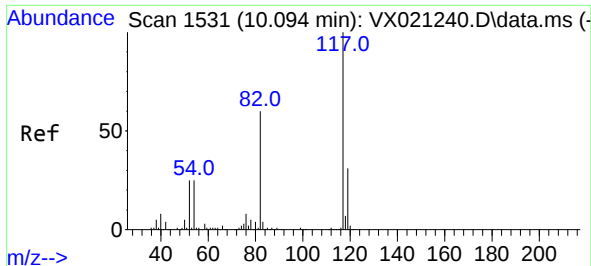

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 110478
Ion Ratio Lower Upper
117 100
82 60.5 47.4 71.2
119 33.8 26.6 39.8

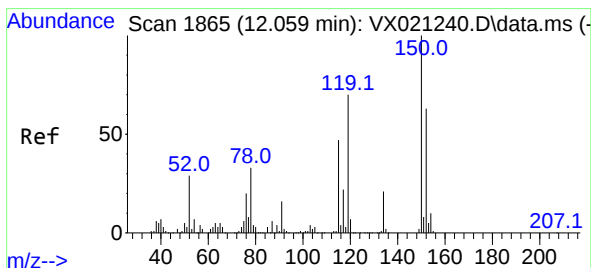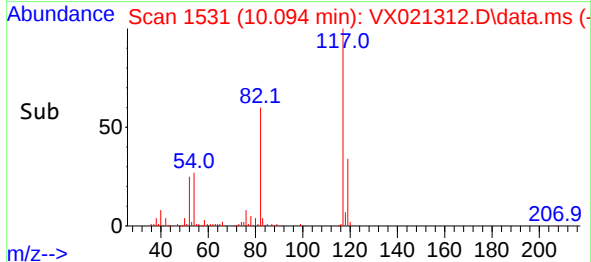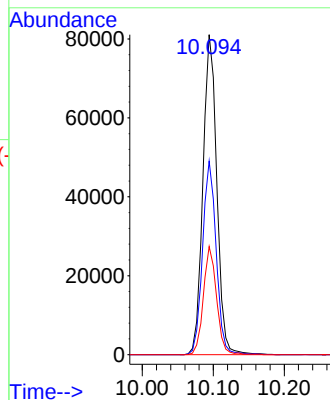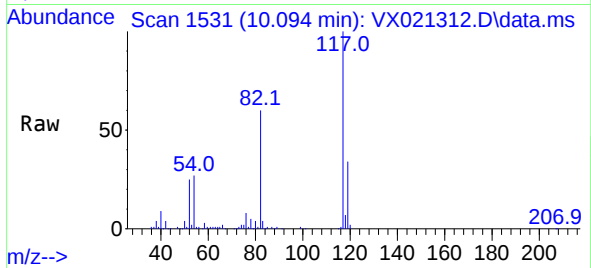

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021312.D
Acq: 19 Mar 2021 19:10

Tgt Ion:152 Resp: 46966
Ion Ratio Lower Upper
152 100
115 62.9 41.1 123.3
150 157.1 0.0 349.0

