

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021313.D
 Acq On : 19 Mar 2021 19:33
 Operator : JC/MD
 Sample : M1687-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1033-1042

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260

Signal : TIC: VX021313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.605	76	88	90	rBV7	4250	10416	2.38%	0.376%
2	2.422	221	227	236	rBV	22307	38488	8.79%	1.389%
3	2.581	246	254	260	rBV	5138	10031	2.29%	0.362%
4	4.634	592	603	621	rBV	49717	146813	33.51%	5.299%
5	5.464	732	744	758	rBB	51669	147604	33.69%	5.327%
6	5.629	760	772	784	rBV	91686	251790	57.47%	9.087%
7	6.029	830	840	852	rBV	62046	161571	36.88%	5.831%
8	6.829	964	976	991	rBV	136345	324157	73.99%	11.699%
9	8.694	1286	1293	1300	rBV	281025	438096	100.00%	15.811%
10	8.764	1300	1305	1315	rVB	100521	153300	34.99%	5.533%
11	9.317	1393	1399	1405	rVB	27448	39332	8.98%	1.420%
12	9.559	1433	1440	1448	rVB3	3743	5989	1.37%	0.216%
13	10.094	1525	1531	1550	rVB	279499	371803	84.87%	13.419%
14	10.341	1568	1573	1577	rBV	4535	6113	1.40%	0.221%
15	10.682	1627	1631	1635	rBV	5434	6899	1.57%	0.249%
16	11.118	1699	1705	1717	rBV	223208	286120	65.31%	10.326%
17	12.059	1860	1865	1871	rBV	271323	330717	75.49%	11.936%
18	12.253	1894	1898	1908	rBV3	4249	8074	1.84%	0.291%
19	13.583	2110	2124	2140	rVB10	4819	18913	4.32%	0.683%
20	13.818	2159	2164	2168	rBV	5794	7064	1.61%	0.255%
21	16.389	2595	2601	2607	rVB2	3882	7485	1.71%	0.270%




Sum of corrected areas: 2770775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021313.D
Acq On : 19 Mar 2021 19:33
Operator : JC/MD
Sample : M1687-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1033-1042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

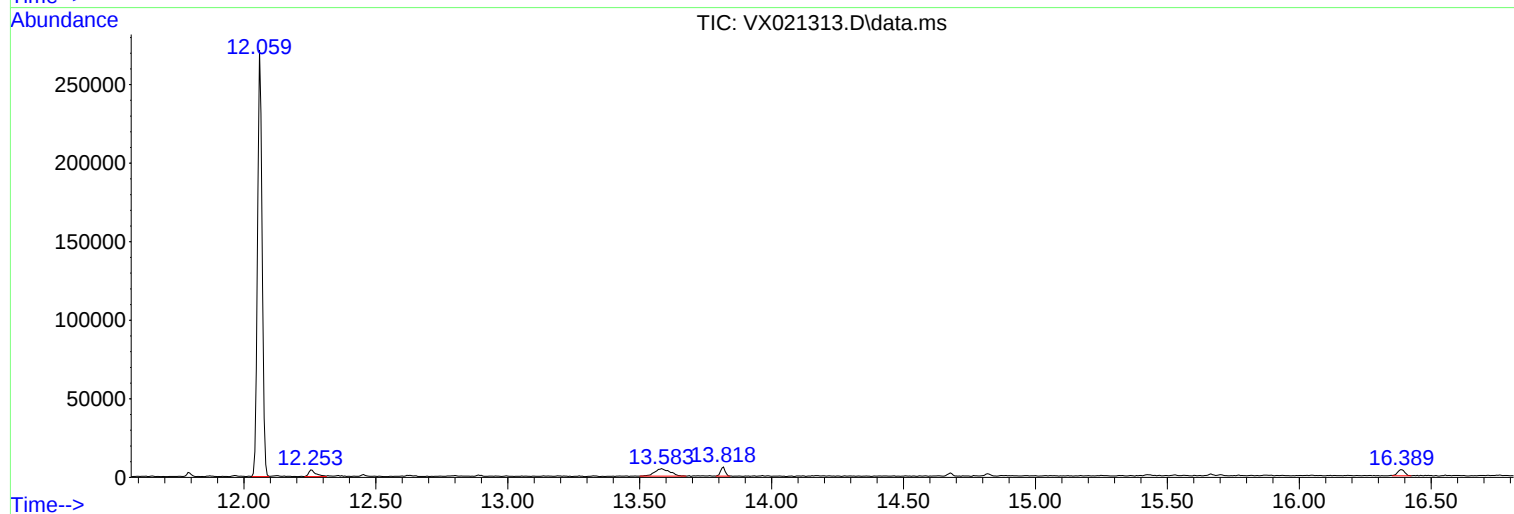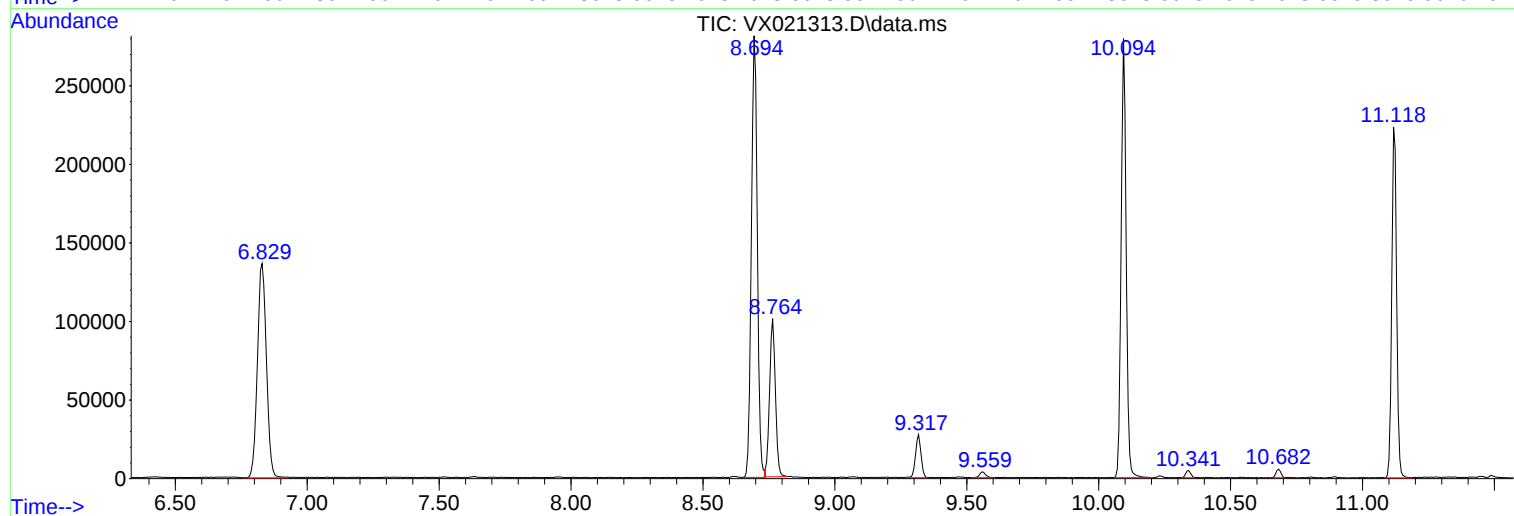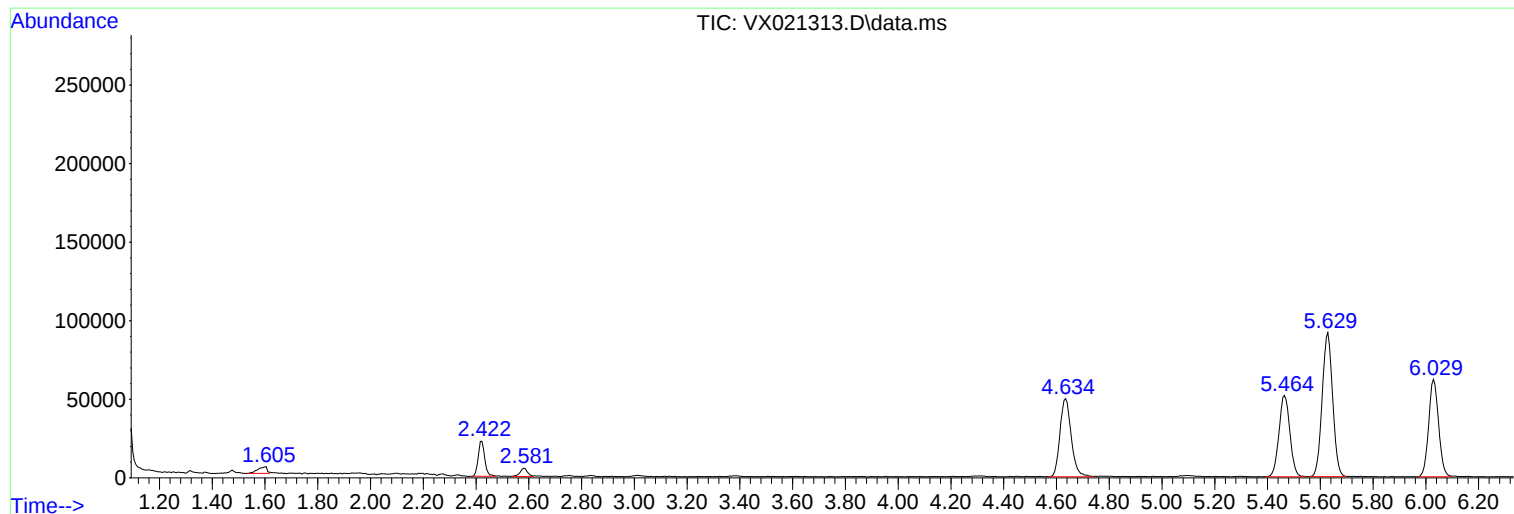

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021313.D
Acq On : 19 Mar 2021 19:33
Operator : JC/MD
Sample : M1687-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1033-1042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021313.D
Acq On : 19 Mar 2021 19:33
Operator : JC/MD
Sample : M1687-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1033-1042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
