

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021317.D
 Acq On : 19 Mar 2021 21:07
 Operator : JC/MD
 Sample : M1736-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D2-20210317

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260

Signal : TIC: VX021317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	208	217	225	rBV2	59874	117369	3.20%	1.878%
2	5.464	733	744	759	rBV	54462	157918	4.31%	2.526%
3	5.629	760	772	785	rBV2	96289	269165	7.34%	4.306%
4	6.029	828	840	853	rBV	65031	172258	4.70%	2.756%
5	6.829	965	976	989	rBV	149133	344921	9.40%	5.518%
6	7.188	1025	1037	1056	rBV	1764269	3667466	100.00%	58.673%
7	8.694	1285	1293	1307	rBV	299730	468916	12.79%	7.502%
8	9.318	1393	1399	1407	rVB	36218	53183	1.45%	0.851%
9	10.094	1524	1531	1549	rVB	278093	386076	10.53%	6.177%
10	11.118	1699	1705	1716	rBV	225856	289158	7.88%	4.626%
11	12.059	1860	1865	1878	rVB	263852	324289	8.84%	5.188%




Sum of corrected areas: 6250719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021317.D
Acq On : 19 Mar 2021 21:07
Operator : JC/MD
Sample : M1736-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

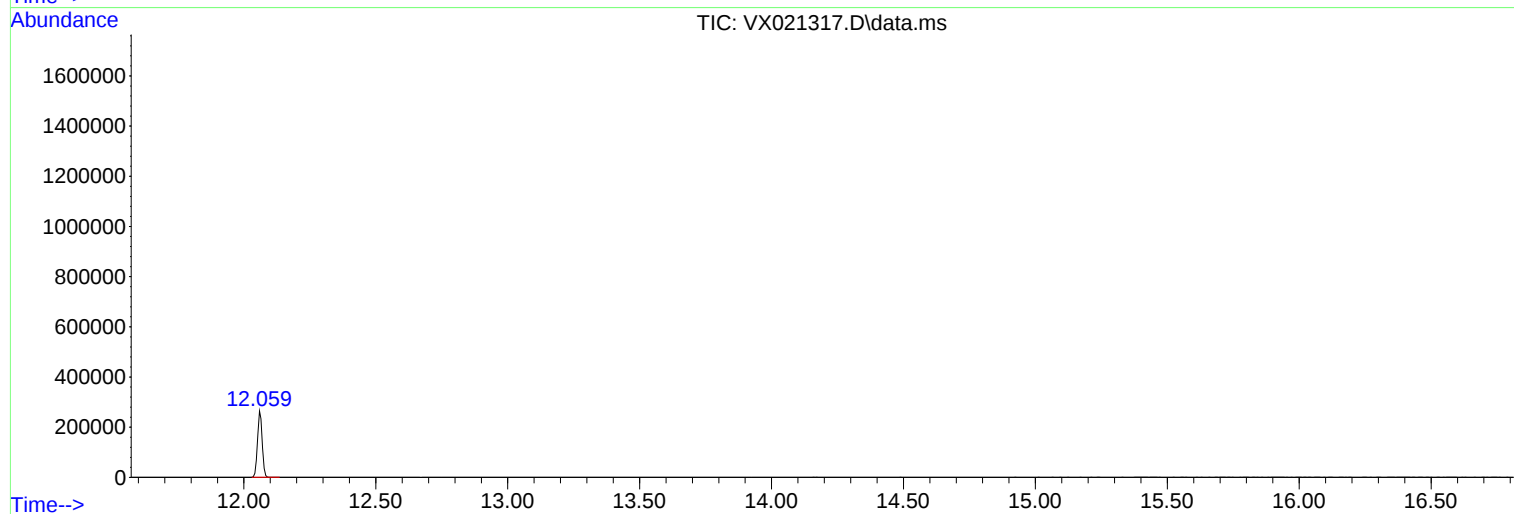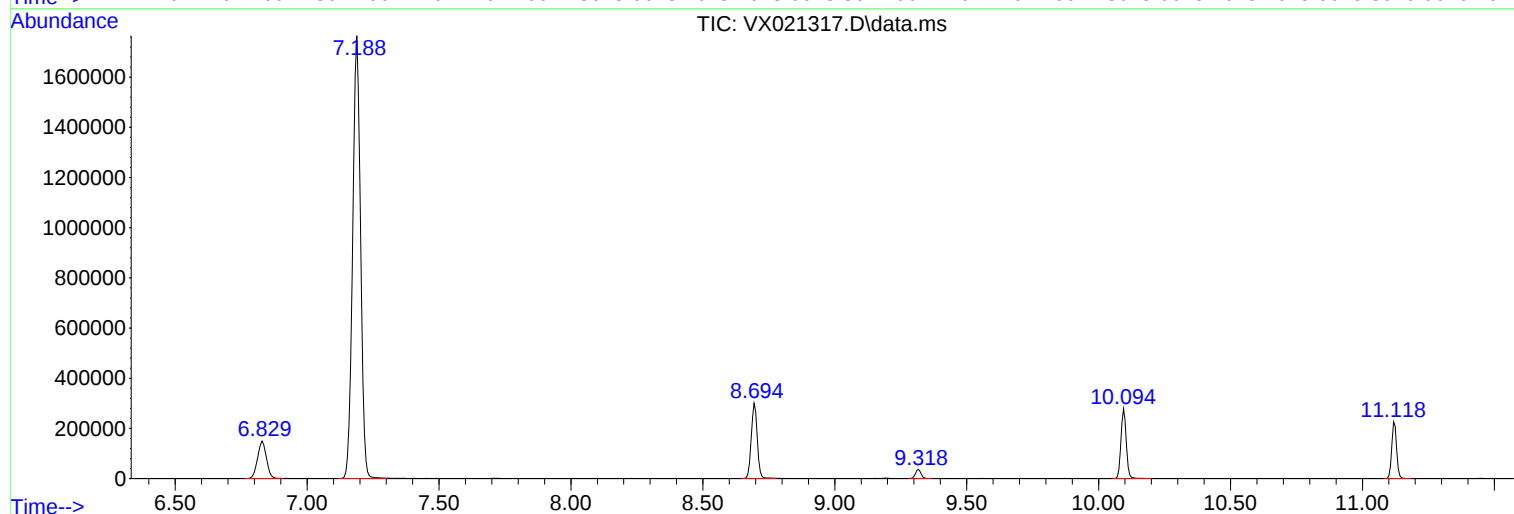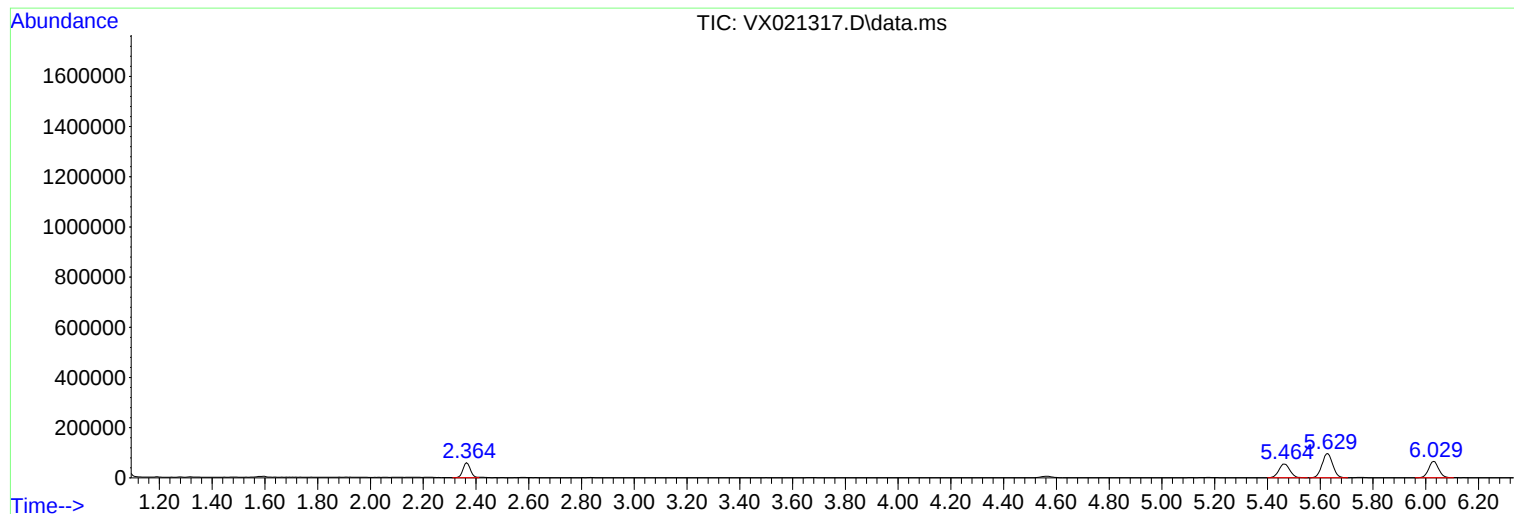

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021317.D
Acq On : 19 Mar 2021 21:07
Operator : JC/MD
Sample : M1736-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021317.D
Acq On : 19 Mar 2021 21:07
Operator : JC/MD
Sample : M1736-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
