

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021318.D
 Acq On : 19 Mar 2021 21:30
 Operator : JC/MD
 Sample : M1736-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20210317

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	79	85	90	rVB3	2929	6098	1.39%	0.253%
2	2.582	246	254	264	rBV	2918	6386	1.46%	0.265%
3	5.464	731	744	758	rBV2	53100	151270	34.57%	6.273%
4	5.629	761	772	784	rVV	92008	255181	58.32%	10.582%
5	6.029	829	840	854	rBV	62346	164553	37.61%	6.824%
6	6.829	965	976	989	rBV	140293	328462	75.07%	13.621%
7	7.188	1025	1037	1046	rBV	80854	173404	39.63%	7.191%
8	8.694	1286	1293	1301	rBV	286689	437529	100.00%	18.144%
9	10.094	1523	1531	1546	rBV	263404	354659	81.06%	14.707%
10	11.118	1699	1705	1716	rBV	202251	257220	58.79%	10.667%
11	12.059	1860	1865	1877	rVB	229463	276667	63.23%	11.473%




Sum of corrected areas: 2411429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021318\
Data File : VX021318.D
Acq On : 19 Mar 2021 21:30
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

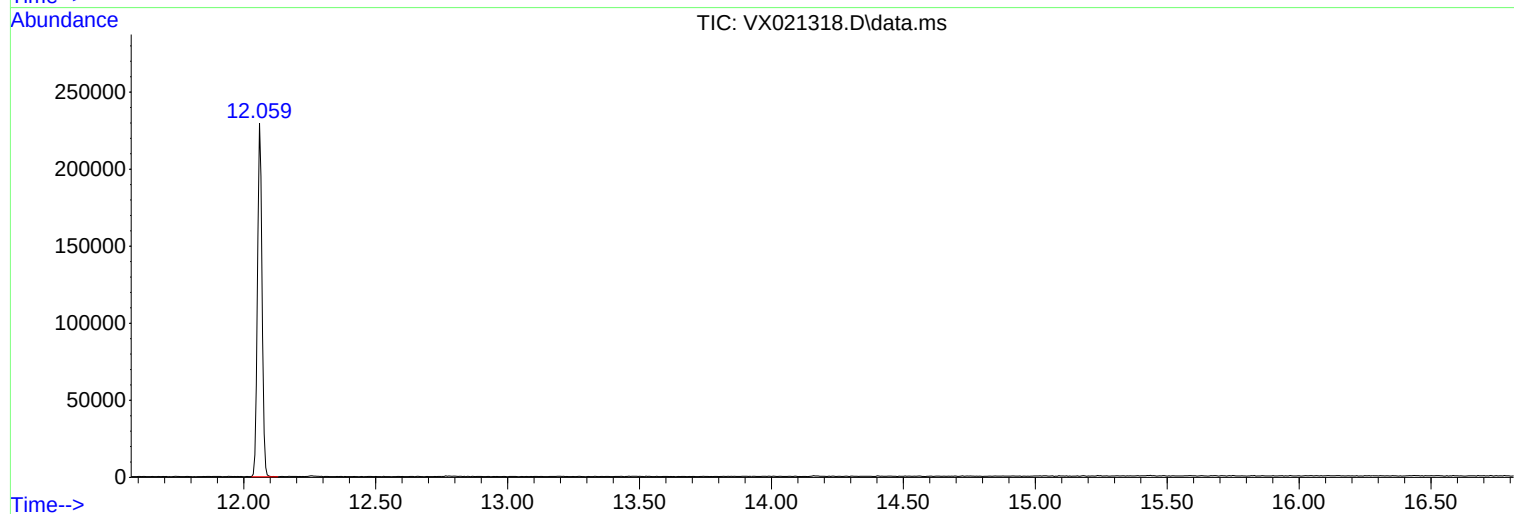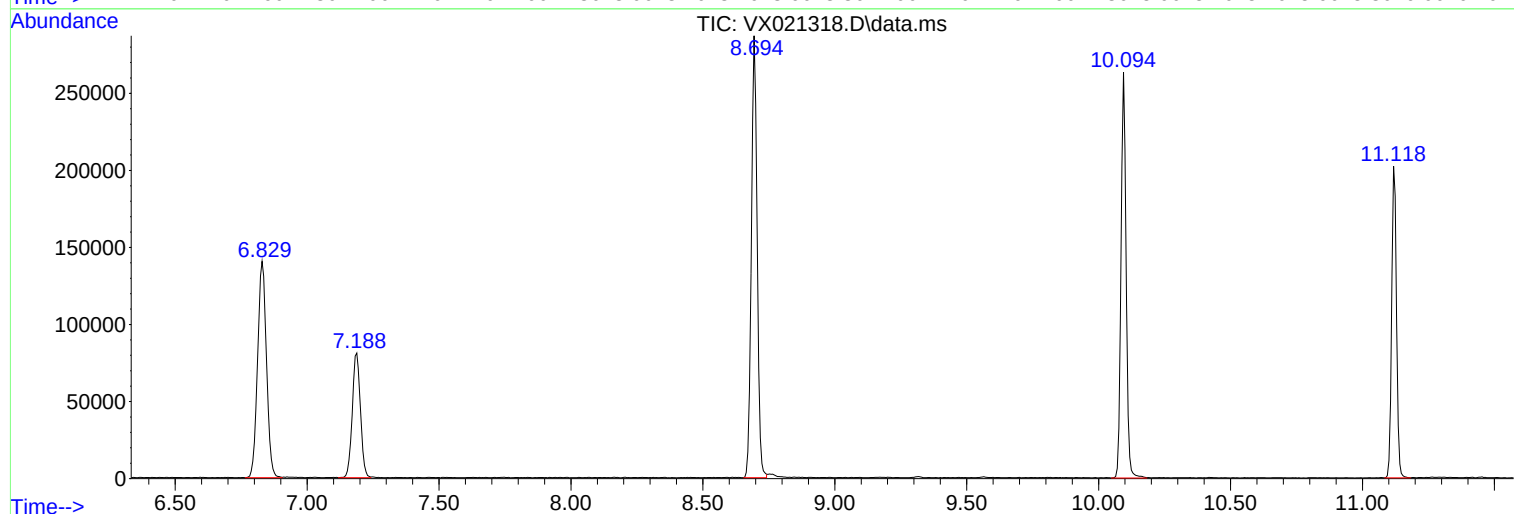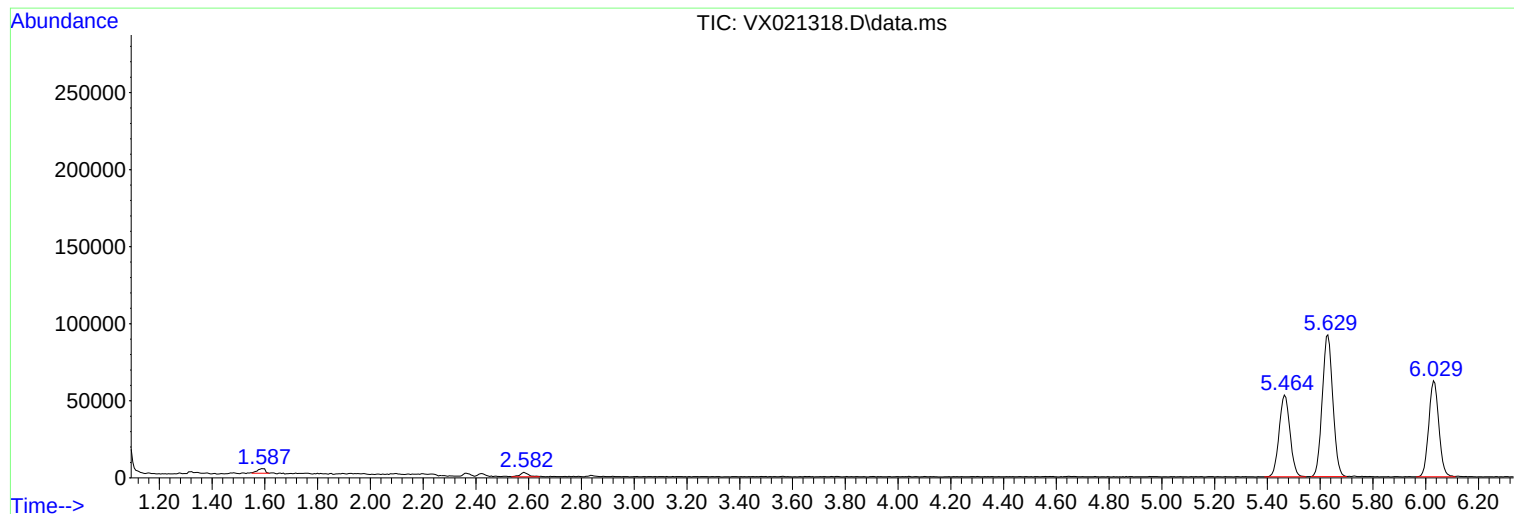

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021318.D
Acq On : 19 Mar 2021 21:30
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021318.D
Acq On : 19 Mar 2021 21:30
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
