

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021327.D
 Acq On : 20 Mar 2021 05:29
 Operator : JC/MD
 Sample : M1735-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE134D4-20210315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	207	217	233	rVB	603742	1151278	100.00%	30.774%
2	5.464	732	744	758	rBV2	54419	154087	13.38%	4.119%
3	5.623	760	771	789	rVV2	89312	255823	22.22%	6.838%
4	6.029	828	840	852	rBV	64773	166327	14.45%	4.446%
5	6.829	966	976	991	rBV	143592	332404	28.87%	8.885%
6	7.188	1027	1037	1050	rBV	85330	183208	15.91%	4.897%
7	8.694	1286	1293	1304	rBV	283886	441336	38.33%	11.797%
8	9.318	1393	1399	1406	rVB	82787	119203	10.35%	3.186%
9	10.094	1525	1531	1541	rBV	270135	364978	31.70%	9.756%
10	11.118	1700	1705	1715	rVB	211018	268057	23.28%	7.165%
11	12.059	1860	1865	1873	rVB	252415	304394	26.44%	8.136%




Sum of corrected areas: 3741095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021327.D
Acq On : 20 Mar 2021 05:29
Operator : JC/MD
Sample : M1735-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D4-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

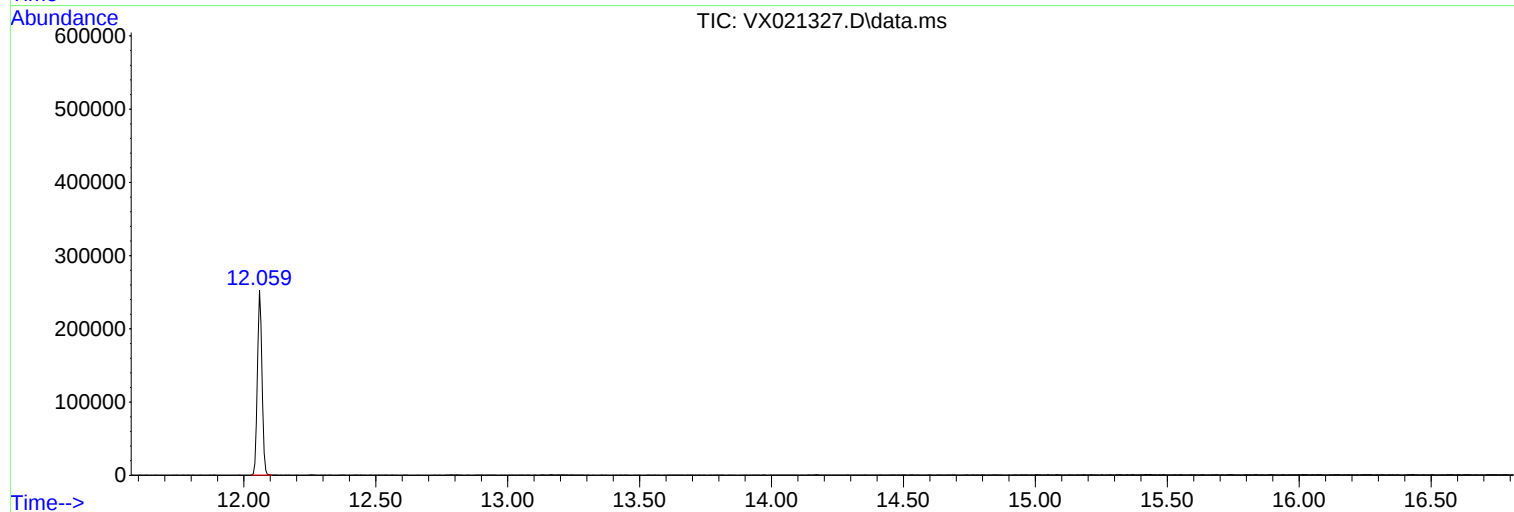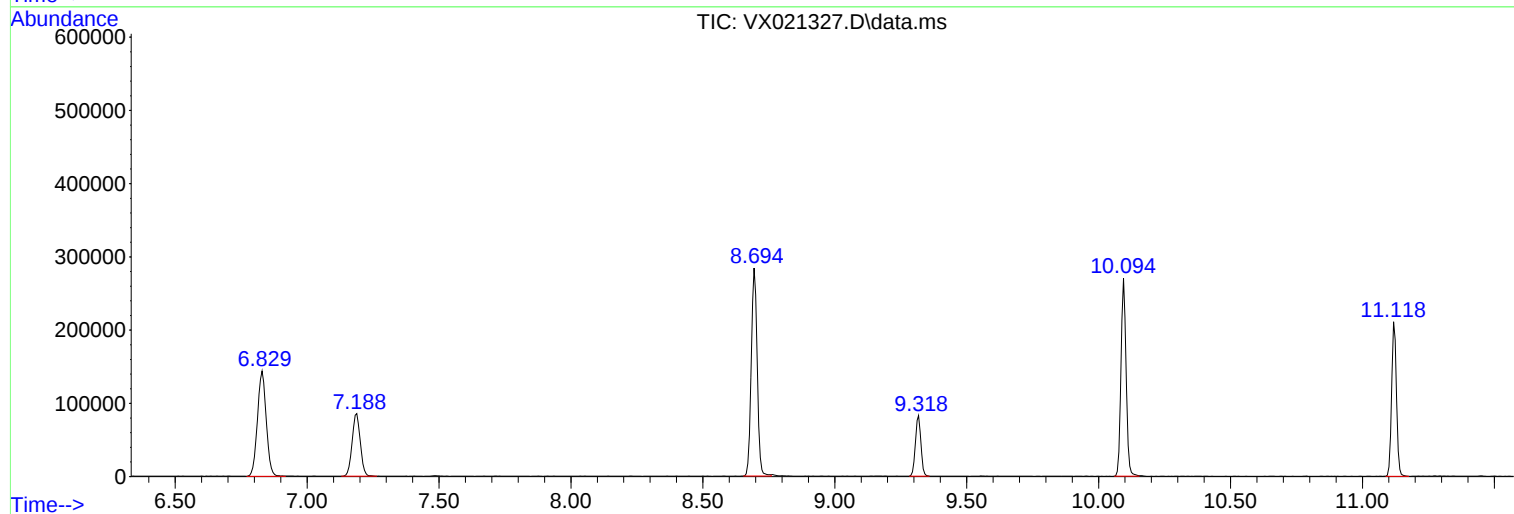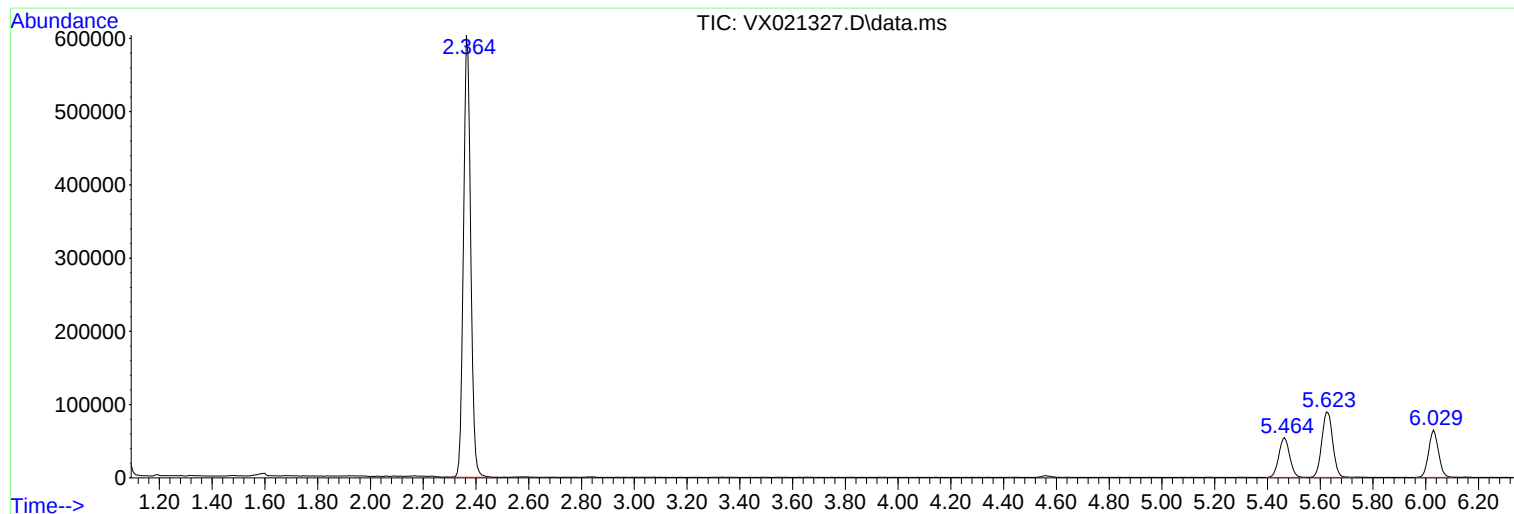

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021327.D
Acq On : 20 Mar 2021 05:29
Operator : JC/MD
Sample : M1735-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D4-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021327.D
Acq On : 20 Mar 2021 05:29
Operator : JC/MD
Sample : M1735-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D4-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
